

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032423\
 Data File : P0093511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 14:17
 Operator : YP/AJ
 Sample : 02052-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1846

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/27/2023
 Supervised By :Ankita Jodhani 03/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:22:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.630	50691036	17996028	16.187	15.956
2) SA Decachlor...	10.257	8.658	40549564	17277696	18.736	17.646
Target Compounds						
26) L6 AR-1254-1	6.465	5.518	10105842	5016435	86.478	79.926
27) L6 AR-1254-2	6.685	5.666	26263706	6362908	153.708	112.914 #
28) L6 AR-1254-3	7.054	6.071	26782538	11555169	161.110	134.216
29) L6 AR-1254-4	7.343	6.301	24693601	8950252	231.650	195.716
30) L6 AR-1254-5	7.765	6.721	38425355	19679025	283.773m	266.466

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032423\
Data File : PO093511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 14:17
Operator : YP/AJ
Sample : 02052-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1846


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/27/2023
Supervised By :Ankita Jodhani 03/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:22:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

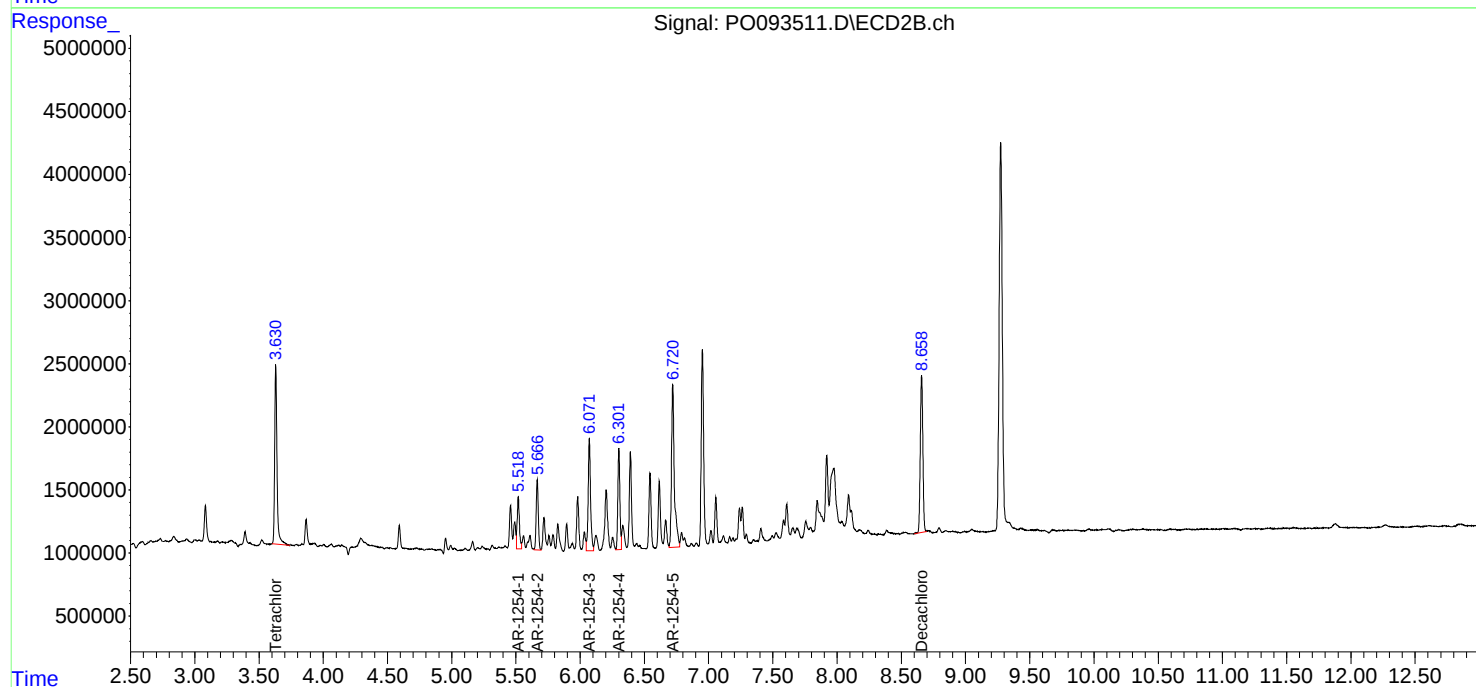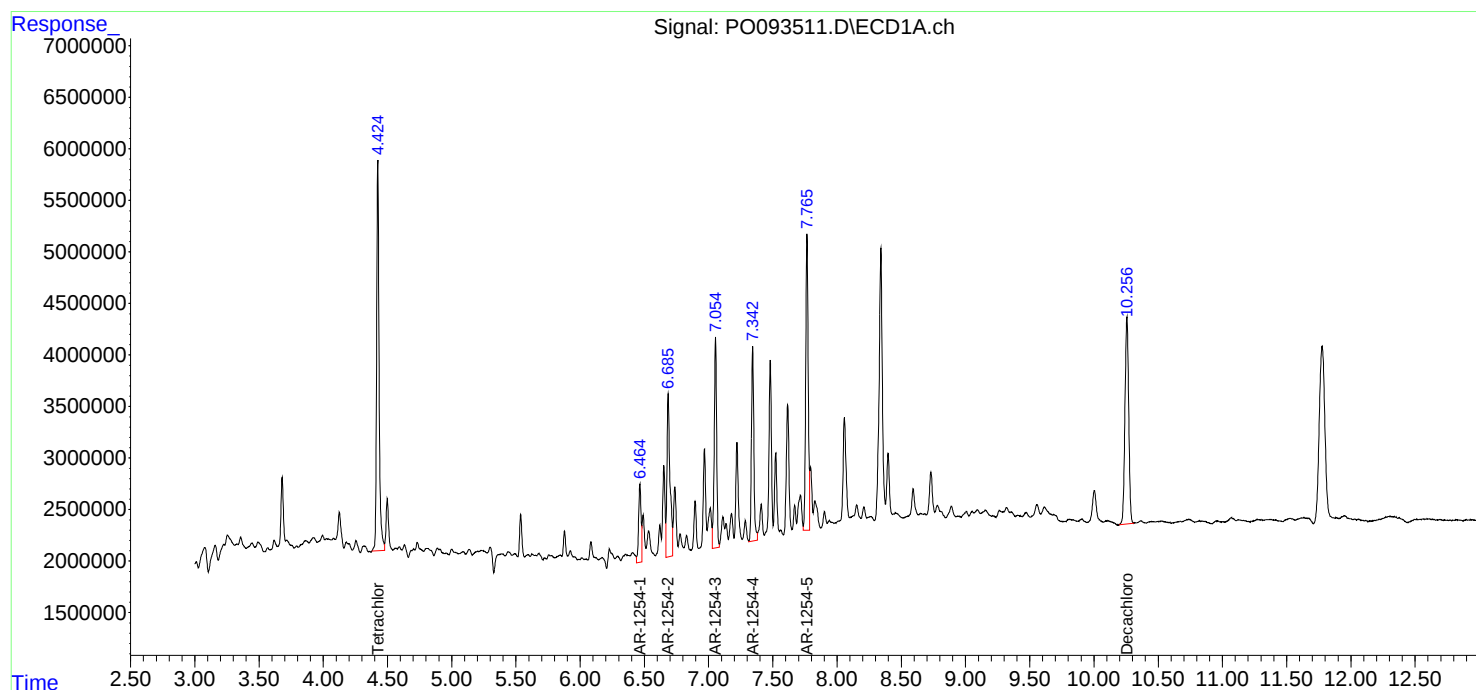

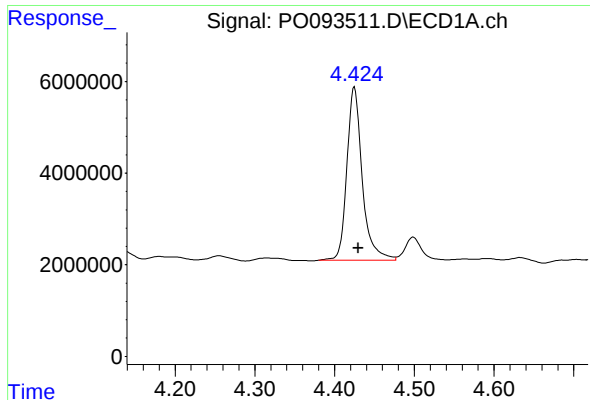


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 50691036
Conc: 16.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1846


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/27/2023
Supervised By :Ankita Jodhani 03/27/2023

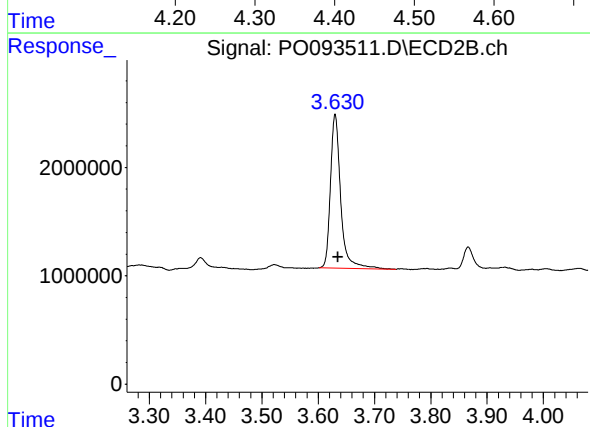


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.005 min
Response: 17996028
Conc: 15.96 ng/ml

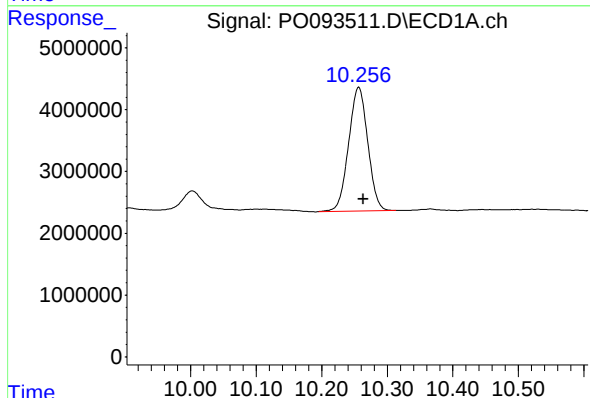


#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: -0.007 min
Response: 40549564
Conc: 18.74 ng/ml

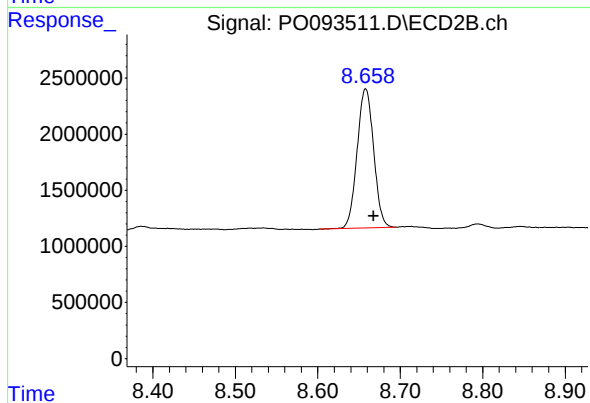

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.010 min
Response: 17277696
Conc: 17.65 ng/ml

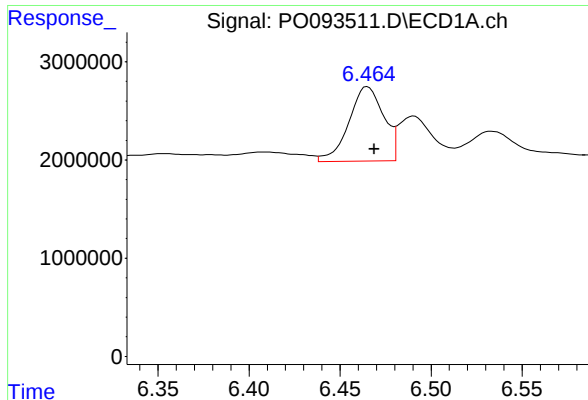


#26 AR-1254-1

R.T.: 6.465 min
Delta R.T.: -0.004 min
Response: 10105842
Conc: 86.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1846


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/27/2023
Supervised By :Ankita Jodhani 03/27/2023

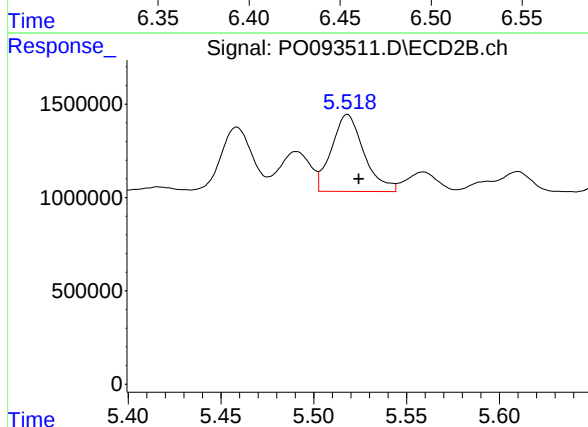


#26 AR-1254-1

R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 5016435
Conc: 79.93 ng/ml

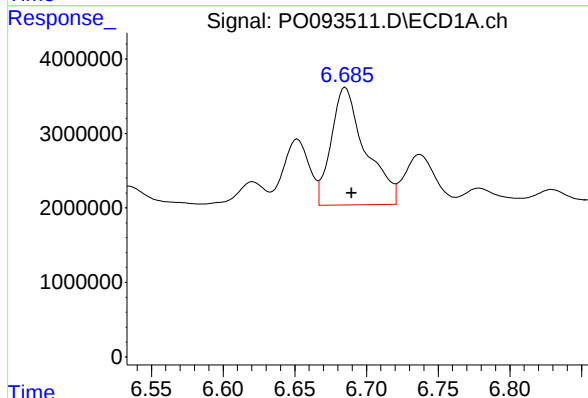


#27 AR-1254-2

R.T.: 6.685 min
Delta R.T.: -0.004 min
Response: 26263706
Conc: 153.71 ng/ml

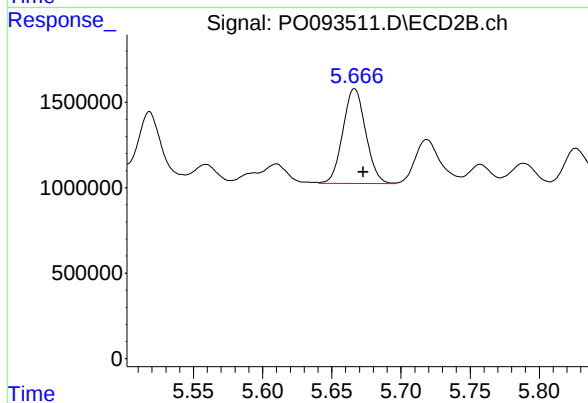

#27 AR-1254-2

R.T.: 5.666 min
Delta R.T.: -0.006 min
Response: 6362908
Conc: 112.91 ng/ml

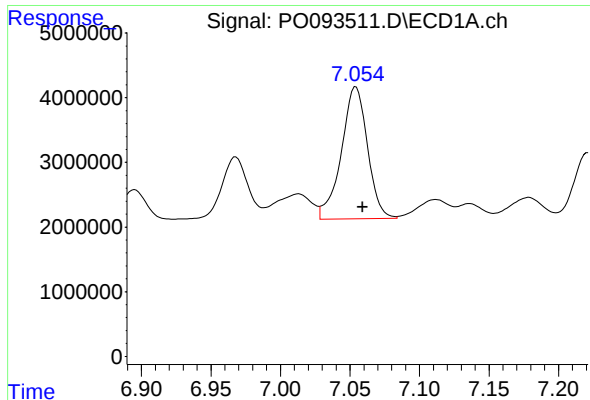


#28 AR-1254-3

R.T.: 7.054 min
Delta R.T.: -0.005 min
Response: 26782538
Conc: 161.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1846


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/27/2023
Supervised By :Ankita Jodhani 03/27/2023

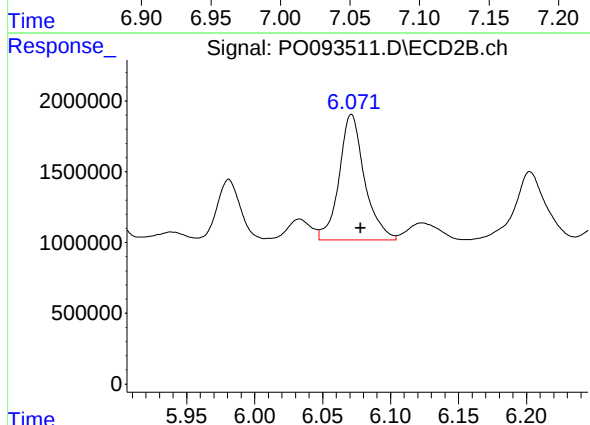


#28 AR-1254-3

R.T.: 6.071 min
Delta R.T.: -0.007 min
Response: 11555169
Conc: 134.22 ng/ml

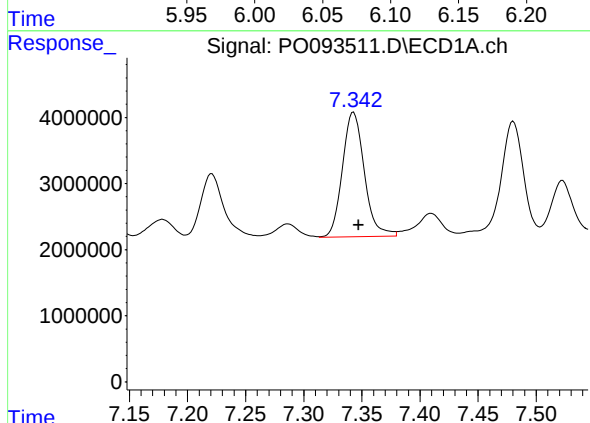


#29 AR-1254-4

R.T.: 7.343 min
Delta R.T.: -0.004 min
Response: 24693601
Conc: 231.65 ng/ml

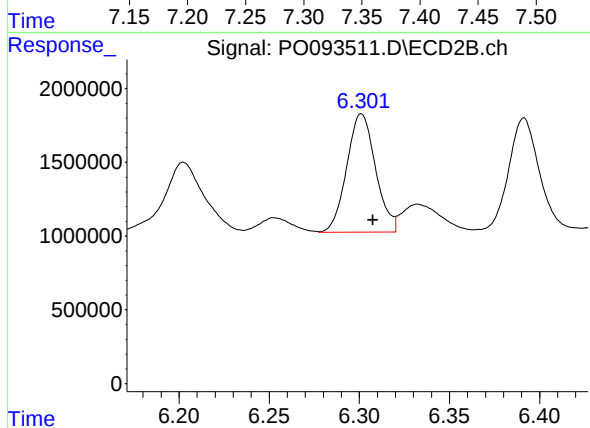

#29 AR-1254-4

R.T.: 6.301 min
Delta R.T.: -0.006 min
Response: 8950252
Conc: 195.72 ng/ml

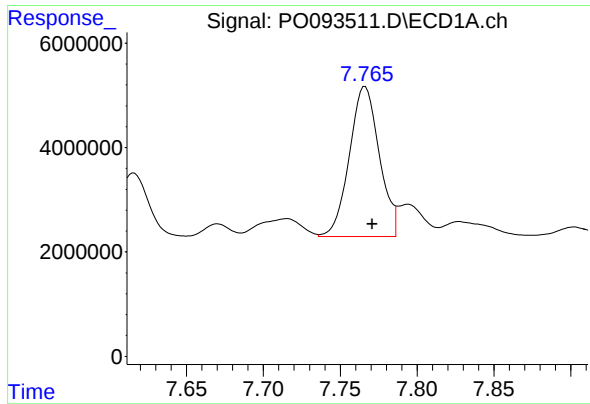


#30 AR-1254-5

R.T.: 7.765 min
Delta R.T.: -0.005 min
Response: 38425355
Conc: 283.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1846

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/27/2023
Supervised By :Ankita Jodhani 03/27/2023

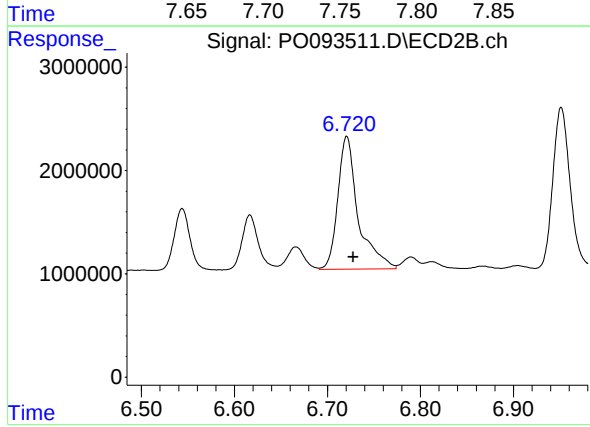

#30 AR-1254-5

R.T.: 6.721 min
Delta R.T.: -0.007 min
Response: 19679025
Conc: 266.47 ng/ml