

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032423\
 Data File : P0093513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 14:52
 Operator : YP/AJ
 Sample : 02058-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHAMBER-B-72-EAST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:23:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.630	37430757	17055798	11.953	15.122 #
2) SA Decachlor...	10.256	8.657	21614975	10549228	9.987	10.774
Target Compounds						
31) L7 AR-1260-1	7.220	6.202	9238300	5928188	71.309	97.505 #
32) L7 AR-1260-2	7.479	6.391	10927847	5755838	74.024	79.614
33) L7 AR-1260-3	7.843	6.545	6456243	4305319	57.399	64.385
34) L7 AR-1260-4	8.069	7.019	8749146	3269986	68.226	59.420
35) L7 AR-1260-5	8.397	7.263	13371457	7097889	59.845	60.289



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032423\
Data File : P0093513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 14:52
Operator : YP/AJ
Sample : 02058-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CHAMBER-B-72-EAST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:23:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

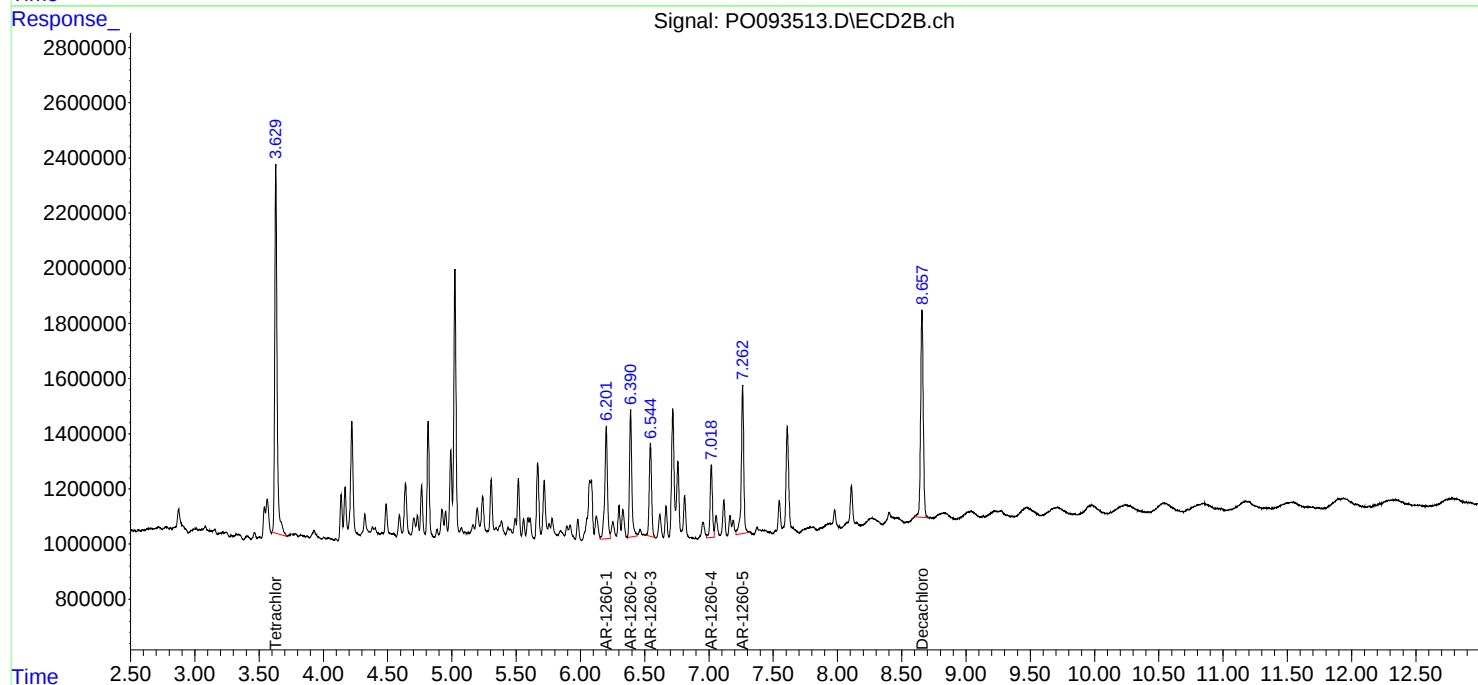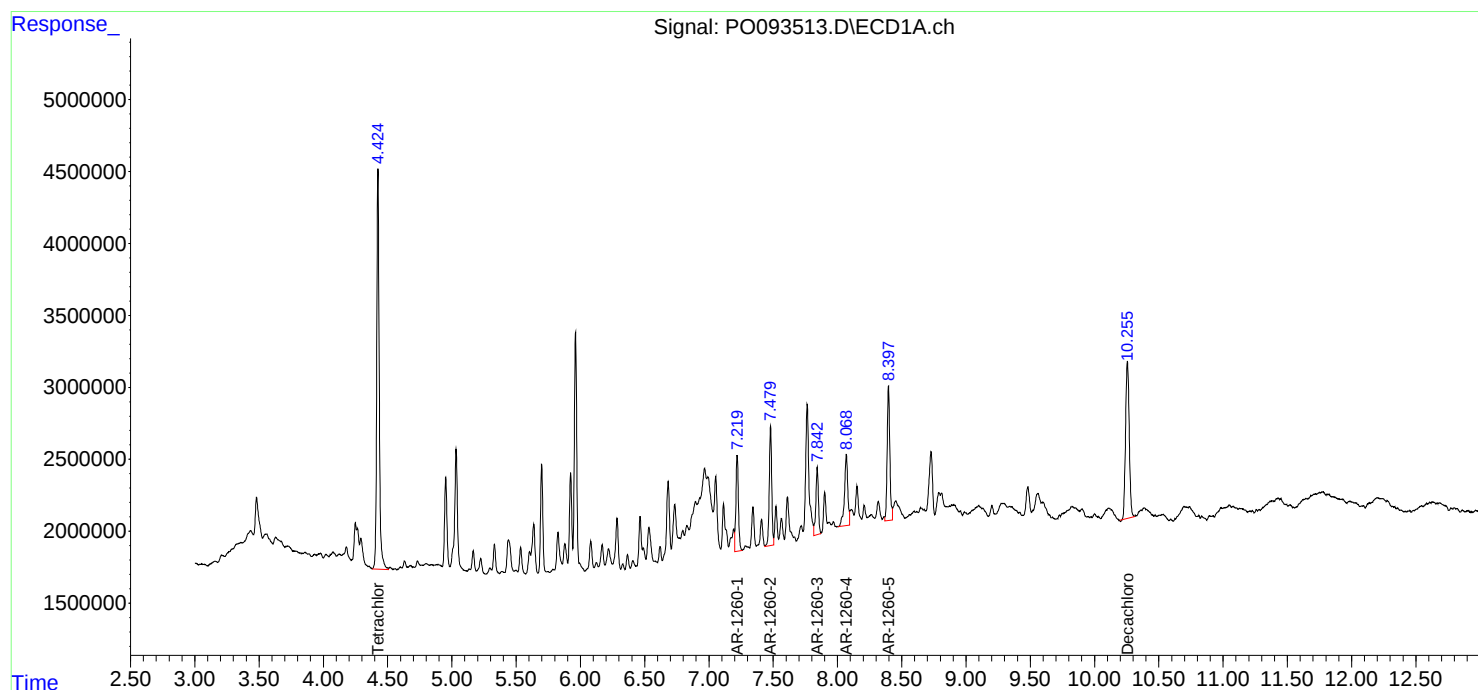


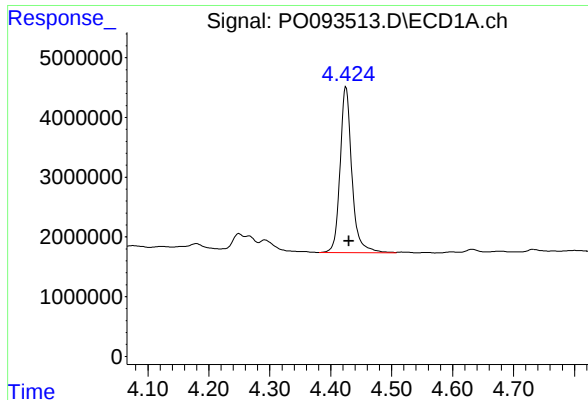

#1 Tetrachloro-m-xylene


R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 37430757
Conc: 11.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-B-72-EAST

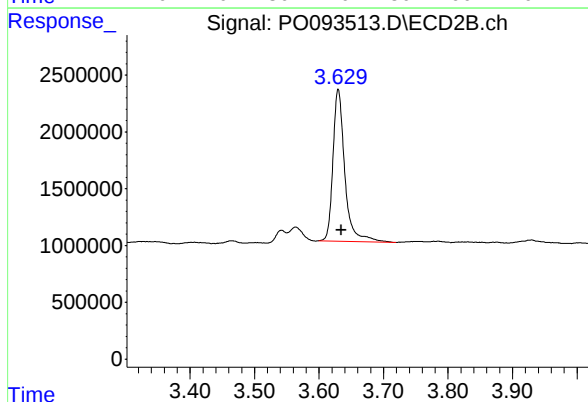


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.005 min
Response: 17055798
Conc: 15.12 ng/ml

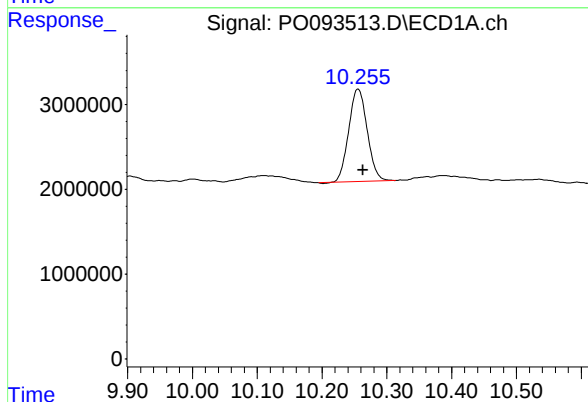


#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: -0.008 min
Response: 21614975
Conc: 9.99 ng/ml

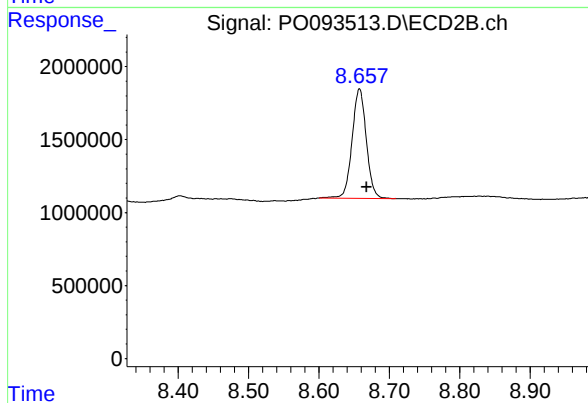

#2 Decachlorobiphenyl


R.T.: 8.657 min
Delta R.T.: -0.011 min
Response: 10549228
Conc: 10.77 ng/ml

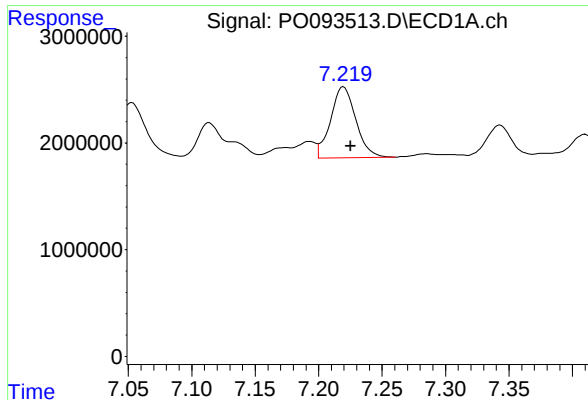

#31 AR-1260-1


R.T.: 7.220 min
Delta R.T.: -0.006 min
Response: 9238300
Conc: 71.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-B-72-EAST

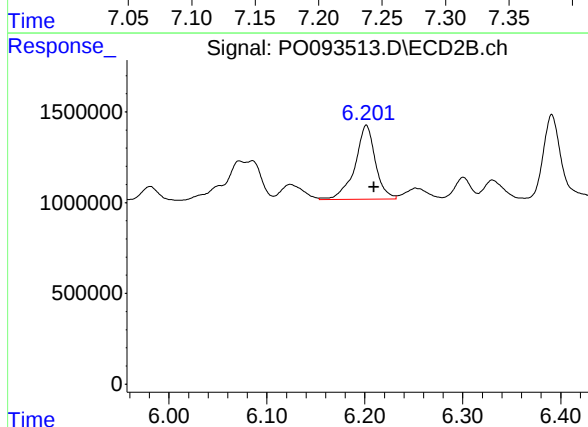


#31 AR-1260-1

R.T.: 6.202 min
Delta R.T.: -0.008 min
Response: 5928188
Conc: 97.51 ng/ml

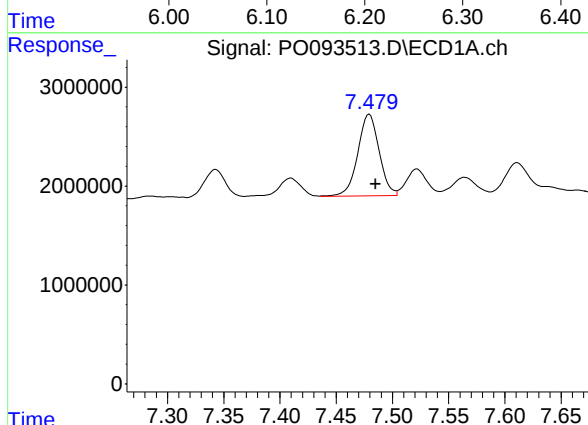


#32 AR-1260-2

R.T.: 7.479 min
Delta R.T.: -0.006 min
Response: 10927847
Conc: 74.02 ng/ml

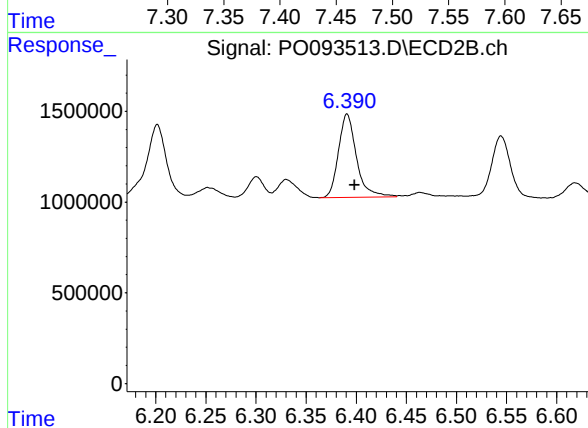

#32 AR-1260-2


R.T.: 6.391 min
Delta R.T.: -0.007 min
Response: 5755838
Conc: 79.61 ng/ml

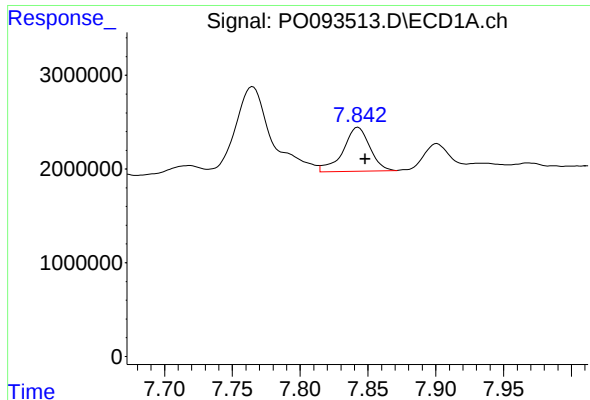

#33 AR-1260-3


R.T.: 7.843 min
Delta R.T.: -0.005 min
Response: 6456243
Conc: 57.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-B-72-EAST

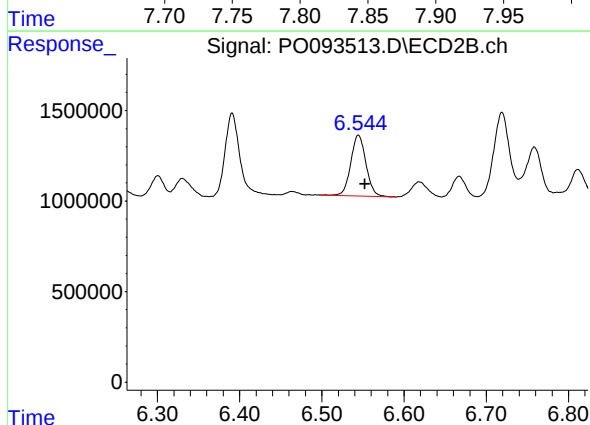


#33 AR-1260-3

R.T.: 6.545 min
Delta R.T.: -0.008 min
Response: 4305319
Conc: 64.38 ng/ml

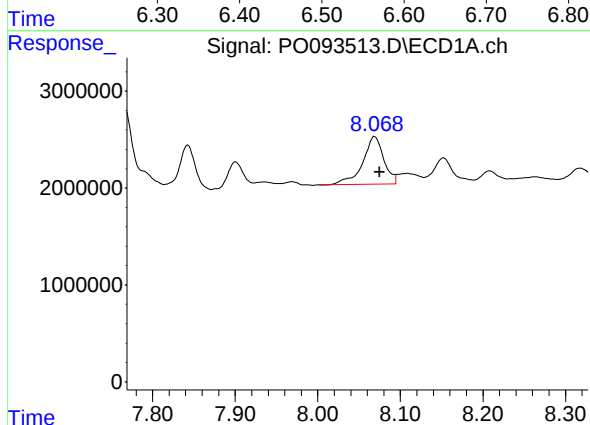


#34 AR-1260-4

R.T.: 8.069 min
Delta R.T.: -0.006 min
Response: 8749146
Conc: 68.23 ng/ml

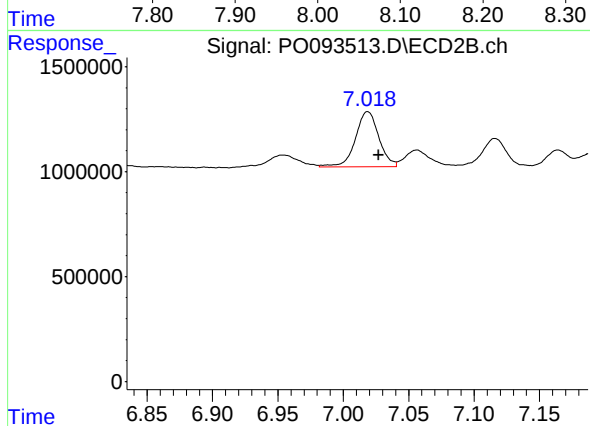

#34 AR-1260-4


R.T.: 7.019 min
Delta R.T.: -0.008 min
Response: 3269986
Conc: 59.42 ng/ml

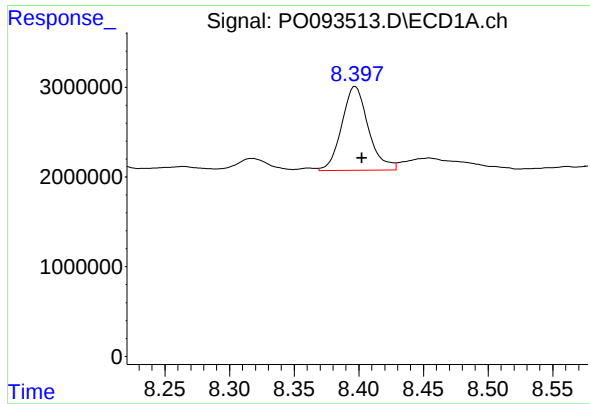

#35 AR-1260-5

R.T.: 8.397 min
Delta R.T.: -0.005 min
Response: 13371457
Conc: 59.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-B-72-EAST

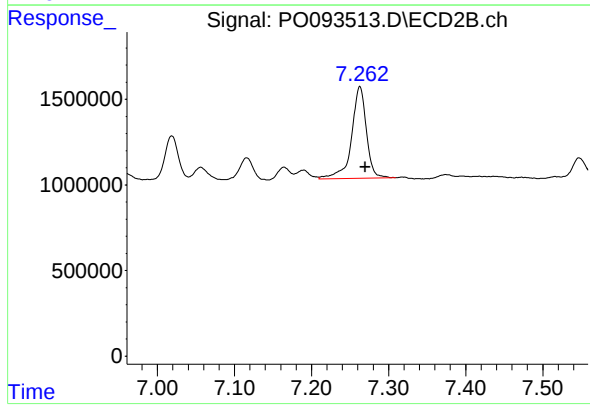

#35 AR-1260-5

R.T.: 7.263 min
Delta R.T.: -0.007 min
Response: 7097889
Conc: 60.29 ng/ml