

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032423\
 Data File : P0093550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2023 07:44
 Operator : YP/AJ
 Sample : 02065-02 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1161

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:39:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.423	3.628	6091330	2092426	1.945	1.855
2) SA Decachlor...	10.253	8.656	5314121	2002138	2.455	2.045

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032423\
Data File : PO093550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2023 07:44
Operator : YP/AJ
Sample : 02065-02 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1161

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:39:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

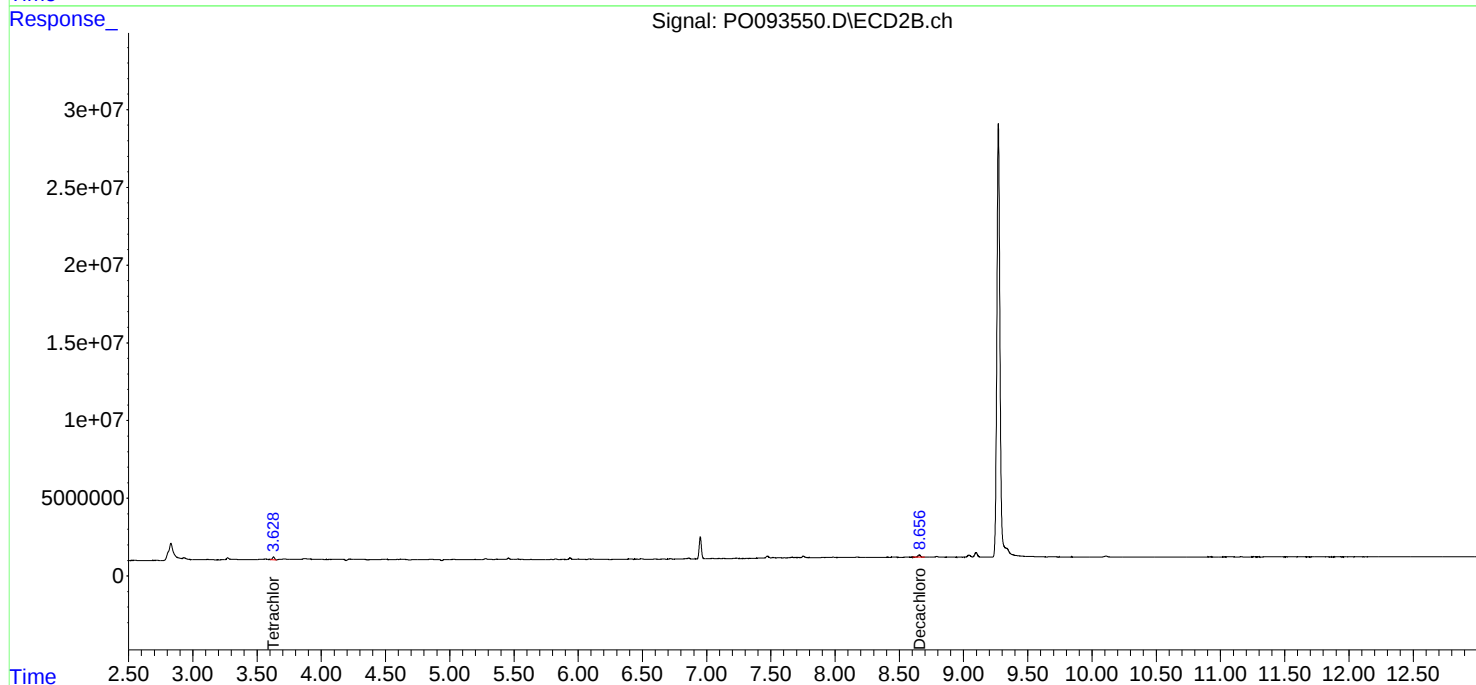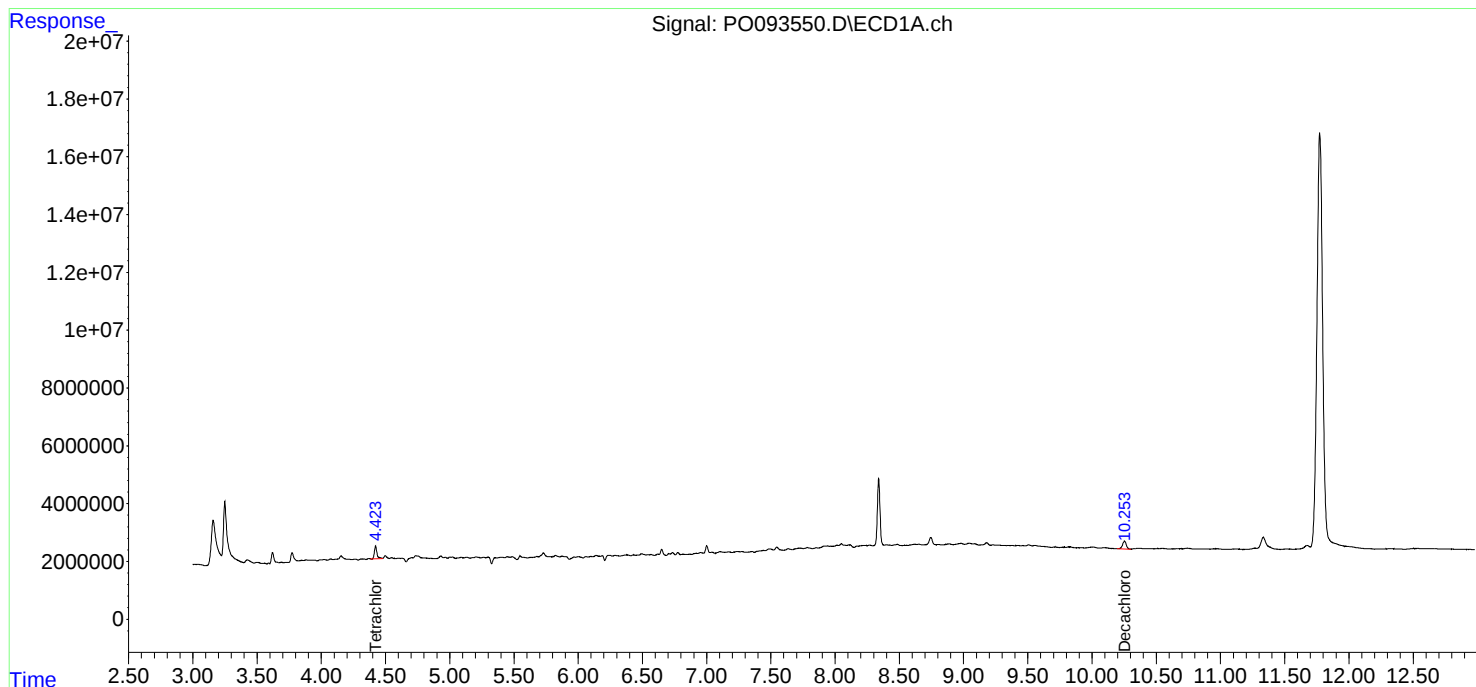


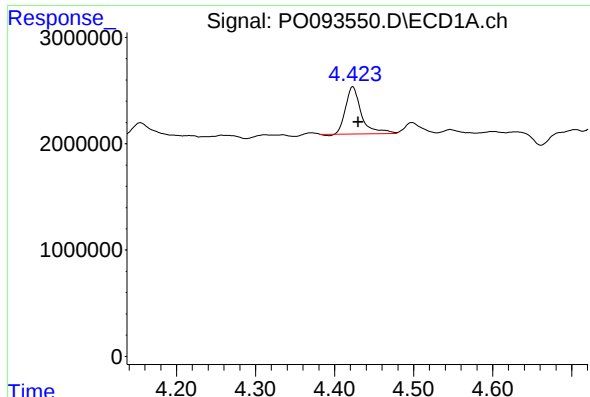

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.007 min
Response: 6091330
Conc: 1.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
1161

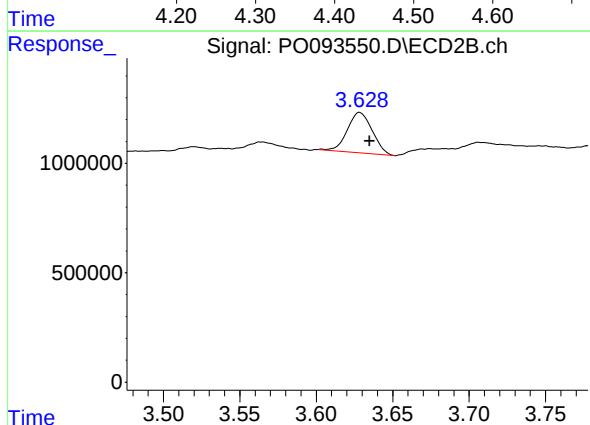


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.006 min
Response: 2092426
Conc: 1.86 ng/ml

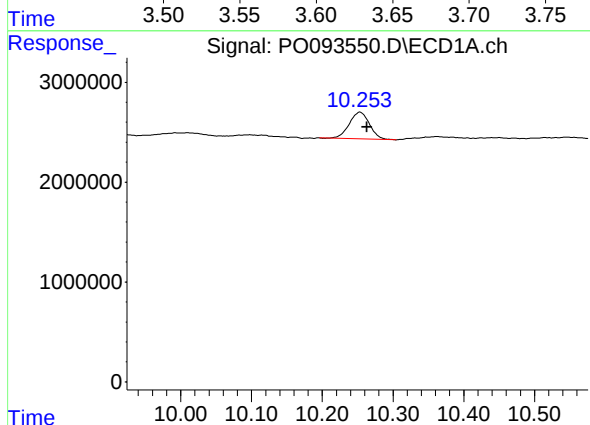

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: -0.010 min
Response: 5314121
Conc: 2.46 ng/ml

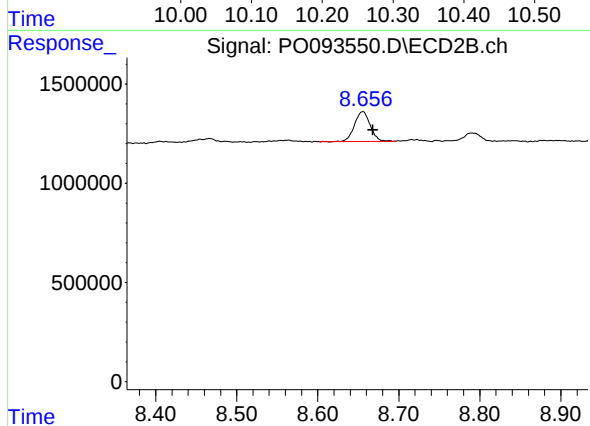

#2 Decachlorobiphenyl

R.T.: 8.656 min
Delta R.T.: -0.012 min
Response: 2002138
Conc: 2.04 ng/ml