

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
 Data File : P0076526.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 12:43
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:10:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:44:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.917	3.928	4730290	2703946	54.011	49.294
2) SA Decachlor...	10.889	9.184	3627364	2425879	55.724	51.481
Target Compounds						
21) L5 AR-1248-1	6.239	5.177	859986	484941	519.538	483.859
22) L5 AR-1248-2	6.531	5.436	1297451	830059	531.513	509.802
23) L5 AR-1248-3	6.748	5.480	1542434	843753	538.390	511.165
24) L5 AR-1248-4	7.176	5.663	1701203	987193	544.812	507.781
25) L5 AR-1248-5	7.216	6.085	1752640	955479	562.853	515.650m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032521\
Data File : PO076526.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 12:43
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:44:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

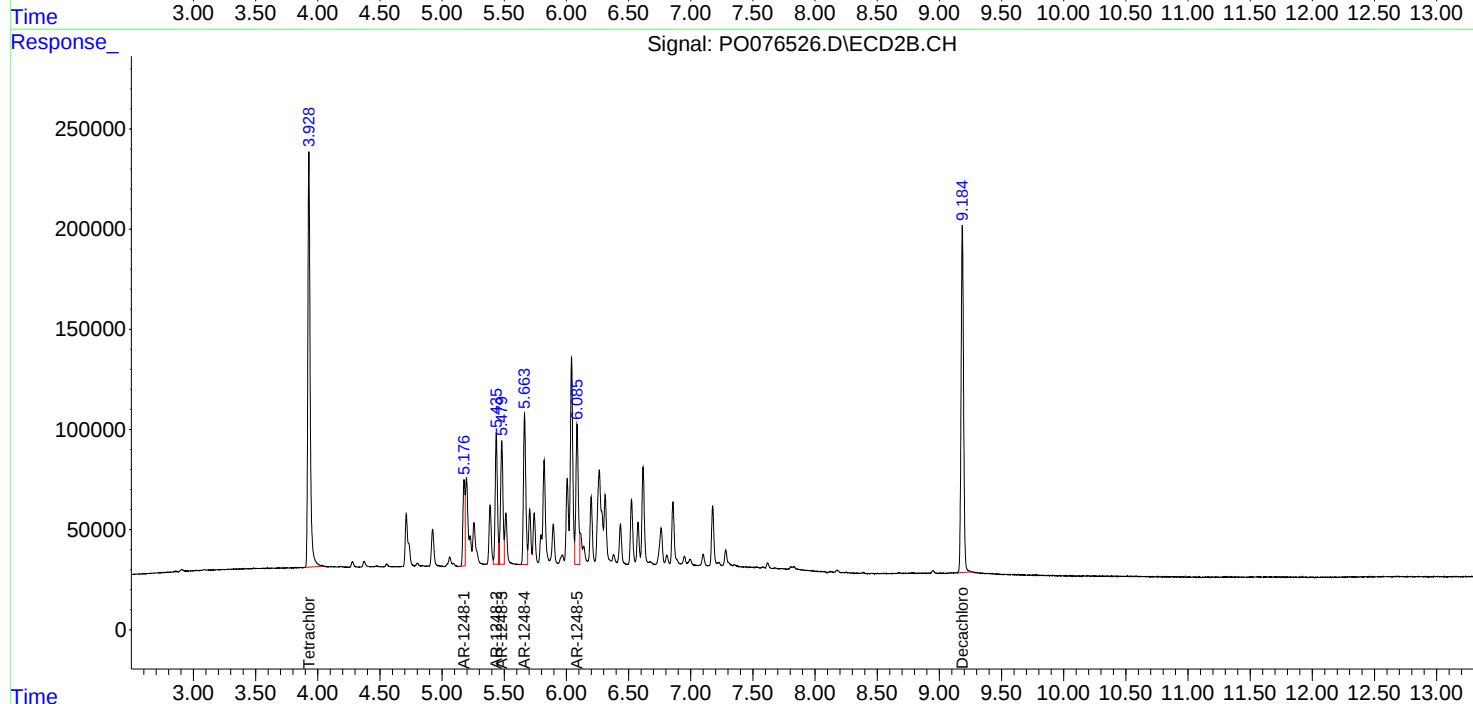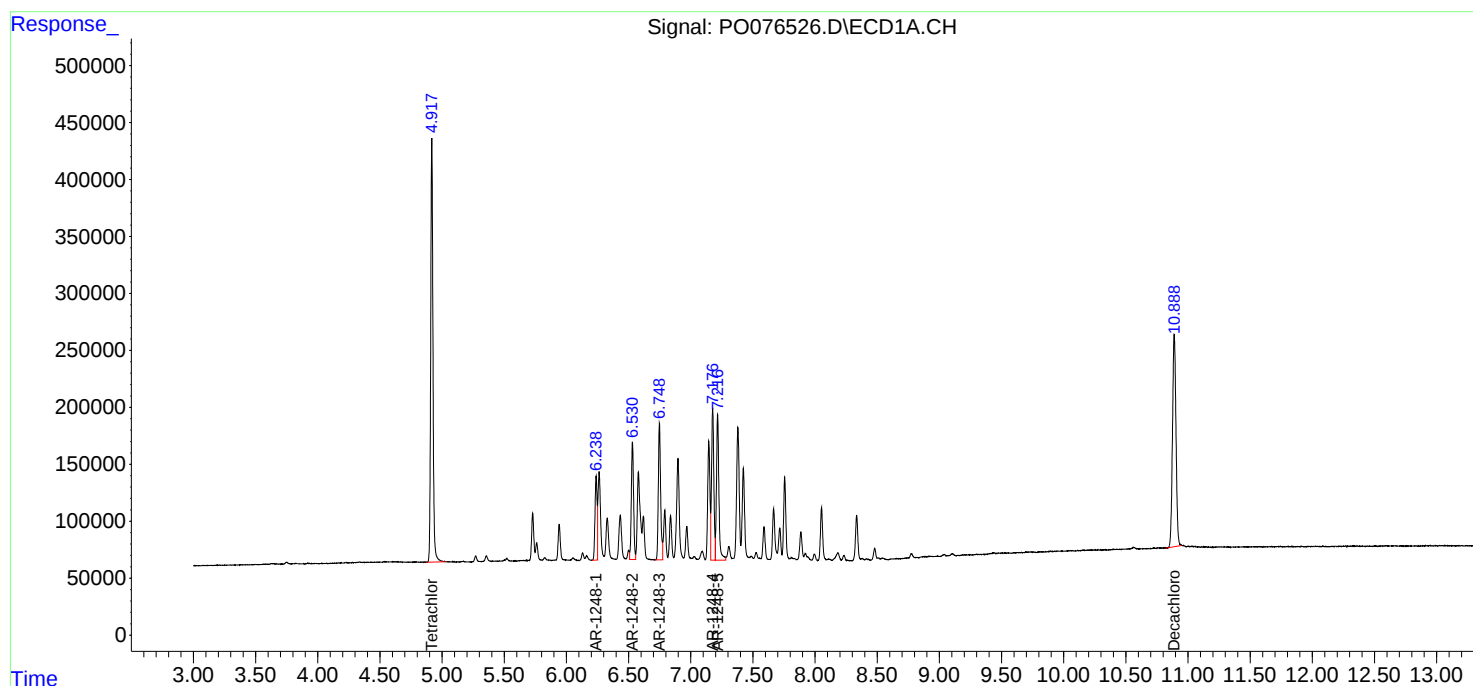

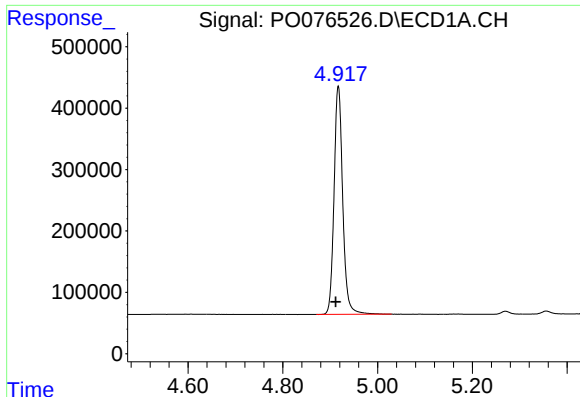


#1 Tetrachloro-m-xylene

R.T.: 4.917 min
Delta R.T.: 0.005 min
Response: 4730290
Conc: 54.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:31 AM

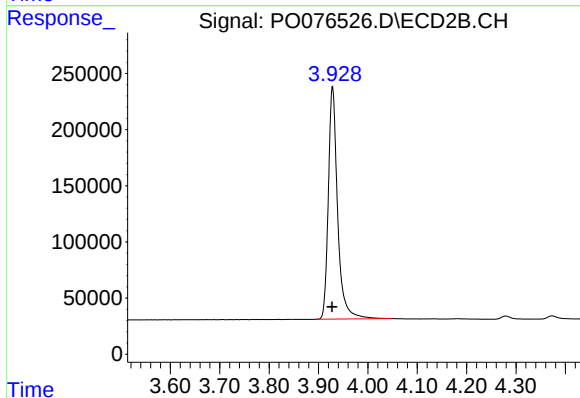


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.001 min
Response: 2703946
Conc: 49.29 ng/ml

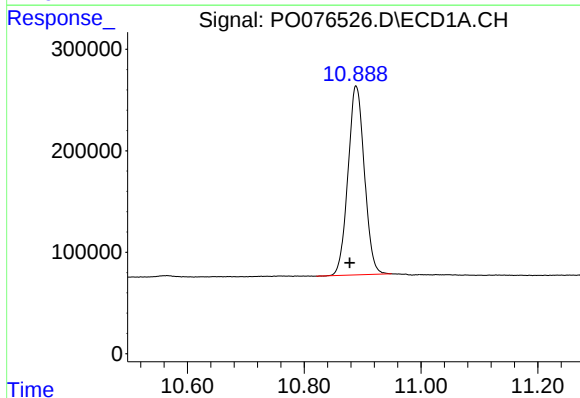


#2 Decachlorobiphenyl

R.T.: 10.889 min
Delta R.T.: 0.010 min
Response: 3627364
Conc: 55.72 ng/ml

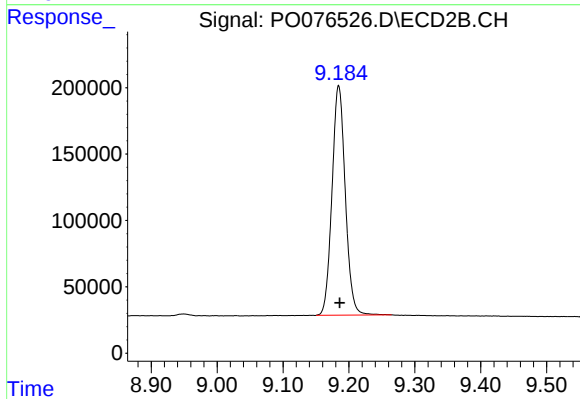

#2 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: -0.001 min
Response: 2425879
Conc: 51.48 ng/ml

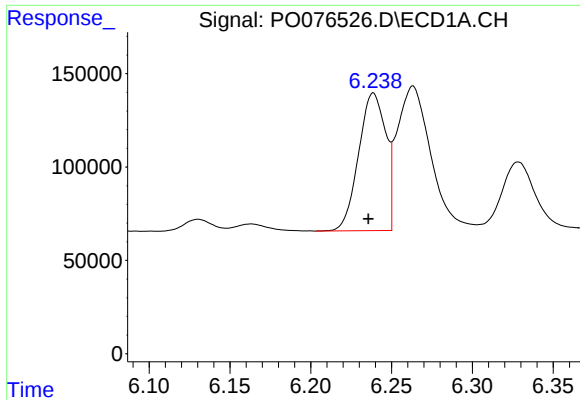


#21 AR-1248-1

R.T.: 6.239 min
Delta R.T.: 0.003 min
Response: 859986
Conc: 519.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:31 AM

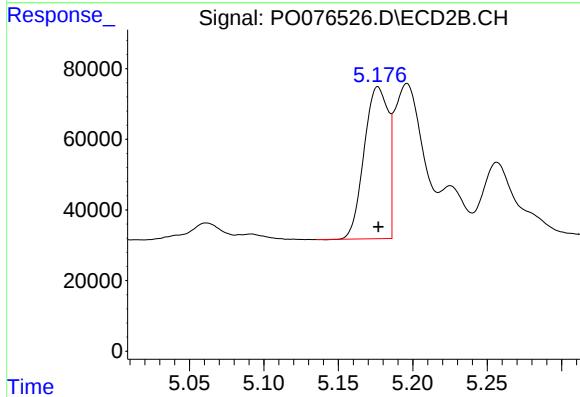


#21 AR-1248-1

R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 484941
Conc: 483.86 ng/ml

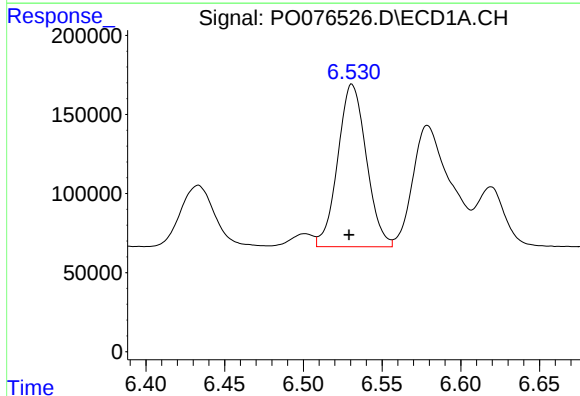


#22 AR-1248-2

R.T.: 6.531 min
Delta R.T.: 0.002 min
Response: 1297451
Conc: 531.51 ng/ml

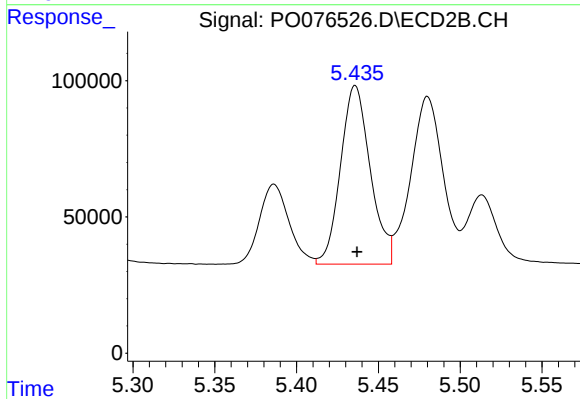

#22 AR-1248-2

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 830059
Conc: 509.80 ng/ml

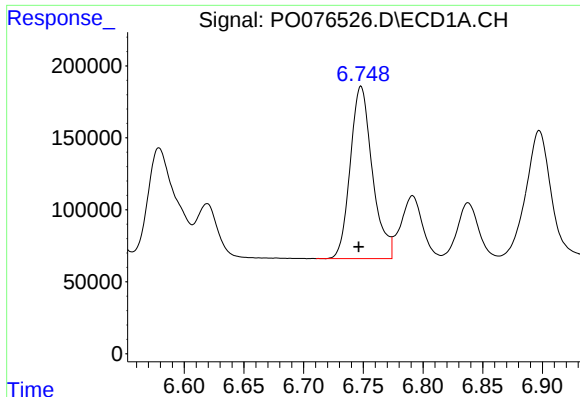


#23 AR-1248-3

R.T.: 6.748 min
Delta R.T.: 0.002 min
Response: 1542434
Conc: 538.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:31 AM

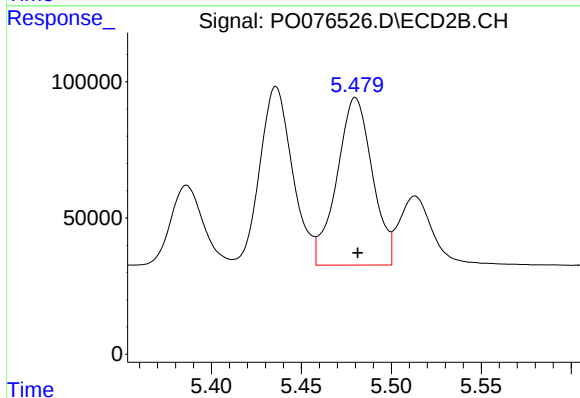


#23 AR-1248-3

R.T.: 5.480 min
Delta R.T.: -0.001 min
Response: 843753
Conc: 511.16 ng/ml

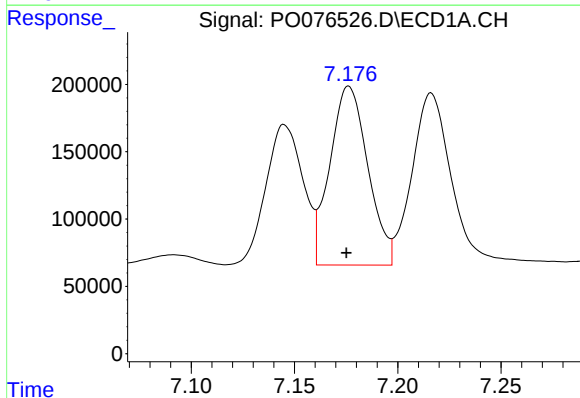


#24 AR-1248-4

R.T.: 7.176 min
Delta R.T.: 0.001 min
Response: 1701203
Conc: 544.81 ng/ml

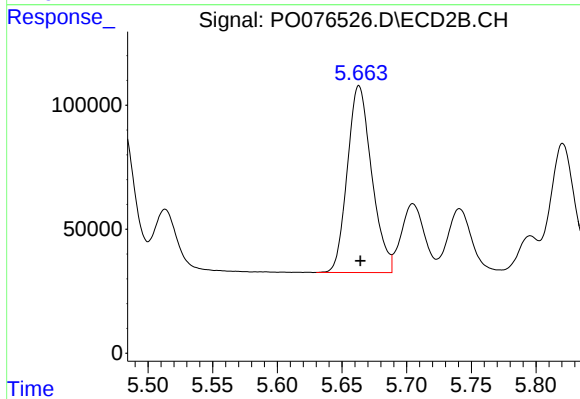

#24 AR-1248-4

R.T.: 5.663 min
Delta R.T.: -0.001 min
Response: 987193
Conc: 507.78 ng/ml

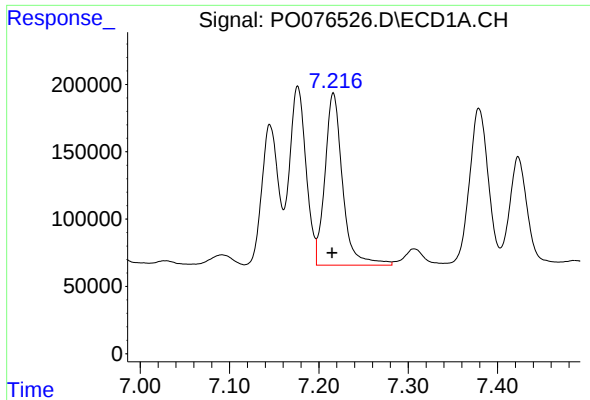


#25 AR-1248-5

R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 1752640
Conc: 562.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:31 AM

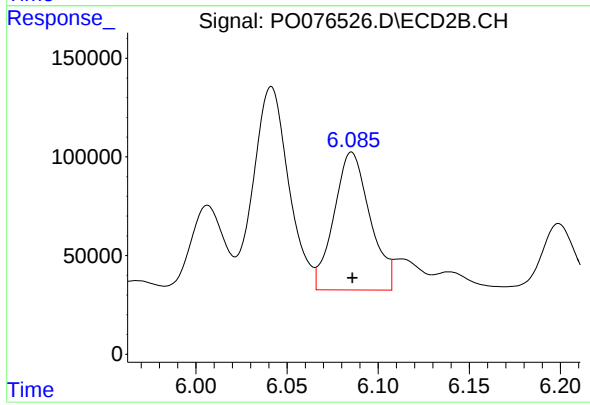

#25 AR-1248-5

R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 955479
Conc: 515.65 ng/ml m