

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
 Data File : P0076531.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 14:09
 Operator : DD\AJ
 Sample : M1772-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUM-1-2-COMP

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:10:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:46:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.950f	951895	912526	10.869m	16.636m#
2) SA Decachlor...	10.891	9.190	1244082	855020	19.112m	18.145

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
Data File : P0076531.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 14:09
Operator : DD\AJ
Sample : M1772-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUM-1-2-COMP


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:46:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

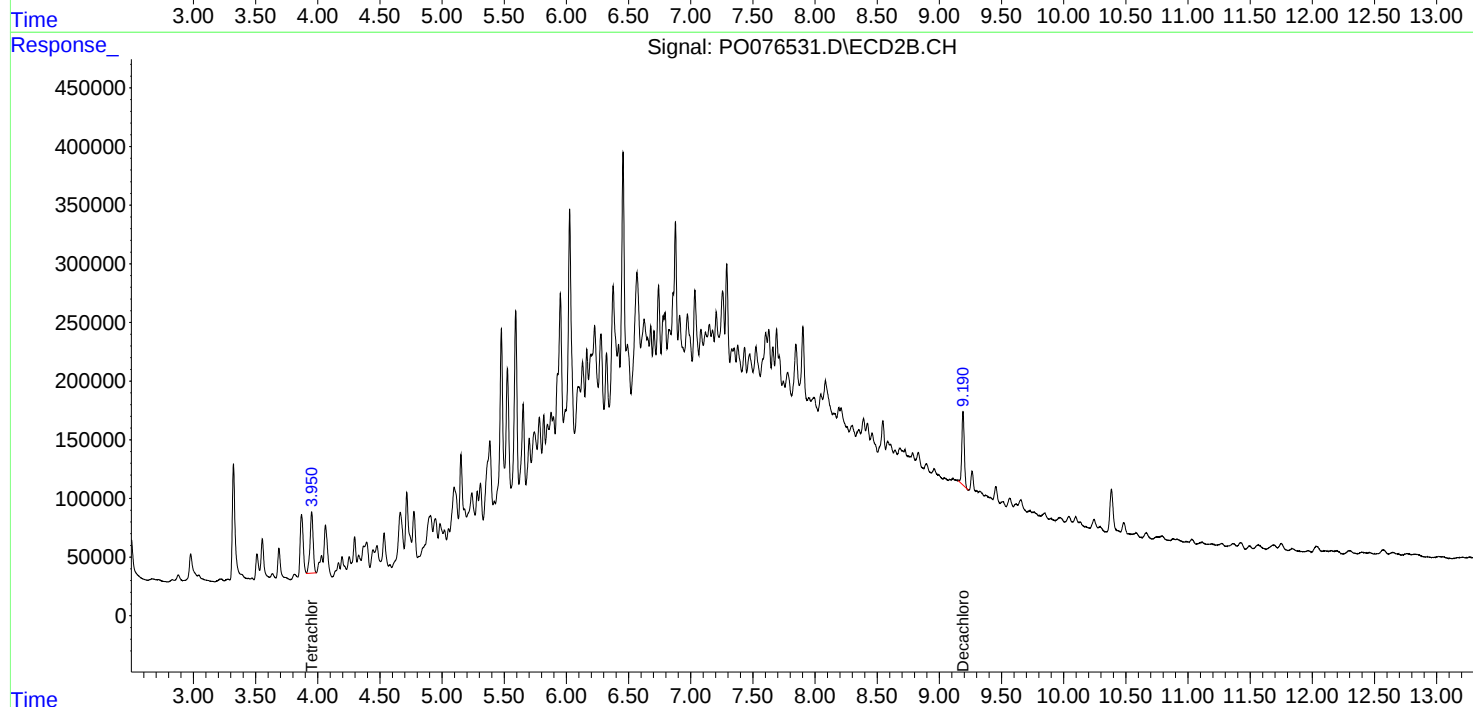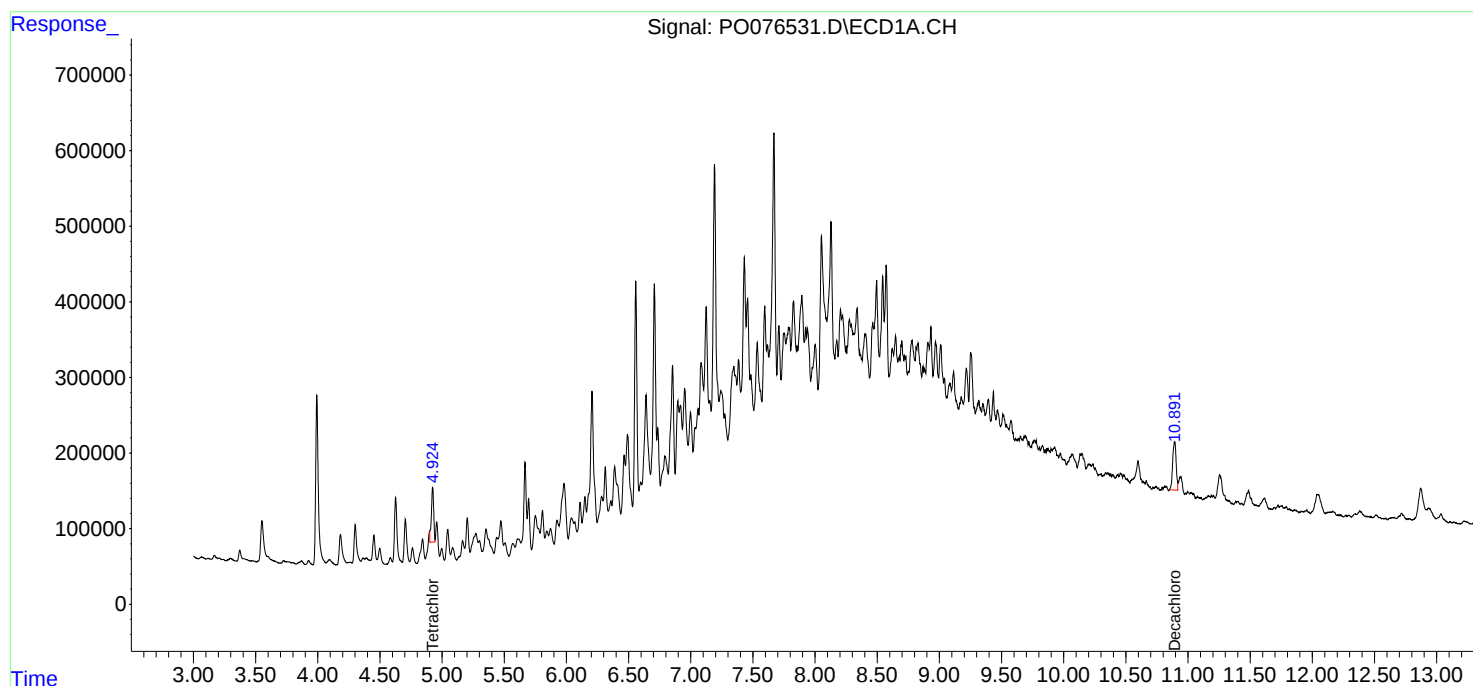

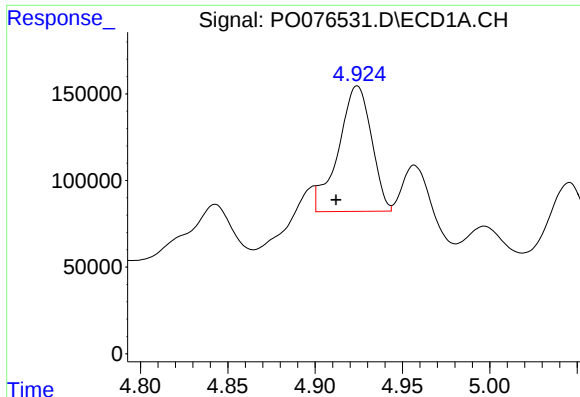


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: 0.012 min
Response: 951895
Conc: 10.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DRUM-1-2-COMP


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:32 AM

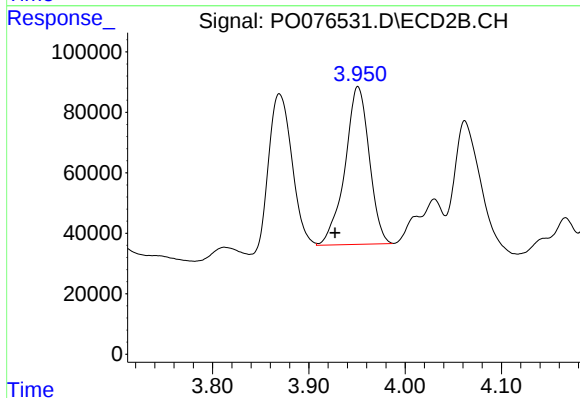


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.023 min
Response: 912526
Conc: 16.64 ng/ml m

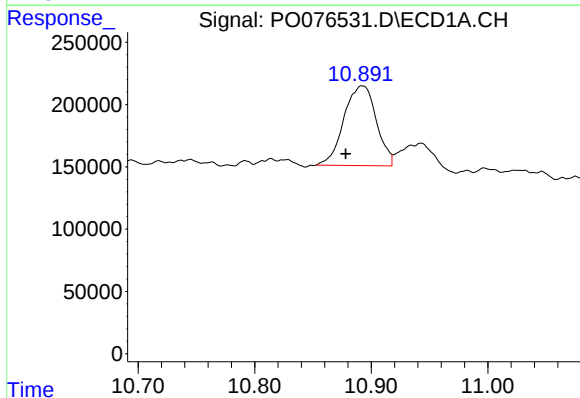

#2 Decachlorobiphenyl

R.T.: 10.891 min
Delta R.T.: 0.013 min
Response: 1244082
Conc: 19.11 ng/ml m

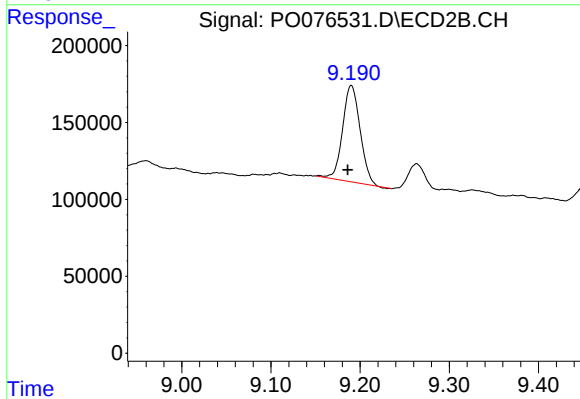

#2 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: 0.004 min
Response: 855020
Conc: 18.14 ng/ml