

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
 Data File : P0076532.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 14:26
 Operator : DD\AJ
 Sample : M1769-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SVE-03

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:10:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:46:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.928	128888	111353	1.472	2.030 #
2) SA Decachlor...	10.884	9.184	325259	125695	4.997	2.667m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
Data File : P0076532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 14:26
Operator : DD\AJ
Sample : M1769-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SVE-03


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:46:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

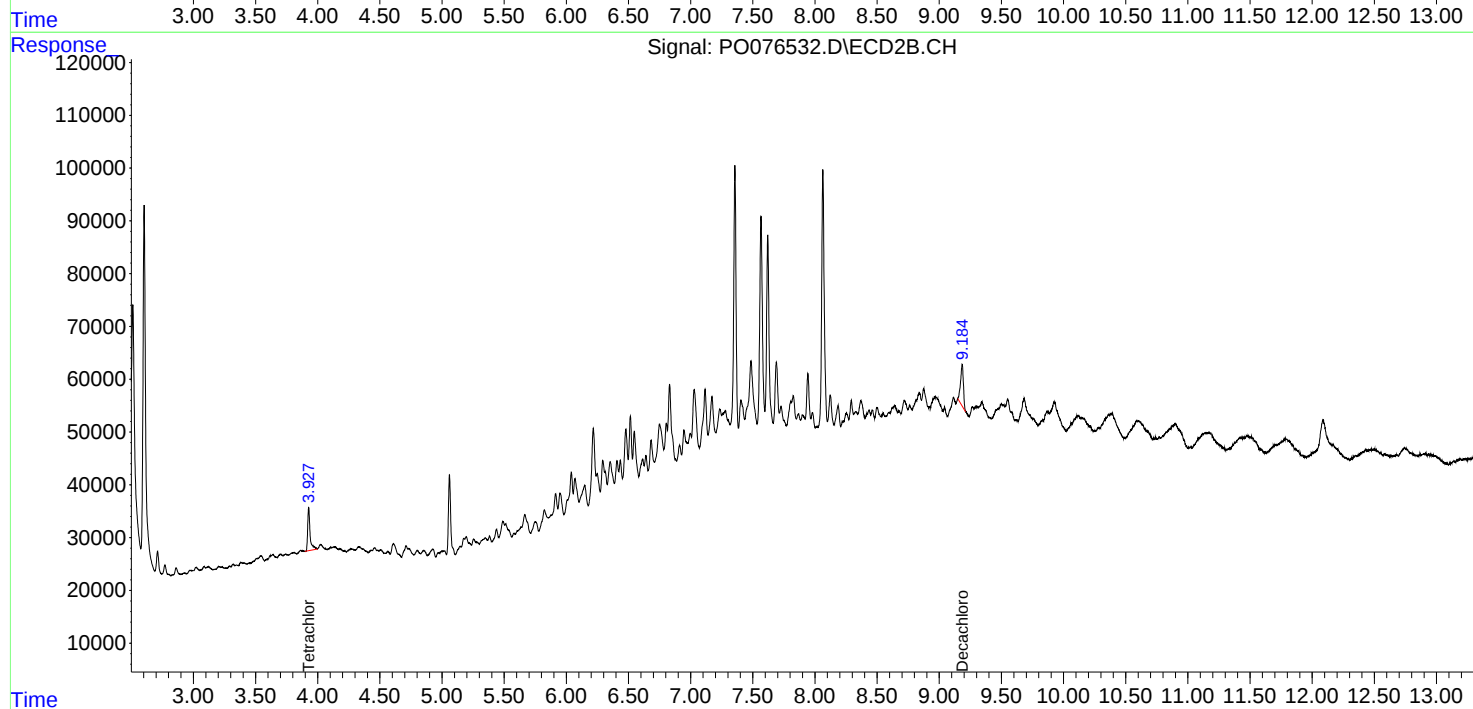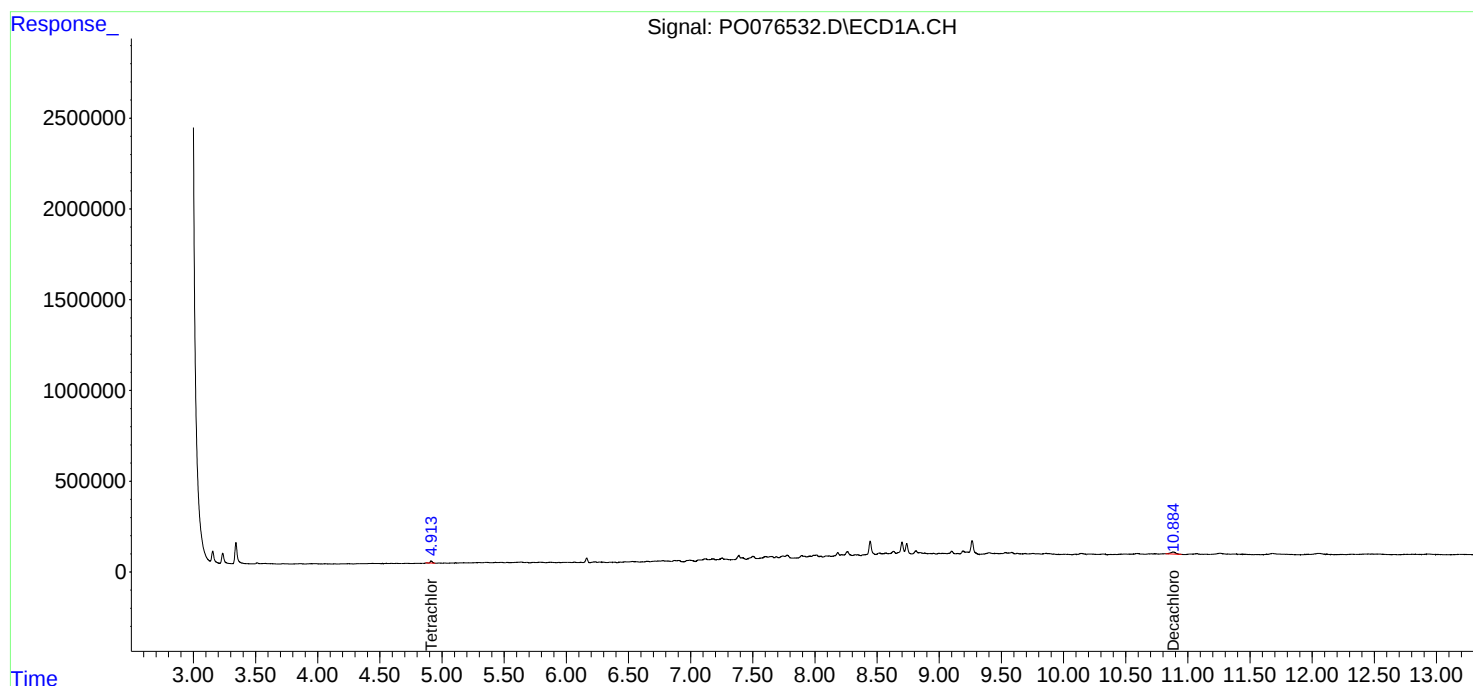

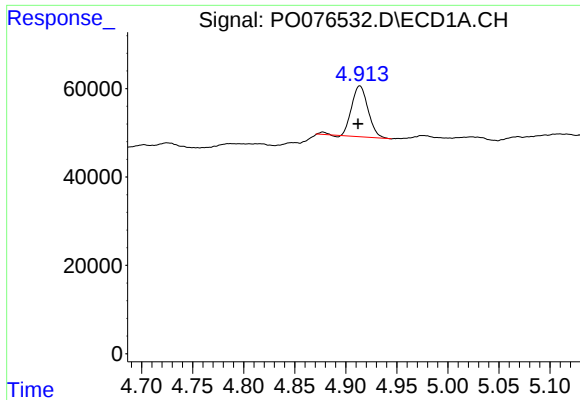


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: 0.002 min
Response: 128888
Conc: 1.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
SVE-03


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:34 AM

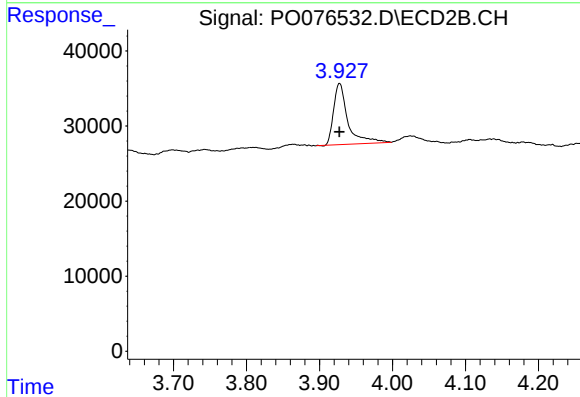


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 111353
Conc: 2.03 ng/ml

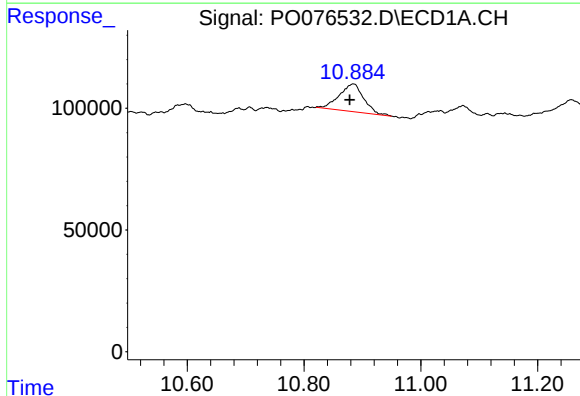

#2 Decachlorobiphenyl

R.T.: 10.884 min
Delta R.T.: 0.006 min
Response: 325259
Conc: 5.00 ng/ml

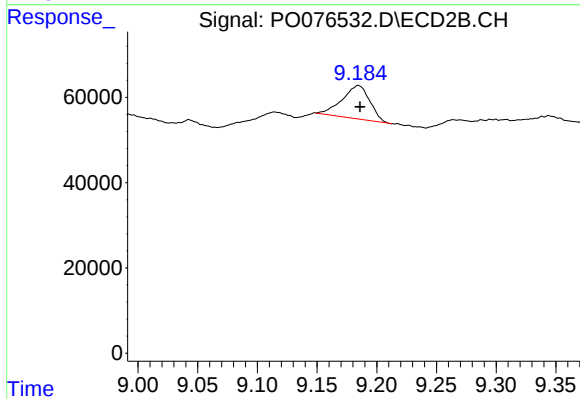

#2 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: -0.002 min
Response: 125695
Conc: 2.67 ng/ml m