

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0032521\
 Data File : P0076536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 15:35
 Operator : DD\AJ
 Sample : M1775-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11979

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:10:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:47:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.912	3.927	758840	462547	8.665	8.432
2) SA Decachlor...	10.886	9.184	328313	204734	5.044	4.345
Target Compounds						
31) L7 AR-1260-1	7.917	6.752	40071	34975	11.661m	13.647
32) L7 AR-1260-2	8.183	6.948	85428	35684	21.070	11.506 #
33) L7 AR-1260-3	8.548	7.098	51476	34455	17.039	11.728m#
34) L7 AR-1260-4	8.777	7.582	51714	17622	14.840m	7.394 #
35) L7 AR-1260-5	9.104	7.828	99805	49857	14.769	8.788m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032521\
Data File : P0076536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 15:35
Operator : DD\AJ
Sample : M1775-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
11979


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:47:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

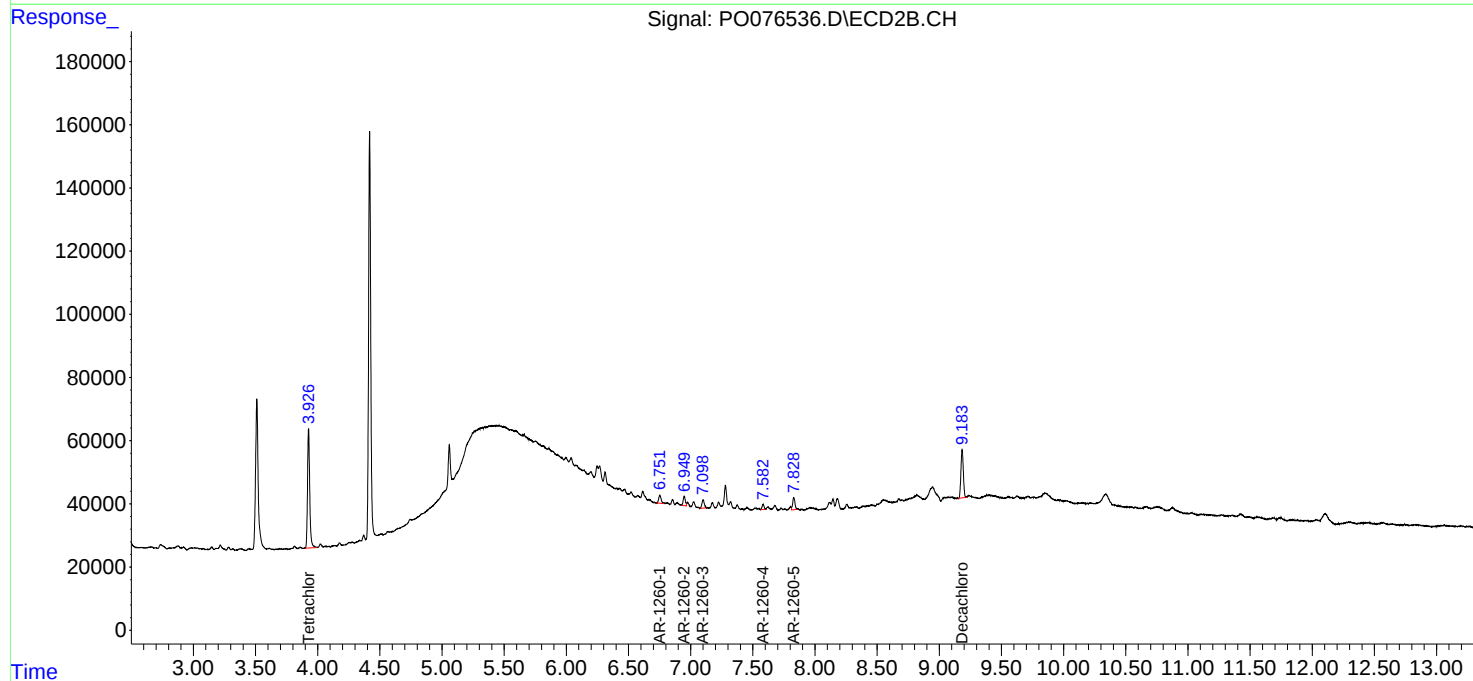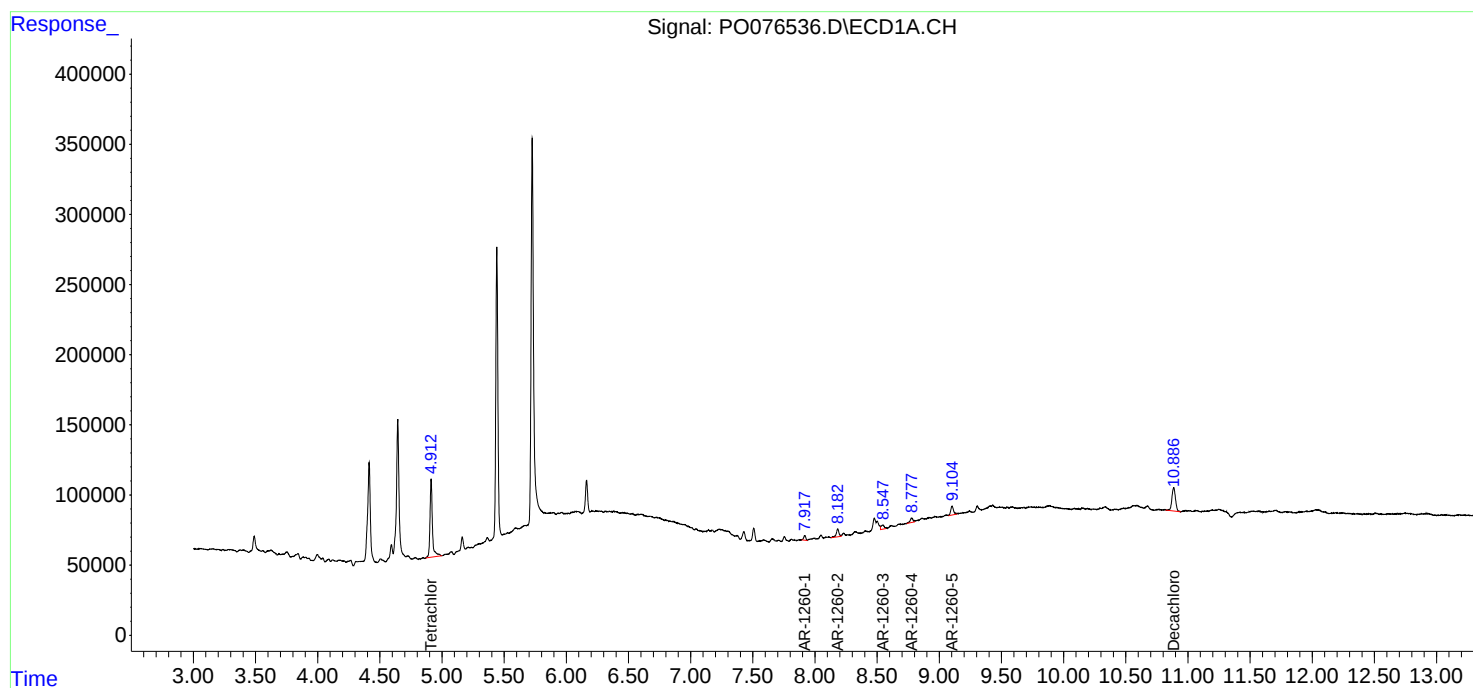

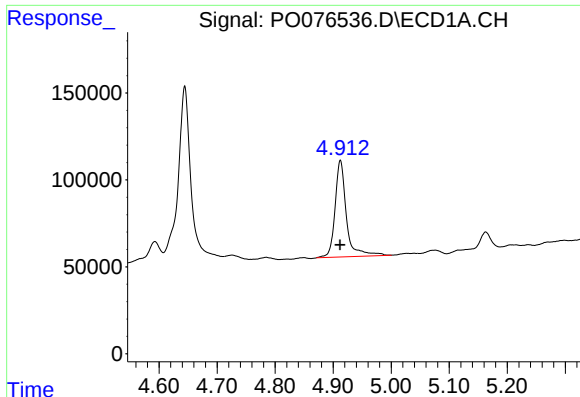


#1 Tetrachloro-m-xylene

R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 758840
Conc: 8.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
11979


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:36 AM

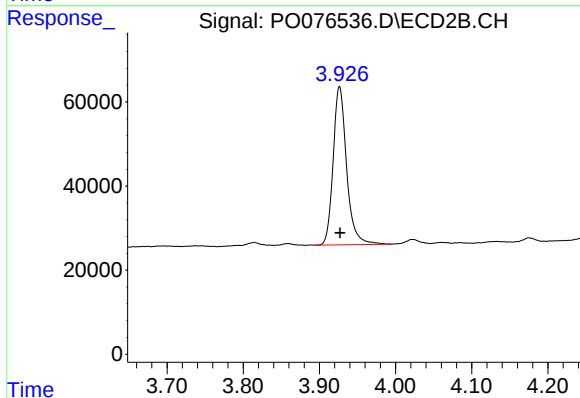


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 462547
Conc: 8.43 ng/ml

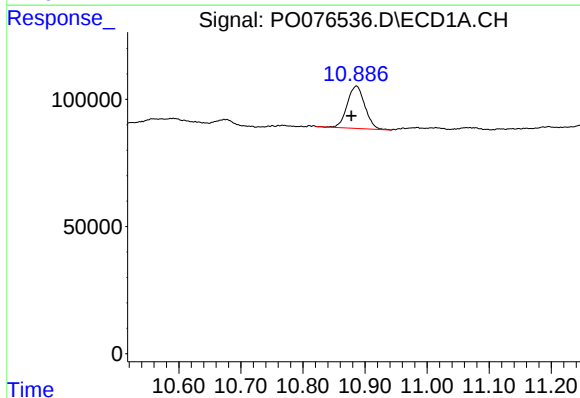


#2 Decachlorobiphenyl

R.T.: 10.886 min
Delta R.T.: 0.008 min
Response: 328313
Conc: 5.04 ng/ml

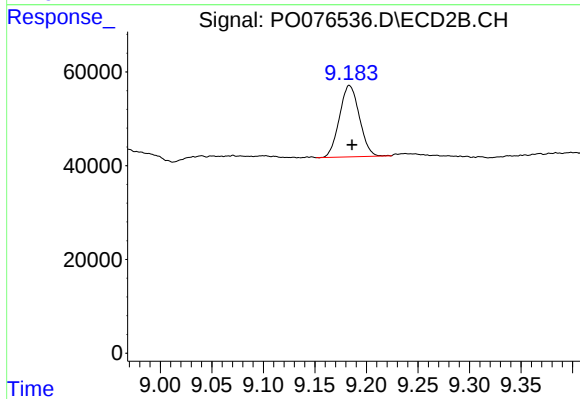

#2 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: -0.002 min
Response: 204734
Conc: 4.34 ng/ml

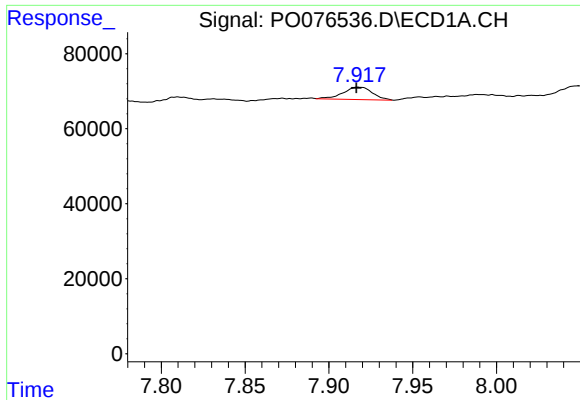


#31 AR-1260-1

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 40071
Conc: 11.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
11979


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:36 AM

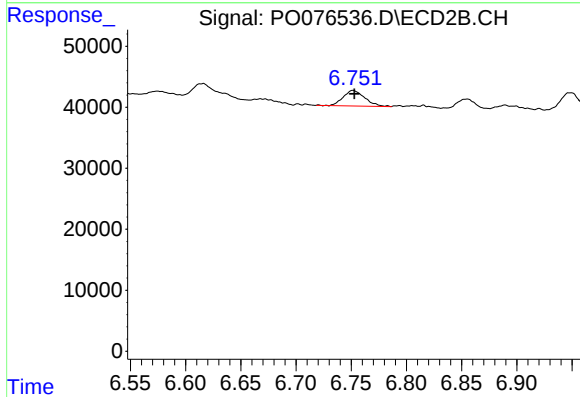


#31 AR-1260-1

R.T.: 6.752 min
Delta R.T.: -0.001 min
Response: 34975
Conc: 13.65 ng/ml

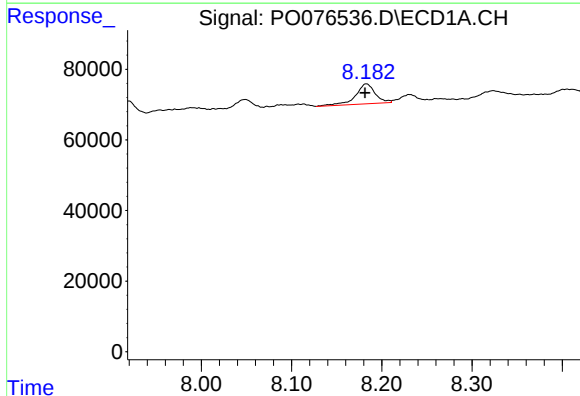


#32 AR-1260-2

R.T.: 8.183 min
Delta R.T.: 0.002 min
Response: 85428
Conc: 21.07 ng/ml

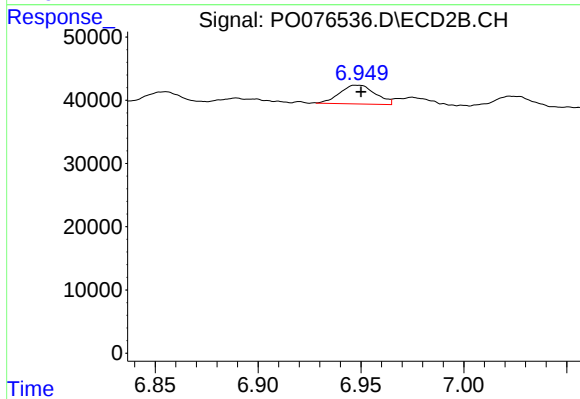

#32 AR-1260-2

R.T.: 6.948 min
Delta R.T.: -0.002 min
Response: 35684
Conc: 11.51 ng/ml

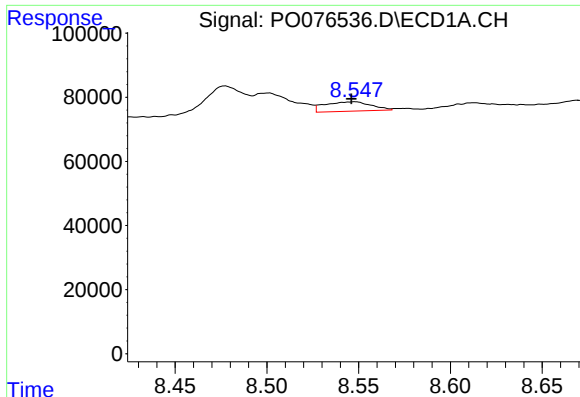


#33 AR-1260-3

R.T.: 8.548 min
Delta R.T.: 0.002 min
Response: 51476
Conc: 17.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
11979


Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:36 AM

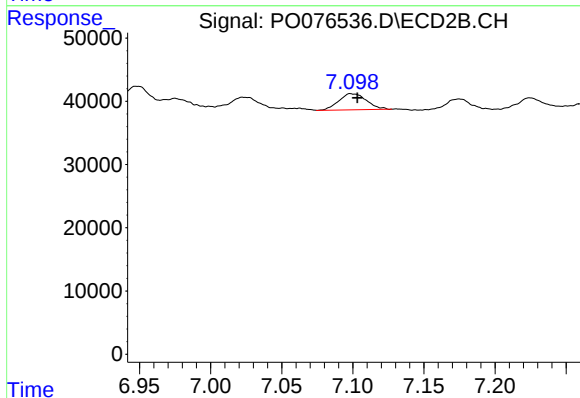


#33 AR-1260-3

R.T.: 7.098 min
Delta R.T.: -0.006 min
Response: 34455
Conc: 11.73 ng/ml m

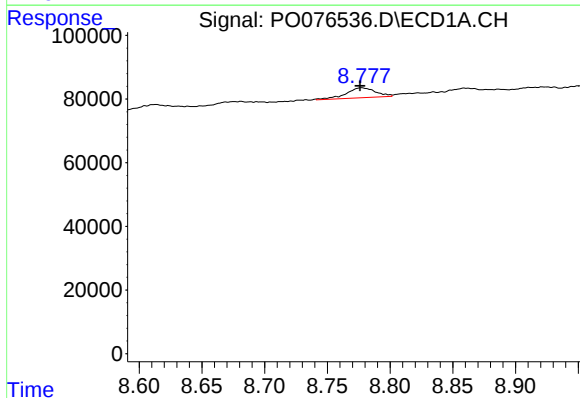


#34 AR-1260-4

R.T.: 8.777 min
Delta R.T.: 0.001 min
Response: 51714
Conc: 14.84 ng/ml m

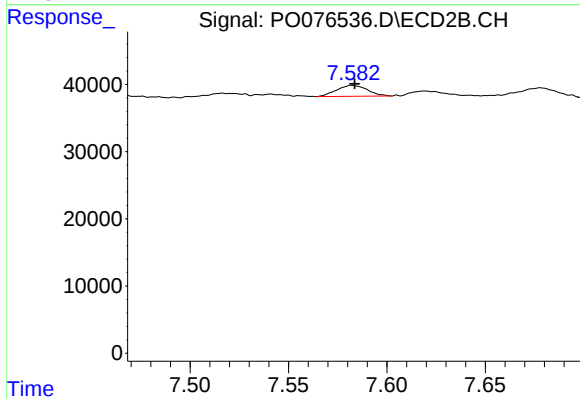

#34 AR-1260-4

R.T.: 7.582 min
Delta R.T.: -0.001 min
Response: 17622
Conc: 7.39 ng/ml

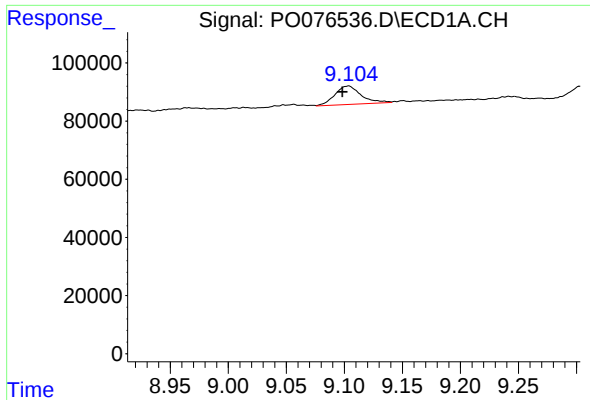


#35 AR-1260-5

R.T.: 9.104 min
Delta R.T.: 0.005 min
Response: 99805
Conc: 14.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
11979

Manual Integrations
APPROVED

Ankita
3/25/2021 9:10:36 AM

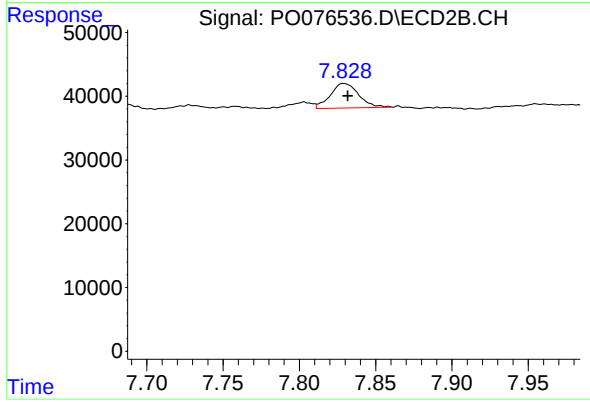

#35 AR-1260-5

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 49857
Conc: 8.79 ng/ml m