

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032621\
 Data File : P0076551.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2021 14:08
 Operator : DD\AJ
 Sample : M1802-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3D-(4.5-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 18:41:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.912	3.926	2169386	1268978	24.770	23.134
2) SA Decachlor...	10.887	9.183	2016330	1280980	30.975	27.185

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032621\
Data File : P0076551.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2021 14:08
Operator : DD\AJ
Sample : M1802-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-3D-(4.5-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 18:41:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

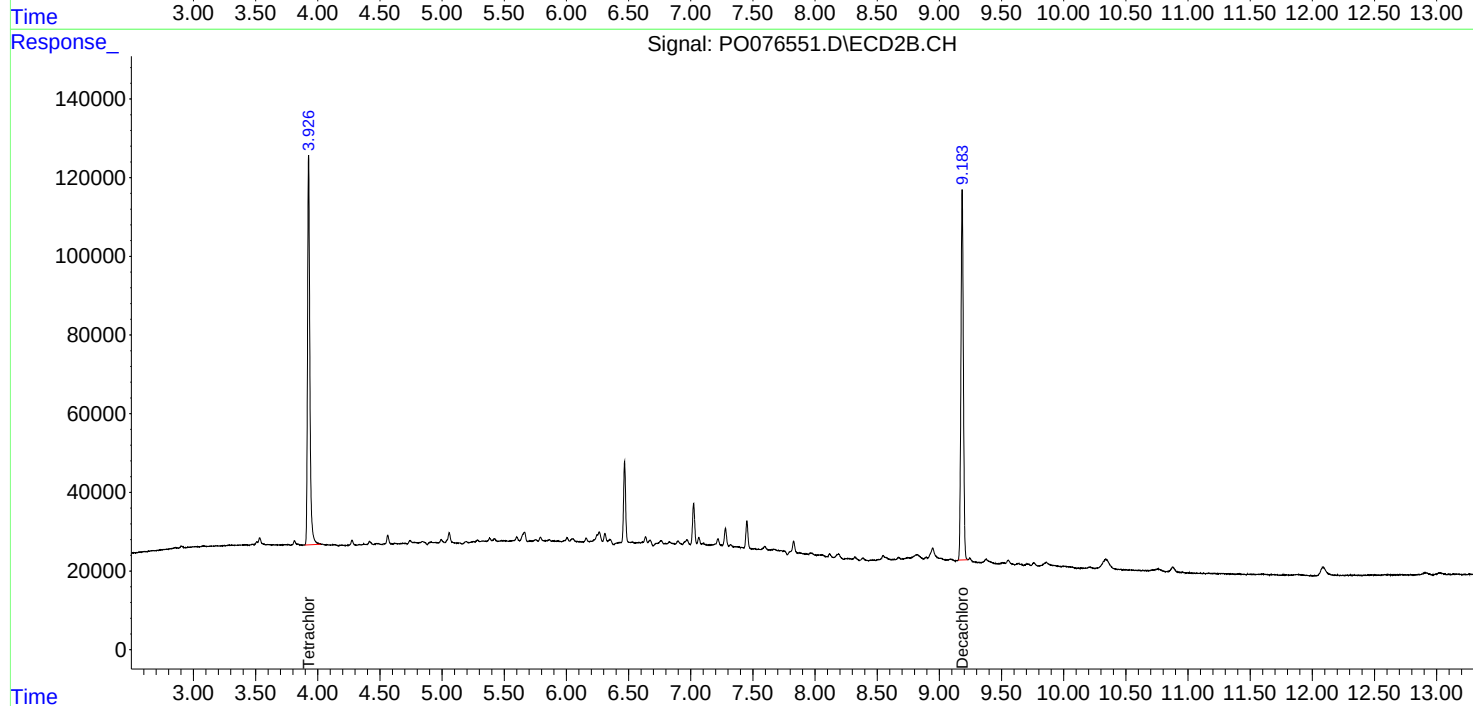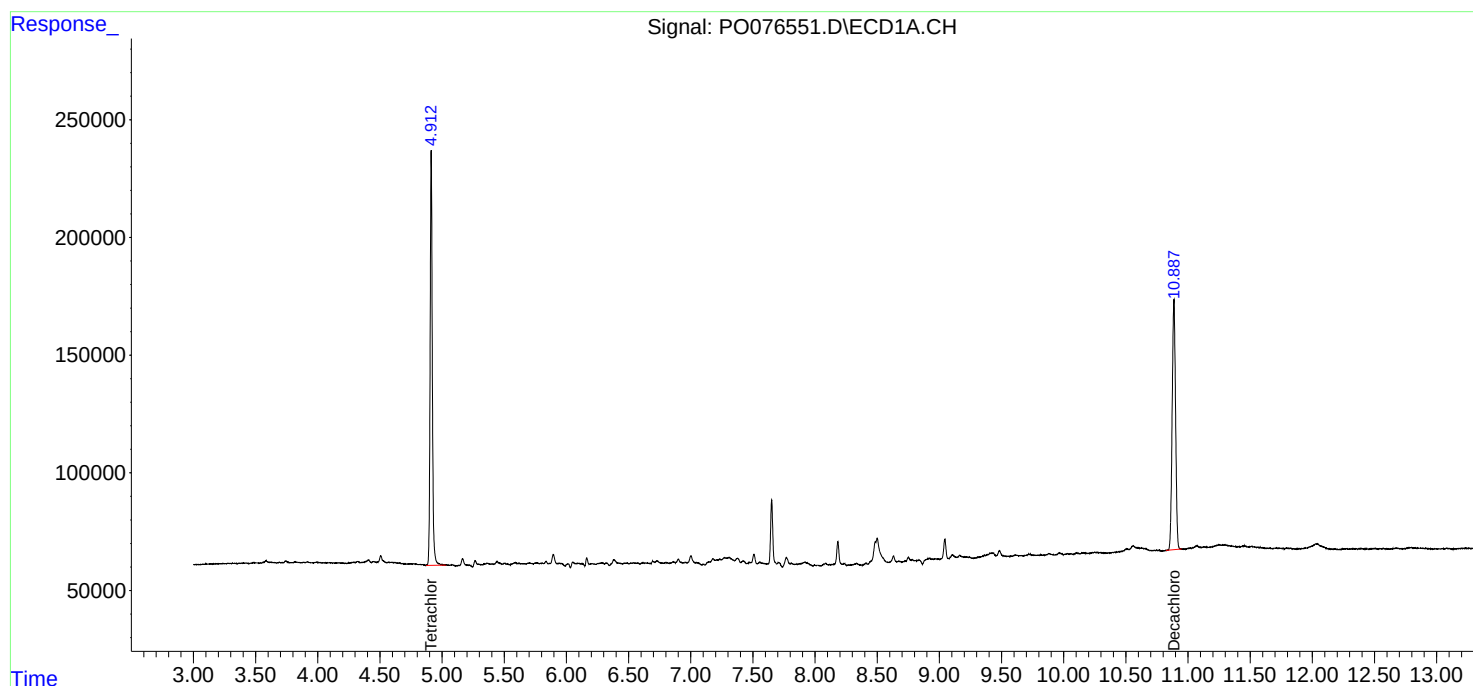


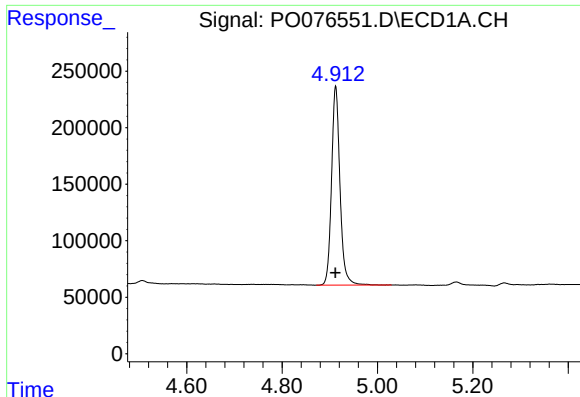

#1 Tetrachloro-m-xylene


R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 2169386
Conc: 24.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-3D-(4.5-5)

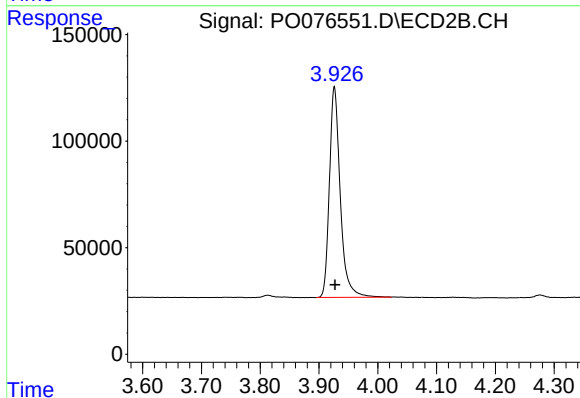


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 1268978
Conc: 23.13 ng/ml

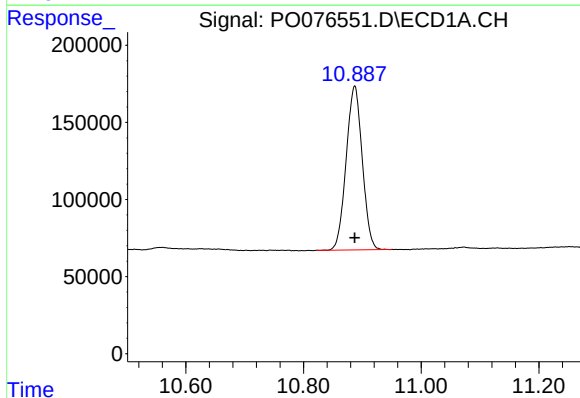

#2 Decachlorobiphenyl

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 2016330
Conc: 30.98 ng/ml

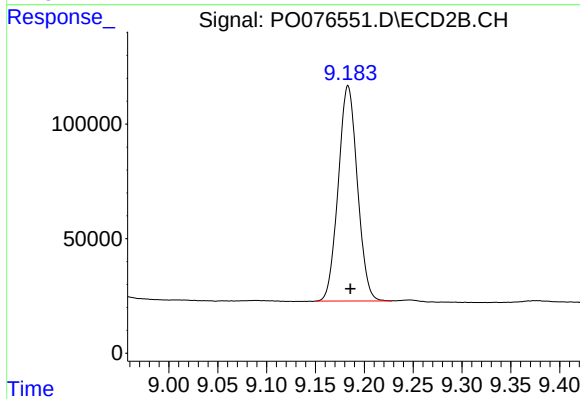

#2 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: -0.003 min
Response: 1280980
Conc: 27.18 ng/ml