

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032723\
 Data File : P0093584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2023 16:51
 Operator : YP/AJ
 Sample : 02102-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHAMBER-C-72-EAST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 21:20:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.631	39772239	14531567	12.701	12.884
2) SA Decachlor...	10.255	8.657	22341473	9864388	10.323	10.075
Target Compounds						
31) L7 AR-1260-1	7.220	6.201	6587998	3673518	50.852	60.421
32) L7 AR-1260-2	7.479	6.390	7167596	3852078	48.553	53.282
33) L7 AR-1260-3	7.842	6.544	4647009	2751357	41.314	41.146
34) L7 AR-1260-4	8.068	7.017	6108881	1810138	47.637	32.893 #
35) L7 AR-1260-5	8.396	7.261	9458263	4187358	42.331	35.567



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032723\
Data File : P0093584.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2023 16:51
Operator : YP/AJ
Sample : 02102-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-EAST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 21:20:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

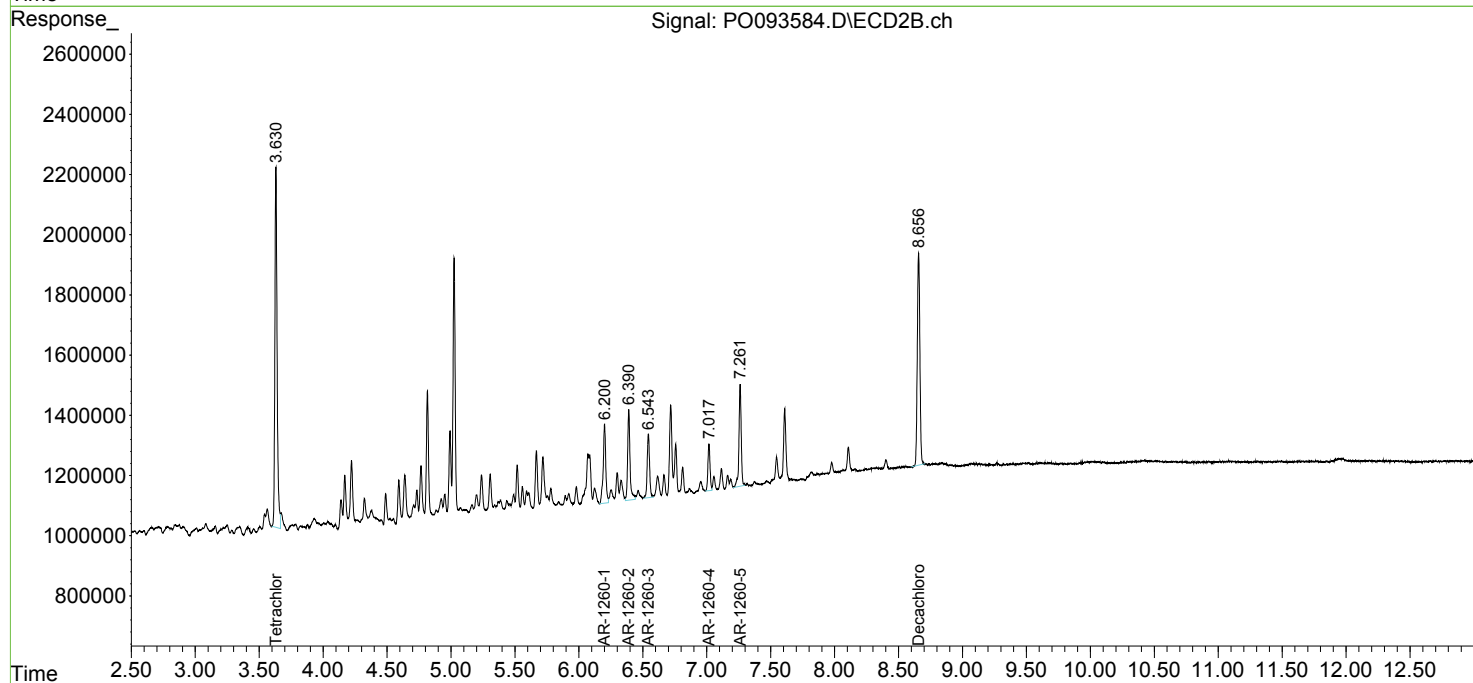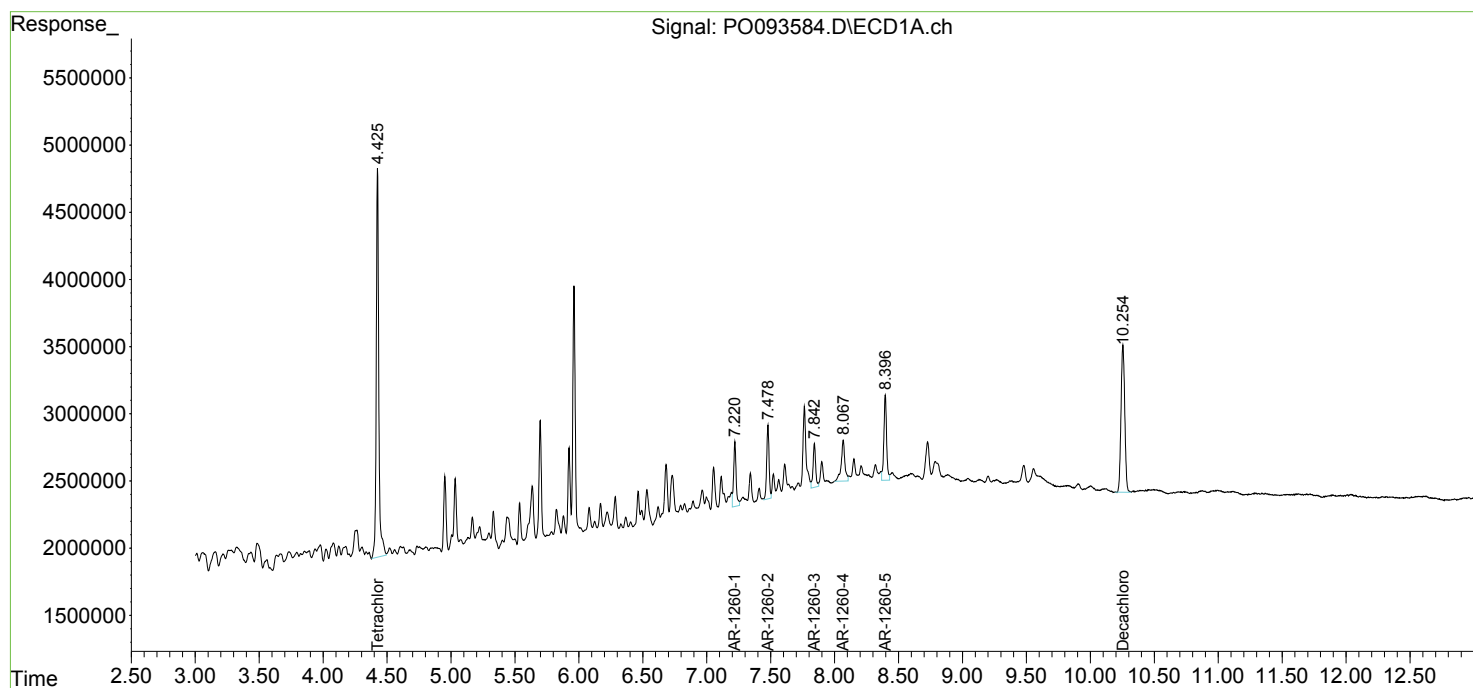


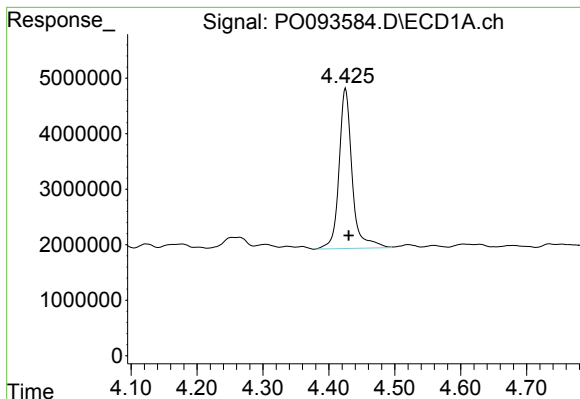

#1 Tetrachloro-m-xylene


R.T.: 4.425 min
Delta R.T.: -0.005 min
Response: 39772239
Conc: 12.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-EAST

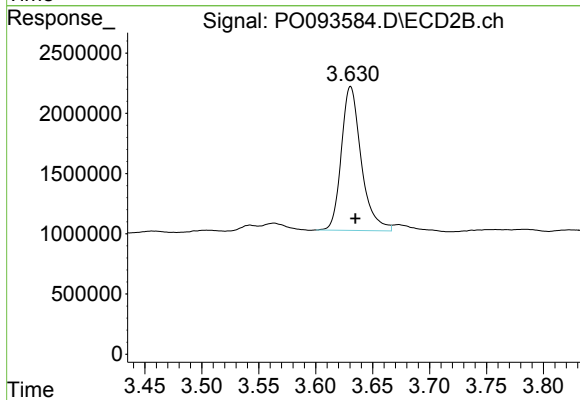


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 14531567
Conc: 12.88 ng/ml

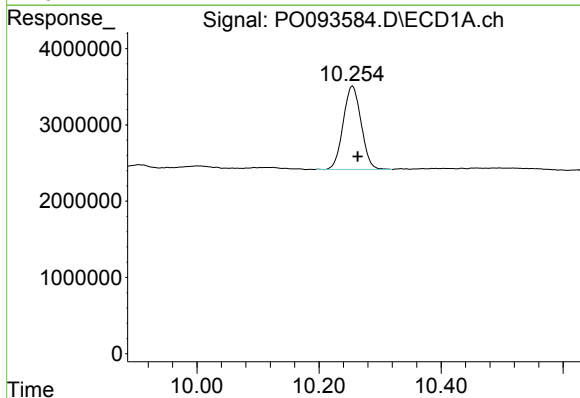


#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: -0.009 min
Response: 22341473
Conc: 10.32 ng/ml

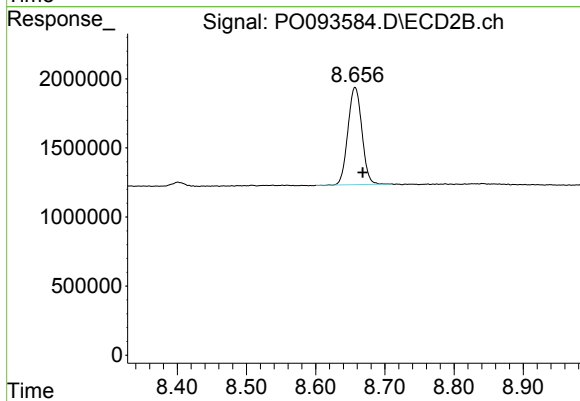

#2 Decachlorobiphenyl


R.T.: 8.657 min
Delta R.T.: -0.011 min
Response: 9864388
Conc: 10.07 ng/ml

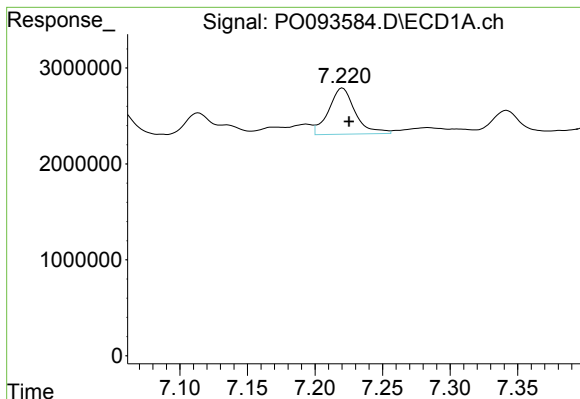

#31 AR-1260-1


R.T.: 7.220 min
Delta R.T.: -0.005 min
Response: 6587998
Conc: 50.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-EAST

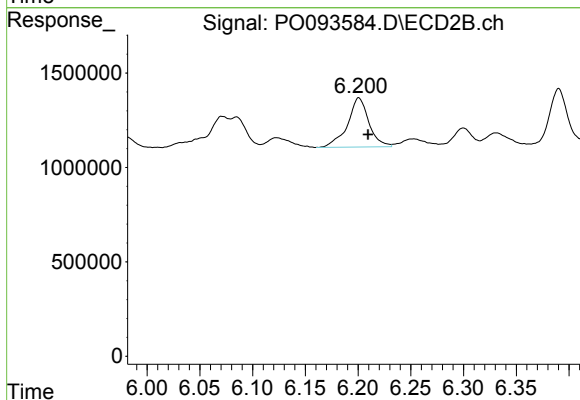


#31 AR-1260-1

R.T.: 6.201 min
Delta R.T.: -0.009 min
Response: 3673518
Conc: 60.42 ng/ml

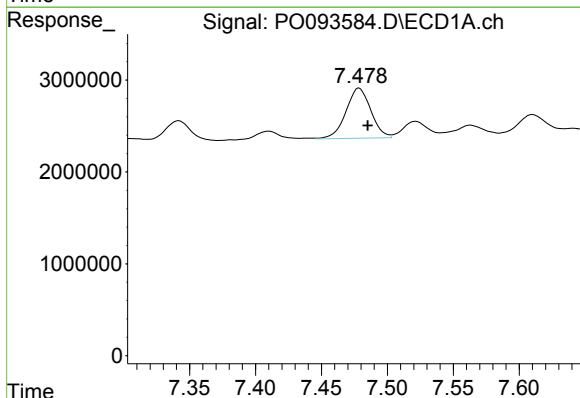


#32 AR-1260-2

R.T.: 7.479 min
Delta R.T.: -0.006 min
Response: 7167596
Conc: 48.55 ng/ml

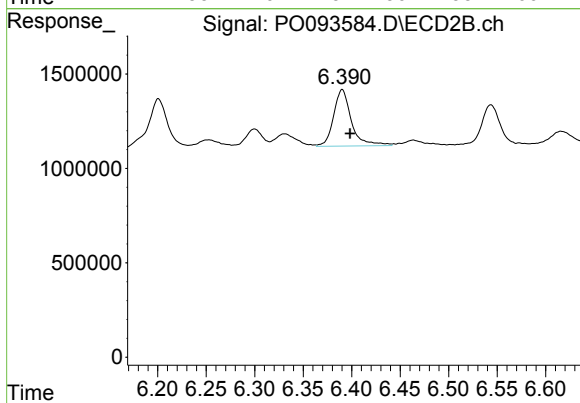

#32 AR-1260-2


R.T.: 6.390 min
Delta R.T.: -0.008 min
Response: 3852078
Conc: 53.28 ng/ml

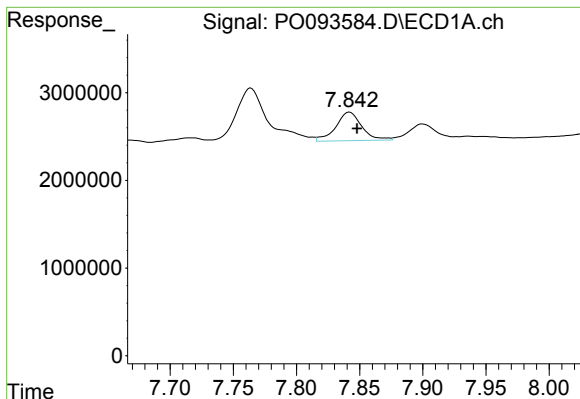

#33 AR-1260-3


R.T.: 7.842 min
Delta R.T.: -0.006 min
Response: 4647009
Conc: 41.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-EAST

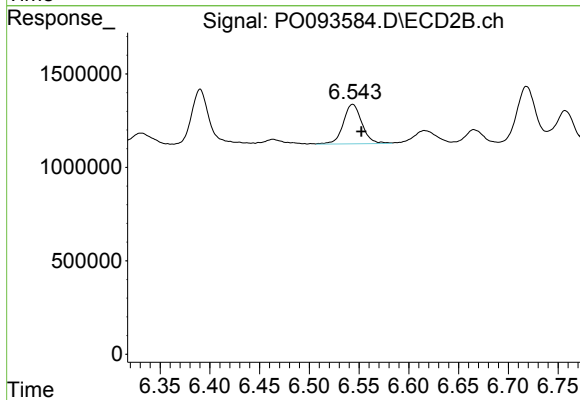


#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: -0.009 min
Response: 2751357
Conc: 41.15 ng/ml

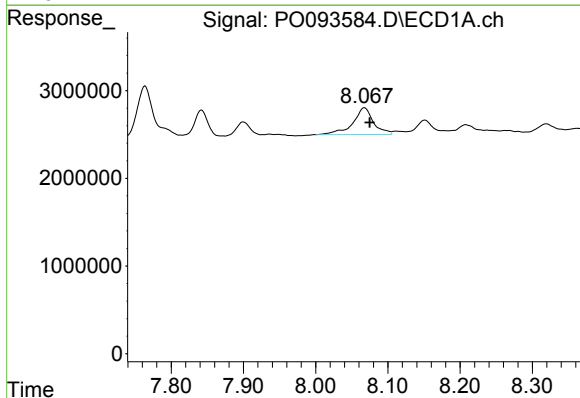


#34 AR-1260-4

R.T.: 8.068 min
Delta R.T.: -0.007 min
Response: 6108881
Conc: 47.64 ng/ml

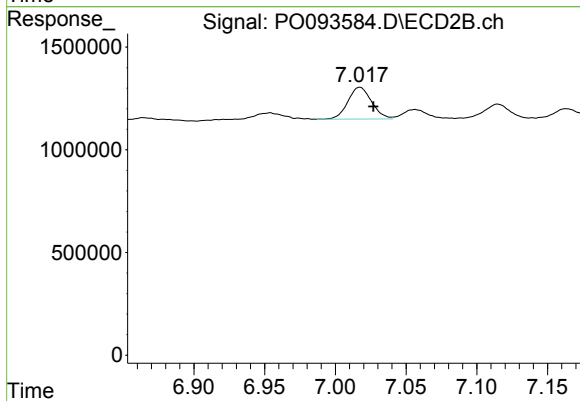

#34 AR-1260-4


R.T.: 7.017 min
Delta R.T.: -0.010 min
Response: 1810138
Conc: 32.89 ng/ml

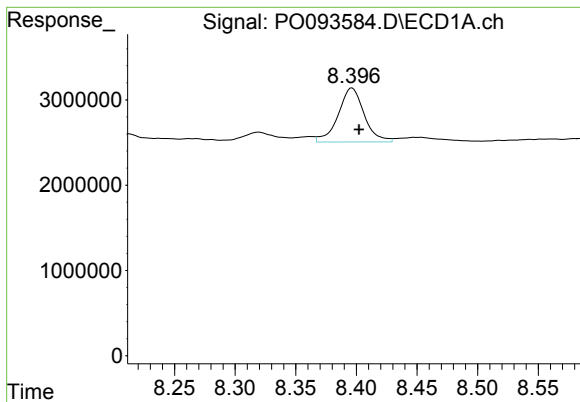

#35 AR-1260-5

R.T.: 8.396 min
Delta R.T.: -0.006 min
Response: 9458263
Conc: 42.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHAMBER-C-72-EAST

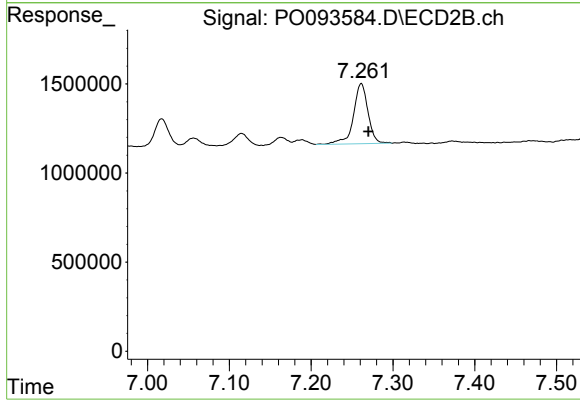

#35 AR-1260-5

R.T.: 7.261 min
Delta R.T.: -0.009 min
Response: 4187358
Conc: 35.57 ng/ml