

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032823\
 Data File : P0093632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2023 21:05
 Operator : YP/AJ
 Sample : 02109-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EB-2023-03-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:03:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.629	59634918	20723064	19.044	18.374
2) SA Decachlor...	10.247	8.651	24903251	11221096	11.506	11.460

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032823\
Data File : PO093632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2023 21:05
Operator : YP/AJ
Sample : 02109-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EB-2023-03-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:03:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

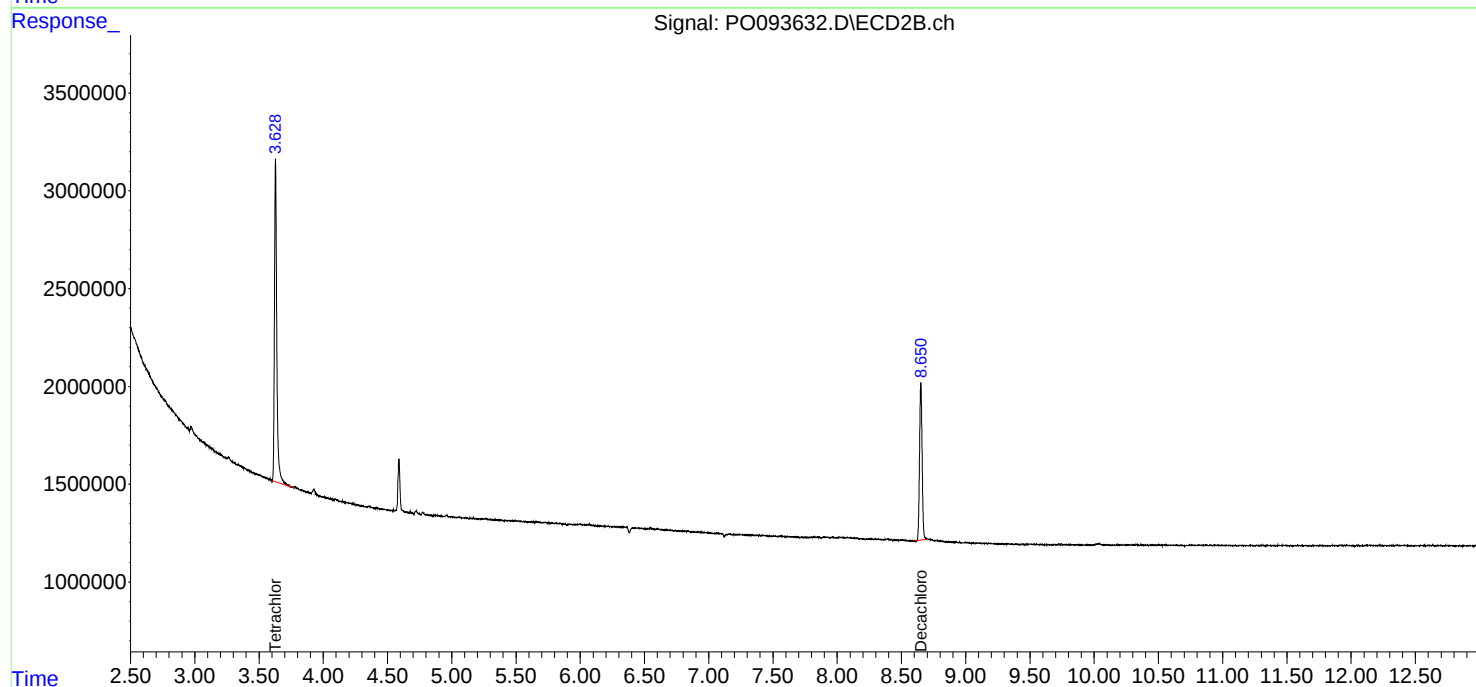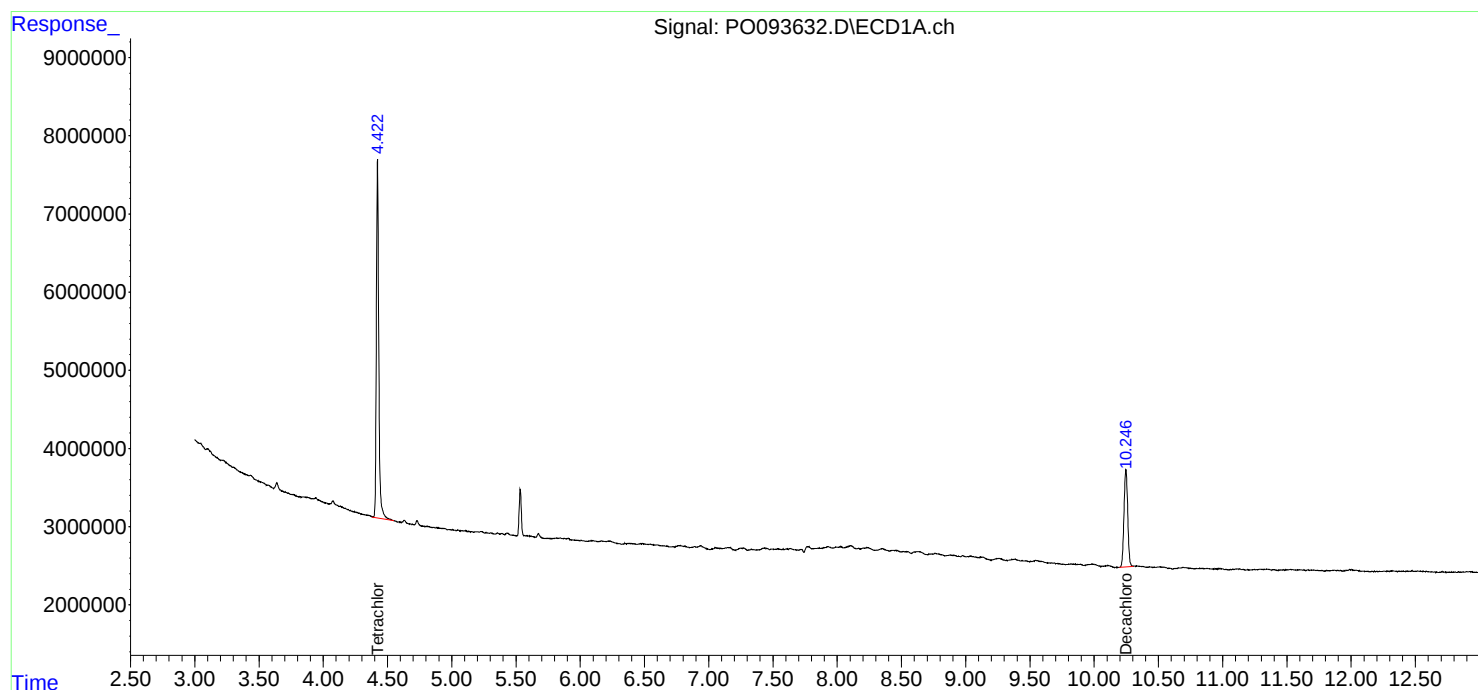


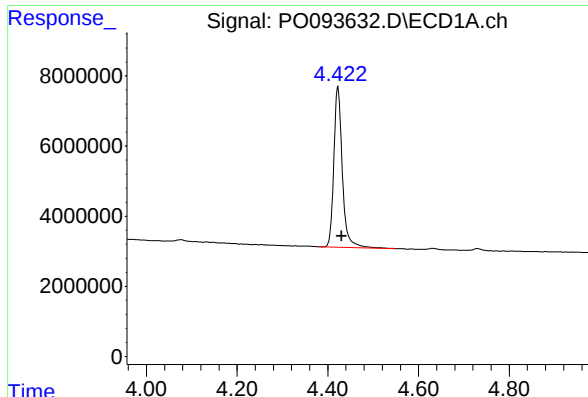

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: -0.008 min
Response: 59634918
Conc: 19.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
EB-2023-03-26

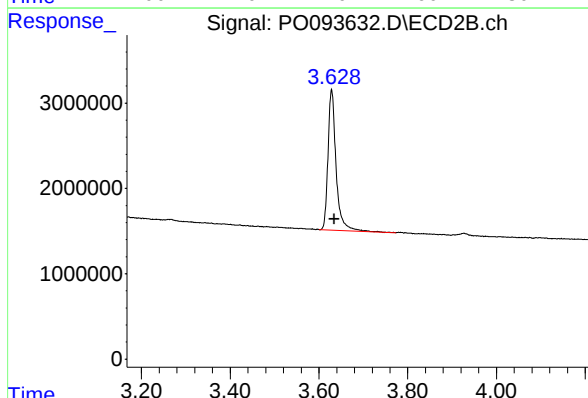


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.006 min
Response: 20723064
Conc: 18.37 ng/ml

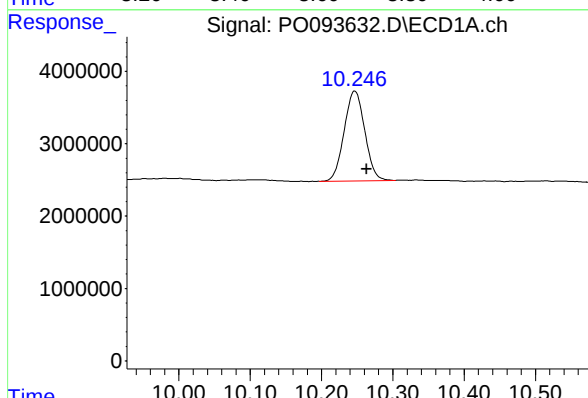

#2 Decachlorobiphenyl

R.T.: 10.247 min
Delta R.T.: -0.017 min
Response: 24903251
Conc: 11.51 ng/ml

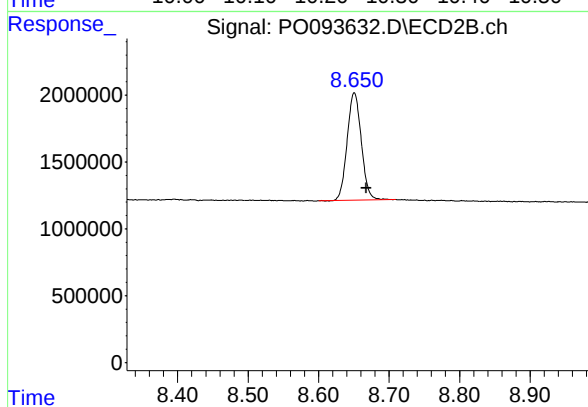

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.017 min
Response: 11221096
Conc: 11.46 ng/ml