

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032922\
 Data File : P0085696.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2022 11:25
 Operator : YP\AJ
 Sample : PB143642BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB143642BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 03:13:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 29 06:17:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.474	3.567	4360966	973875	21.860	20.257
2)	SA Decachlor...	10.382	8.592	3070819	811199	23.417	22.812

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032922\
Data File : P0085696.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2022 11:25
Operator : YP\AJ
Sample : PB143642BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB143642BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 03:13:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 29 06:17:49 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

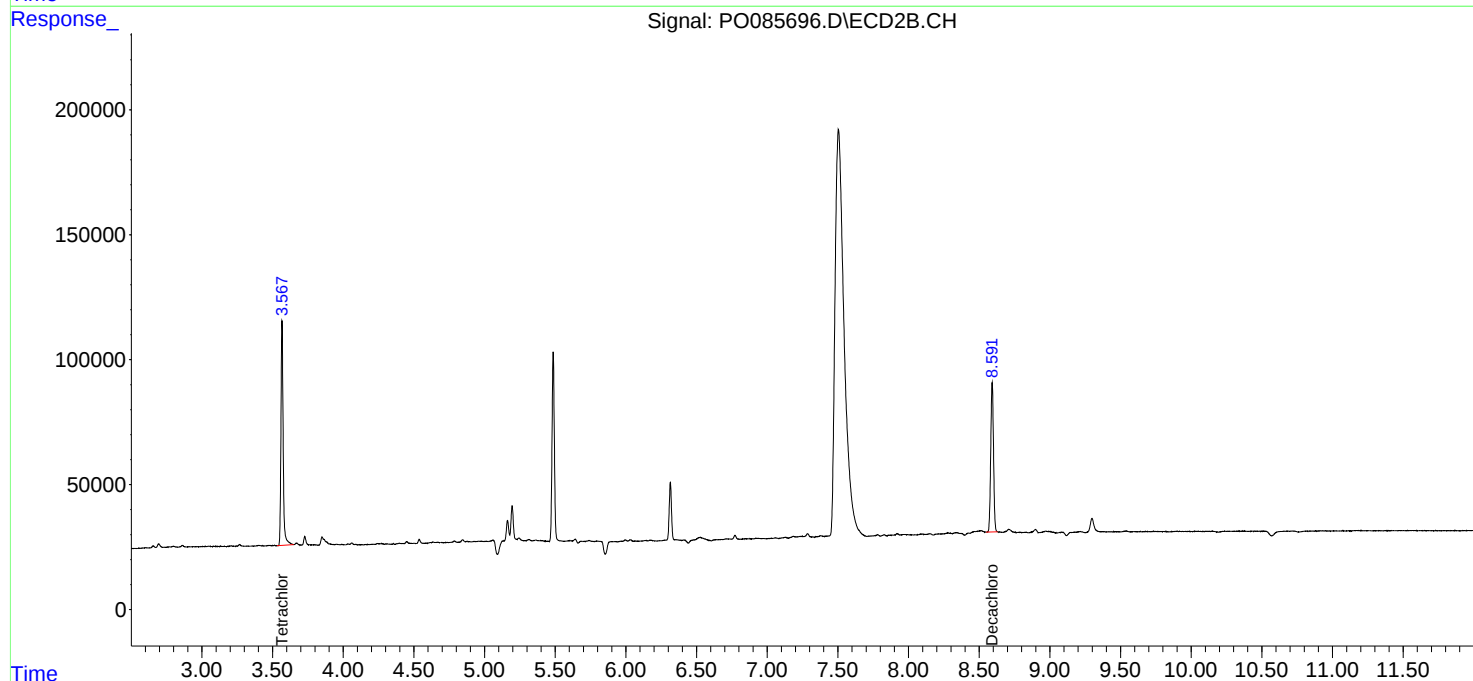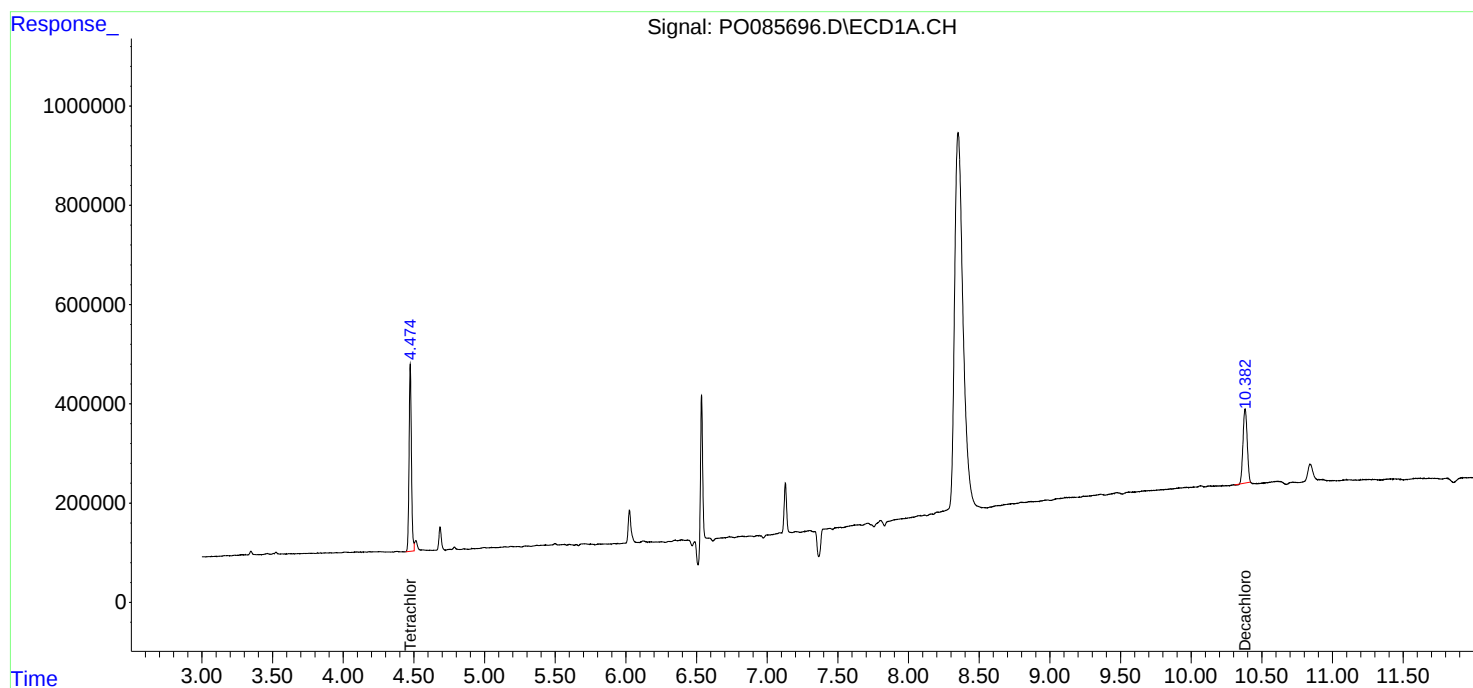


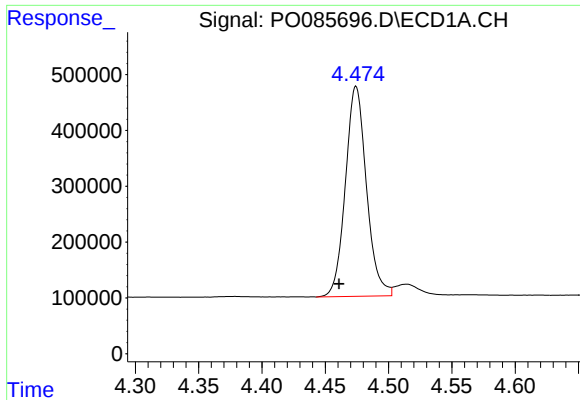

#1 Tetrachloro-m-xylene


R.T.: 4.474 min
Delta R.T.: 0.013 min
Response: 4360966
Conc: 21.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB143642BL

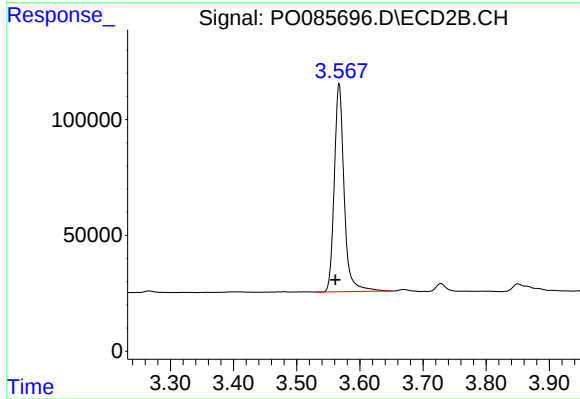


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.006 min
Response: 973875
Conc: 20.26 ng/ml

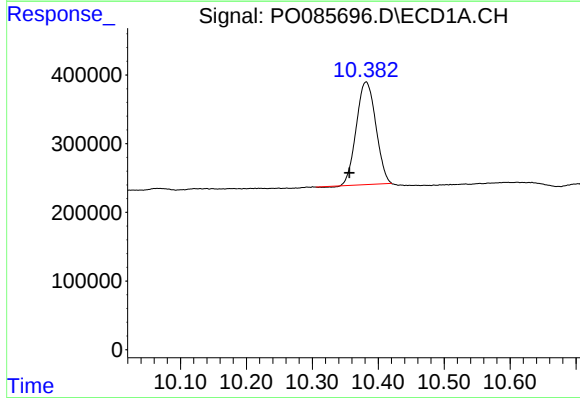

#2 Decachlorobiphenyl

R.T.: 10.382 min
Delta R.T.: 0.025 min
Response: 3070819
Conc: 23.42 ng/ml

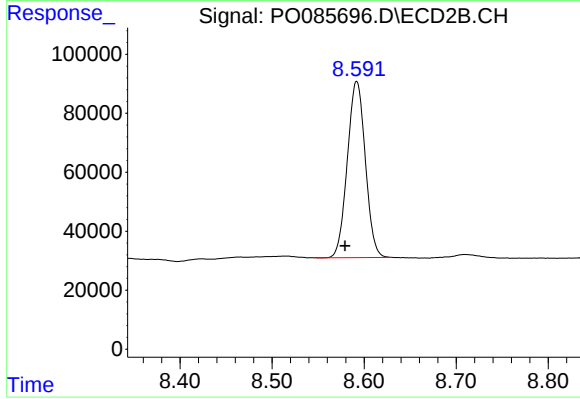

#2 Decachlorobiphenyl

R.T.: 8.592 min
Delta R.T.: 0.013 min
Response: 811199
Conc: 22.81 ng/ml