

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032922\
 Data File : P0085713.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2022 17:07
 Operator : YP\AJ
 Sample : N2123-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-COMP-CS-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/30/2022
 Supervised By :mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 03:20:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 29 06:17:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.460	3.563	3515179	977094	17.620m	20.324
2) SA Decachlor...	10.363	8.581	3188436	751309	24.314	21.128

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032922\
Data File : PO085713.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2022 17:07
Operator : YP\AJ
Sample : N2123-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 03:20:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 29 06:17:49 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

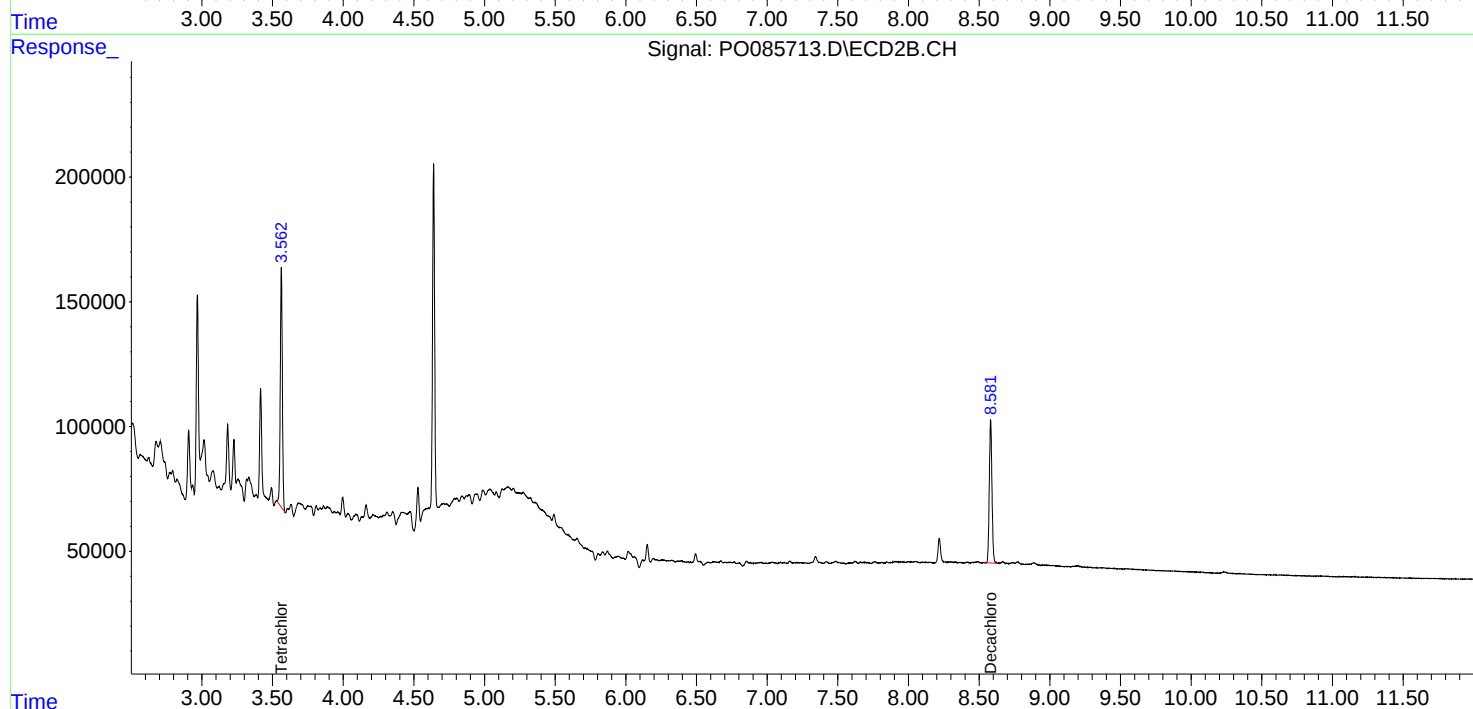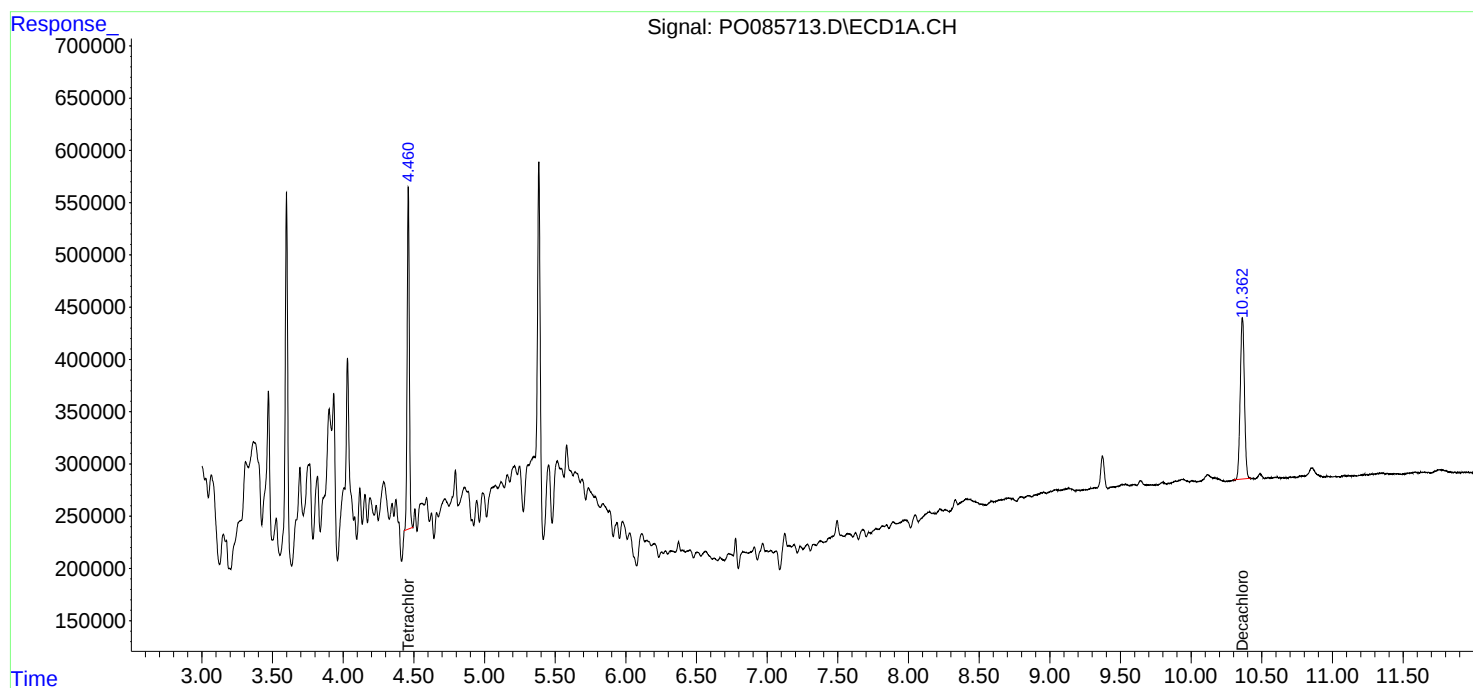

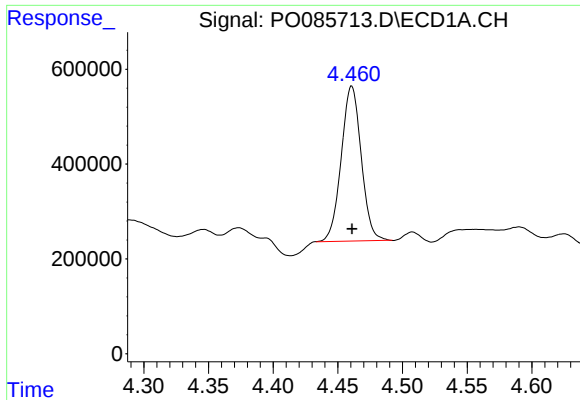


#1 Tetrachloro-m-xylene

R.T.: 4.460 min
Delta R.T.: 0.000 min
Response: 3515179
Conc: 17.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-CS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2022
Supervised By :mohammad ahmed 03/30/2022

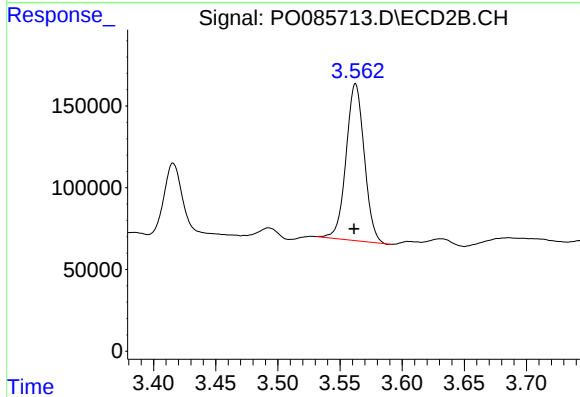


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.001 min
Response: 977094
Conc: 20.32 ng/ml

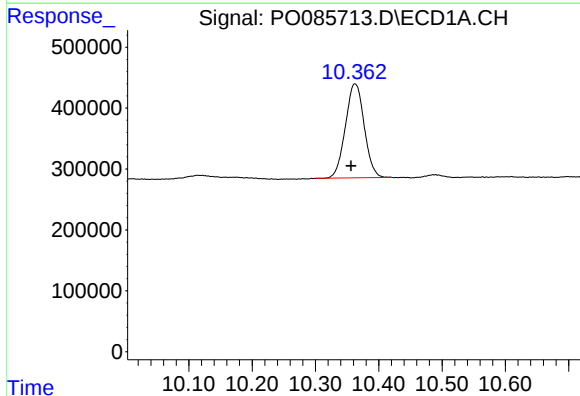

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.006 min
Response: 3188436
Conc: 24.31 ng/ml

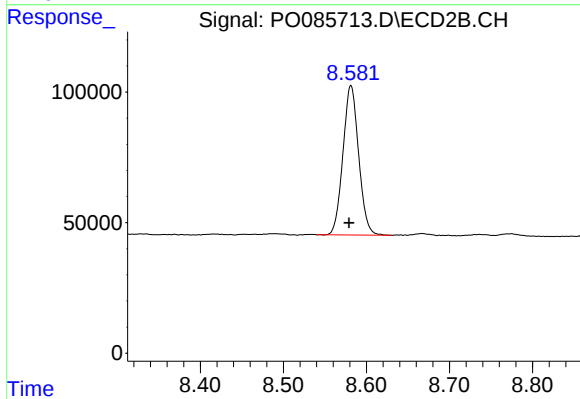

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: 0.002 min
Response: 751309
Conc: 21.13 ng/ml