

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032923\
 Data File : P0093647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2023 13:27
 Operator : YP/AJ
 Sample : 02114-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 15091

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/30/2023
 Supervised By :Ankita Jodhani 03/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 17:11:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

 System Monitoring Compounds

1) SA Tetrachlo...	4.420	3.626	7839588	2637522	2.503m	2.339
2) SA Decachlor...	10.249	8.654	5721045	2390242	2.643	2.441

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032923\
Data File : P0093647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2023 13:27
Operator : YP/AJ
Sample : 02114-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
15091


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2023
Supervised By :Ankita Jodhani 03/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 17:11:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

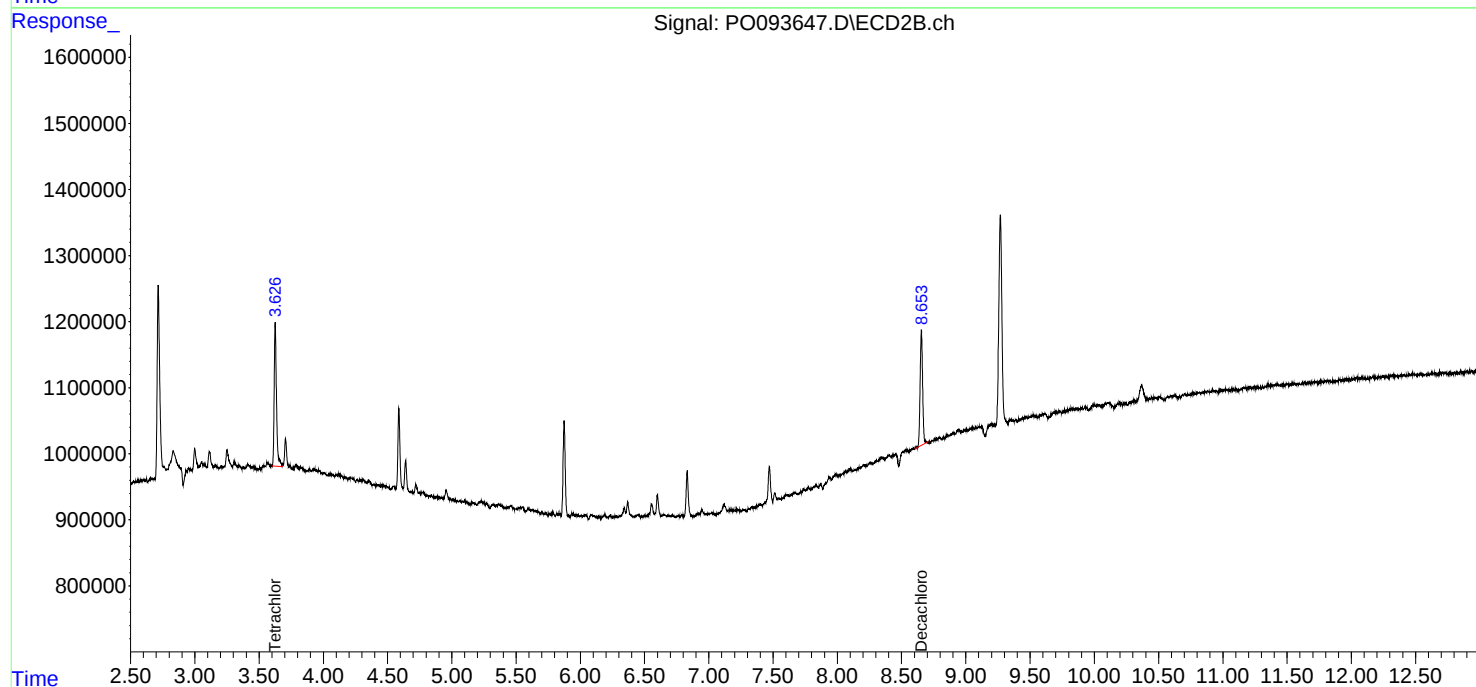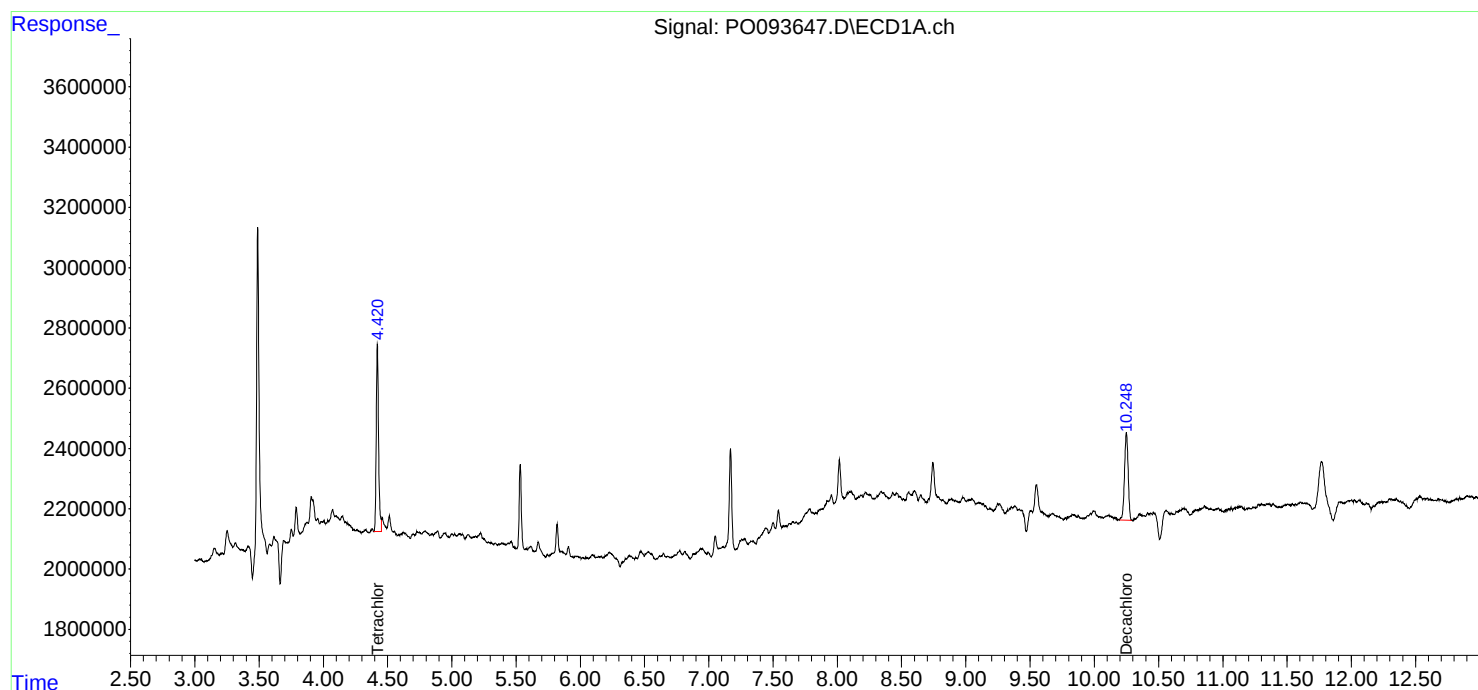

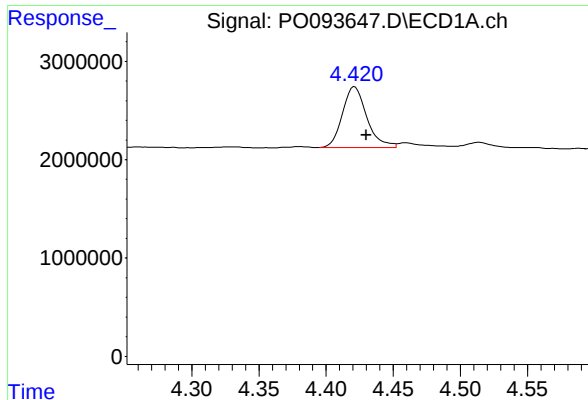


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.010 min
Response: 7839588
Conc: 2.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
15091


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2023
Supervised By :Ankita Jodhani 03/30/2023

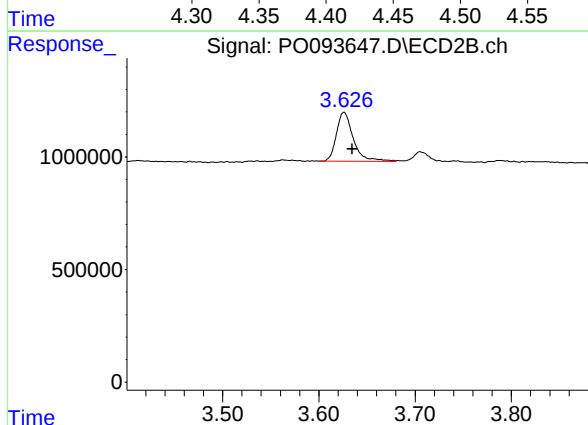


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: -0.009 min
Response: 2637522
Conc: 2.34 ng/ml

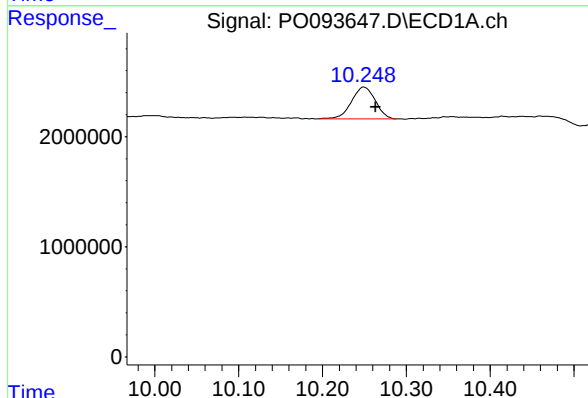

#2 Decachlorobiphenyl

R.T.: 10.249 min
Delta R.T.: -0.014 min
Response: 5721045
Conc: 2.64 ng/ml

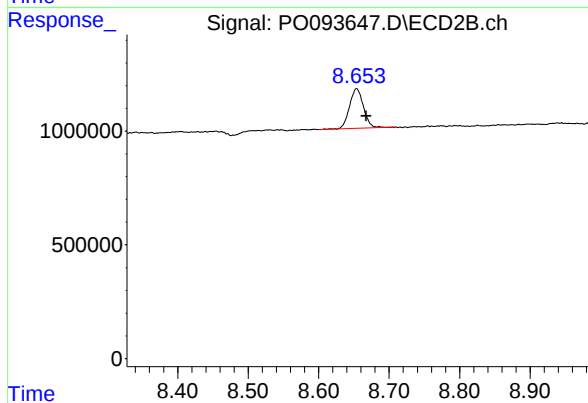

#2 Decachlorobiphenyl

R.T.: 8.654 min
Delta R.T.: -0.014 min
Response: 2390242
Conc: 2.44 ng/ml