

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032923\
 Data File : P0093650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2023 14:18
 Operator : YP/AJ
 Sample : 02113-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-287

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 17:12:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.423	3.628	64487944	22466164	20.593	19.919
2) SA Decachlor...	10.250	8.652	52249627	22302973	24.142	22.778

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032923\
Data File : PO093650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2023 14:18
Operator : YP/AJ
Sample : 02113-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ETGI-287

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 17:12:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

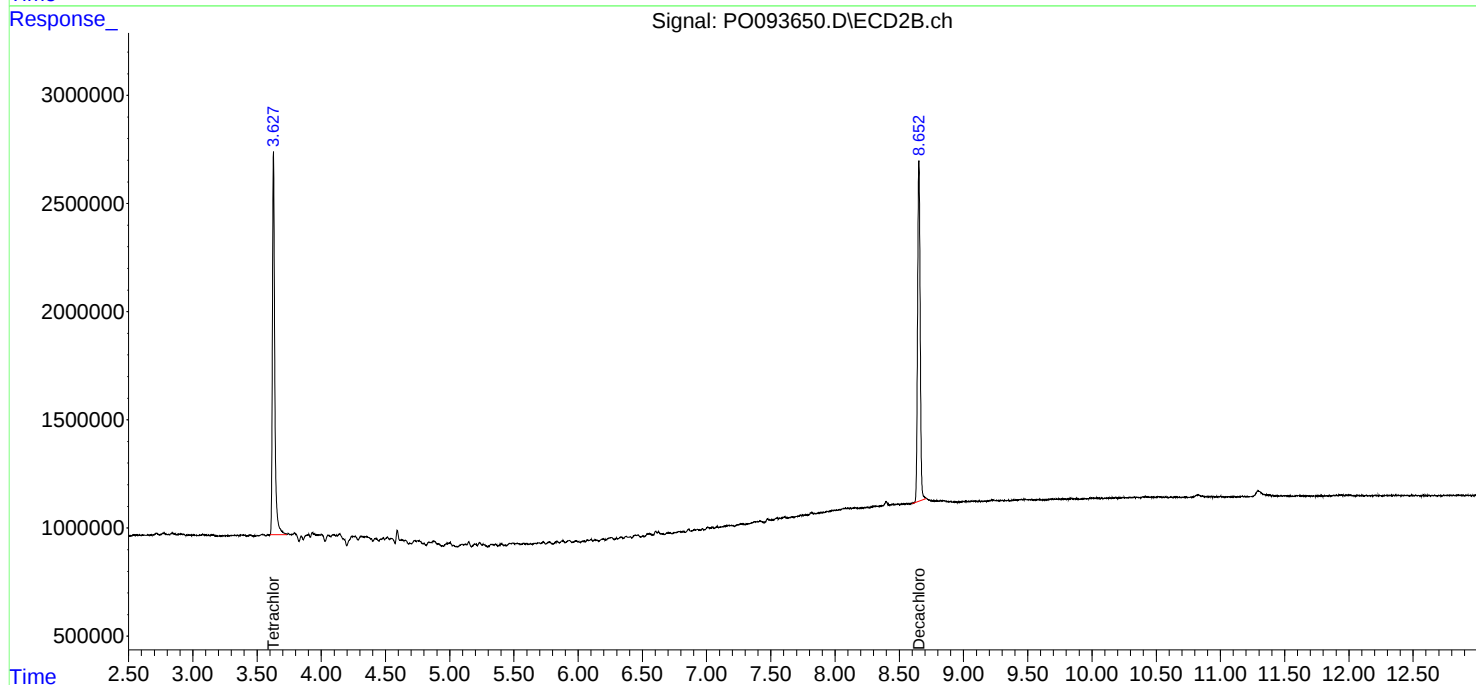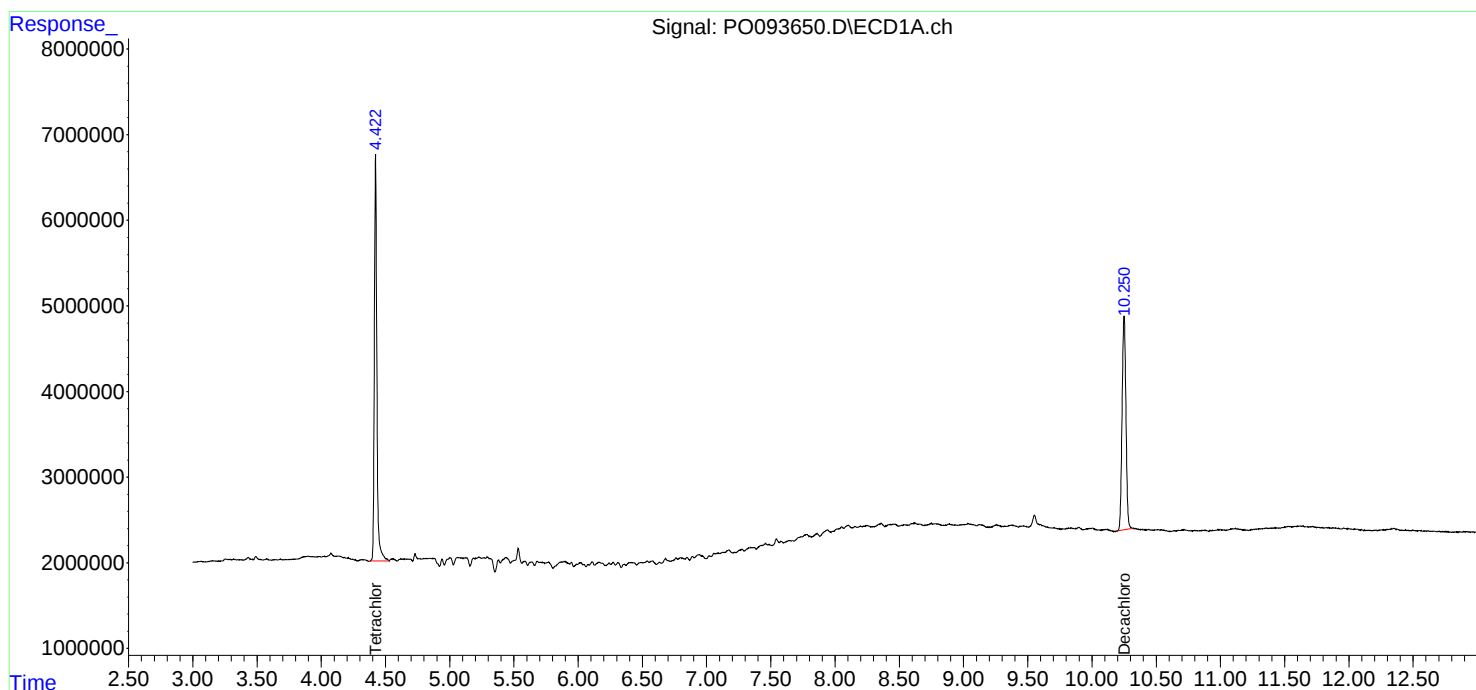


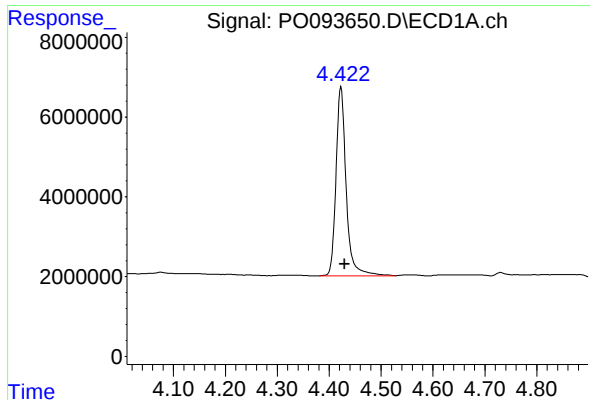

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.007 min
Response: 64487944
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-287

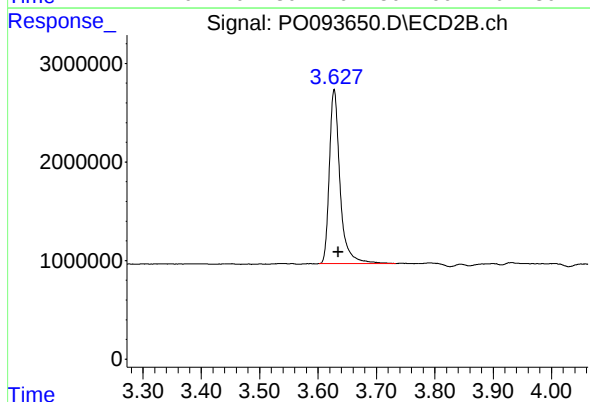


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.007 min
Response: 22466164
Conc: 19.92 ng/ml

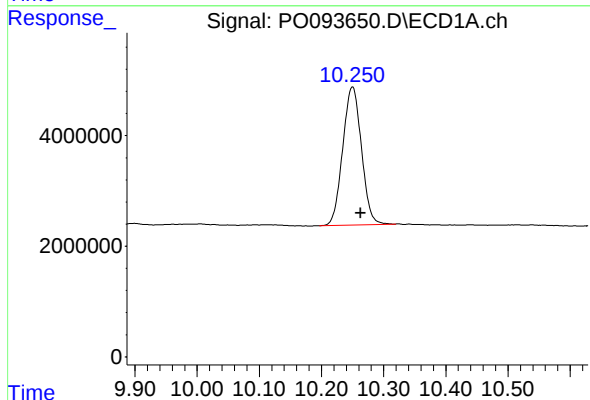

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: -0.013 min
Response: 52249627
Conc: 24.14 ng/ml

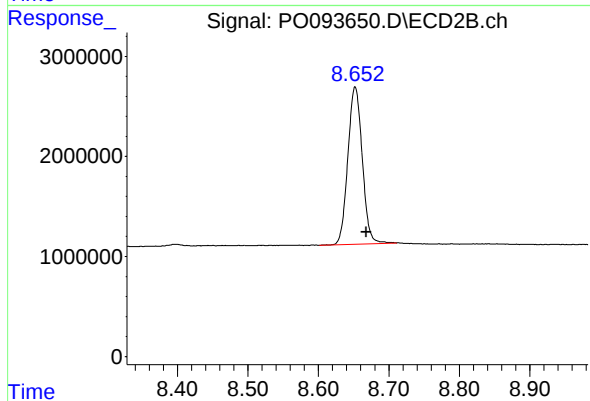

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.016 min
Response: 22302973
Conc: 22.78 ng/ml