

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076587.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2021 9:36
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 13:46:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.911	3.925	4509761	2606185	51.493	47.511
2) SA Decachlor...	10.882	9.179	3508040	2484767	53.891	52.731
Target Compounds						
16) L4 AR-1242-1	6.234	5.172	1036815	569543	463.783	442.200
17) L4 AR-1242-2	6.257	5.192	1633632	1099162	480.815	469.028
18) L4 AR-1242-3	6.323	5.382	949324	498447	469.753	460.327
19) L4 AR-1242-4	6.429	5.476	780693	479528	484.730	432.809
20) L4 AR-1242-5	7.211	6.037	756873	662422	433.324m	499.404

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO033021\
Data File : PO076587.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2021 9:36
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 13:46:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

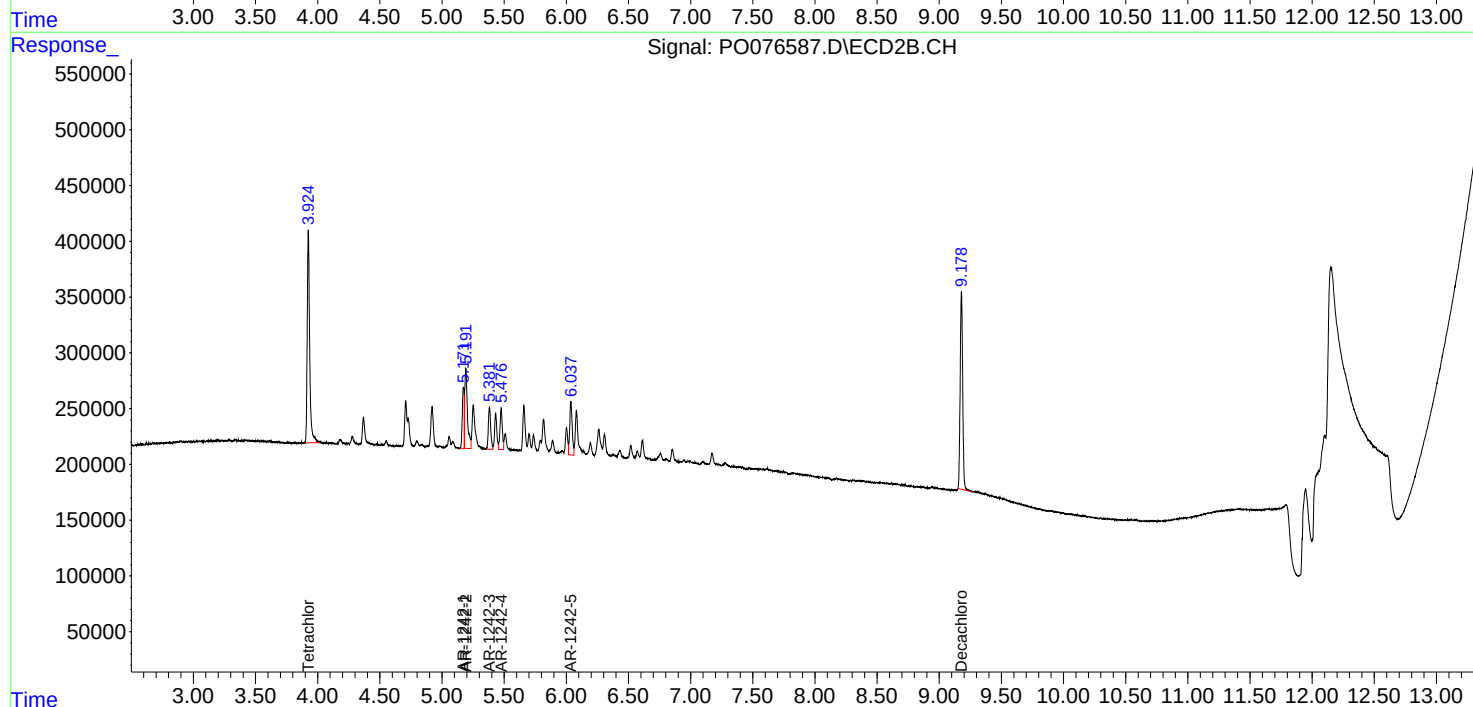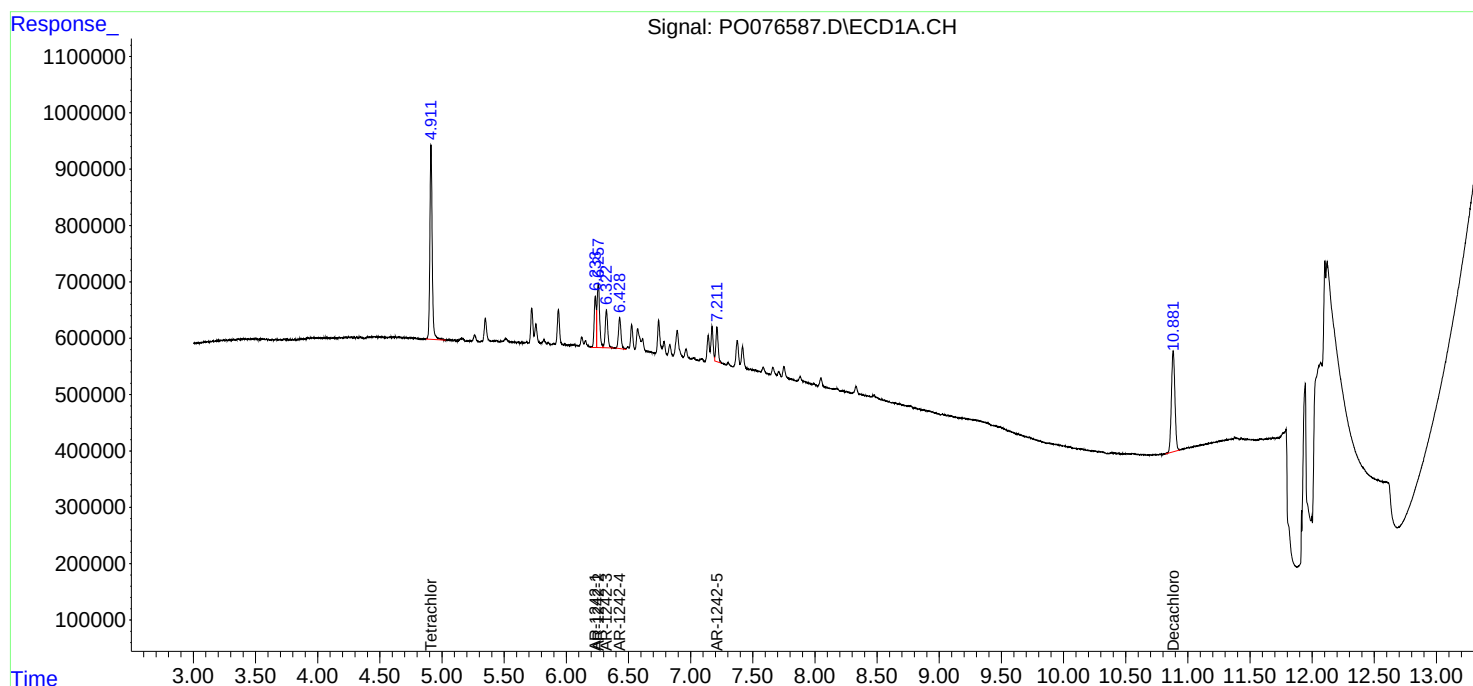

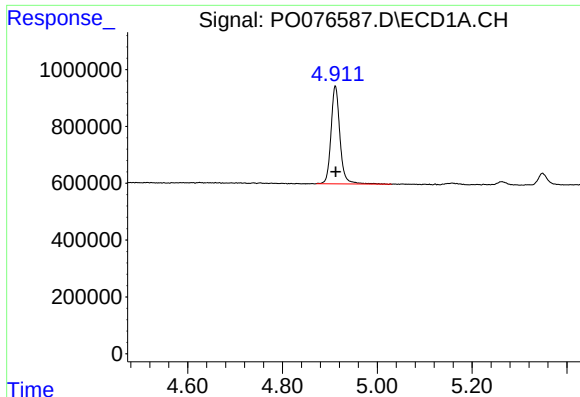


#1 Tetrachloro-m-xylene

R.T.: 4.911 min
Delta R.T.: 0.000 min
Response: 4509761
Conc: 51.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:08 PM

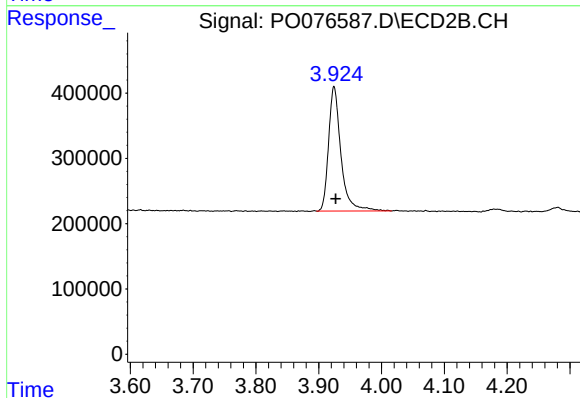


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.003 min
Response: 2606185
Conc: 47.51 ng/ml

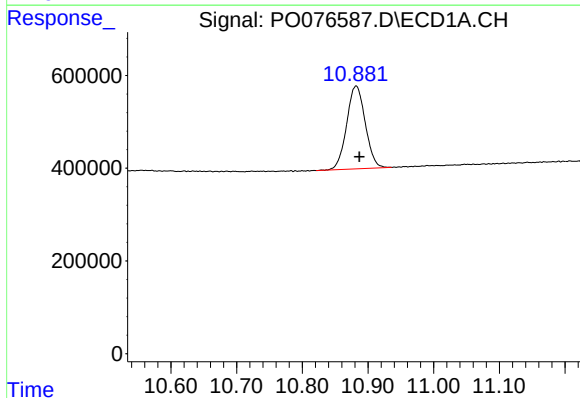


#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.005 min
Response: 3508040
Conc: 53.89 ng/ml

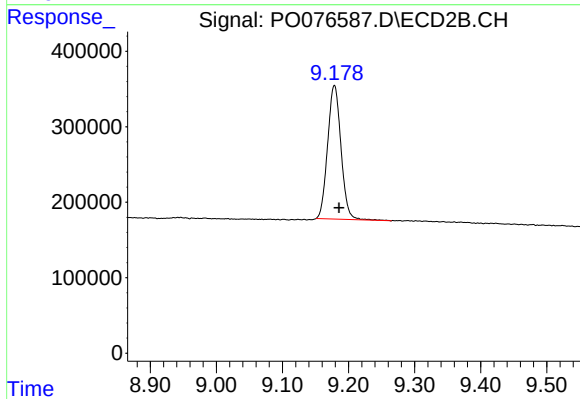

#2 Decachlorobiphenyl

R.T.: 9.179 min
Delta R.T.: -0.007 min
Response: 2484767
Conc: 52.73 ng/ml

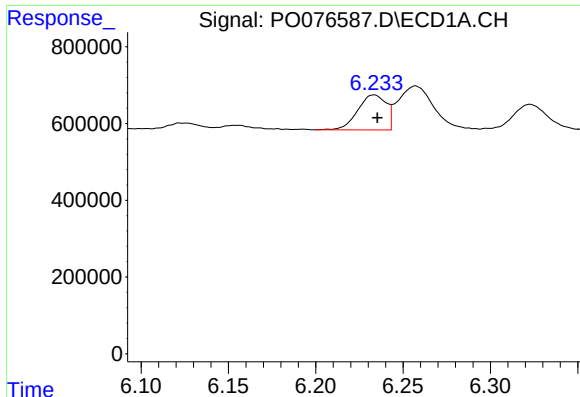


#16 AR-1242-1

R.T.: 6.234 min
Delta R.T.: -0.002 min
Response: 1036815
Conc: 463.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:08 PM

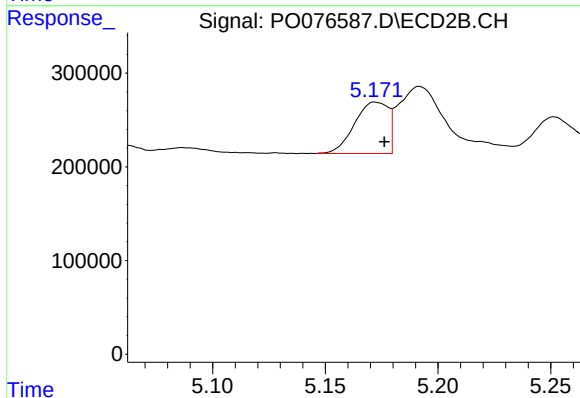


#16 AR-1242-1

R.T.: 5.172 min
Delta R.T.: -0.004 min
Response: 569543
Conc: 442.20 ng/ml

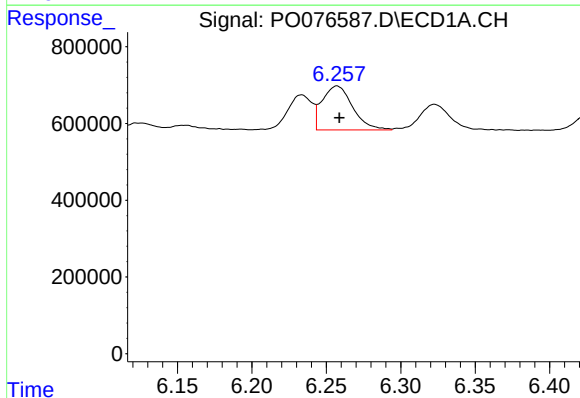


#17 AR-1242-2

R.T.: 6.257 min
Delta R.T.: -0.002 min
Response: 1633632
Conc: 480.82 ng/ml

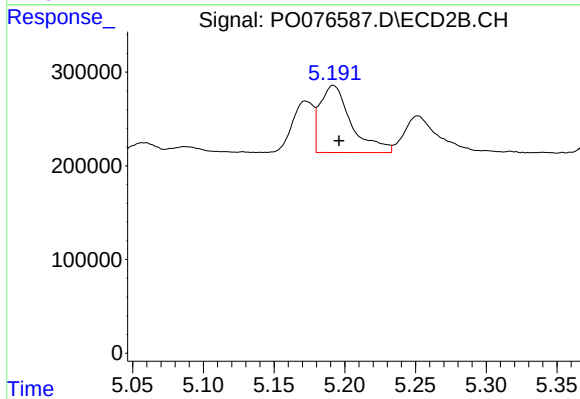

#17 AR-1242-2

R.T.: 5.192 min
Delta R.T.: -0.004 min
Response: 1099162
Conc: 469.03 ng/ml

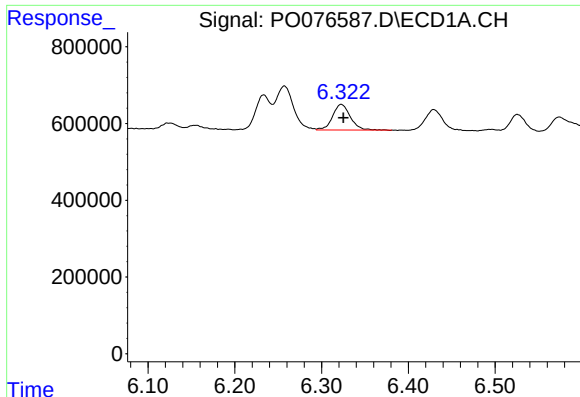


#18 AR-1242-3

R.T.: 6.323 min
Delta R.T.: -0.002 min
Response: 949324
Conc: 469.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:08 PM

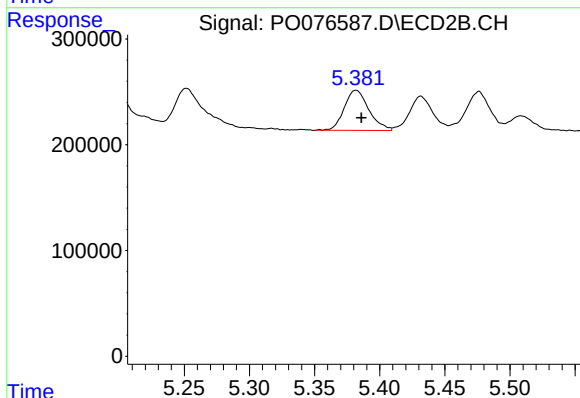


#18 AR-1242-3

R.T.: 5.382 min
Delta R.T.: -0.004 min
Response: 498447
Conc: 460.33 ng/ml

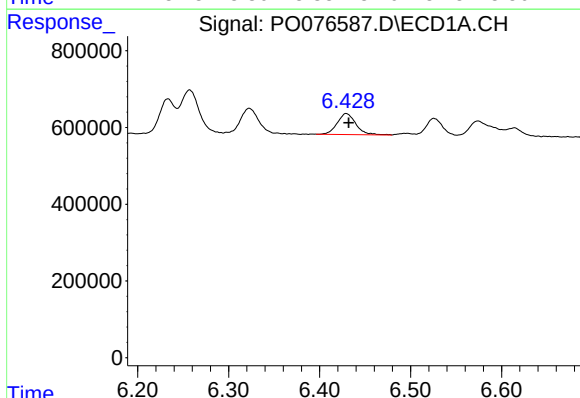


#19 AR-1242-4

R.T.: 6.429 min
Delta R.T.: -0.003 min
Response: 780693
Conc: 484.73 ng/ml

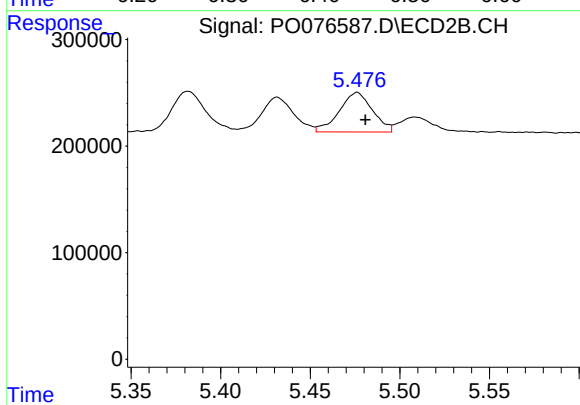

#19 AR-1242-4

R.T.: 5.476 min
Delta R.T.: -0.005 min
Response: 479528
Conc: 432.81 ng/ml

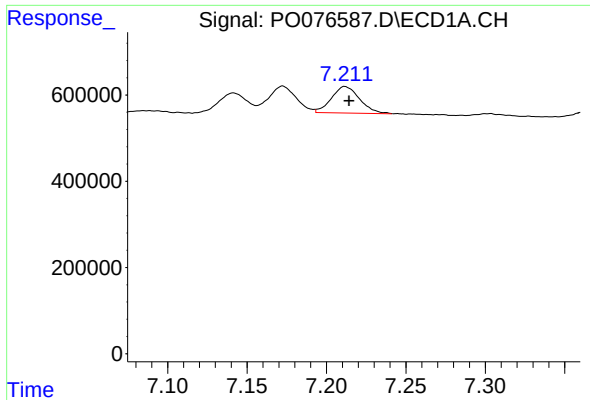


#20 AR-1242-5

R.T.: 7.211 min
Delta R.T.: -0.003 min
Response: 756873
Conc: 433.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:08 PM

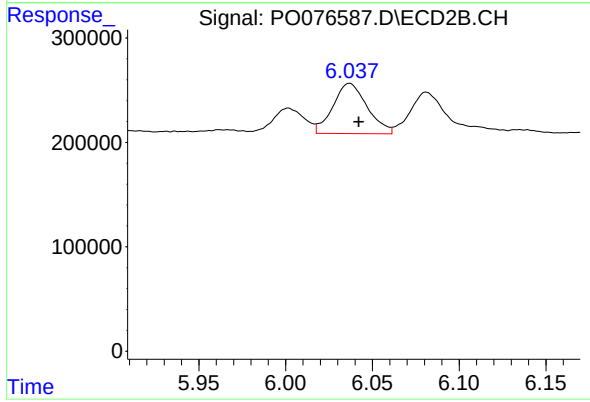

#20 AR-1242-5

R.T.: 6.037 min
Delta R.T.: -0.005 min
Response: 662422
Conc: 499.40 ng/ml