

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2021 11:31
 Operator : DD\AJ
 Sample : M1776-05RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 107

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 13:48:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.927	1016785	571265	11.610	10.414m
2) SA Decachlor...	10.882	9.185	924311	2666072	14.199m	56.578m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2021 11:31
Operator : DD\AJ
Sample : M1776-05RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
107


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 13:48:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

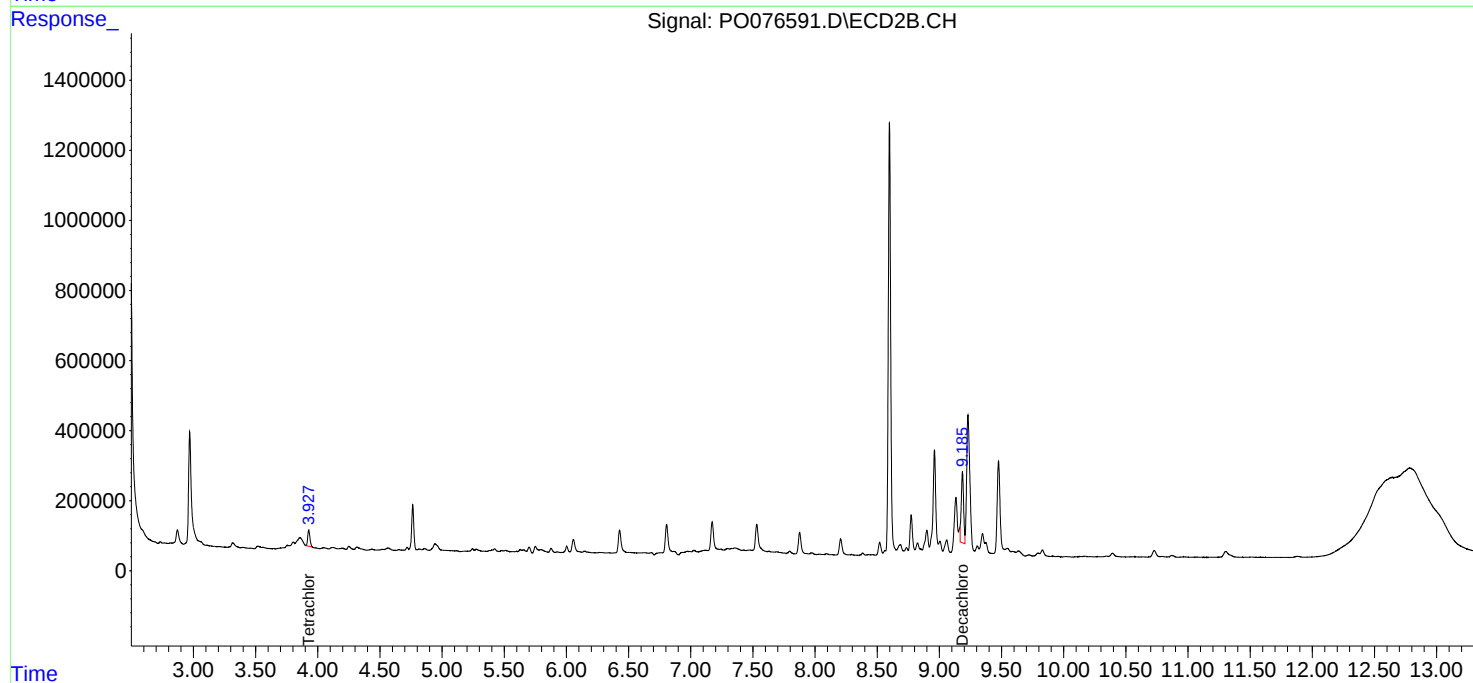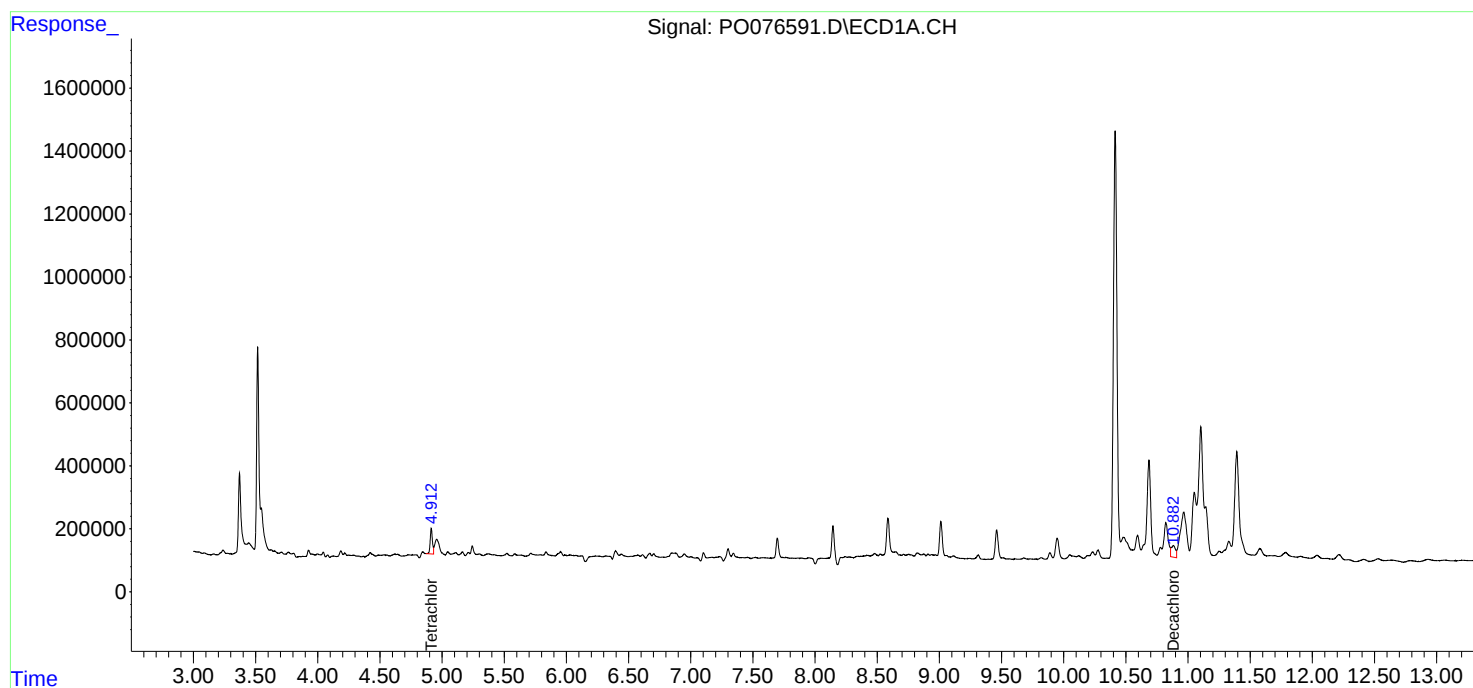

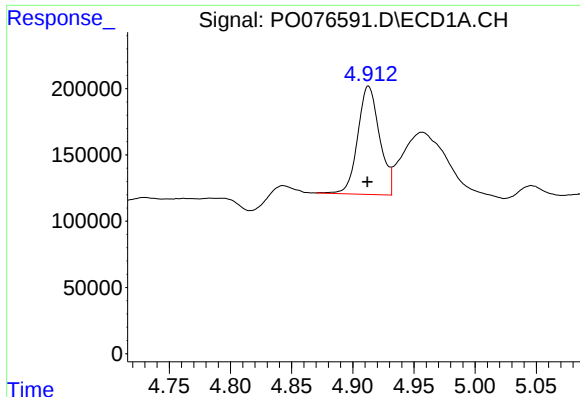


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 1016785
Conc: 11.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
107


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:10 PM

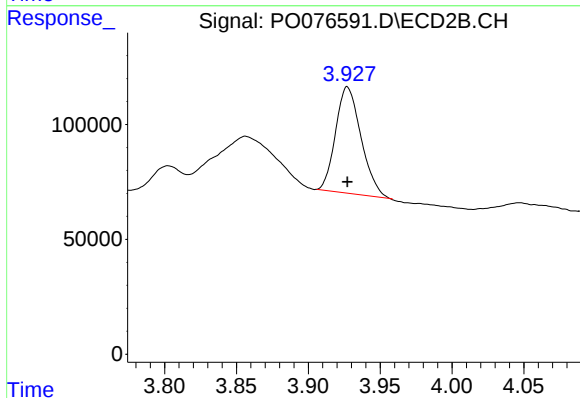


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 571265
Conc: 10.41 ng/ml m

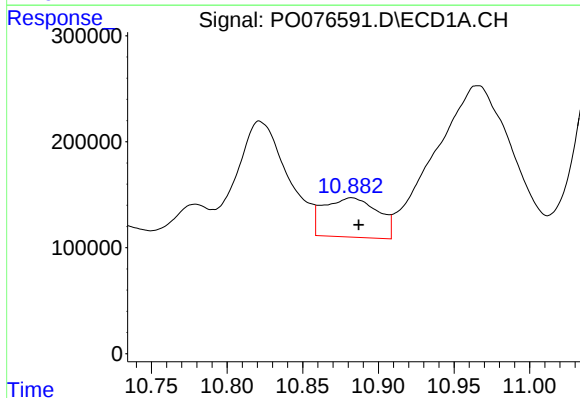

#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.005 min
Response: 924311
Conc: 14.20 ng/ml m

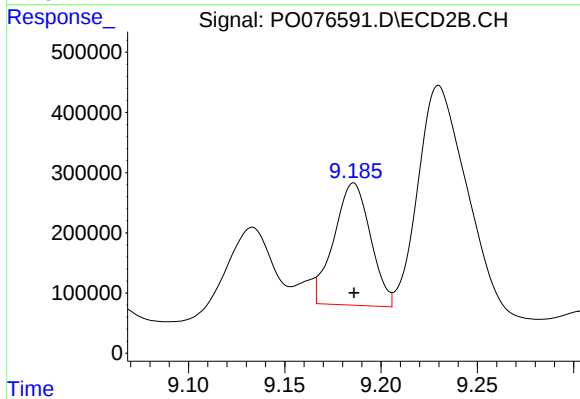

#2 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.000 min
Response: 2666072
Conc: 56.58 ng/ml m