

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2021 11:48
 Operator : DD\AJ
 Sample : M1814-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-1A-(0.0-0.5)

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 13:49:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.926	2546388	1442291	29.075	26.293
2) SA Decachlor...	10.885	9.181	1972995	1153279	30.310m	24.474

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2021 11:48
Operator : DD\AJ
Sample : M1814-11
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-1A-(0.0-0.5)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 13:49:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

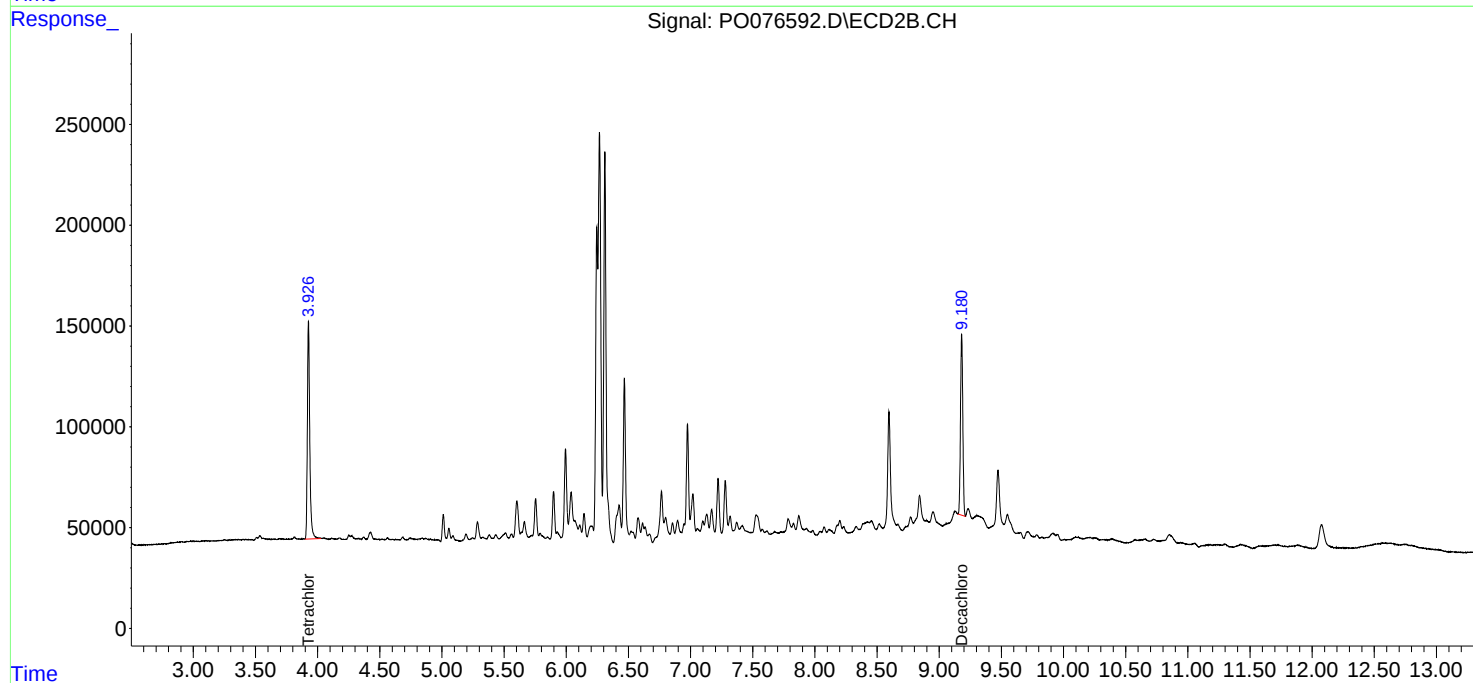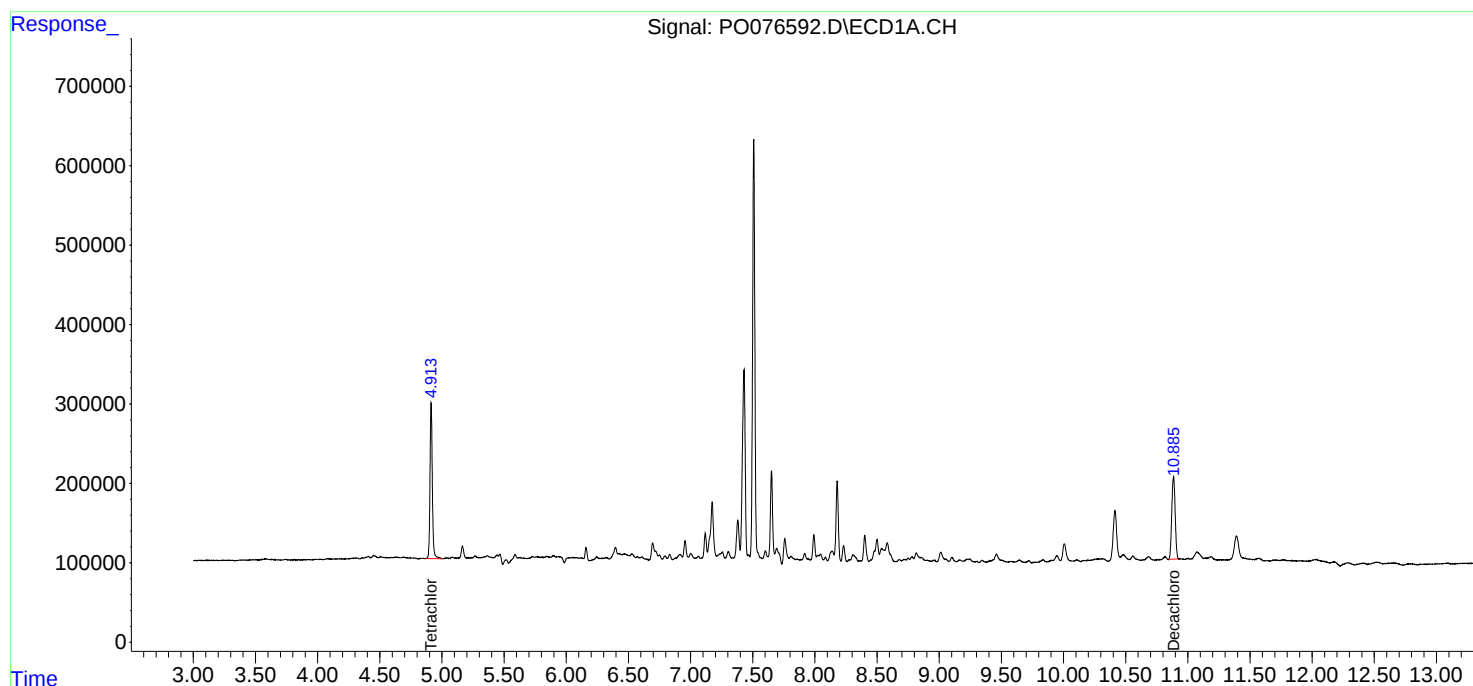

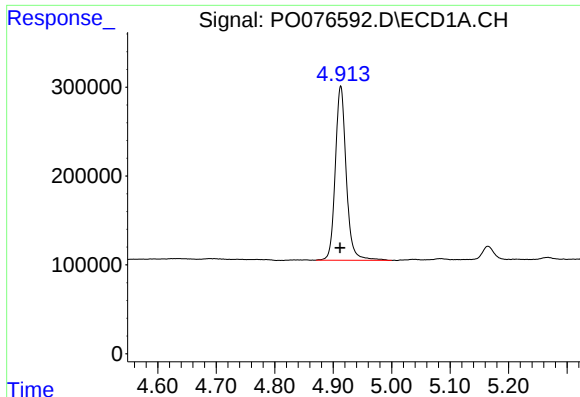


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 2546388
Conc: 29.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-1A-(0.0-0.5)


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:12 PM

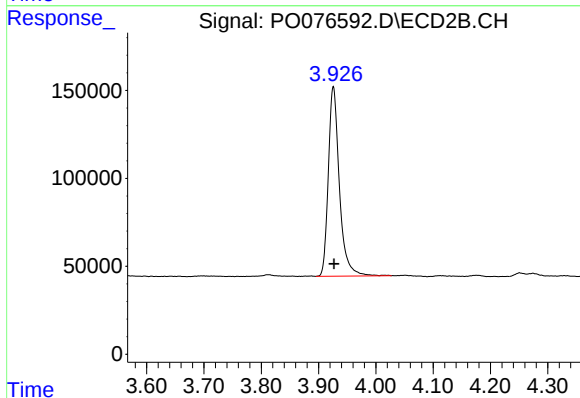


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 1442291
Conc: 26.29 ng/ml

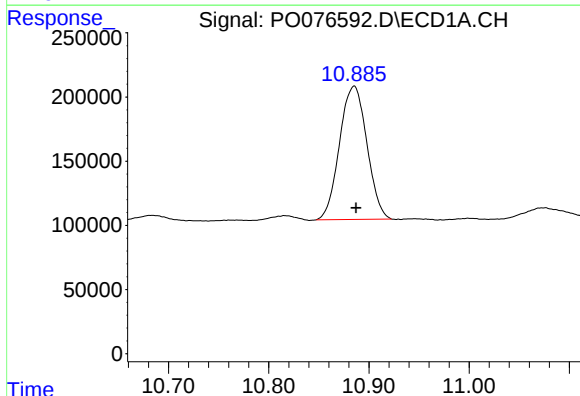

#2 Decachlorobiphenyl

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 1972995
Conc: 30.31 ng/ml m

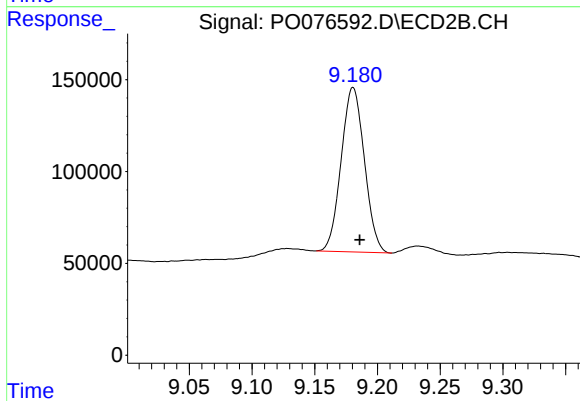

#2 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.005 min
Response: 1153279
Conc: 24.47 ng/ml