

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2021 19:13
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 02:04:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.928	3994718	2266027	45.612	41.310
2) SA Decachlor...	10.885	9.181	3687703	2261700	56.651	47.997
Target Compounds						
16) L4 AR-1242-1	6.235	5.175	965636	519030	431.943	402.982m
17) L4 AR-1242-2	6.259	5.195	1564849	965754	460.571	412.101m
18) L4 AR-1242-3	6.324	5.385	938181	442652	464.239	408.799
19) L4 AR-1242-4	6.432	5.478	738282	479137	458.397	432.456
20) L4 AR-1242-5	7.214	6.040	916135	595664	524.505	449.076

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO033021\
Data File : PO076617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2021 19:13
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 02:04:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

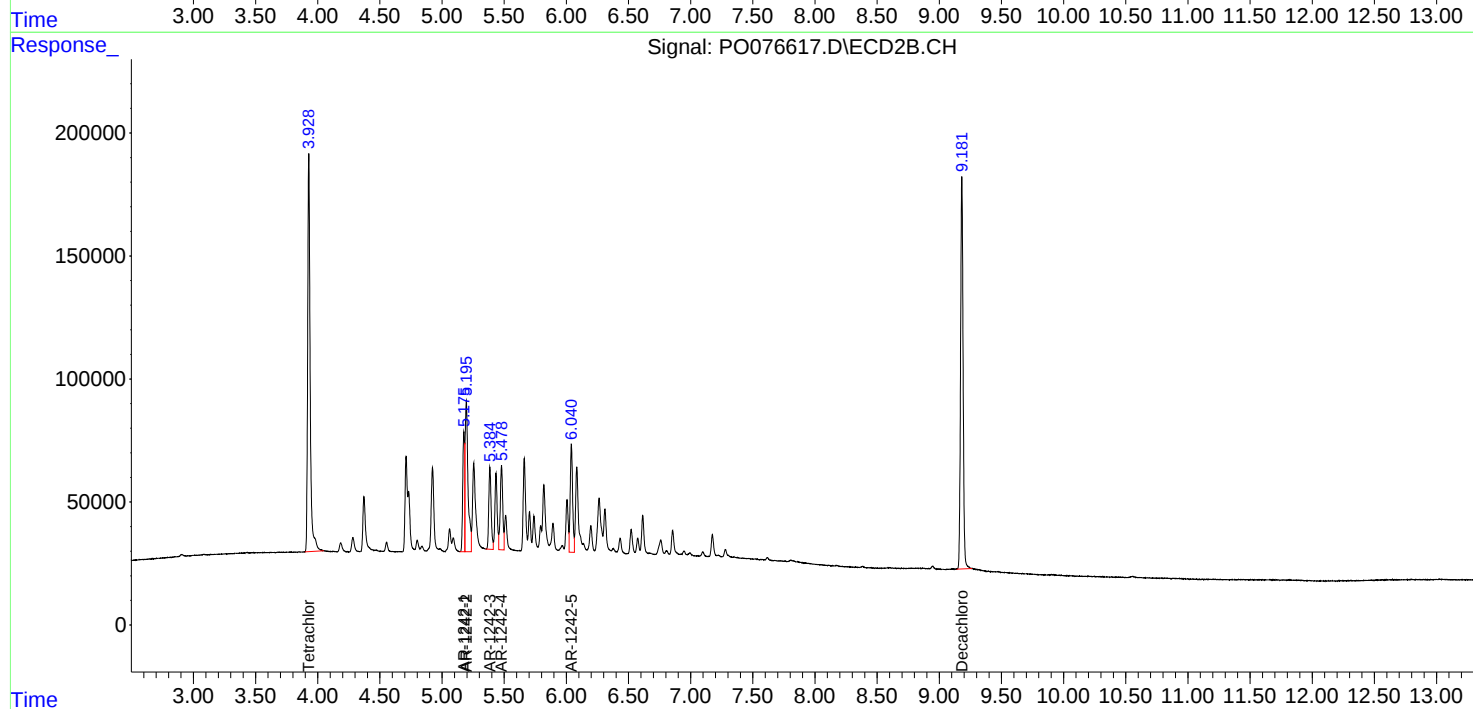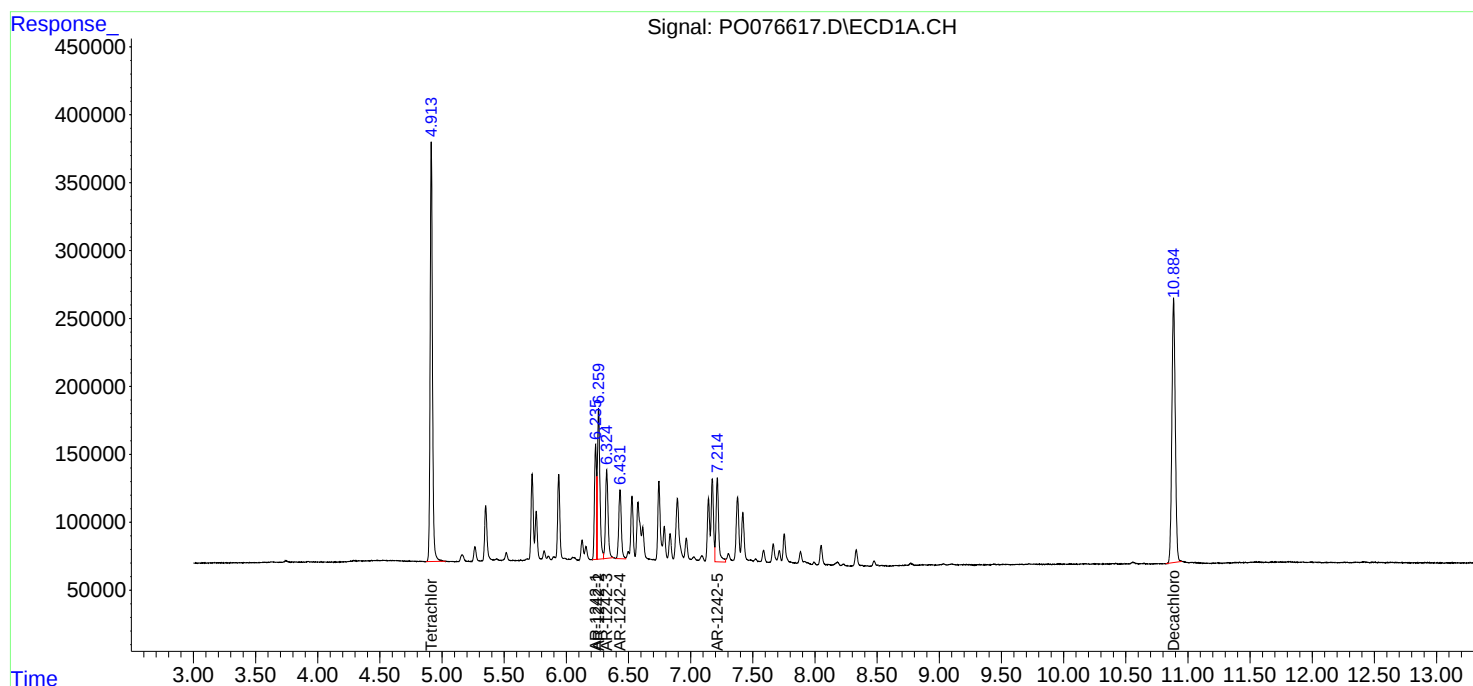

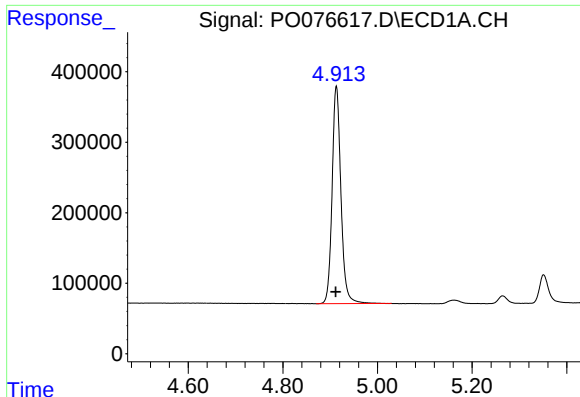


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.001 min
Response: 3994718
Conc: 45.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:25 PM

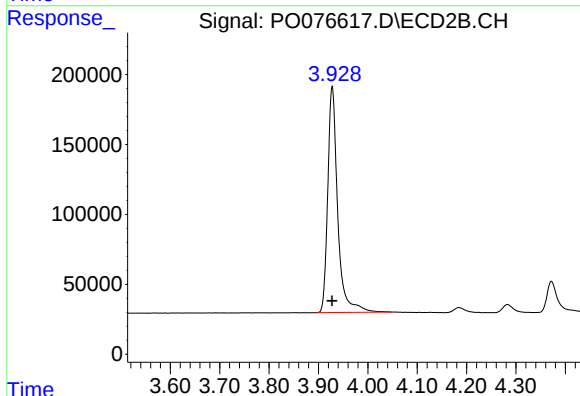


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: 0.000 min
Response: 2266027
Conc: 41.31 ng/ml

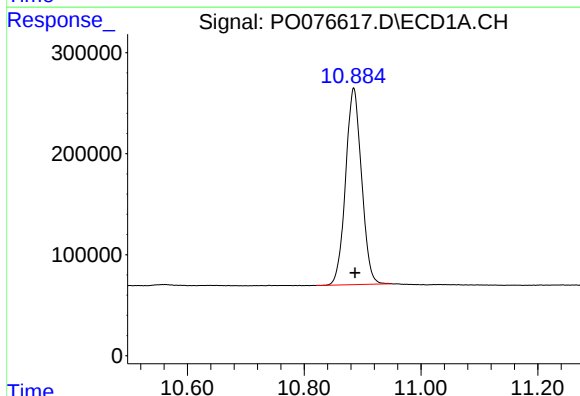


#2 Decachlorobiphenyl

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 3687703
Conc: 56.65 ng/ml

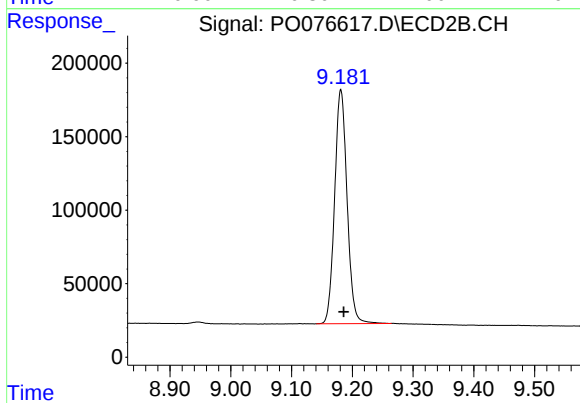

#2 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.005 min
Response: 2261700
Conc: 48.00 ng/ml

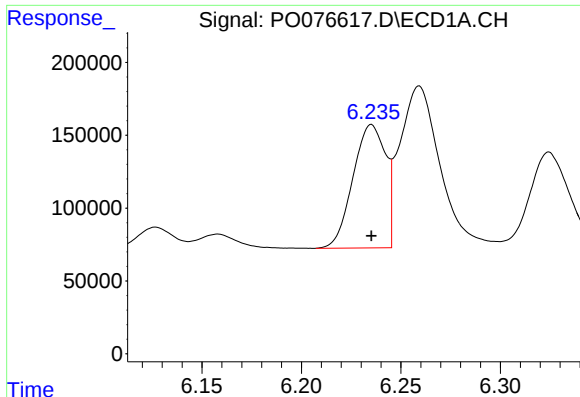


#16 AR-1242-1

R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 965636
Conc: 431.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:25 PM

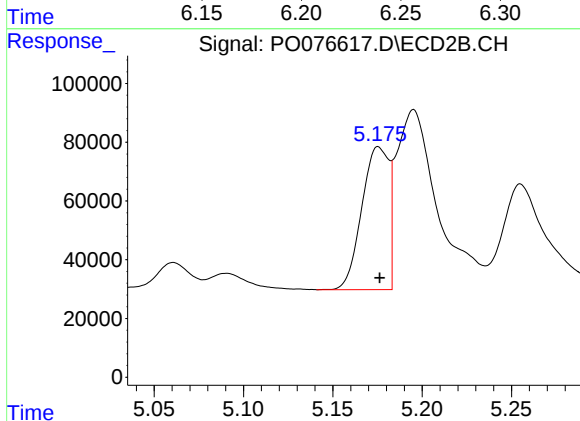


#16 AR-1242-1

R.T.: 5.175 min
Delta R.T.: -0.001 min
Response: 519030
Conc: 402.98 ng/ml m

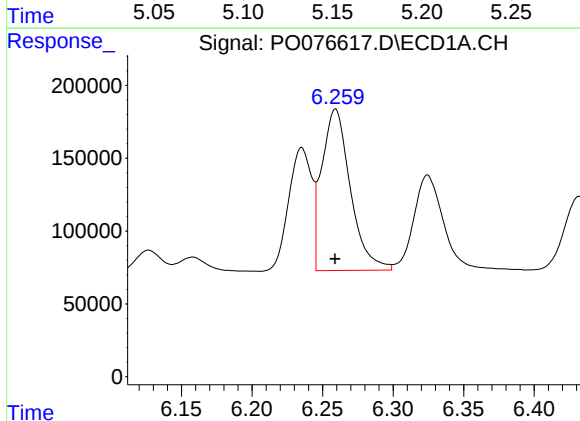


#17 AR-1242-2

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 1564849
Conc: 460.57 ng/ml

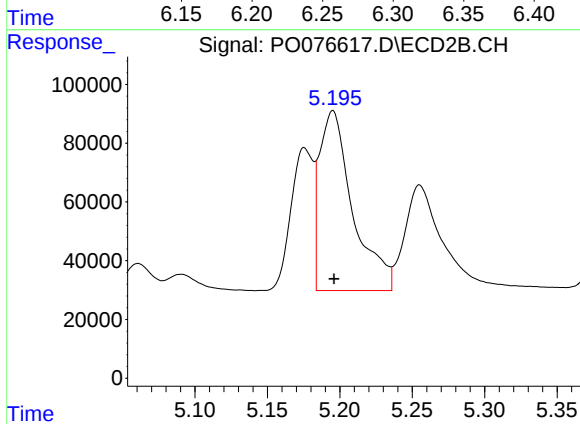

#17 AR-1242-2

R.T.: 5.195 min
Delta R.T.: -0.001 min
Response: 965754
Conc: 412.10 ng/ml m

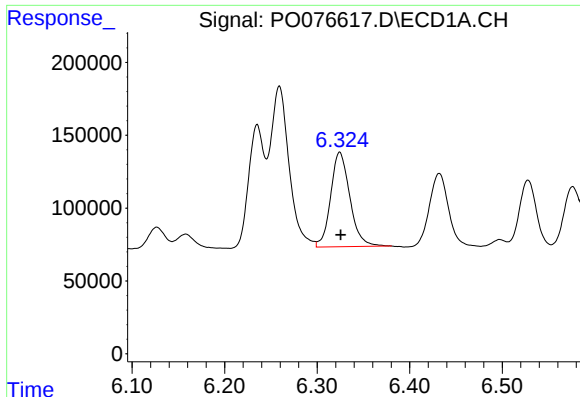


#18 AR-1242-3

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 938181
Conc: 464.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:25 PM

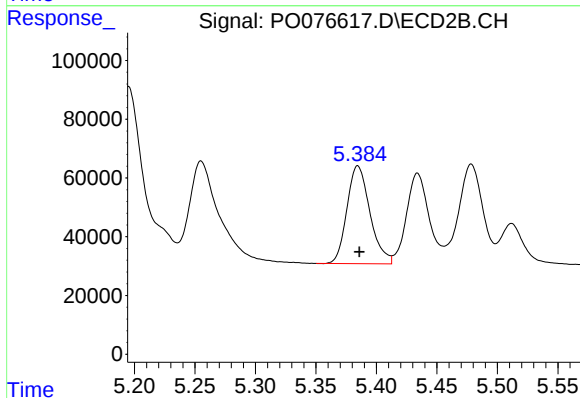


#18 AR-1242-3

R.T.: 5.385 min
Delta R.T.: -0.001 min
Response: 442652
Conc: 408.80 ng/ml

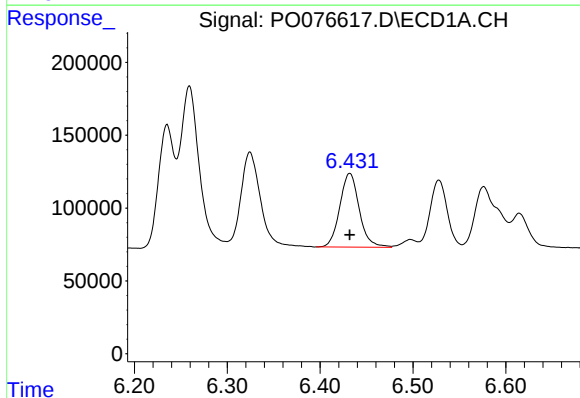


#19 AR-1242-4

R.T.: 6.432 min
Delta R.T.: 0.000 min
Response: 738282
Conc: 458.40 ng/ml

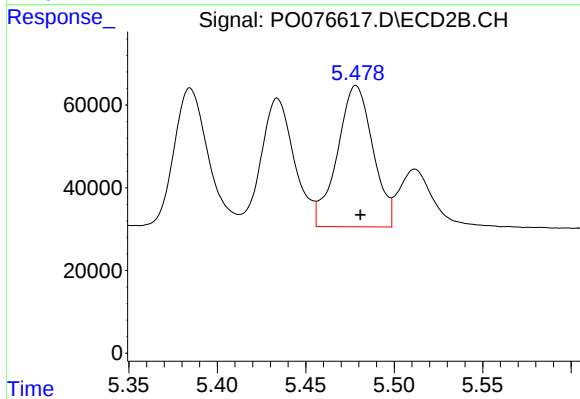

#19 AR-1242-4

R.T.: 5.478 min
Delta R.T.: -0.002 min
Response: 479137
Conc: 432.46 ng/ml

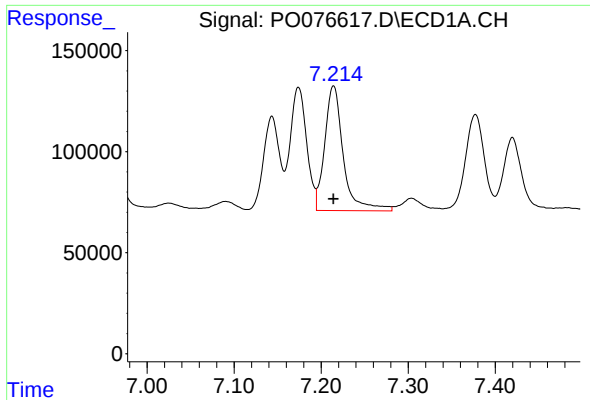


#20 AR-1242-5

R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 916135
Conc: 524.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:25 PM

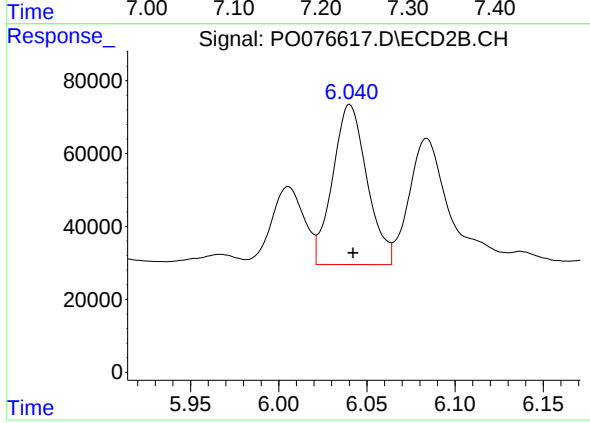

#20 AR-1242-5

R.T.: 6.040 min
Delta R.T.: -0.002 min
Response: 595664
Conc: 449.08 ng/ml