

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076643.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 2:56
 Operator : DD\AJ
 Sample : M1836-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B1-0-2

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 03:50:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.927	2069659	1172997	23.632	21.384
2) SA Decachlor...	10.885	9.180	2095229	1255542	32.187	26.645
Target Compounds						
31) L7 AR-1260-1	7.917	6.748	160340	94186	46.660m	36.750m
32) L7 AR-1260-2	8.182	6.948	177210	144162	43.706m	46.485m
33) L7 AR-1260-3	8.550	7.099	133403	84238	44.156m	28.674 #
34) L7 AR-1260-4	8.778	7.579	153194	104256	43.960m	43.744
35) L7 AR-1260-5	9.102	7.826	282348	214423	41.781	37.795m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076643.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 2:56
Operator : DD\AJ
Sample : M1836-01
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B1-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 03:50:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

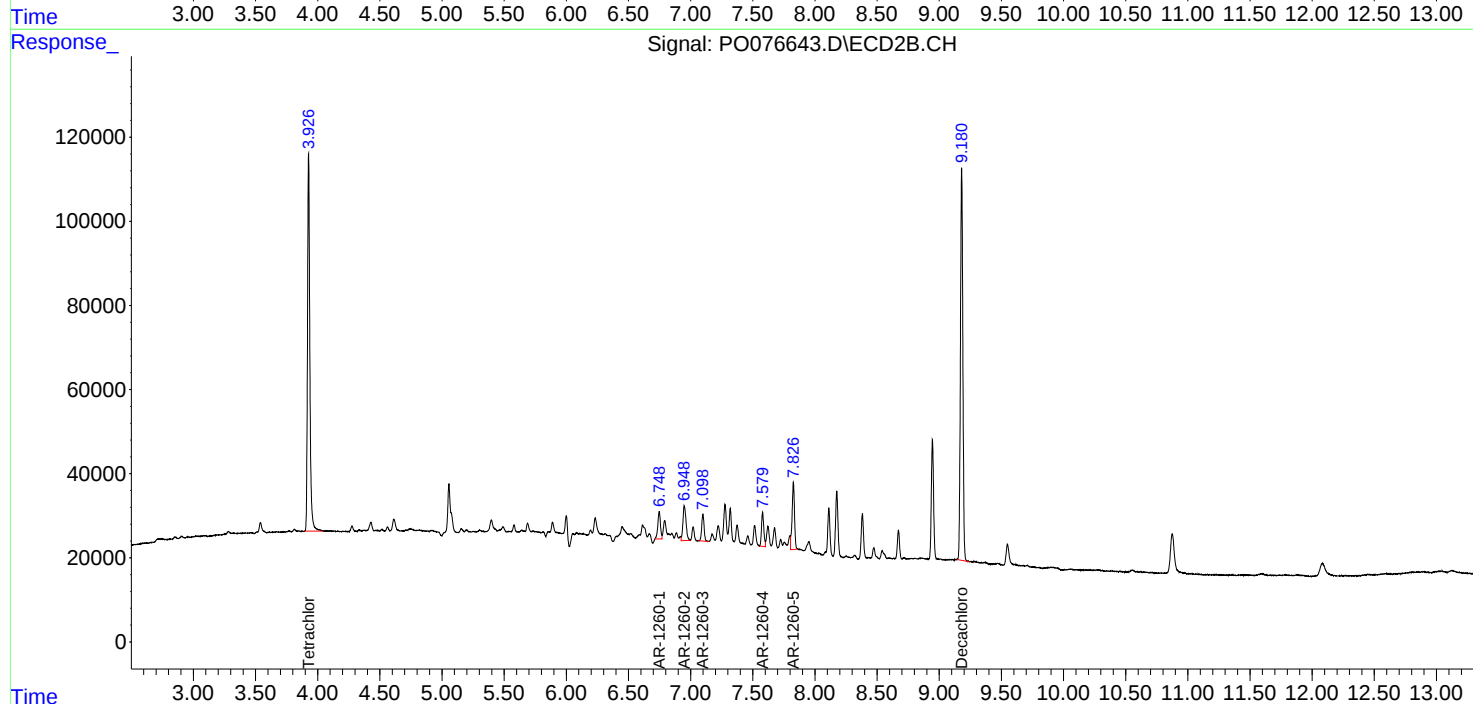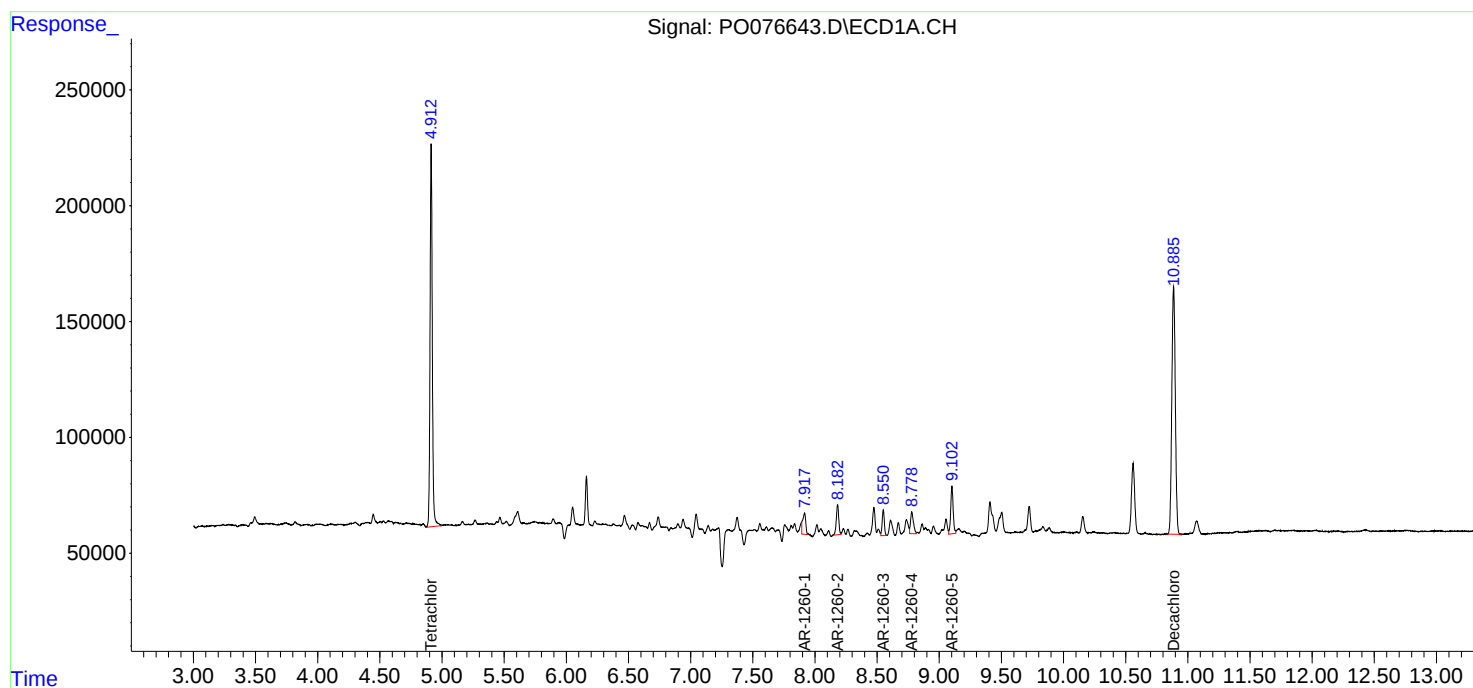

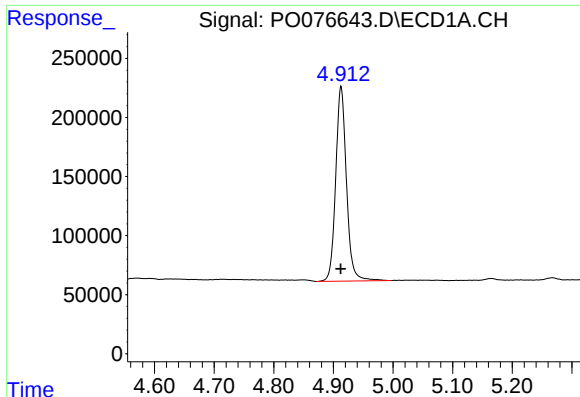


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 2069659
Conc: 23.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
B1-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:30 PM

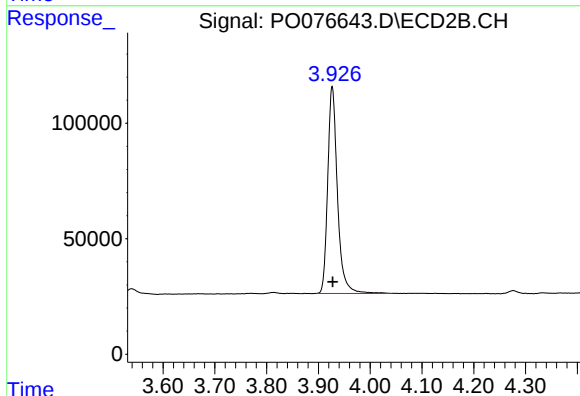


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 1172997
Conc: 21.38 ng/ml

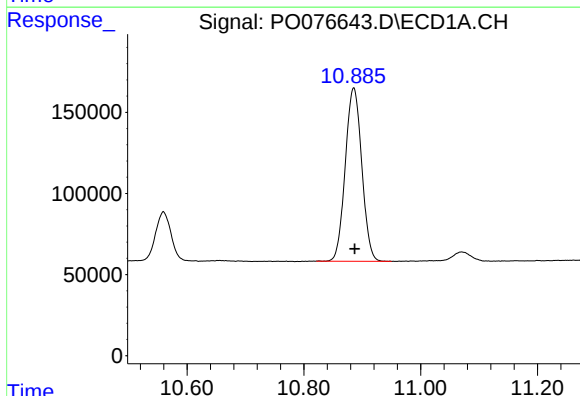


#2 Decachlorobiphenyl

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 2095229
Conc: 32.19 ng/ml

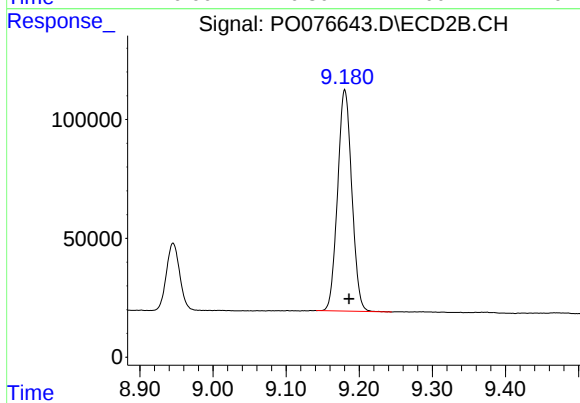

#2 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.006 min
Response: 1255542
Conc: 26.64 ng/ml

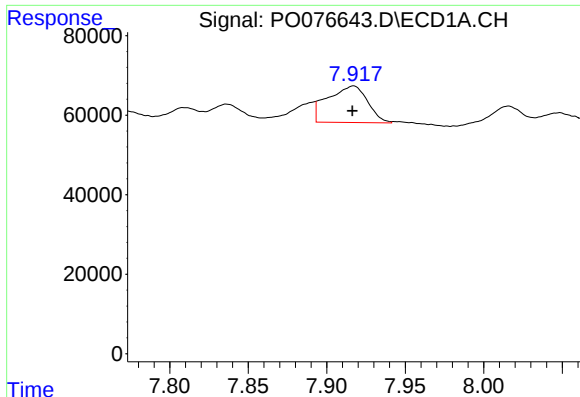


#31 AR-1260-1

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 160340
Conc: 46.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B1-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:30 PM

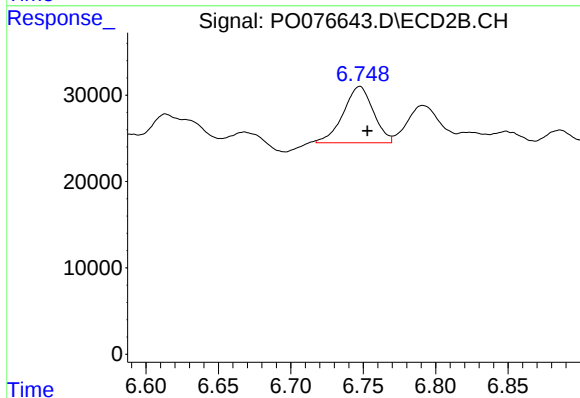


#31 AR-1260-1

R.T.: 6.748 min
Delta R.T.: -0.005 min
Response: 94186
Conc: 36.75 ng/ml m

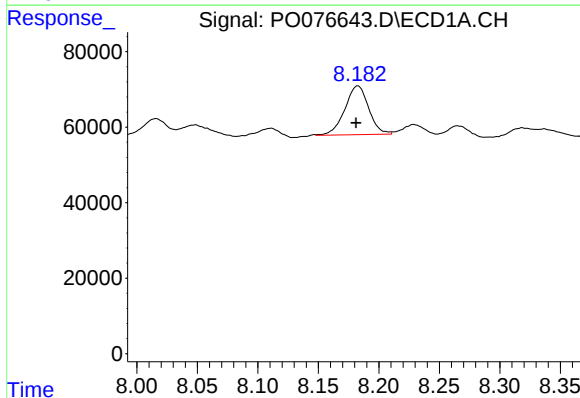


#32 AR-1260-2

R.T.: 8.182 min
Delta R.T.: 0.000 min
Response: 177210
Conc: 43.71 ng/ml m

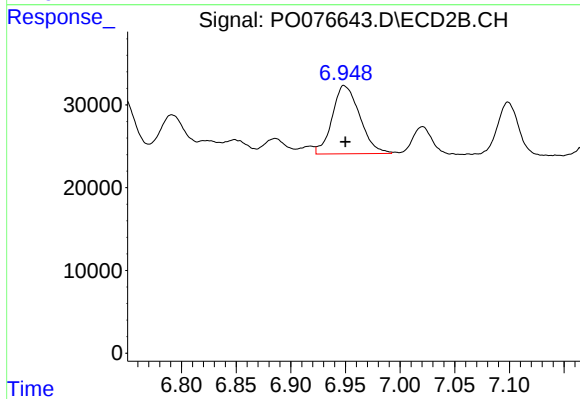

#32 AR-1260-2

R.T.: 6.948 min
Delta R.T.: -0.002 min
Response: 144162
Conc: 46.48 ng/ml m

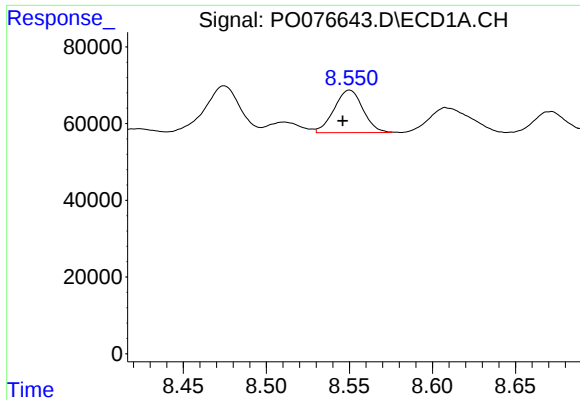


#33 AR-1260-3

R.T.: 8.550 min
Delta R.T.: 0.004 min
Response: 133403
Conc: 44.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B1-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:30 PM

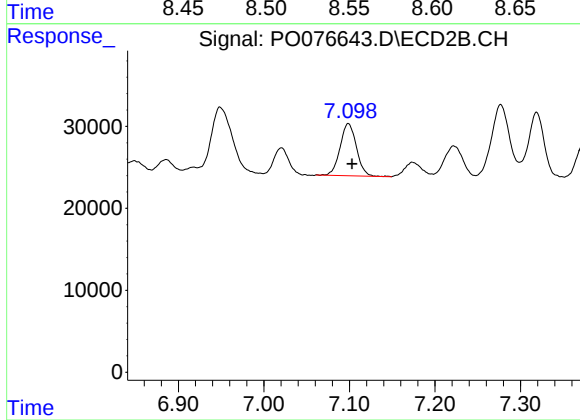


#33 AR-1260-3

R.T.: 7.099 min
Delta R.T.: -0.004 min
Response: 84238
Conc: 28.67 ng/ml

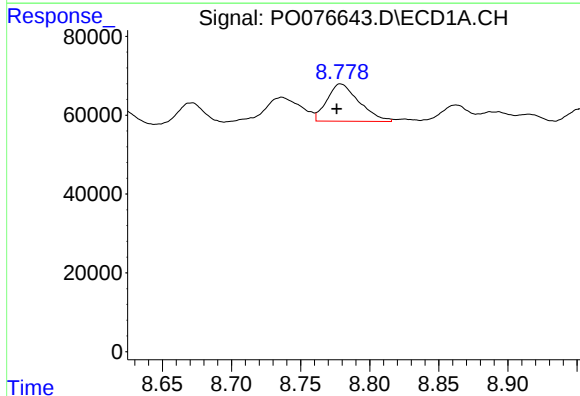


#34 AR-1260-4

R.T.: 8.778 min
Delta R.T.: 0.002 min
Response: 153194
Conc: 43.96 ng/ml m

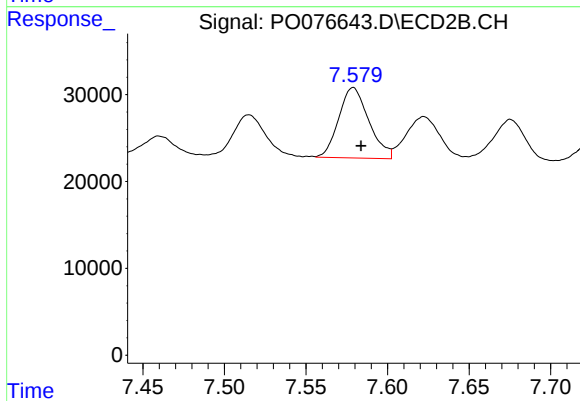

#34 AR-1260-4

R.T.: 7.579 min
Delta R.T.: -0.005 min
Response: 104256
Conc: 43.74 ng/ml

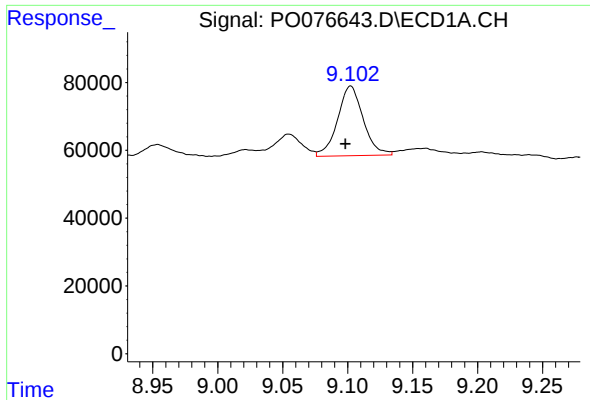


#35 AR-1260-5

R.T.: 9.102 min
Delta R.T.: 0.004 min
Response: 282348
Conc: 41.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
B1-0-2

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:30 PM

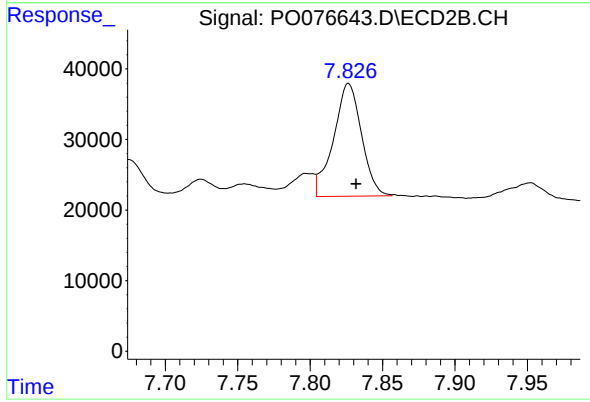

#35 AR-1260-5

R.T.: 7.826 min
Delta R.T.: -0.006 min
Response: 214423
Conc: 37.79 ng/ml m