

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076647.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 4:05
 Operator : DD\AJ
 Sample : M1836-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B3-0-2

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 11:58:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.926	2148327	1131069	24.530	20.620
2) SA Decachlor...	10.887	9.180	2056164	1280157	31.587	27.167m
Target Compounds						
31) L7 AR-1260-1	7.917	6.749	5040943	1494798	1466.936	583.250 #
32) L7 AR-1260-2	8.175	6.959	10893310	7198050	2686.668	2320.982
33) L7 AR-1260-3	8.549	7.100	2728406	1837171	903.105	625.366 #
34) L7 AR-1260-4	8.780	7.580	3536932	1923890	1014.955	807.229
35) L7 AR-1260-5	9.102	7.828	7389037	5154000	1093.401m	908.461

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076647.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 4:05
Operator : DD\AJ
Sample : M1836-05
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 11:58:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

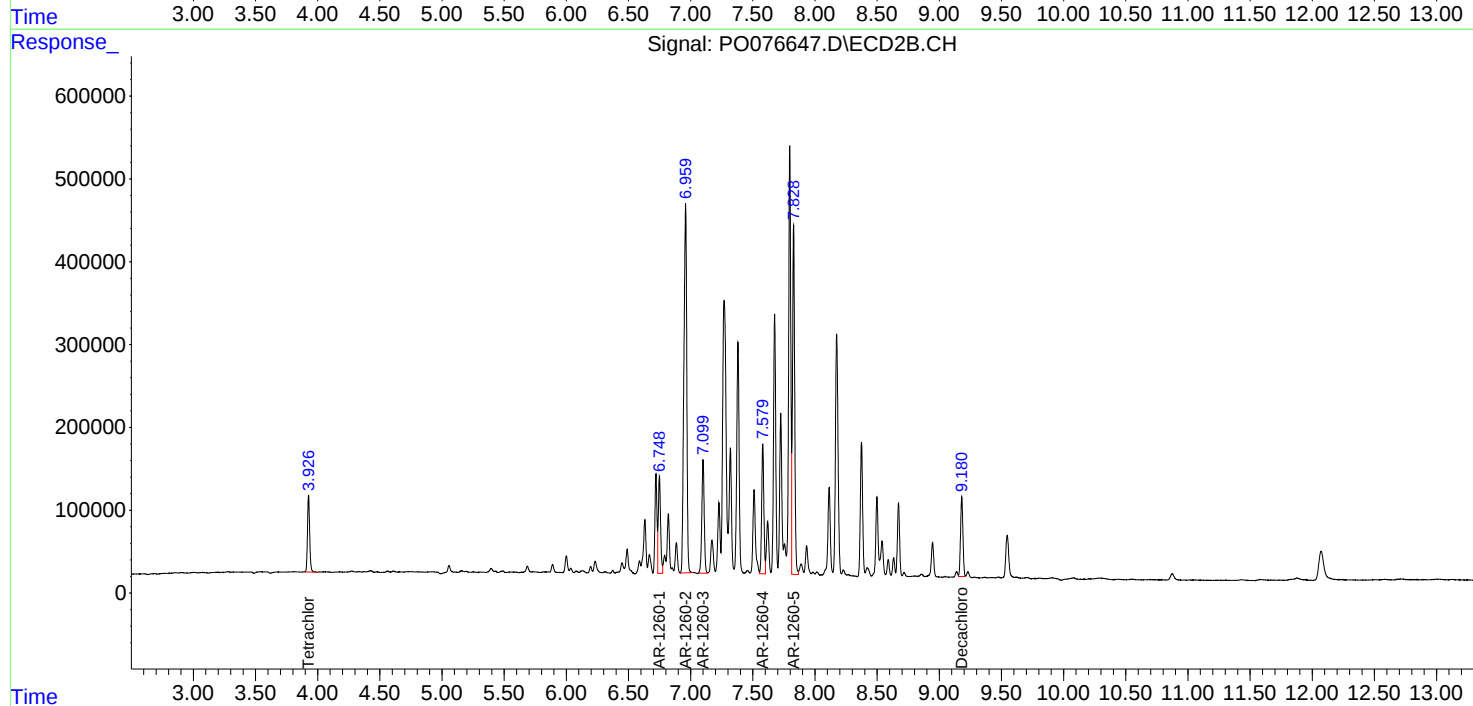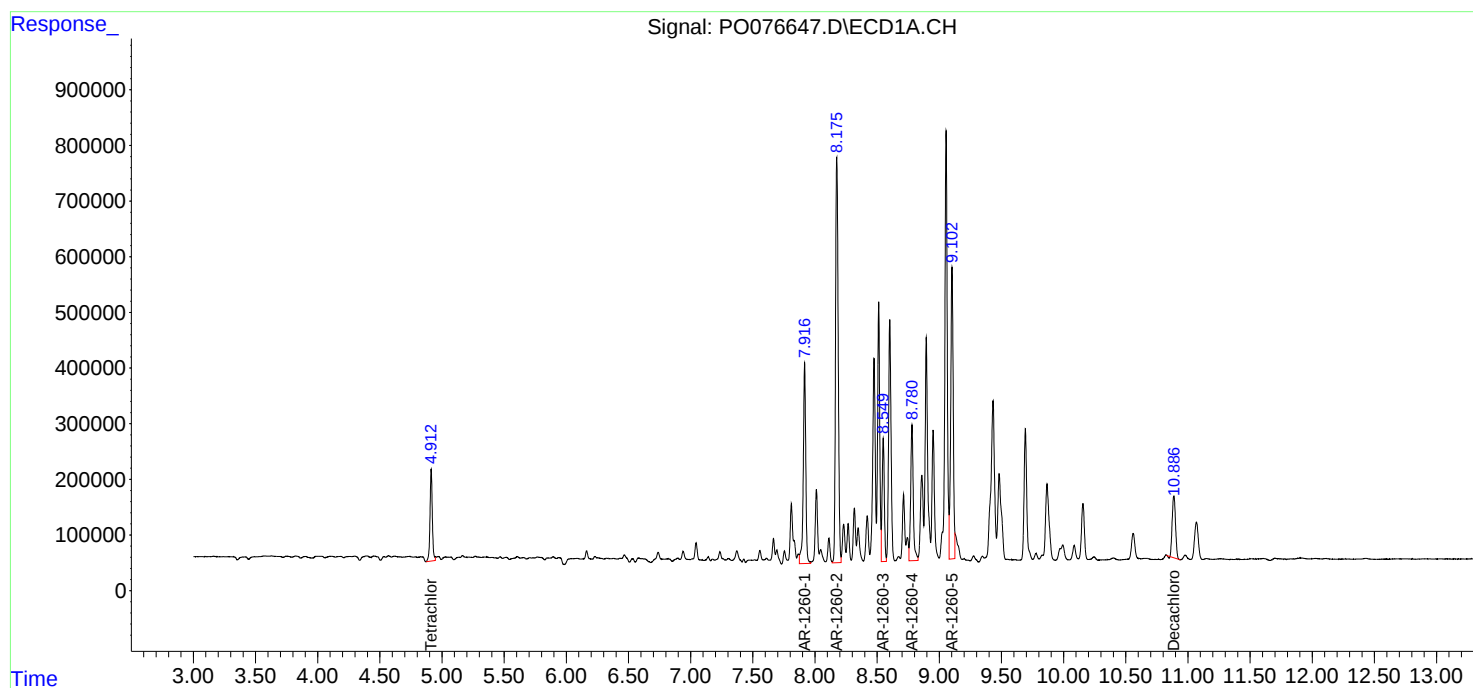

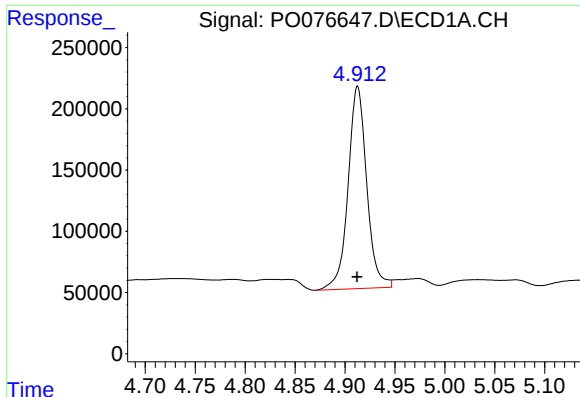


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 2148327
Conc: 24.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:34 PM

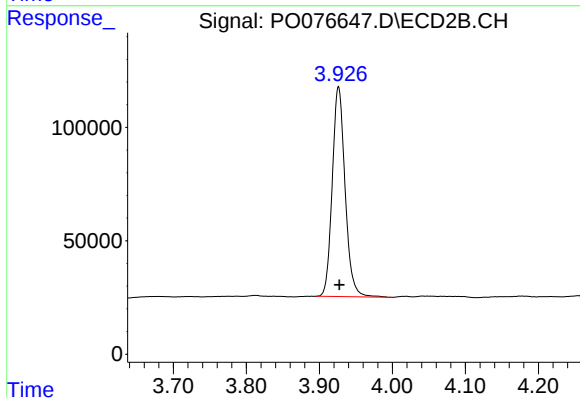


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 1131069
Conc: 20.62 ng/ml

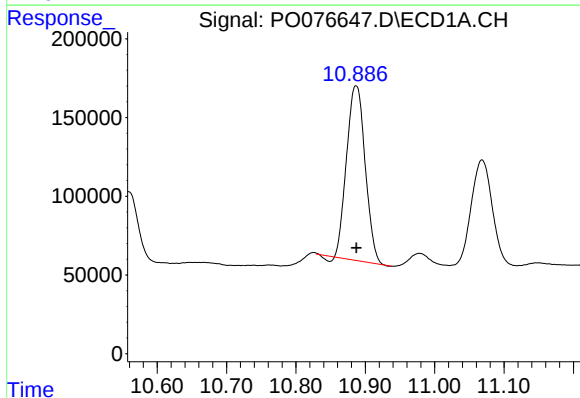


#2 Decachlorobiphenyl

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 2056164
Conc: 31.59 ng/ml

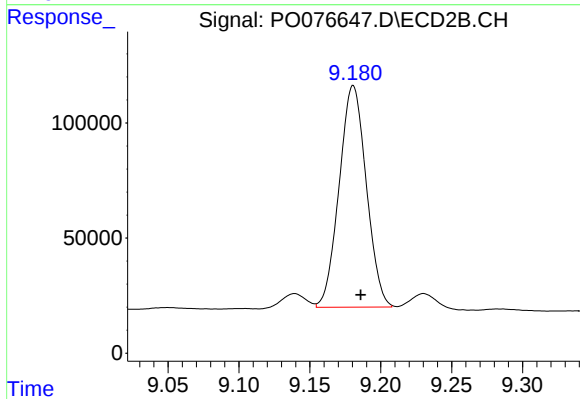

#2 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.006 min
Response: 1280157
Conc: 27.17 ng/ml m

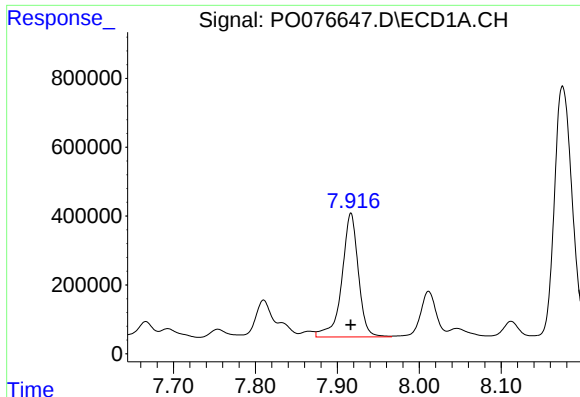


#31 AR-1260-1

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 5040943
Conc: 1466.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:34 PM

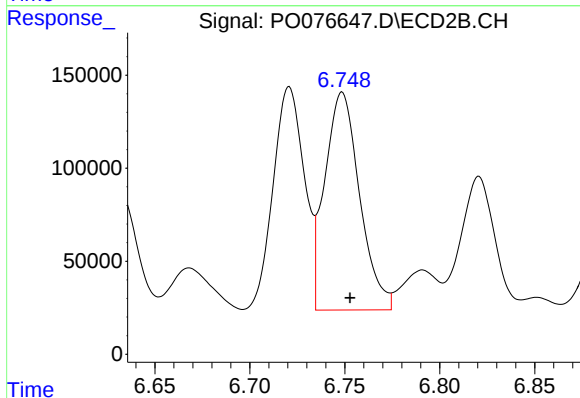


#31 AR-1260-1

R.T.: 6.749 min
Delta R.T.: -0.004 min
Response: 1494798
Conc: 583.25 ng/ml

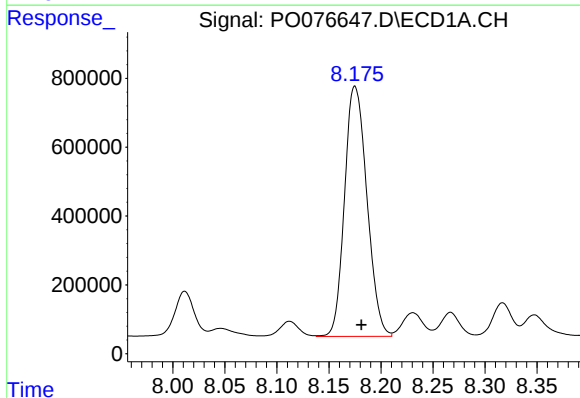


#32 AR-1260-2

R.T.: 8.175 min
Delta R.T.: -0.006 min
Response: 10893310
Conc: 2686.67 ng/ml

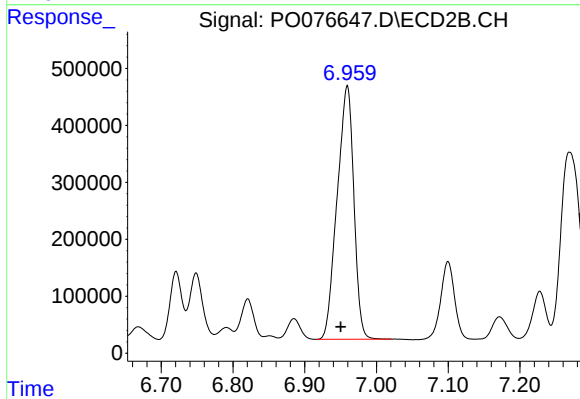

#32 AR-1260-2

R.T.: 6.959 min
Delta R.T.: 0.009 min
Response: 7198050
Conc: 2320.98 ng/ml

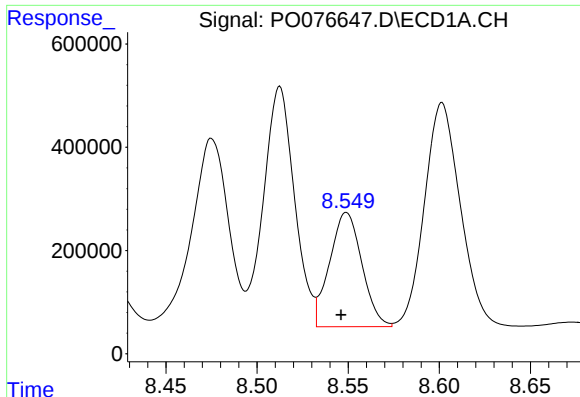


#33 AR-1260-3

R.T.: 8.549 min
Delta R.T.: 0.003 min
Response: 2728406
Conc: 903.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
B3-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:34 PM

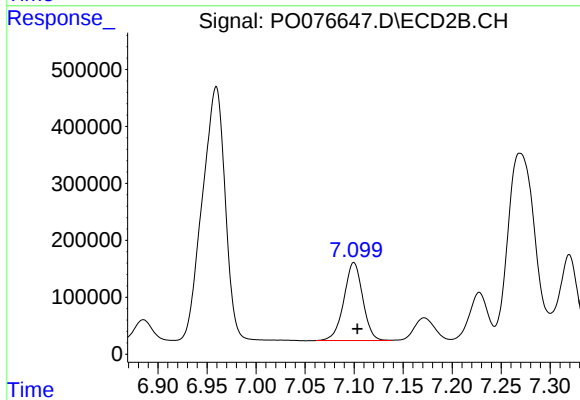


#33 AR-1260-3

R.T.: 7.100 min
Delta R.T.: -0.003 min
Response: 1837171
Conc: 625.37 ng/ml

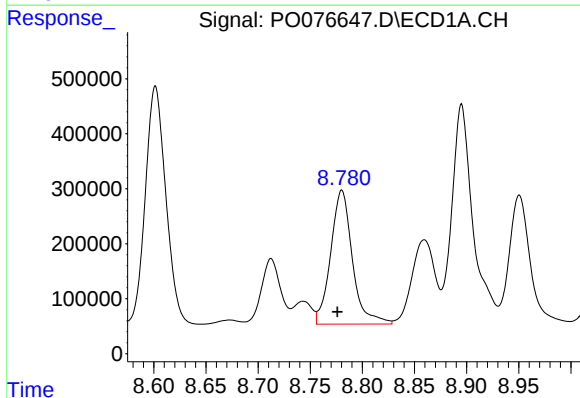


#34 AR-1260-4

R.T.: 8.780 min
Delta R.T.: 0.004 min
Response: 3536932
Conc: 1014.95 ng/ml

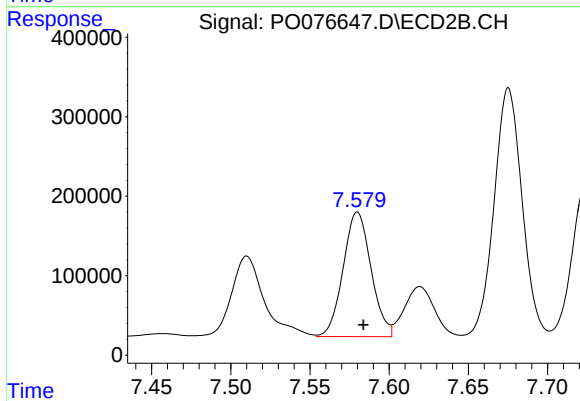

#34 AR-1260-4

R.T.: 7.580 min
Delta R.T.: -0.004 min
Response: 1923890
Conc: 807.23 ng/ml

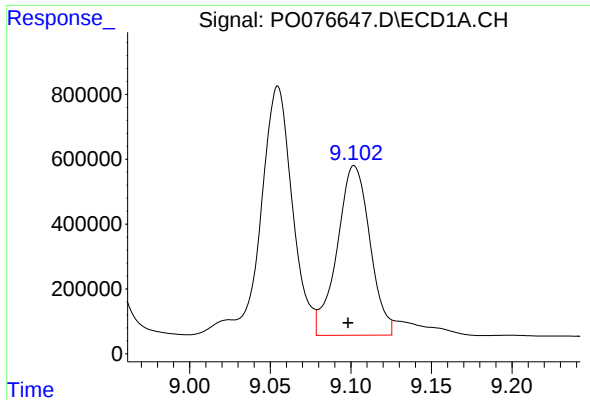


#35 AR-1260-5

R.T.: 9.102 min
Delta R.T.: 0.003 min
Response: 7389037
Conc: 1093.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B3-0-2

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:34 PM

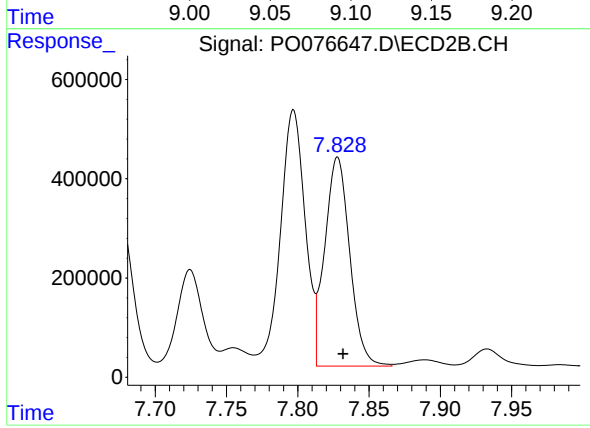

#35 AR-1260-5

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 5154000
Conc: 908.46 ng/ml