

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0033021\
 Data File : P0076652.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 5:31
 Operator : DD\AJ
 Sample : M1836-08
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B4-0-2

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 07:45:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.927	1800039	1062425	20.553	19.368
2) SA Decachlor...	10.888	9.180	2479340	1479952	38.088	31.407
Target Compounds						
31) L7 AR-1260-1	7.917	6.747	94043	88066	27.367m	34.362 #
32) L7 AR-1260-2	8.183	6.949	184183	74932	45.426	24.161m#
33) L7 AR-1260-3	8.549	7.096	52050	50738	17.228	17.271m
34) L7 AR-1260-4	8.777	7.580	94629	40245	27.155	16.886 #
35) L7 AR-1260-5	9.103	7.824	100301	125402	14.842	22.104 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0033021\
Data File : P0076652.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 5:31
Operator : DD\AJ
Sample : M1836-08
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B4-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 07:45:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

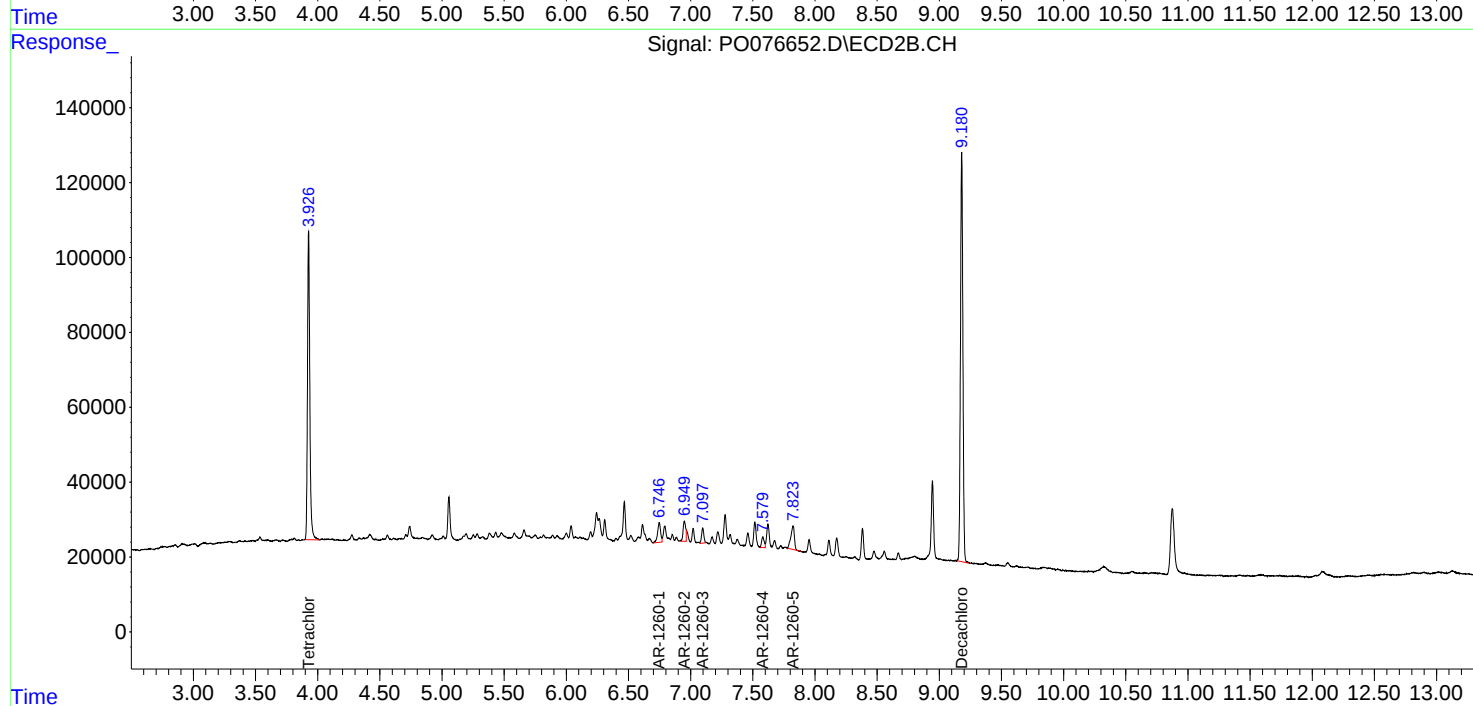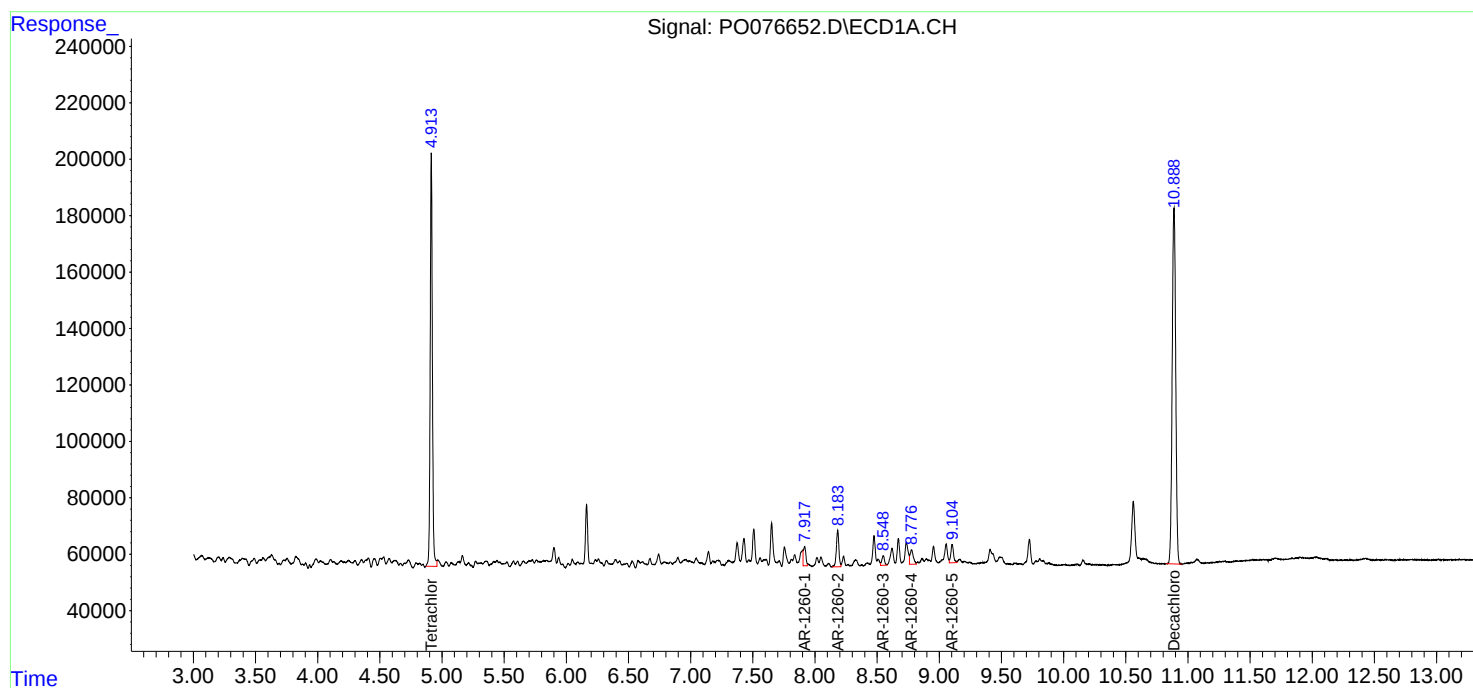

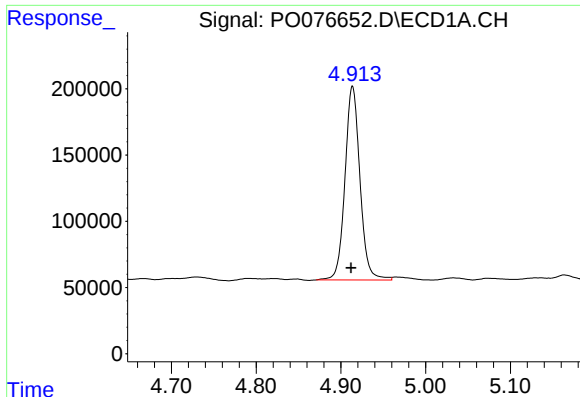


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: 0.002 min
Response: 1800039
Conc: 20.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
B4-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:38 PM

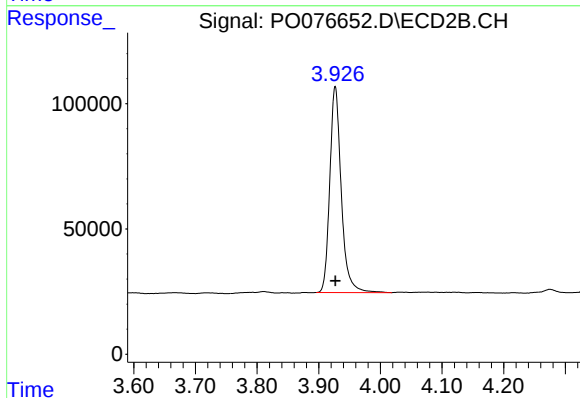


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 1062425
Conc: 19.37 ng/ml

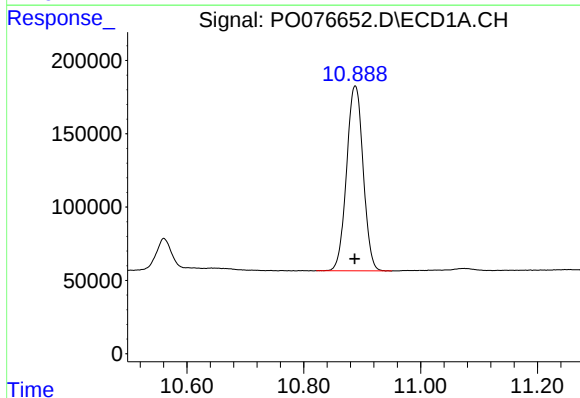


#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.000 min
Response: 2479340
Conc: 38.09 ng/ml

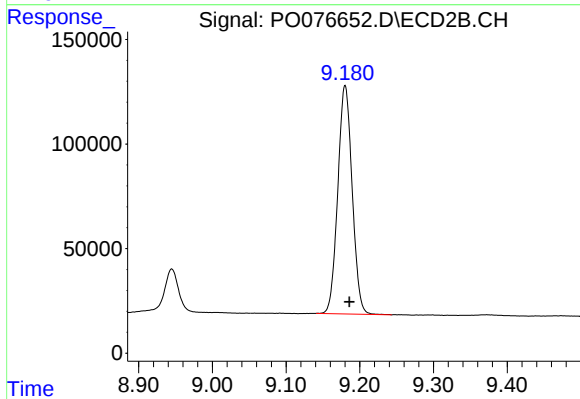

#2 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.006 min
Response: 1479952
Conc: 31.41 ng/ml

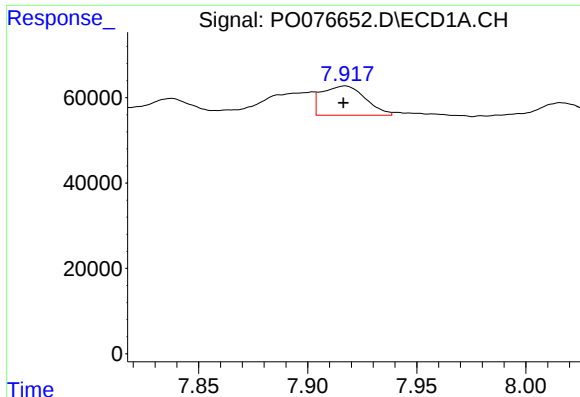


#31 AR-1260-1

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 94043
Conc: 27.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B4-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:38 PM

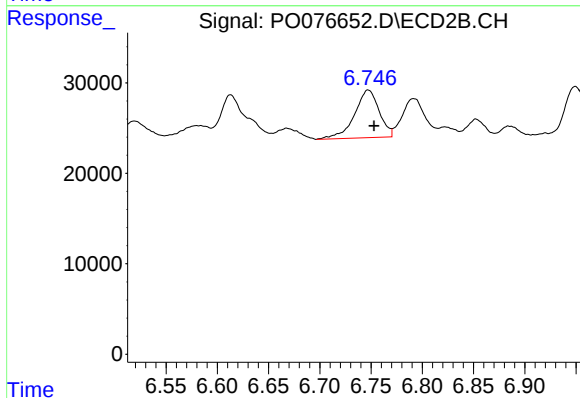


#31 AR-1260-1

R.T.: 6.747 min
Delta R.T.: -0.006 min
Response: 88066
Conc: 34.36 ng/ml

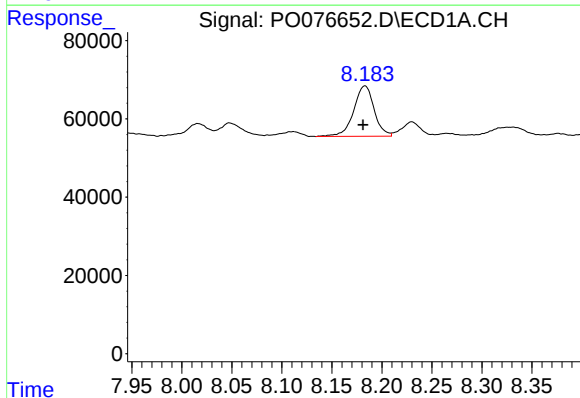


#32 AR-1260-2

R.T.: 8.183 min
Delta R.T.: 0.002 min
Response: 184183
Conc: 45.43 ng/ml

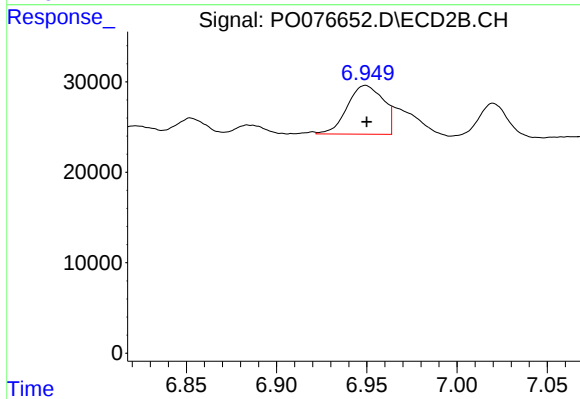

#32 AR-1260-2

R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 74932
Conc: 24.16 ng/ml m

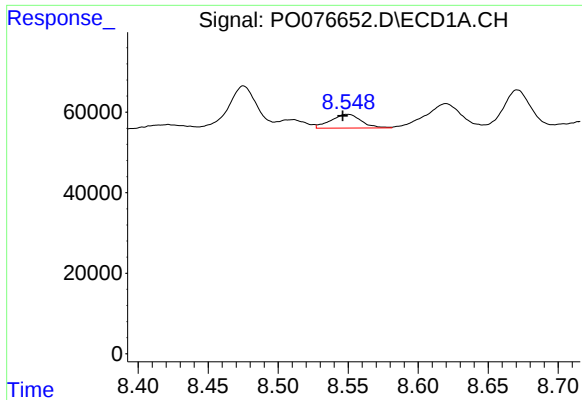


#33 AR-1260-3

R.T.: 8.549 min
Delta R.T.: 0.003 min
Response: 52050
Conc: 17.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
B4-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:38 PM

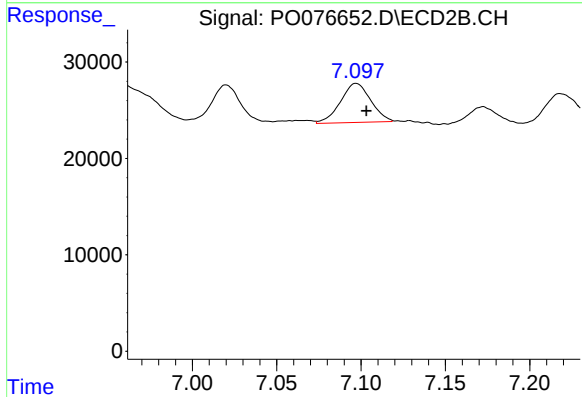


#33 AR-1260-3

R.T.: 7.096 min
Delta R.T.: -0.007 min
Response: 50738
Conc: 17.27 ng/ml m

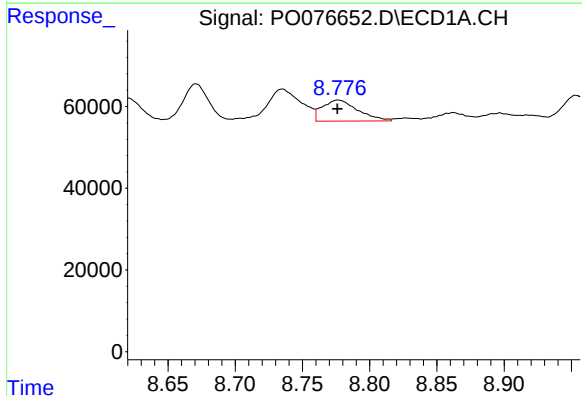


#34 AR-1260-4

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 94629
Conc: 27.15 ng/ml

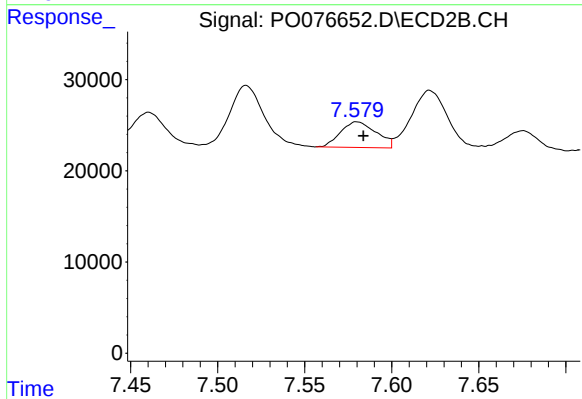

#34 AR-1260-4

R.T.: 7.580 min
Delta R.T.: -0.004 min
Response: 40245
Conc: 16.89 ng/ml

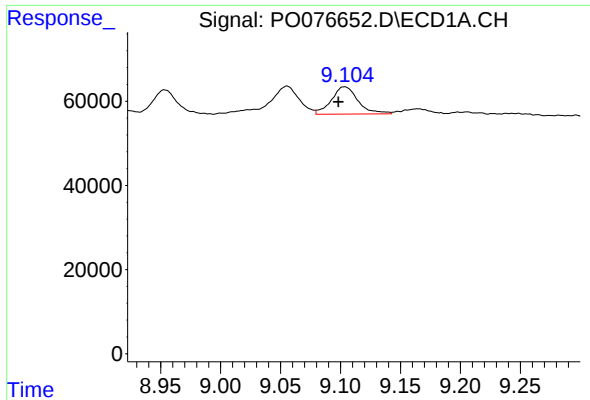


#35 AR-1260-5

R.T.: 9.103 min
Delta R.T.: 0.005 min
Response: 100301
Conc: 14.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
B4-0-2

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:38 PM

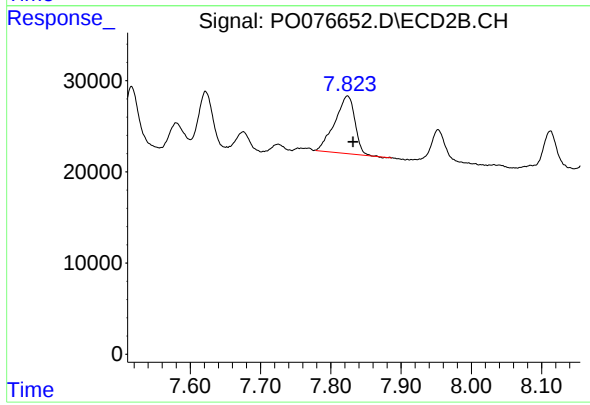

#35 AR-1260-5

R.T.: 7.824 min
Delta R.T.: -0.008 min
Response: 125402
Conc: 22.10 ng/ml