

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076654.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 6:05
 Operator : DD\AJ
 Sample : M1836-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B5-0-2

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 07:46:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.927	2166773	1234150	24.740	22.499
2) SA Decachlor...	10.885	9.181	2567243	1503589	39.439	31.909
Target Compounds						
26) L6 AR-1254-1	7.144	6.039	138697	63627	41.757m	21.482 #
27) L6 AR-1254-2	7.374	6.196	235268	55269	45.711m	21.273 #
28) L6 AR-1254-3	7.755	6.612	239924	94022	45.105	23.475m#
29) L6 AR-1254-4	8.049	6.852	89801	41693	24.898	17.596 #
30) L6 AR-1254-5	8.478	7.277	451610	146049	115.212	41.437 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076654.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 6:05
Operator : DD\AJ
Sample : M1836-10
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B5-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 07:46:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

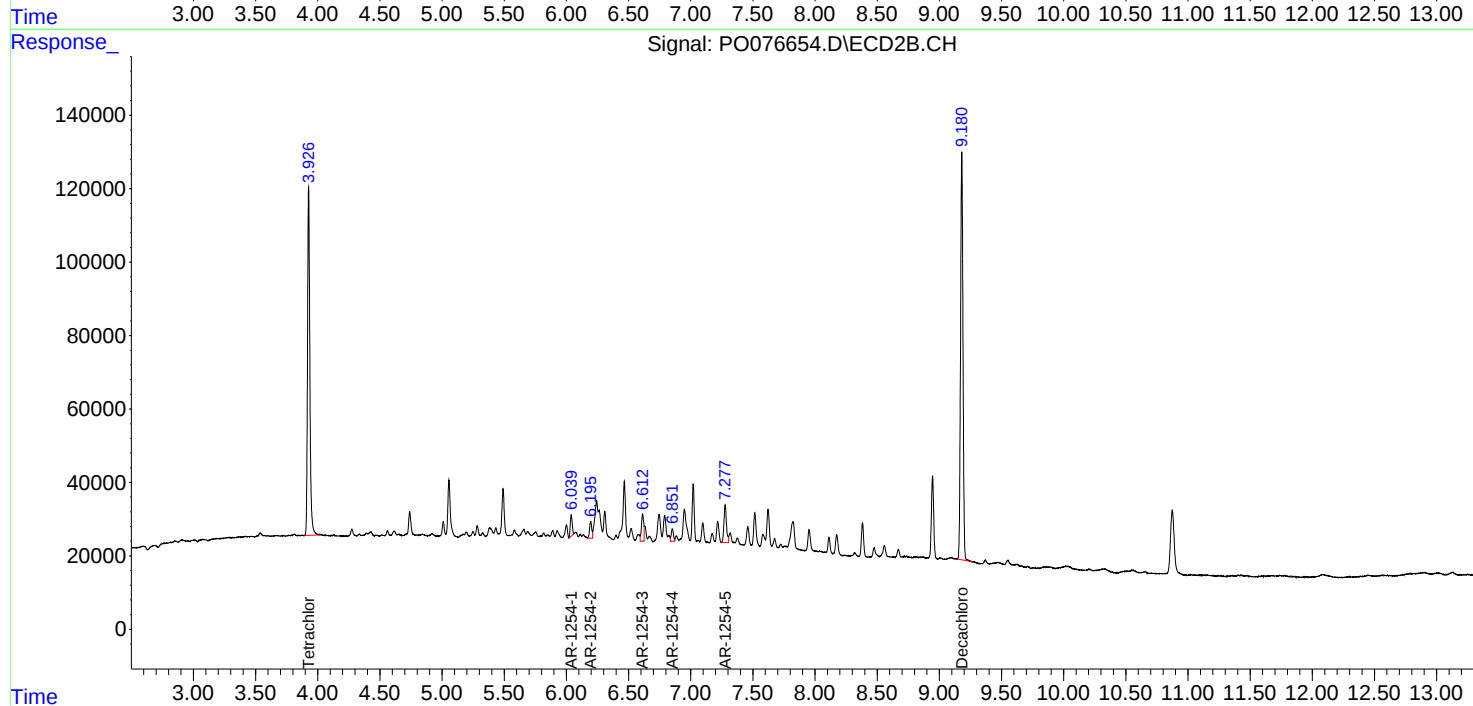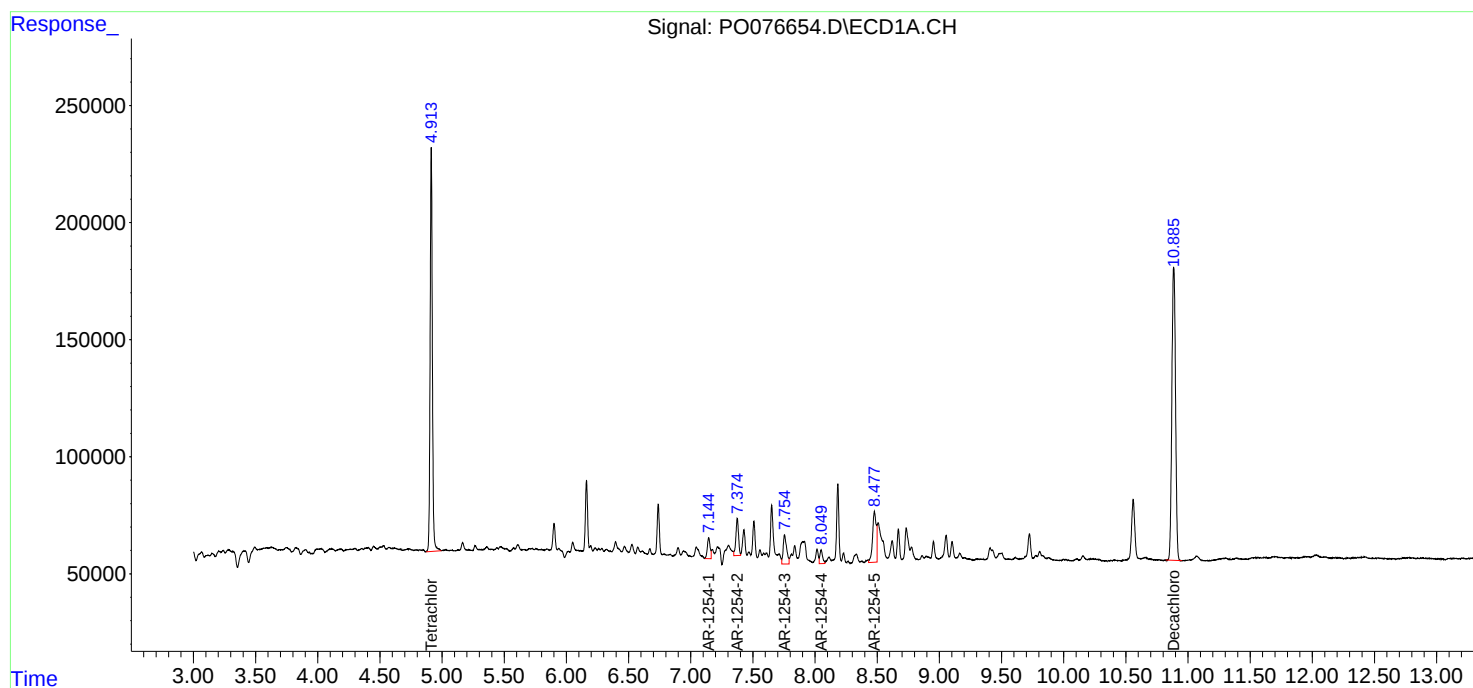

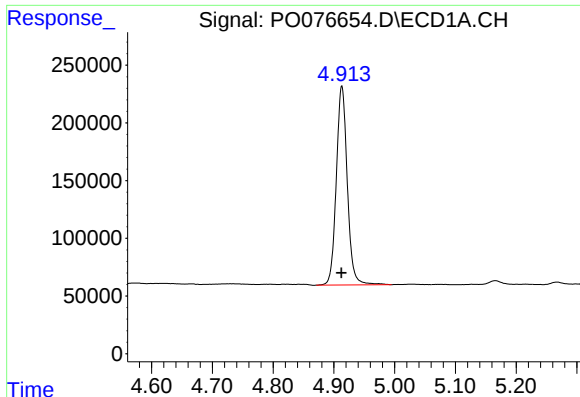


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: 0.001 min
Response: 2166773
Conc: 24.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
B5-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:42 PM

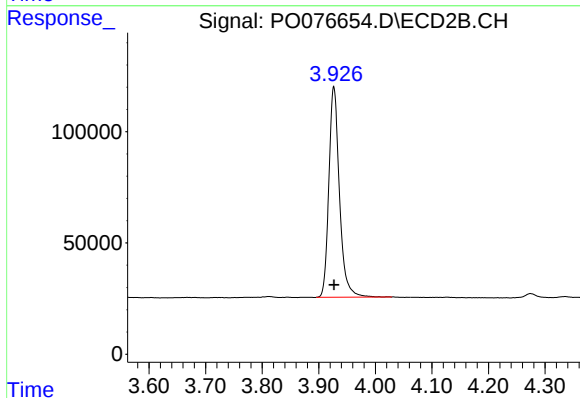


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 1234150
Conc: 22.50 ng/ml

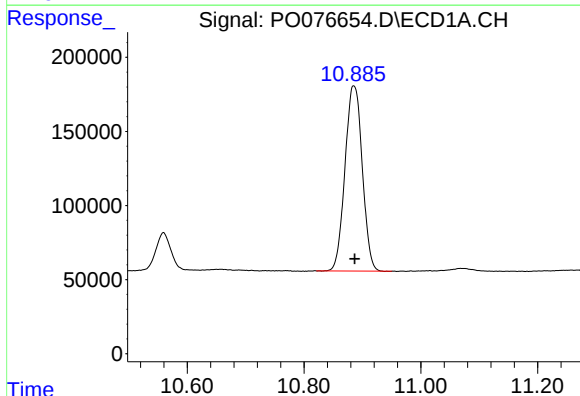


#2 Decachlorobiphenyl

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 2567243
Conc: 39.44 ng/ml

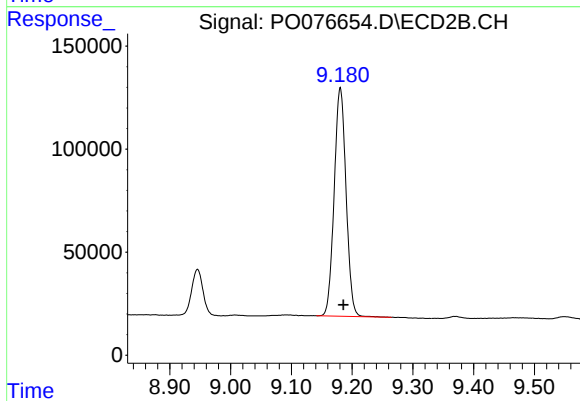

#2 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.005 min
Response: 1503589
Conc: 31.91 ng/ml

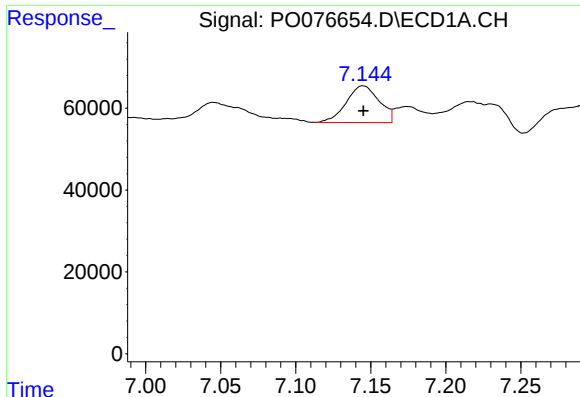


#26 AR-1254-1

R.T.: 7.144 min
Delta R.T.: 0.000 min
Response: 138697
Conc: 41.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B5-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:42 PM

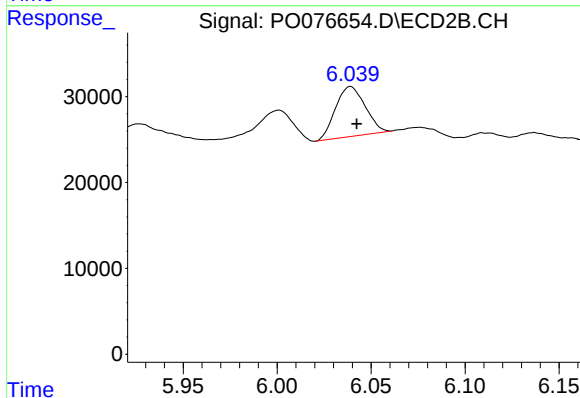


#26 AR-1254-1

R.T.: 6.039 min
Delta R.T.: -0.003 min
Response: 63627
Conc: 21.48 ng/ml

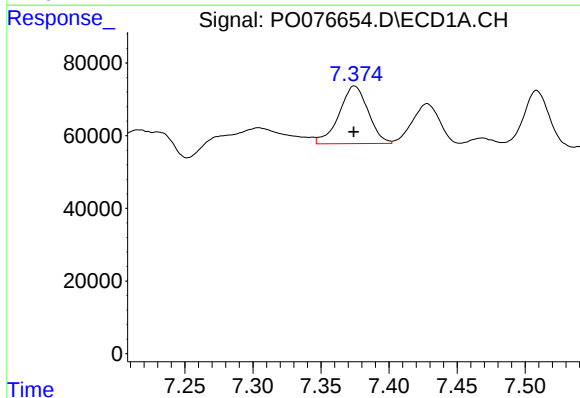


#27 AR-1254-2

R.T.: 7.374 min
Delta R.T.: 0.000 min
Response: 235268
Conc: 45.71 ng/ml m

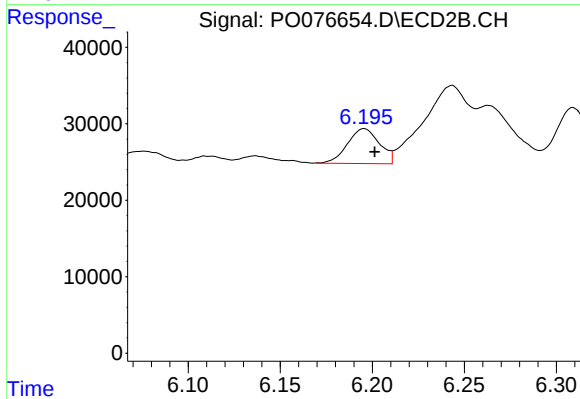

#27 AR-1254-2

R.T.: 6.196 min
Delta R.T.: -0.006 min
Response: 55269
Conc: 21.27 ng/ml

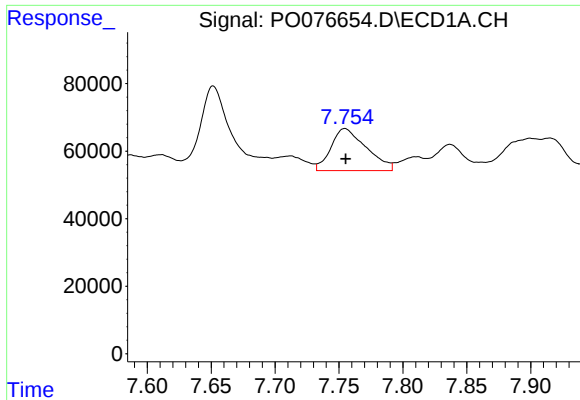


#28 AR-1254-3

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 239924
Conc: 45.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
B5-0-2


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:42 PM

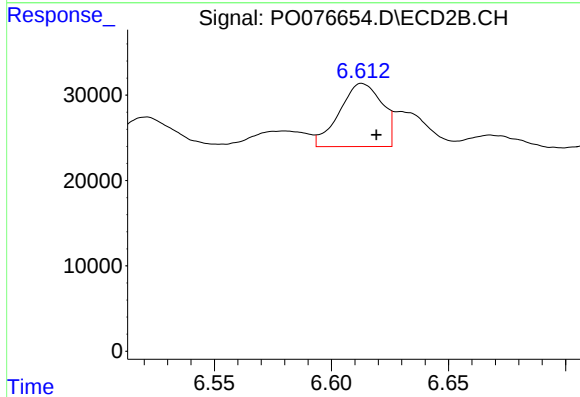


#28 AR-1254-3

R.T.: 6.612 min
Delta R.T.: -0.007 min
Response: 94022
Conc: 23.47 ng/ml m

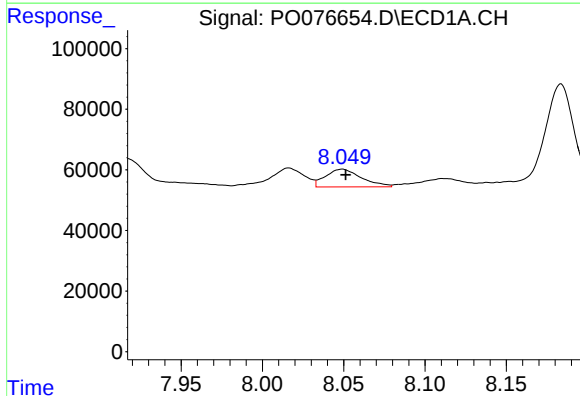


#29 AR-1254-4

R.T.: 8.049 min
Delta R.T.: -0.002 min
Response: 89801
Conc: 24.90 ng/ml

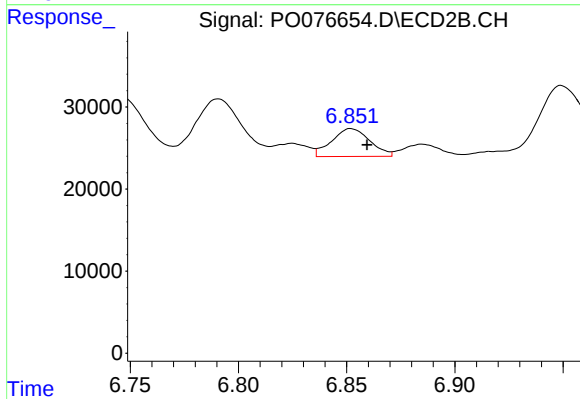

#29 AR-1254-4

R.T.: 6.852 min
Delta R.T.: -0.007 min
Response: 41693
Conc: 17.60 ng/ml

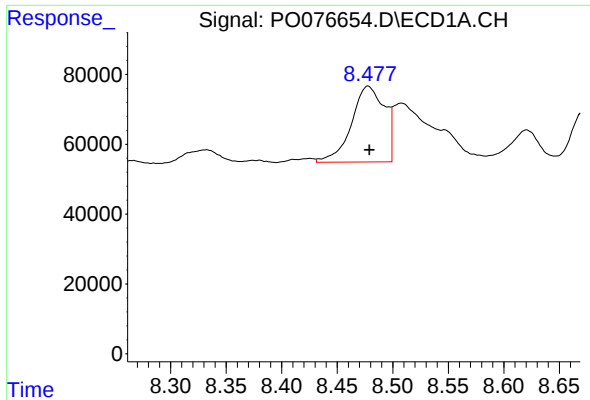


#30 AR-1254-5

R.T.: 8.478 min
Delta R.T.: -0.001 min
Response: 451610
Conc: 115.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
B5-0-2

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:42 PM

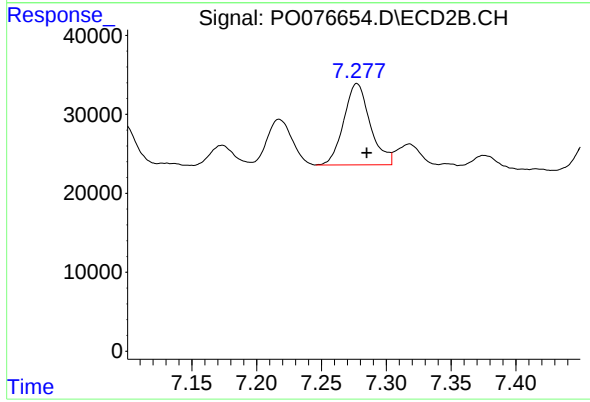

#30 AR-1254-5

R.T.: 7.277 min
Delta R.T.: -0.008 min
Response: 146049
Conc: 41.44 ng/ml