

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 12:24
 Operator : DD\AJ
 Sample : M1823-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MK-3-29-B1

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 17:28:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.914	3.926	1937594	1166756	22.124m	21.270
2) SA Decachlor...	10.889	9.181	1768403	1022936	27.167	21.708

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 12:24
Operator : DD\AJ
Sample : M1823-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
MK-3-29-B1


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 17:28:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

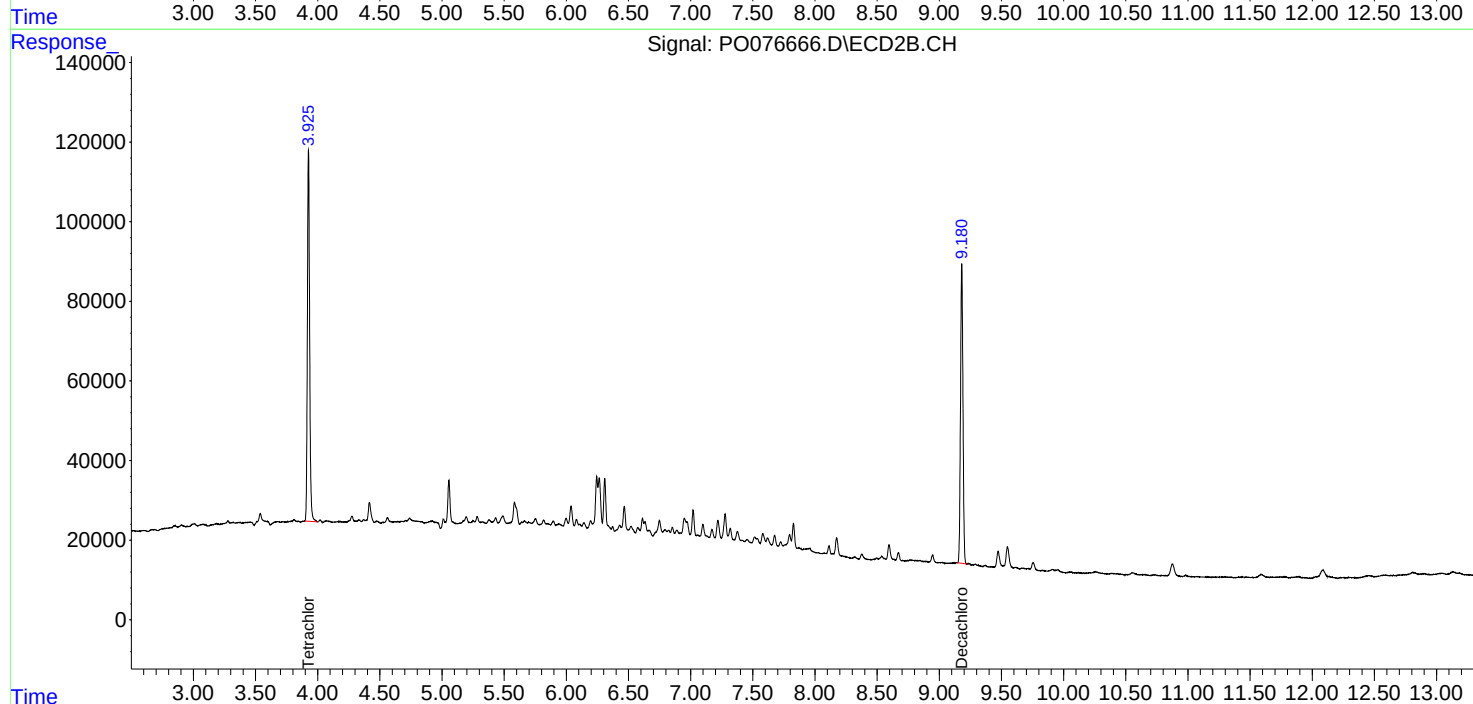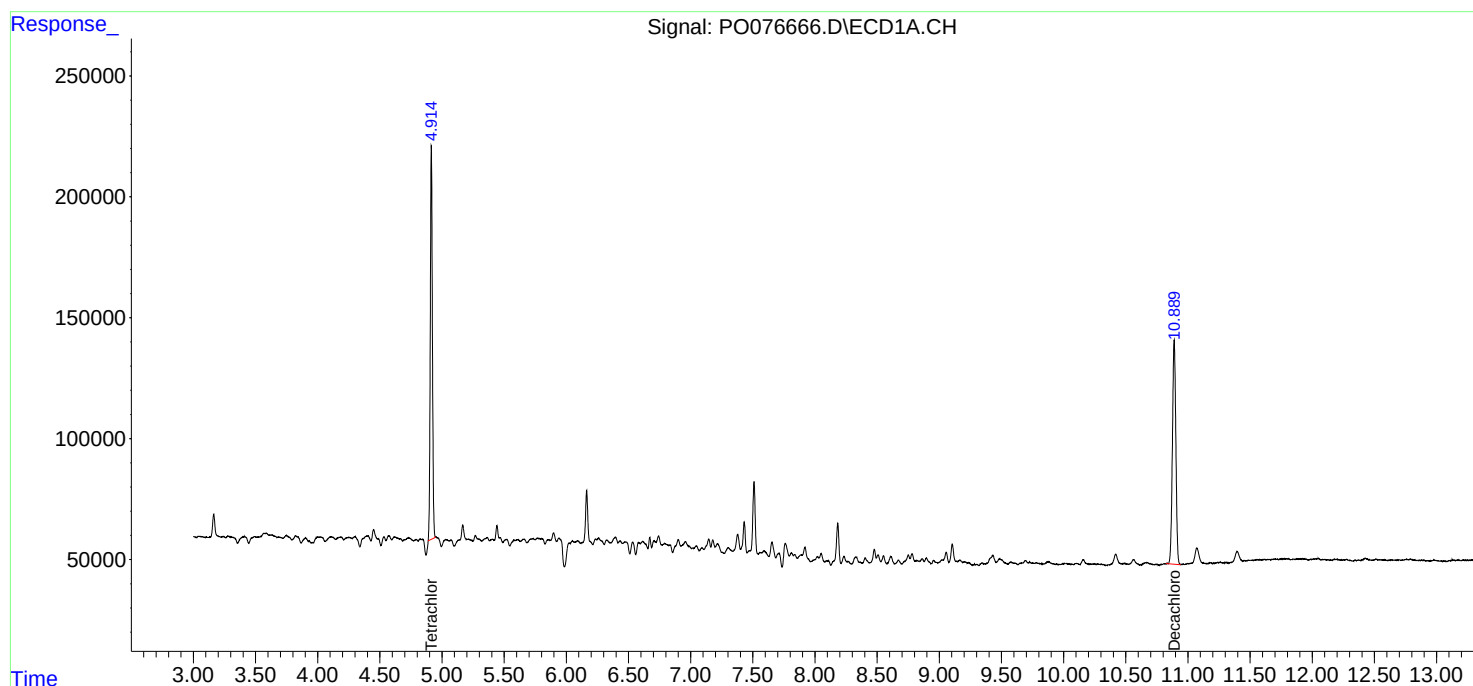

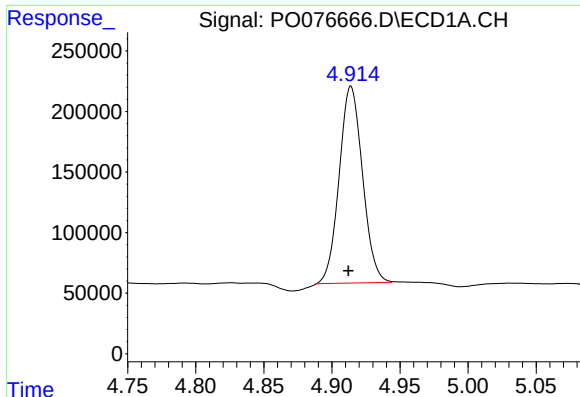


#1 Tetrachloro-m-xylene

R.T.: 4.914 min
Delta R.T.: 0.002 min
Response: 1937594
Conc: 22.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MK-3-29-B1


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:50 PM

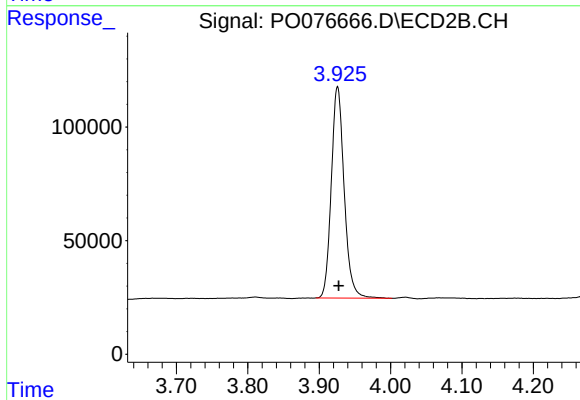


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 1166756
Conc: 21.27 ng/ml

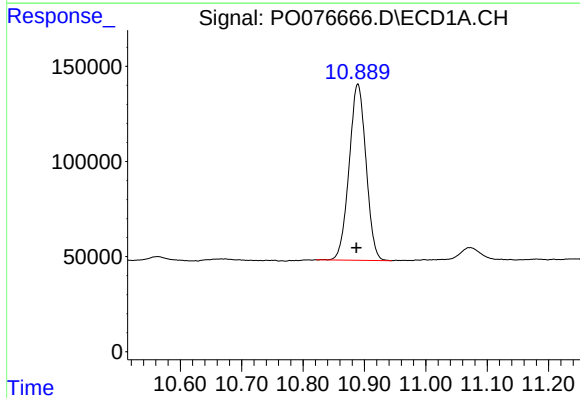

#2 Decachlorobiphenyl

R.T.: 10.889 min
Delta R.T.: 0.002 min
Response: 1768403
Conc: 27.17 ng/ml

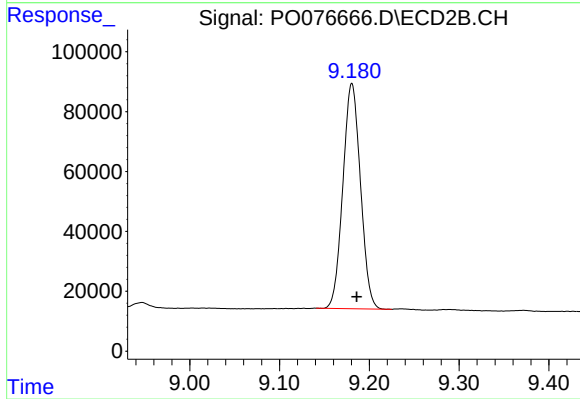

#2 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.005 min
Response: 1022936
Conc: 21.71 ng/ml