

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
 Data File : P0076667.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 12:41
 Operator : DD\AJ
 Sample : M1864-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MMR-SP

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:52:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 17:29:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 24 05:38:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.912	3.926	1795693	1063265	20.503m	19.384
2) SA Decachlor...	10.889	9.181	1472376	896276	22.619	19.020
Target Compounds						
31) L7 AR-1260-1	7.920	6.750	251298	140317	73.129	54.750 #
32) L7 AR-1260-2	8.183	6.947	786454	185110	193.967	59.688 #
33) L7 AR-1260-3	8.551	7.098	181742	167346	60.157	56.964
34) L7 AR-1260-4	8.778	7.580	263254	113416	75.543	47.587 #
35) L7 AR-1260-5	9.104	7.828	328616	255460	48.627	45.028

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033021\
Data File : P0076667.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 12:41
Operator : DD\AJ
Sample : M1864-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
MMR-SP


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 17:29:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 24 05:38:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

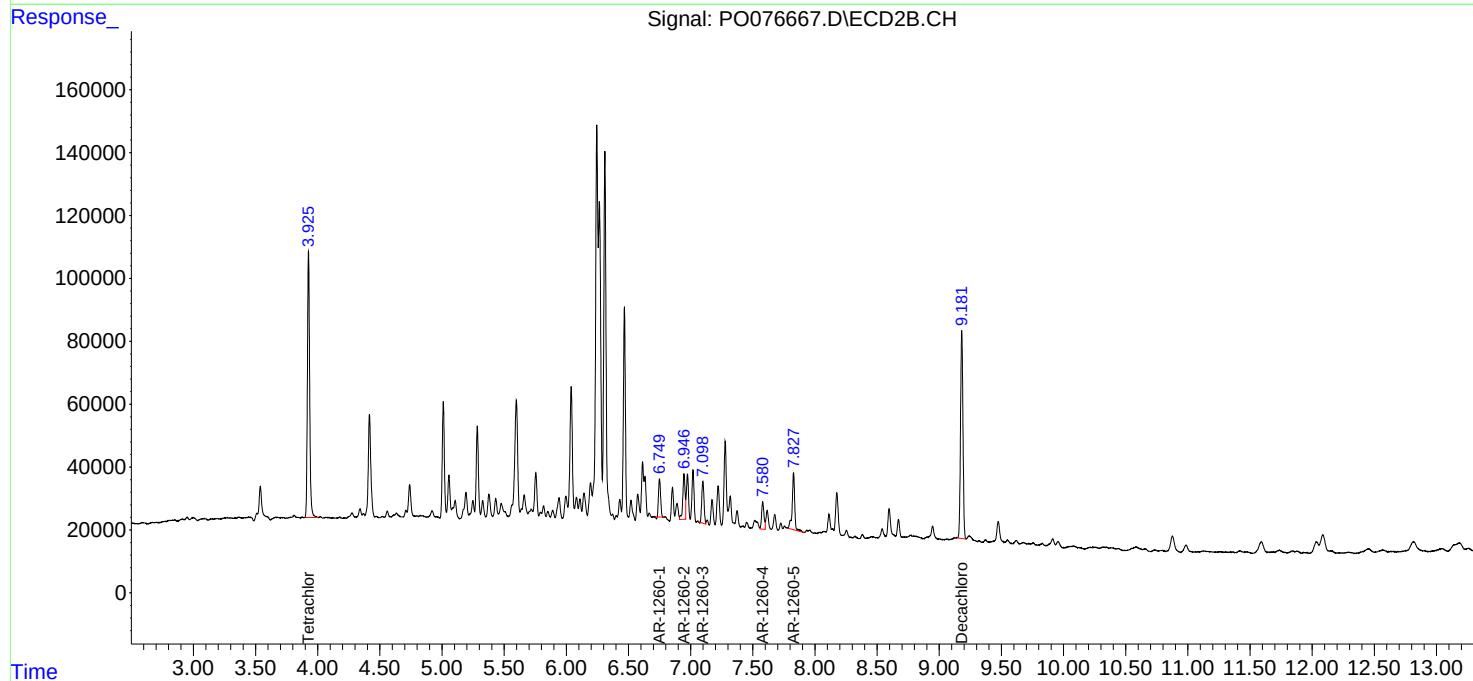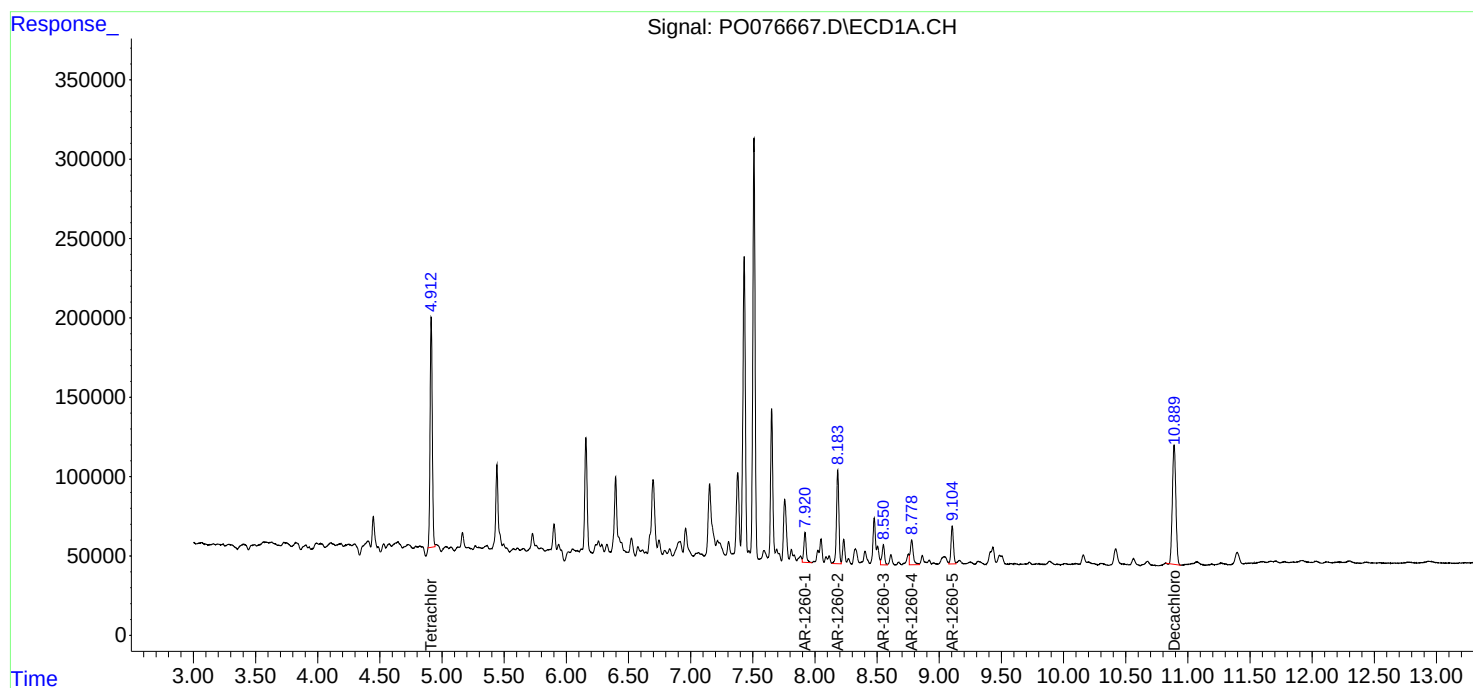

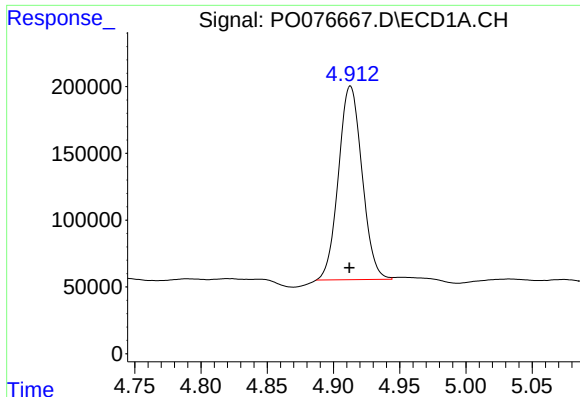


#1 Tetrachloro-m-xylene

R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 1795693
Conc: 20.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MMR-SP


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:52 PM

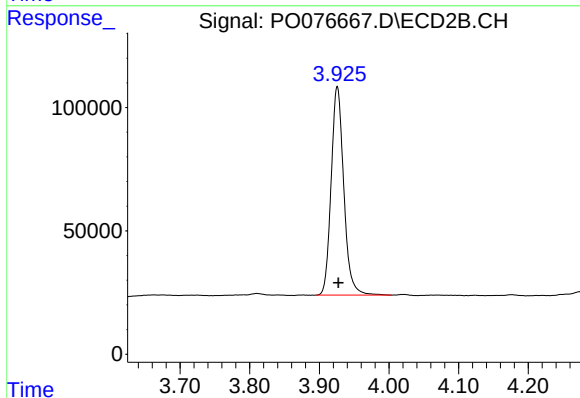


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 1063265
Conc: 19.38 ng/ml

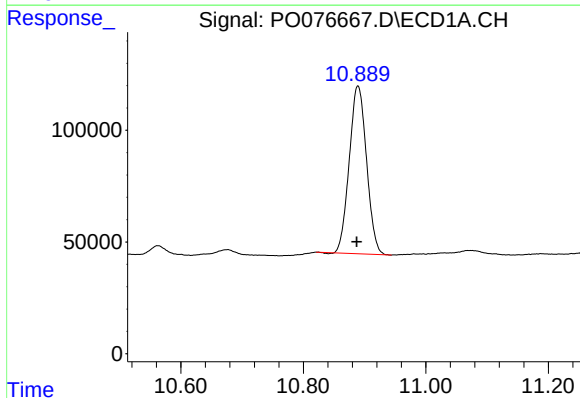


#2 Decachlorobiphenyl

R.T.: 10.889 min
Delta R.T.: 0.002 min
Response: 1472376
Conc: 22.62 ng/ml

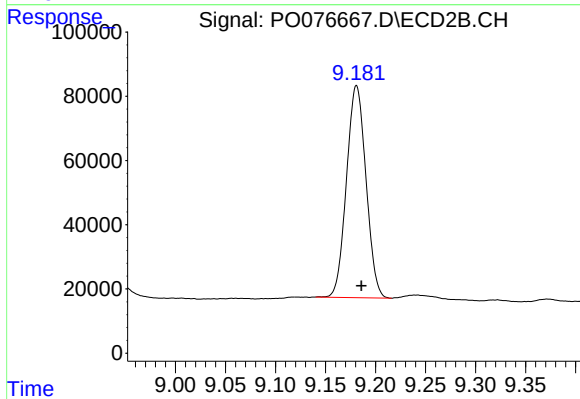

#2 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.005 min
Response: 896276
Conc: 19.02 ng/ml

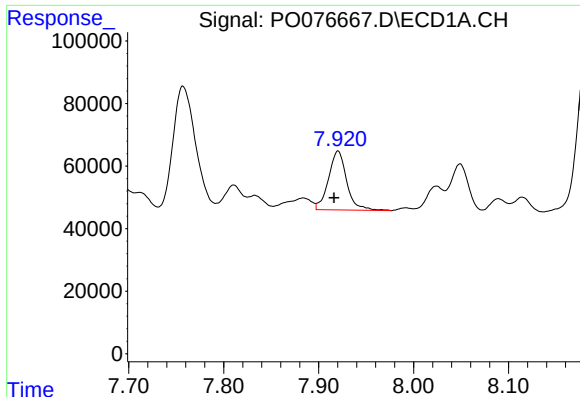


#31 AR-1260-1

R.T.: 7.920 min
Delta R.T.: 0.004 min
Response: 251298
Conc: 73.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
MMR-SP


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:52 PM

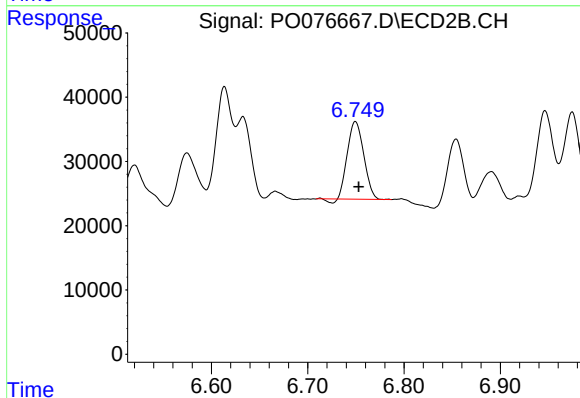


#31 AR-1260-1

R.T.: 6.750 min
Delta R.T.: -0.003 min
Response: 140317
Conc: 54.75 ng/ml

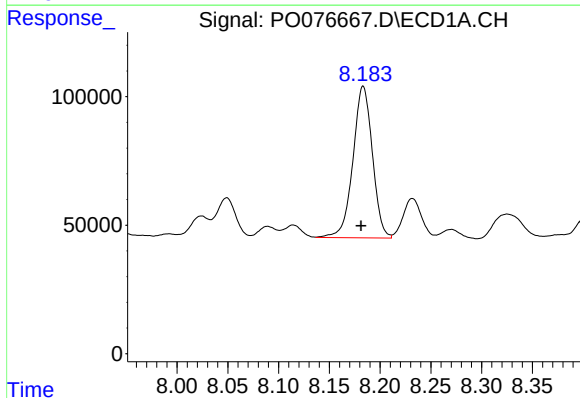


#32 AR-1260-2

R.T.: 8.183 min
Delta R.T.: 0.002 min
Response: 786454
Conc: 193.97 ng/ml

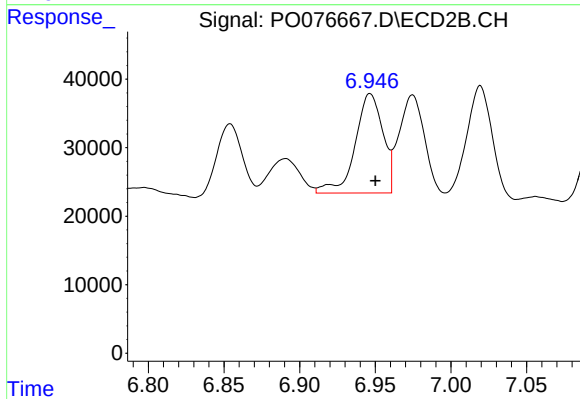

#32 AR-1260-2

R.T.: 6.947 min
Delta R.T.: -0.003 min
Response: 185110
Conc: 59.69 ng/ml

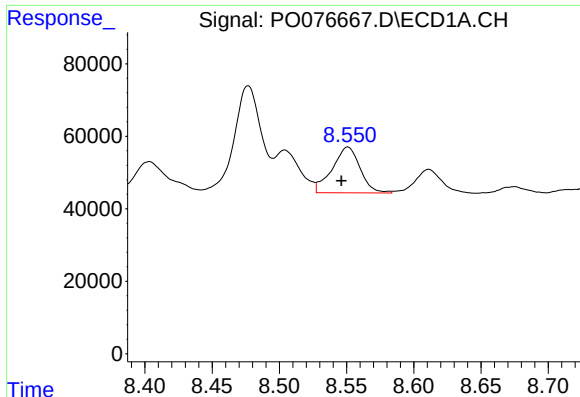


#33 AR-1260-3

R.T.: 8.551 min
Delta R.T.: 0.005 min
Response: 181742
Conc: 60.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MMR-SP


Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:52 PM

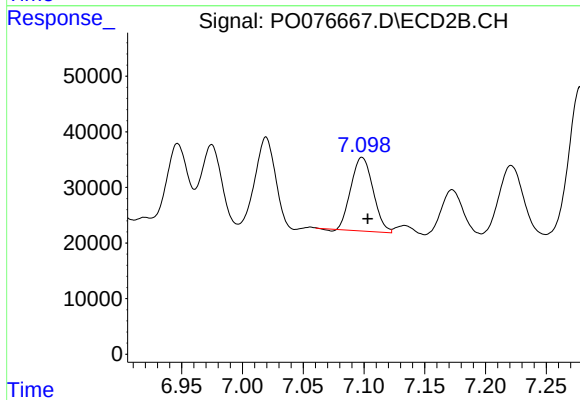


#33 AR-1260-3

R.T.: 7.098 min
Delta R.T.: -0.005 min
Response: 167346
Conc: 56.96 ng/ml

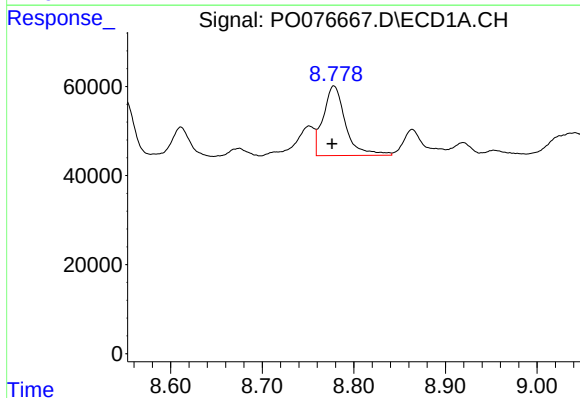


#34 AR-1260-4

R.T.: 8.778 min
Delta R.T.: 0.002 min
Response: 263254
Conc: 75.54 ng/ml

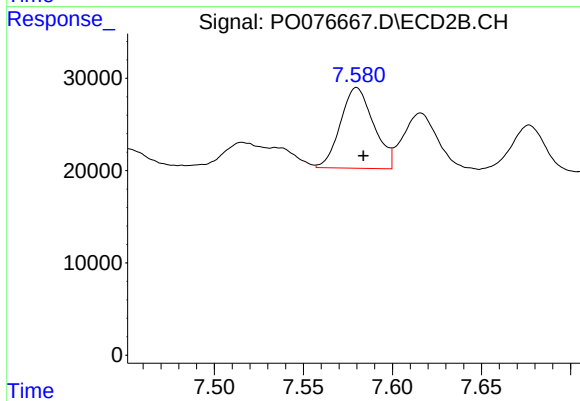

#34 AR-1260-4

R.T.: 7.580 min
Delta R.T.: -0.004 min
Response: 113416
Conc: 47.59 ng/ml

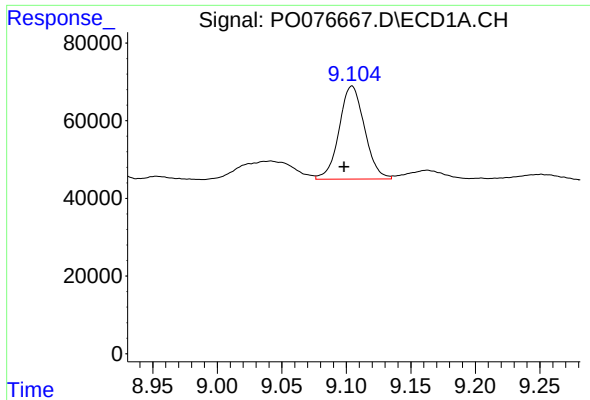


#35 AR-1260-5

R.T.: 9.104 min
Delta R.T.: 0.006 min
Response: 328616
Conc: 48.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MMR-SP

Manual Integrations
APPROVED

Ankita
4/1/2021 12:52:52 PM

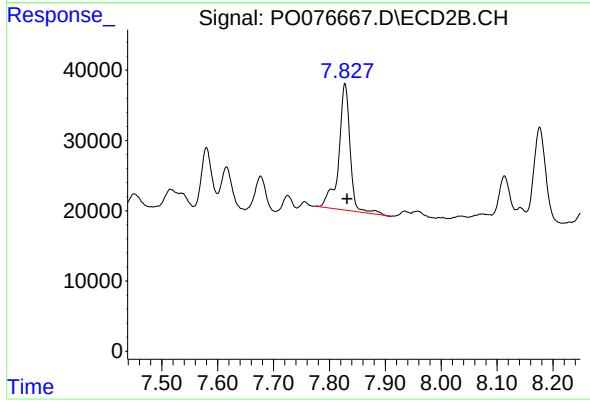

#35 AR-1260-5

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 255460
Conc: 45.03 ng/ml