

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
 Data File : P0085779.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2022 19:17
 Operator : YP\AJ
 Sample : N2152-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIT-11-DEWATERING-EFFL-UNTREATED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:19:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.584	3458686	798167	17.749	16.876
2) SA Decachlor...	10.387	8.599	2437245	635876	18.994	18.111

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
Data File : P0085779.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2022 19:17
Operator : YP\AJ
Sample : N2152-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIT-11-DEWATERING-EFFL-UNTREATED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:19:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

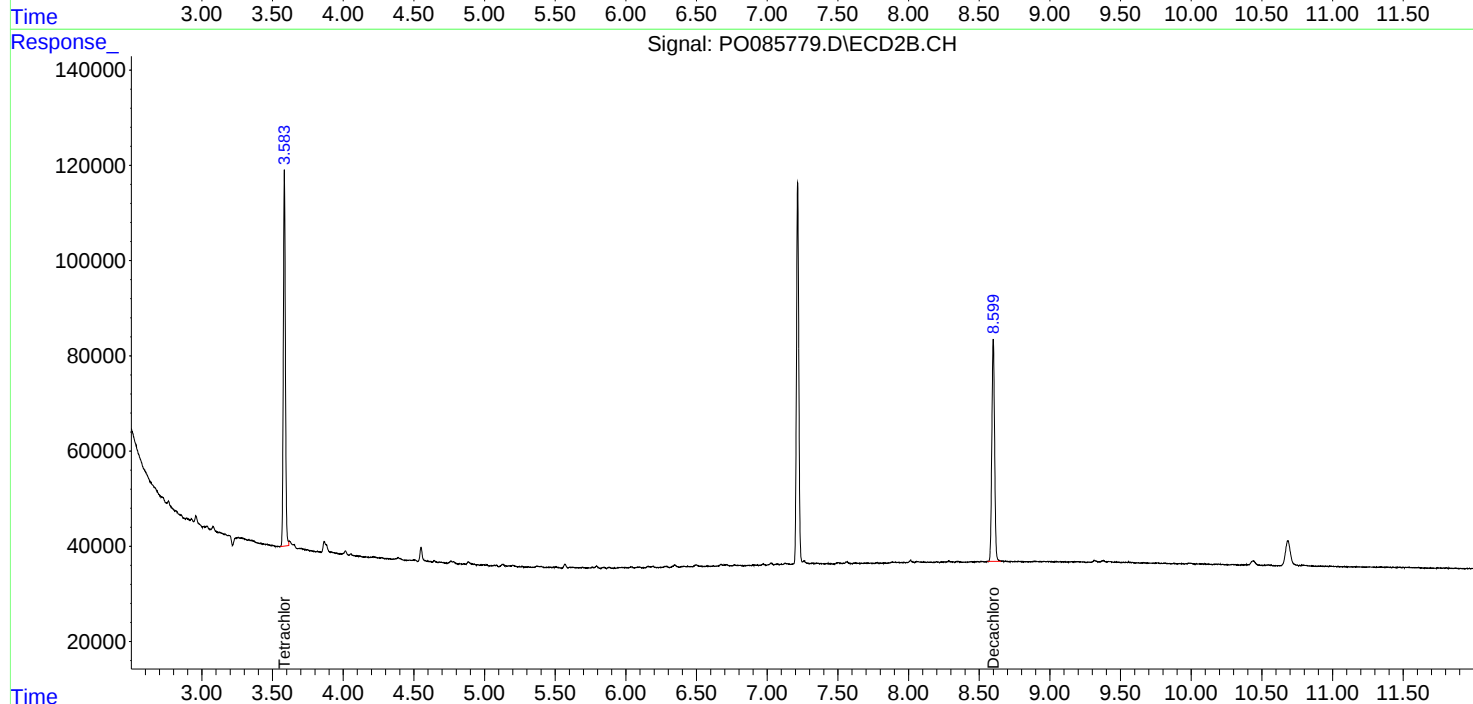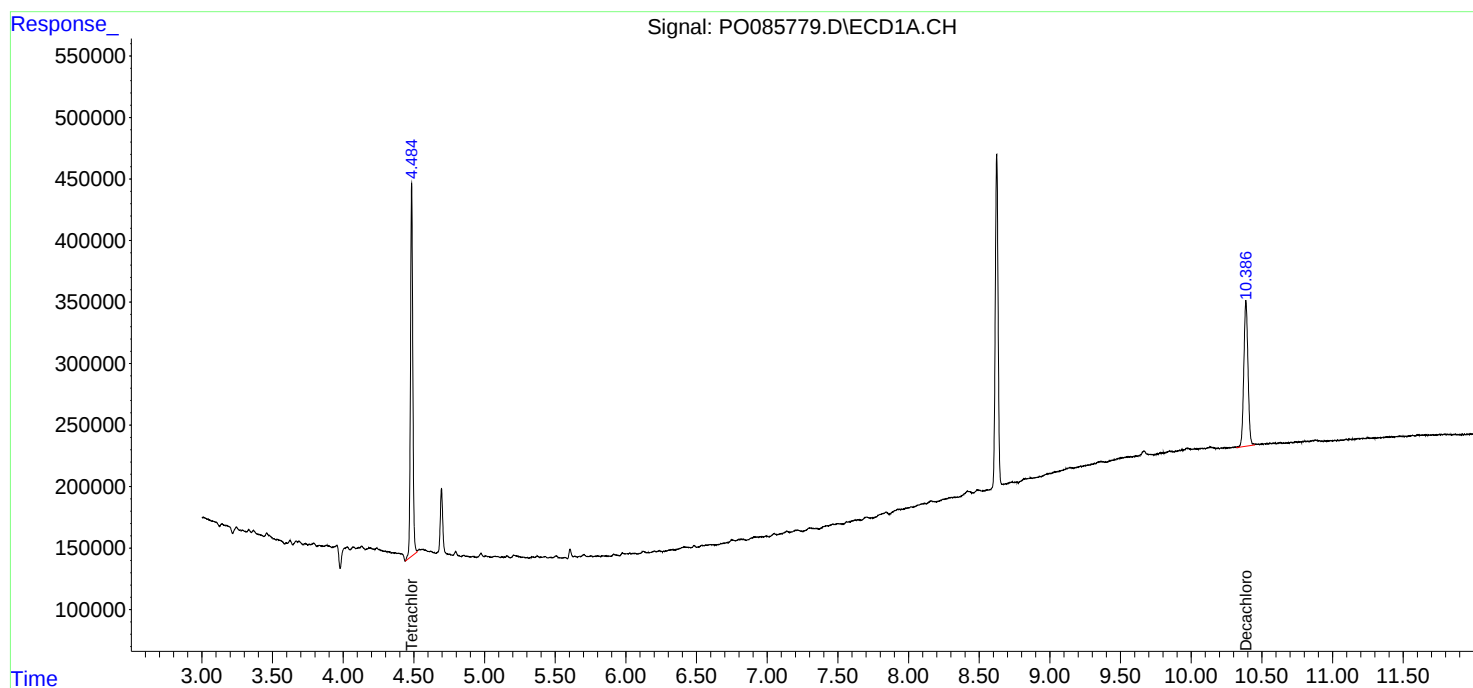

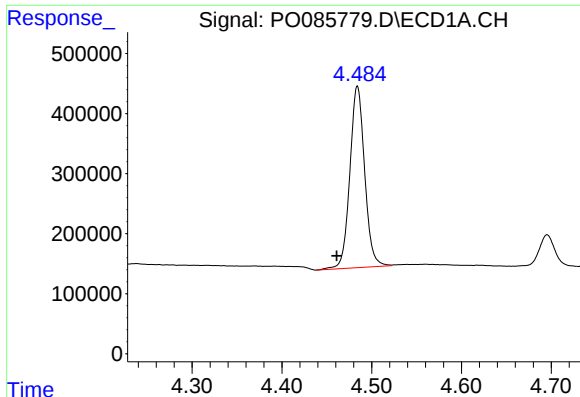

#1 Tetrachloro-m-xylene


R.T.: 4.484 min
Delta R.T.: 0.023 min
Response: 3458686
Conc: 17.75 ng/ml

Instrument :

ECD_O


ClientSampleId :

PIT-11-DEWATERING-EFFL-UNTREATED

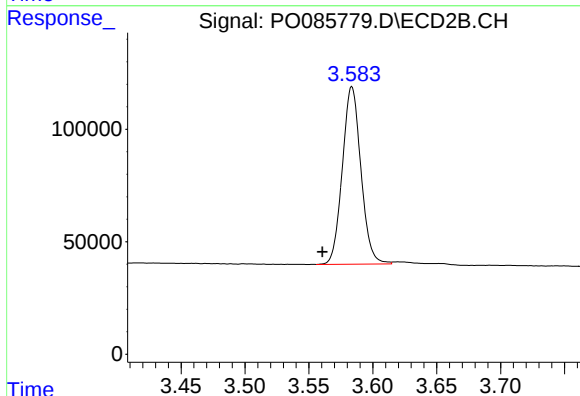


#1 Tetrachloro-m-xylene

R.T.: 3.584 min
Delta R.T.: 0.023 min
Response: 798167
Conc: 16.88 ng/ml

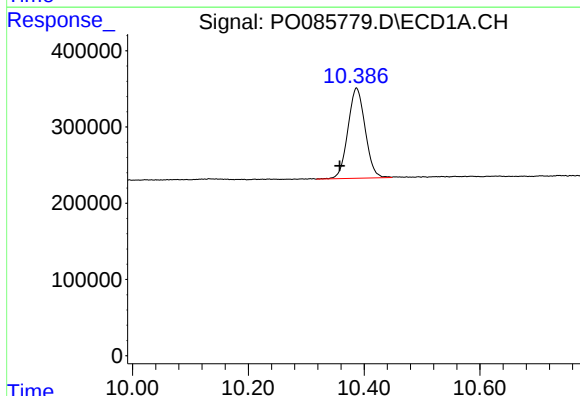

#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.029 min
Response: 2437245
Conc: 18.99 ng/ml

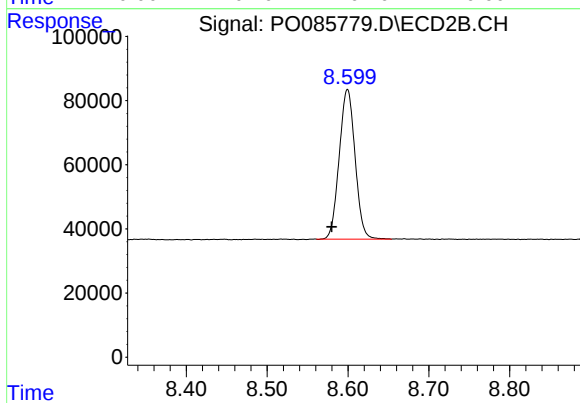

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: 0.020 min
Response: 635876
Conc: 18.11 ng/ml