

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
 Data File : P0085780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2022 19:32
 Operator : YP\AJ
 Sample : N2152-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIT-11-DEWATERING-EFFL-TREATED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:19:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.466	3.567	2995063	753260	15.369	15.927
2) SA Decachlor...	10.375	8.590	1628532	437745	12.691	12.468

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
Data File : P0085780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2022 19:32
Operator : YP\AJ
Sample : N2152-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIT-11-DEWATERING-EFFL-TREATED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:19:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

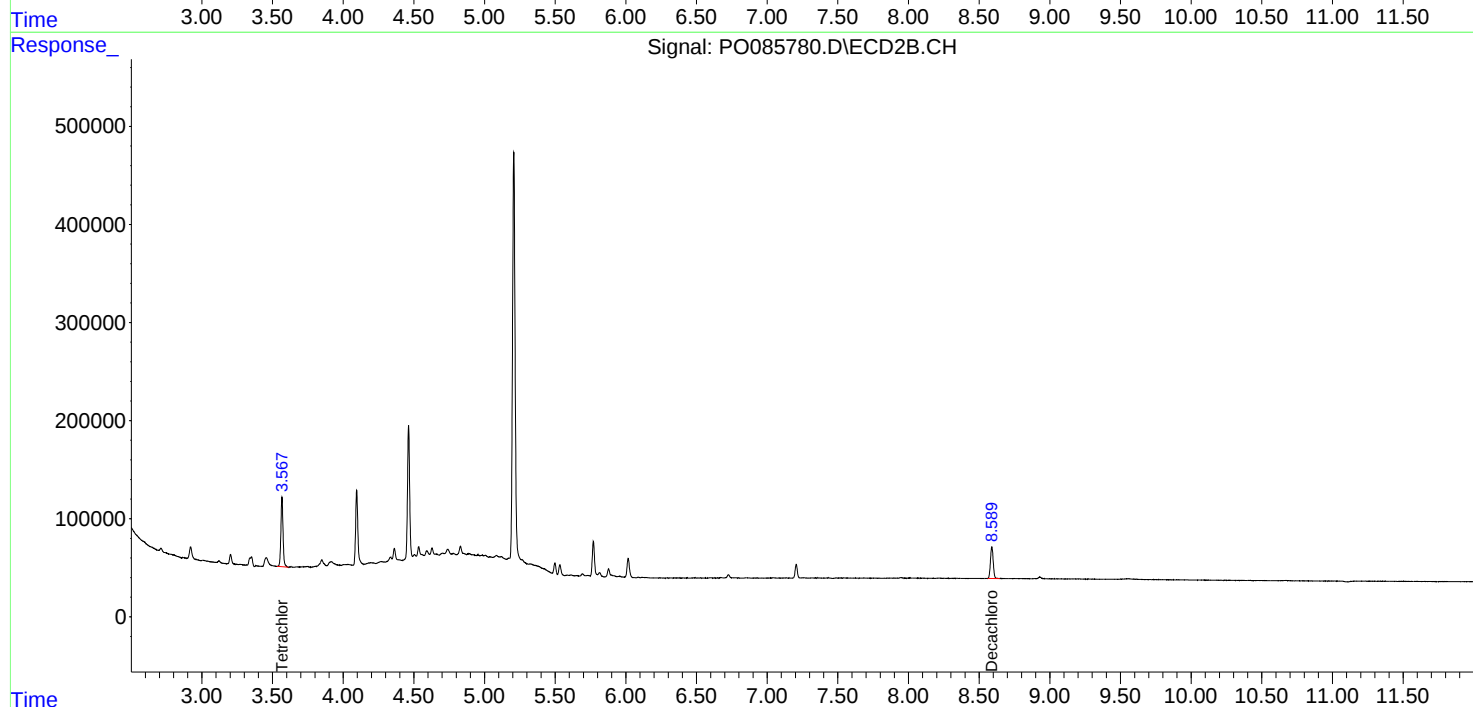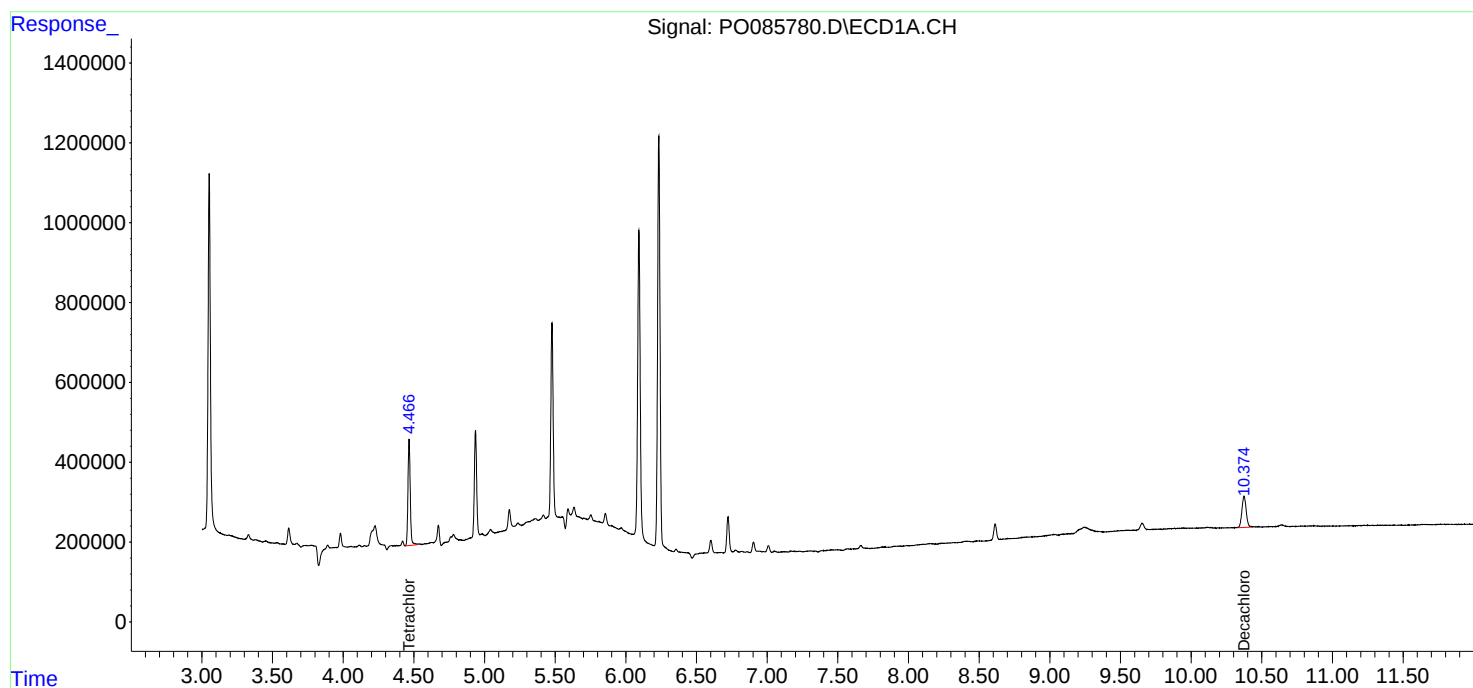

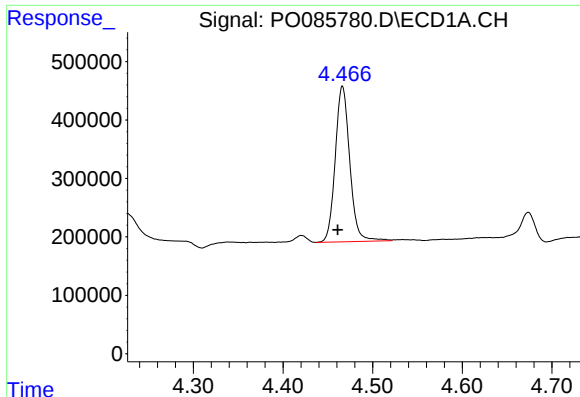

#1 Tetrachloro-m-xylene


R.T.: 4.466 min
Delta R.T.: 0.005 min
Response: 2995063
Conc: 15.37 ng/ml

Instrument :

ECD_O


ClientSampleId :

PIT-11-DEWATERING-EFFL-TREATED

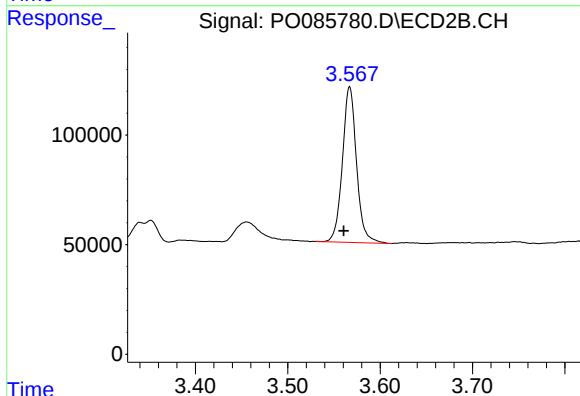


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.006 min
Response: 753260
Conc: 15.93 ng/ml

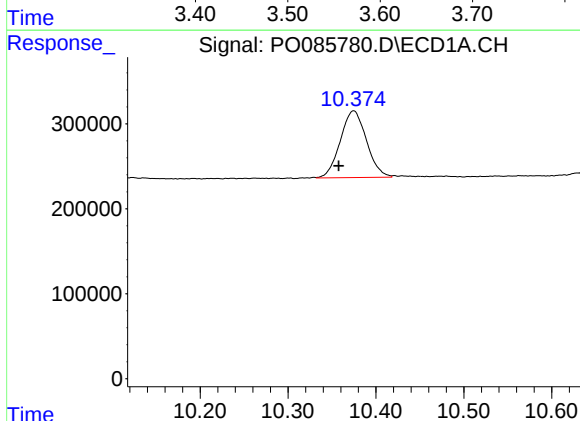

#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.017 min
Response: 1628532
Conc: 12.69 ng/ml

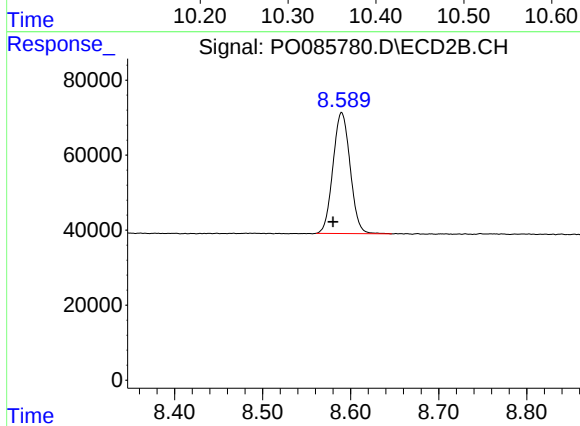

#2 Decachlorobiphenyl

R.T.: 8.590 min
Delta R.T.: 0.010 min
Response: 437745
Conc: 12.47 ng/ml