

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
 Data File : P0085798.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2022 1:21
 Operator : YP\AJ
 Sample : N2149-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PILE-LINDEN-PROPANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:29:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.568	3156434	934509	16.198	19.759
2) SA Decachlor...	10.377	8.593	1888999	521885	14.721	14.864

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
Data File : P0085798.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2022 1:21
Operator : YP\AJ
Sample : N2149-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PILE-LINDEN-PROPANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:29:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

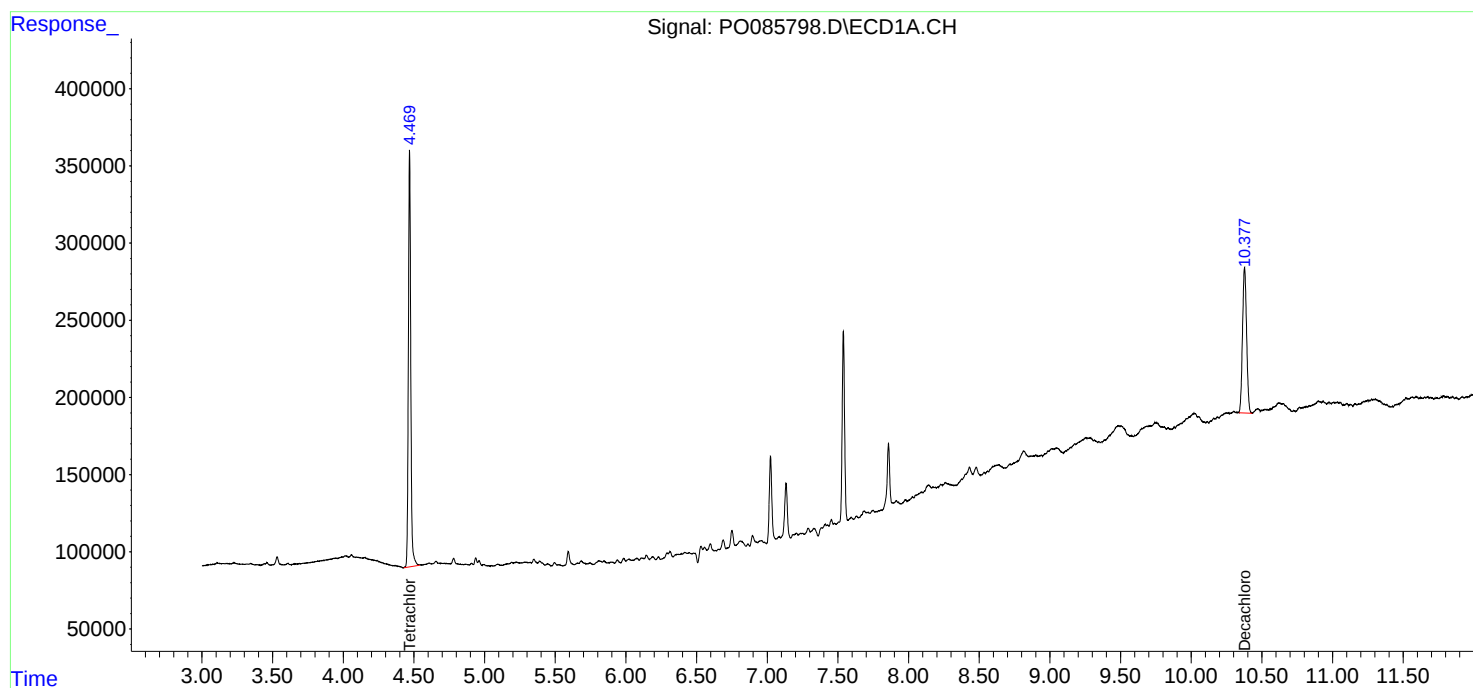


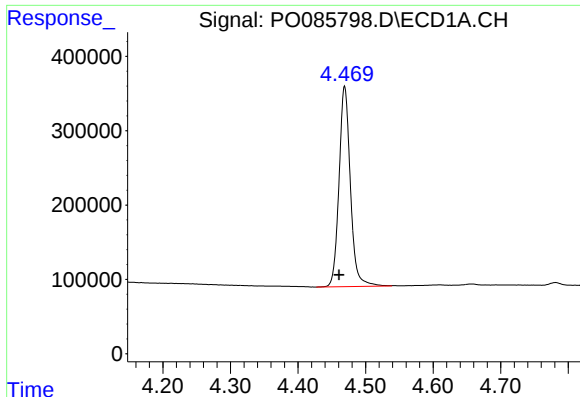

#1 Tetrachloro-m-xylene


R.T.: 4.469 min
Delta R.T.: 0.008 min
Response: 3156434
Conc: 16.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PILE-LINDEN-PROPANE

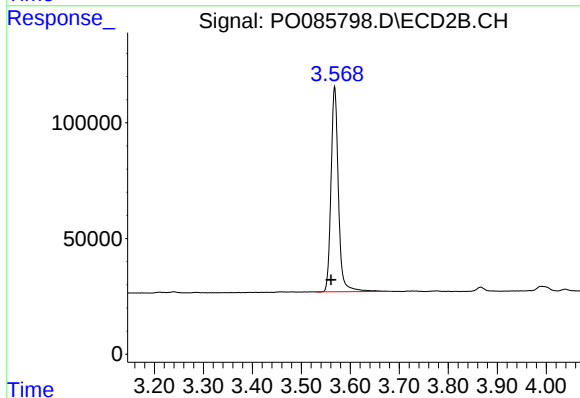


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.007 min
Response: 934509
Conc: 19.76 ng/ml

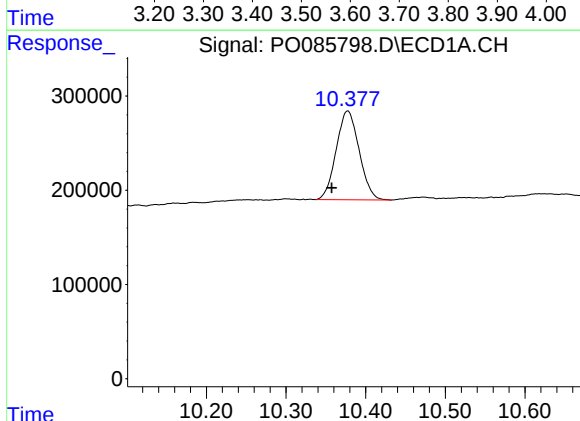

#2 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: 0.020 min
Response: 1888999
Conc: 14.72 ng/ml

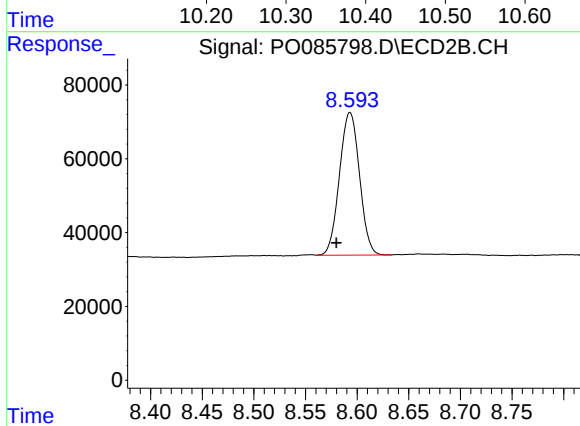

#2 Decachlorobiphenyl

R.T.: 8.593 min
Delta R.T.: 0.013 min
Response: 521885
Conc: 14.86 ng/ml