

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
 Data File : P0085799.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2022 1:37
 Operator : YP\AJ
 Sample : N2156-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-PILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:30:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.567	2977433	852563	15.279	18.027
2) SA Decachlor...	10.380	8.593	2154413	575837	16.790	16.401

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033022\
Data File : P0085799.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2022 1:37
Operator : YP\AJ
Sample : N2156-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:30:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

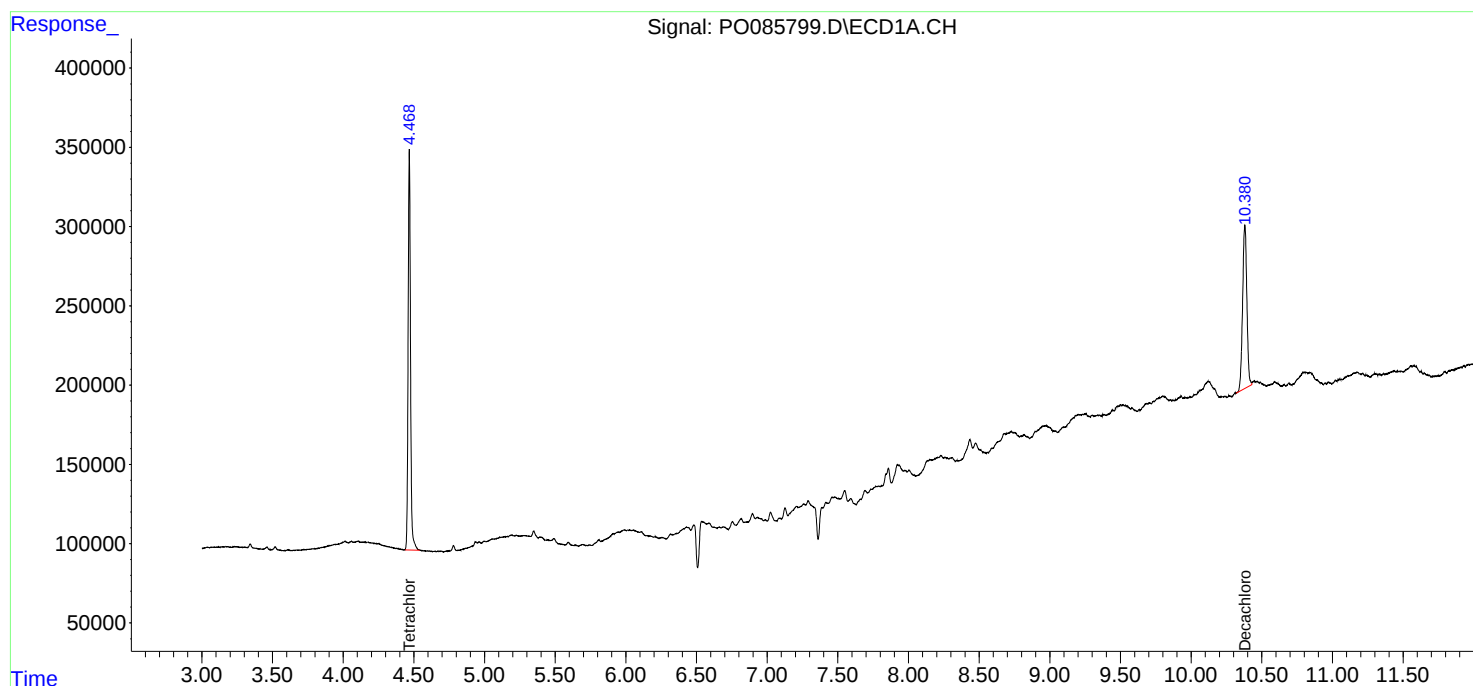


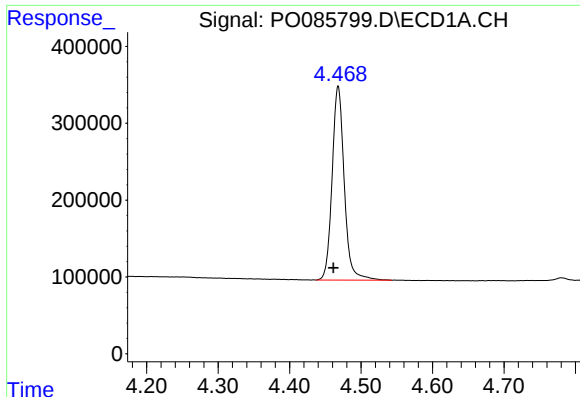

#1 Tetrachloro-m-xylene


R.T.: 4.468 min
Delta R.T.: 0.007 min
Response: 2977433
Conc: 15.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE

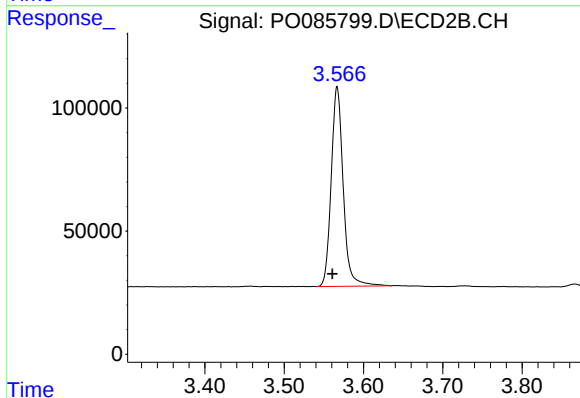


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.006 min
Response: 852563
Conc: 18.03 ng/ml

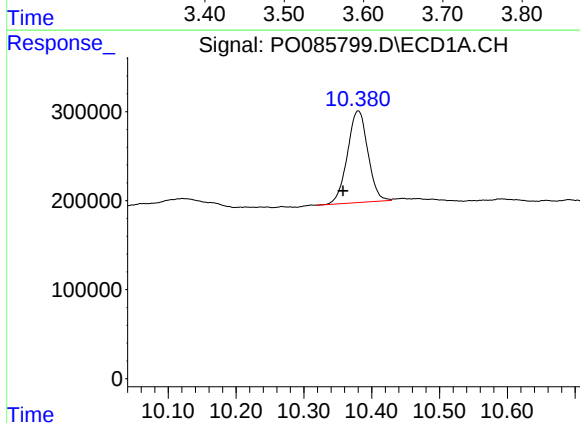

#2 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: 0.023 min
Response: 2154413
Conc: 16.79 ng/ml

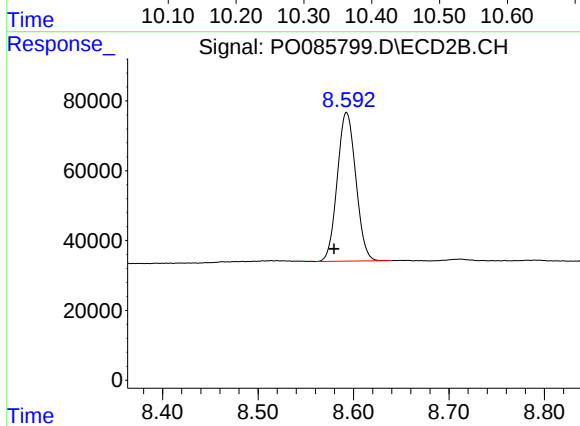

#2 Decachlorobiphenyl

R.T.: 8.593 min
Delta R.T.: 0.013 min
Response: 575837
Conc: 16.40 ng/ml