

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040119\
 Data File : P0054777.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 12:07
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:03:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.302	3.618	723873	680777	20.858	21.333
2)	SA Decachlor...	9.922	8.594	870301	616472	17.654	19.357
Target Compounds							
9)	L2 AR-1221-2	0.000	3.916	0	10968	N.D.	36.587 #
32)	L7 AR-1260-2	0.000	6.353	0	14701	N.D.	5.340 #
35)	L7 AR-1260-5	0.000	7.219	0	12308	N.D.	2.570 #
37)	L8 AR-1262-2	0.000	7.219	0	12308	N.D.	2.511 #
38)	L8 AR-1262-3	0.000	7.566	0	9048	N.D.	4.406 #
39)	L8 AR-1262-4	0.000	7.566	0	9048	N.D.	2.498 #
41)	L9 AR-1268-1	0.000	7.566	0	9048	N.D.	1.600 #
42)	L9 AR-1268-2	0.000	7.566	0	9048	N.D.	1.750 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040119\
Data File : PO054777.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 12:07
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:03:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

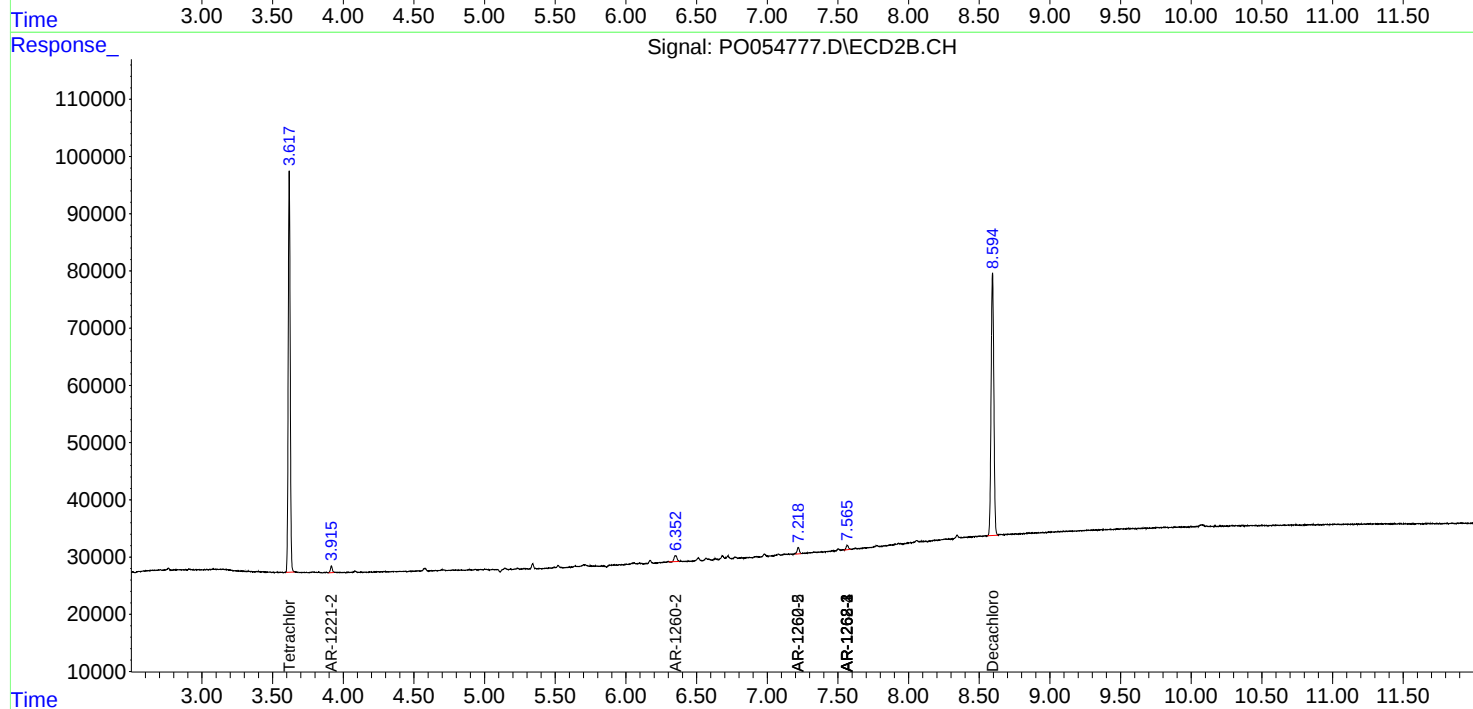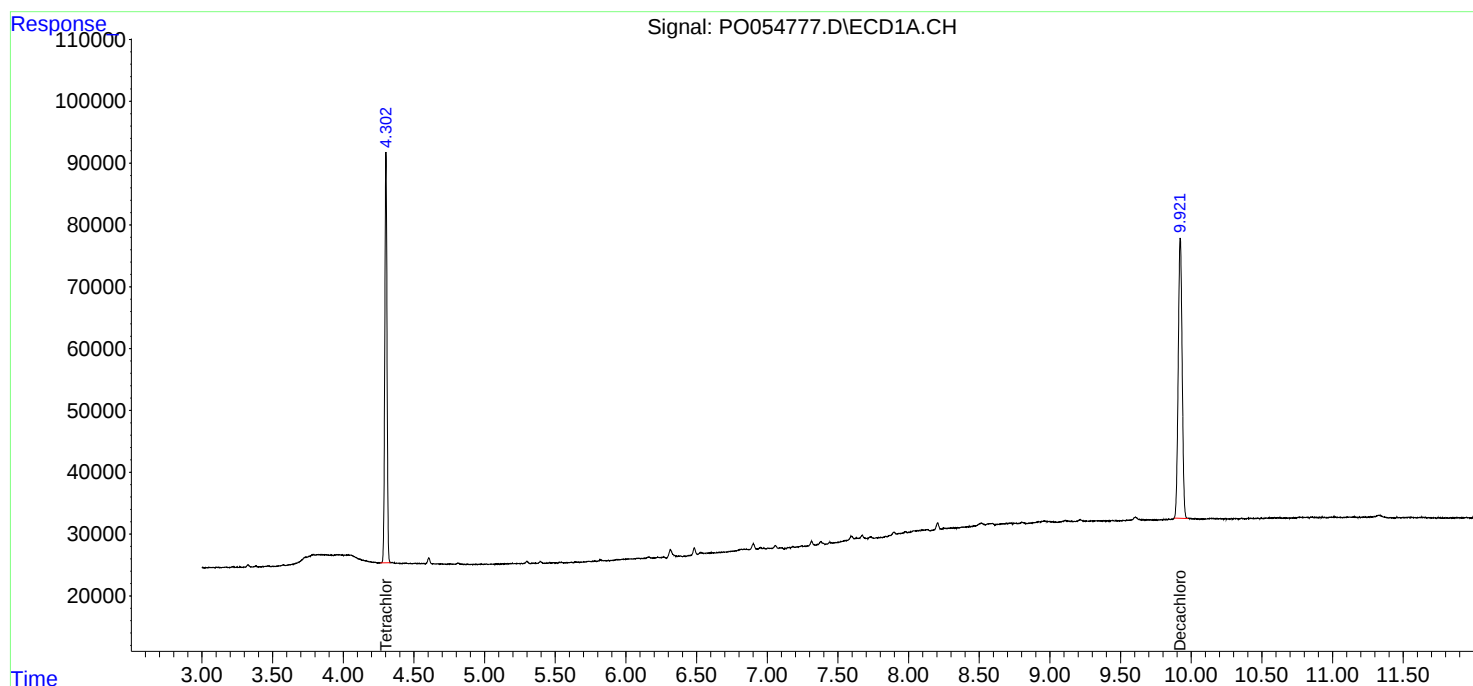


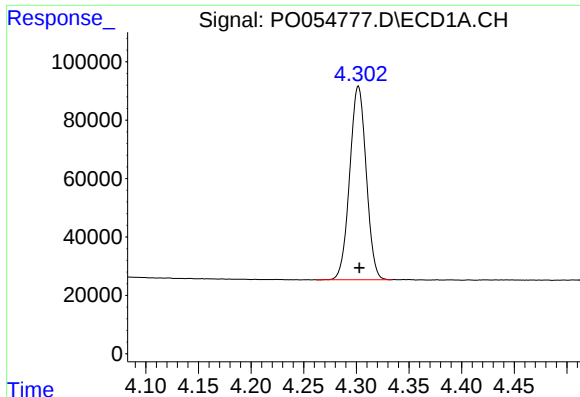

#1 Tetrachloro-m-xylene


R.T.: 4.302 min
Delta R.T.: -0.001 min
Response: 723873
Conc: 20.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

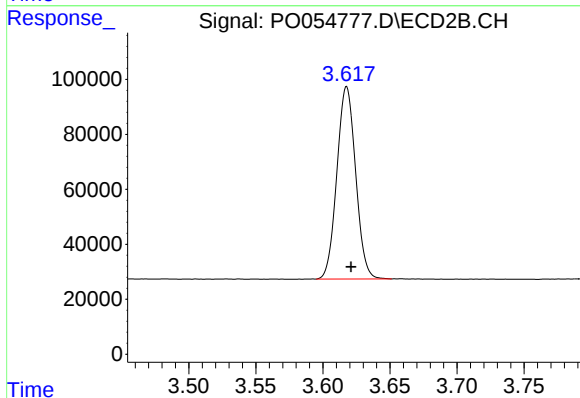


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.003 min
Response: 680777
Conc: 21.33 ng/ml

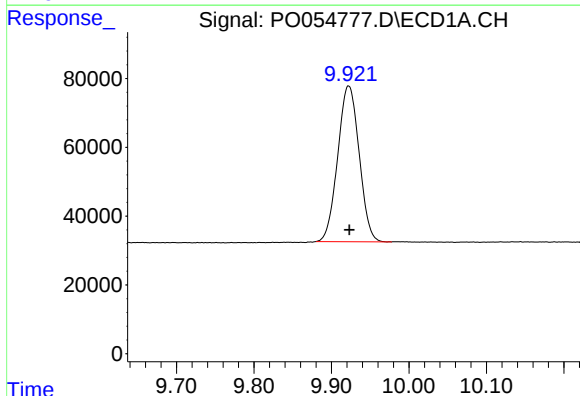


#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.001 min
Response: 870301
Conc: 17.65 ng/ml

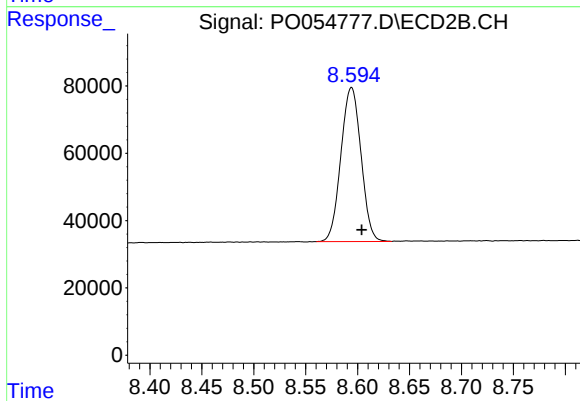

#2 Decachlorobiphenyl


R.T.: 8.594 min
Delta R.T.: -0.010 min
Response: 616472
Conc: 19.36 ng/ml

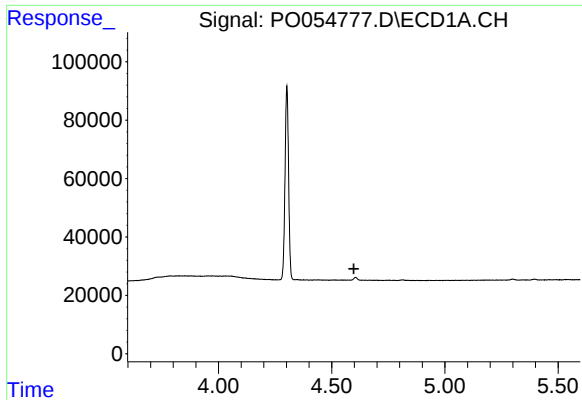

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

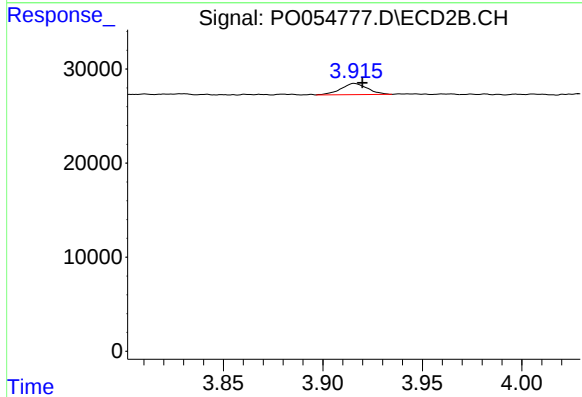


#9 AR-1221-2

R.T.: 3.916 min
Delta R.T.: -0.004 min
Response: 10968
Conc: 36.59 ng/ml

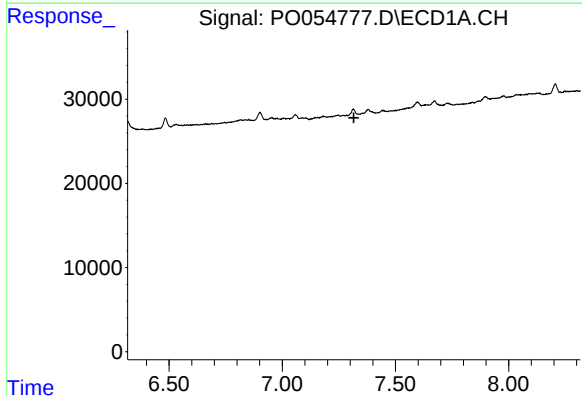


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.316 min
Response: 0
Conc: N.D.

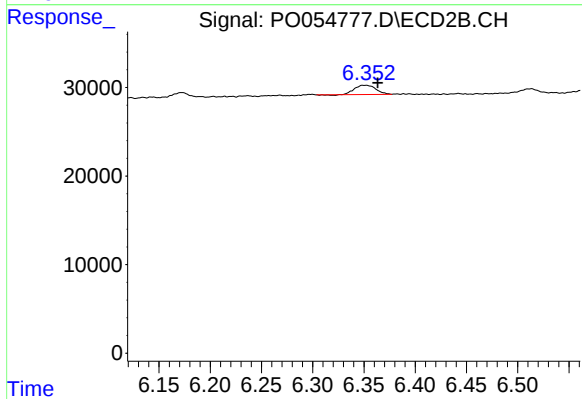

#32 AR-1260-2


R.T.: 6.353 min
Delta R.T.: -0.011 min
Response: 14701
Conc: 5.34 ng/ml

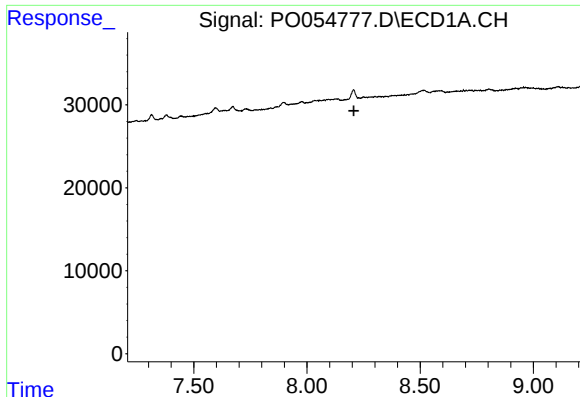

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

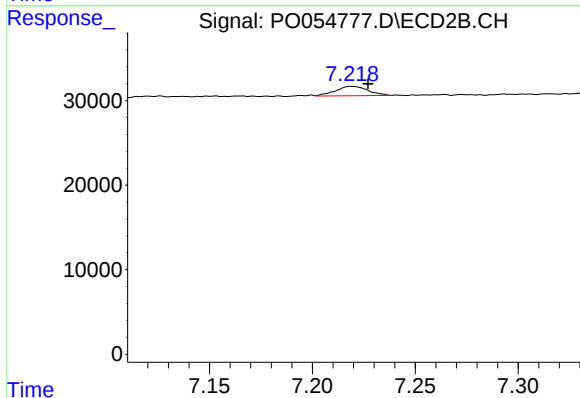


#35 AR-1260-5

R.T.: 7.219 min
Delta R.T.: -0.008 min
Response: 12308
Conc: 2.57 ng/ml

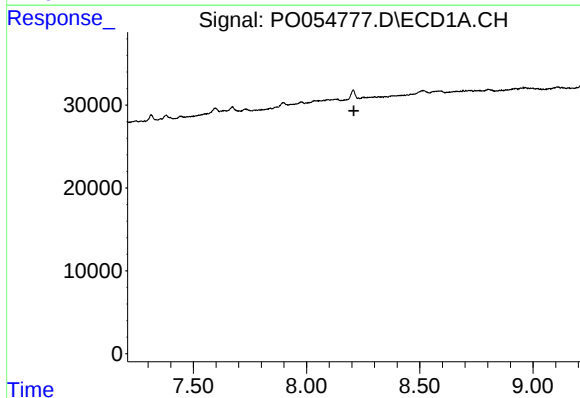


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.209 min
Response: 0
Conc: N.D.

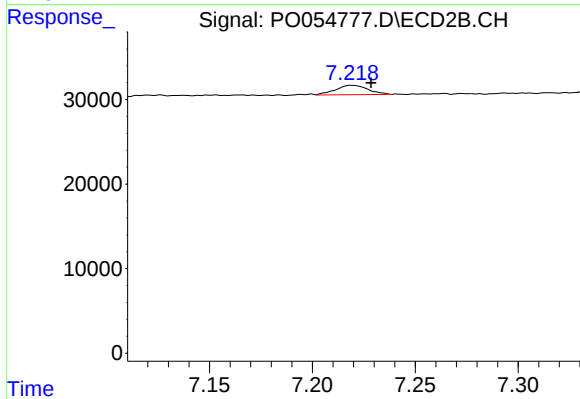

#37 AR-1262-2


R.T.: 7.219 min
Delta R.T.: -0.010 min
Response: 12308
Conc: 2.51 ng/ml

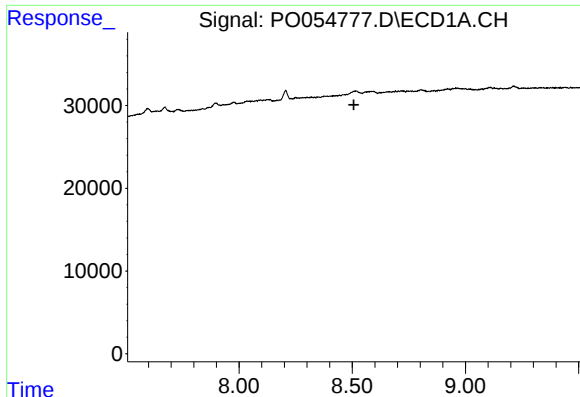

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

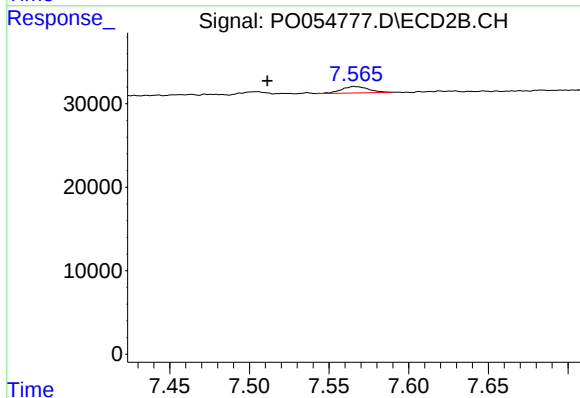


#38 AR-1262-3

R.T.: 7.566 min
Delta R.T.: 0.054 min
Response: 9048
Conc: 4.41 ng/ml

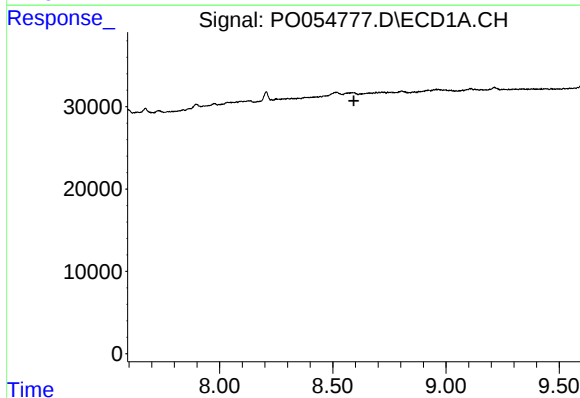


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.593 min
Response: 0
Conc: N.D.

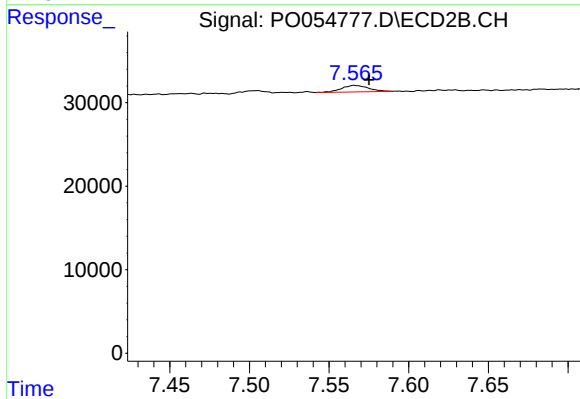

#39 AR-1262-4


R.T.: 7.566 min
Delta R.T.: -0.010 min
Response: 9048
Conc: 2.50 ng/ml

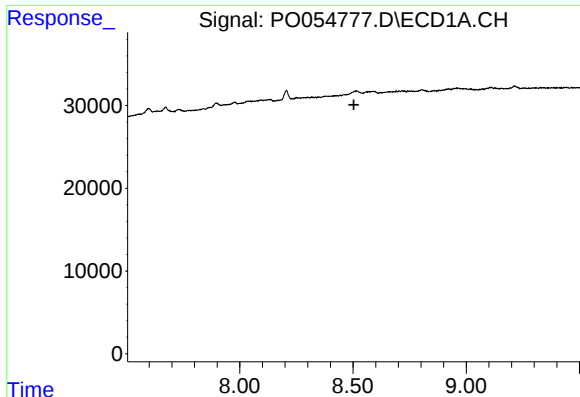

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

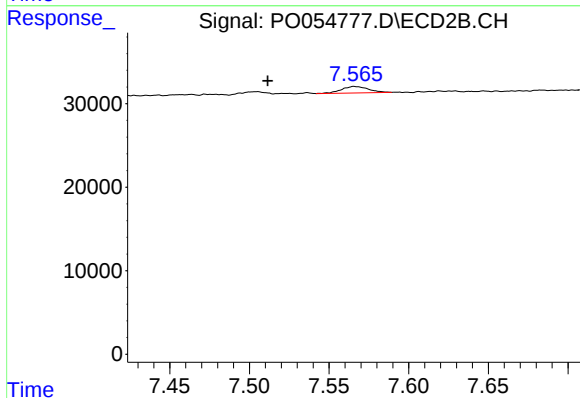


#41 AR-1268-1

R.T.: 7.566 min
Delta R.T.: 0.054 min
Response: 9048
Conc: 1.60 ng/ml

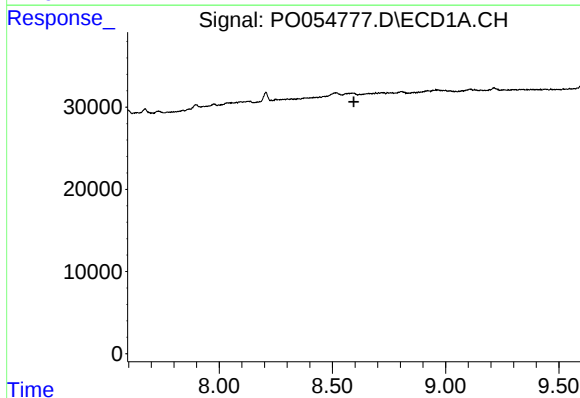

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.594 min
Response: 0
Conc: N.D.

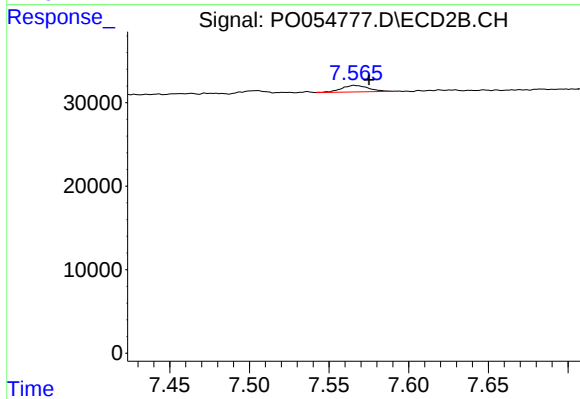

#42 AR-1268-2

R.T.: 7.566 min
Delta R.T.: -0.010 min
Response: 9048
Conc: 1.75 ng/ml