

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040119\
 Data File : P0054776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 11:50
 Operator : SM/SJ
 Sample : K2093-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DL-2-COMP

Manual Integrations
 APPROVED

Sohil
 4/2/2019 4:01:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:02:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.302	3.619	771904	628678	22.242m	19.700
2) SA Decachlor...	9.922	8.595	644927	450949	13.082	14.159

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040119\
Data File : P0054776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 11:50
Operator : SM/SJ
Sample : K2093-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DL-2-COMP


Manual Integrations
APPROVED

Sohil
4/2/2019 4:01:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:02:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

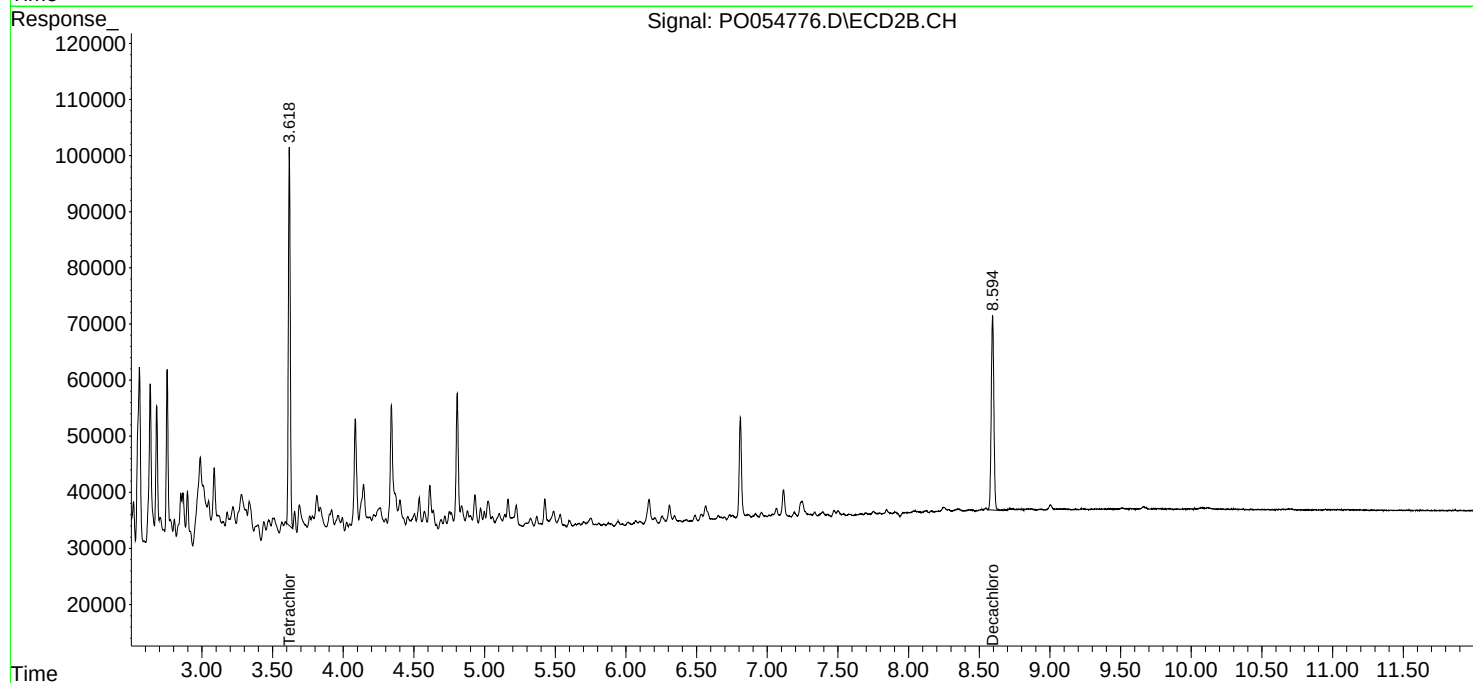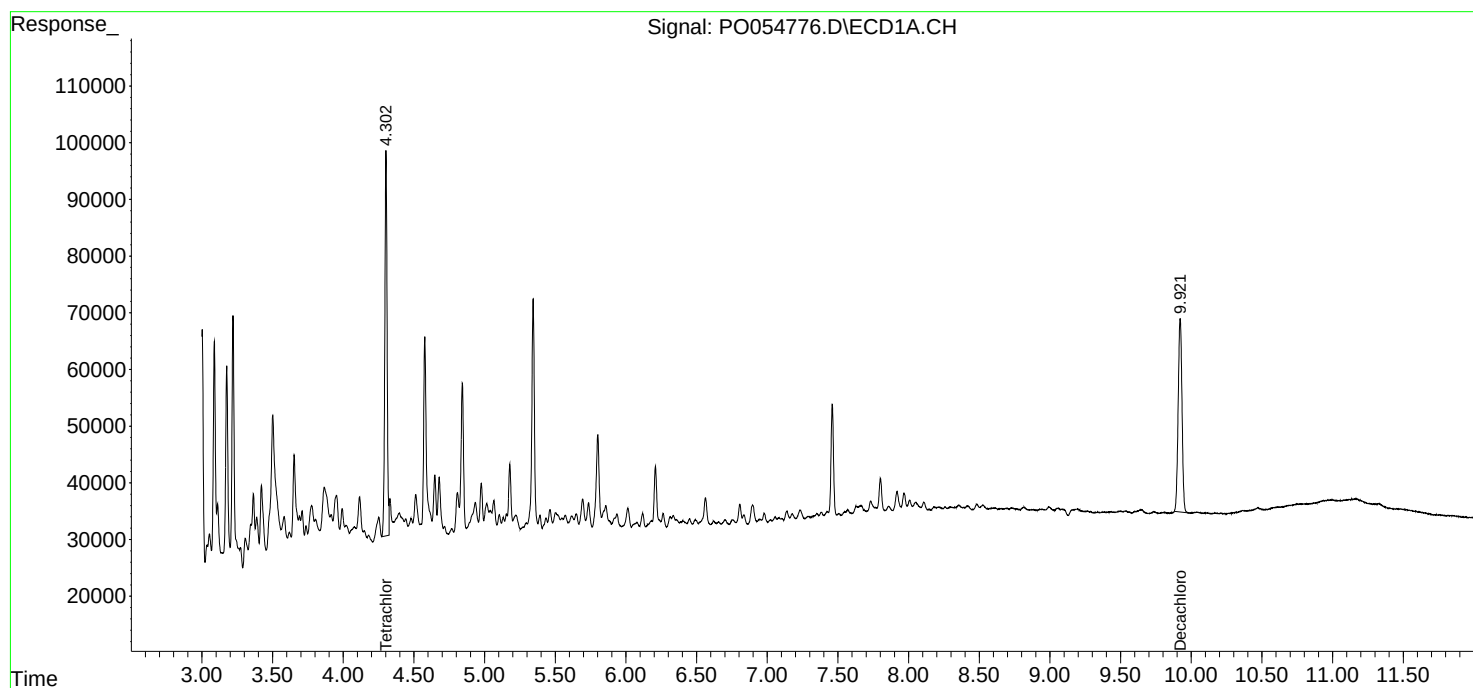

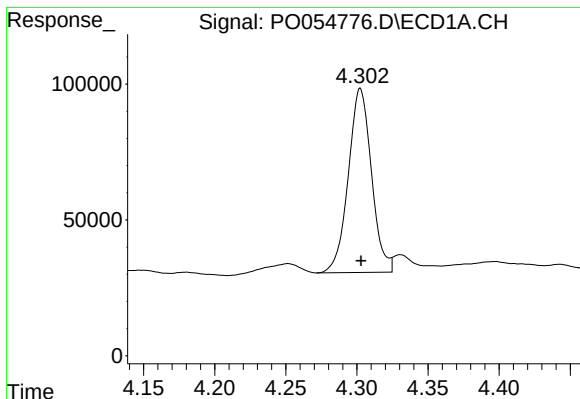


#1 Tetrachloro-m-xylene

R.T.: 4.302 min
Delta R.T.: -0.001 min
Response: 771904
Conc: 22.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DL-2-COMP


Manual Integrations
APPROVED

Sohil
4/2/2019 4:01:46 PM

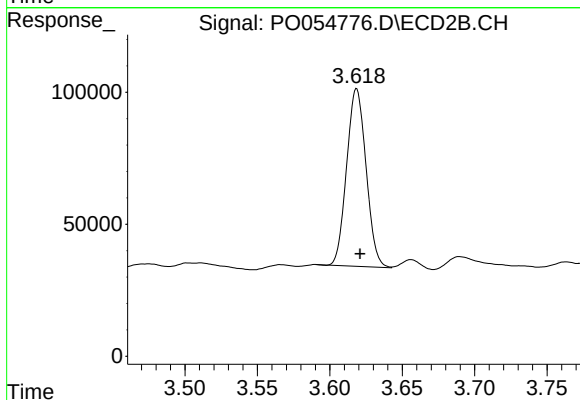


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 628678
Conc: 19.70 ng/ml

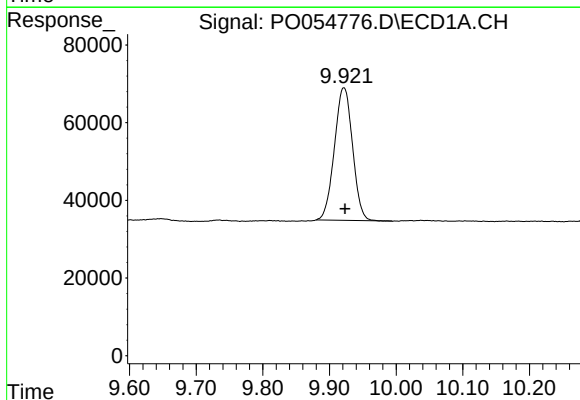

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.002 min
Response: 644927
Conc: 13.08 ng/ml

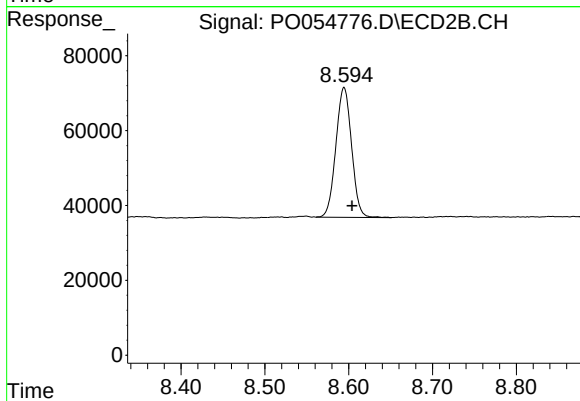

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: -0.010 min
Response: 450949
Conc: 14.16 ng/ml