

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040119\
 Data File : P0054783.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2019 15:55
 Operator : SM/SJ
 Sample : K2056-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 01:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.303	3.619	871620	902496	25.115	28.280
2)	SA Decachlor...	9.923	8.595	773045	542298	15.681	17.028

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040119\
Data File : PO054783.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2019 15:55
Operator : SM/SJ
Sample : K2056-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CS-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 01:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

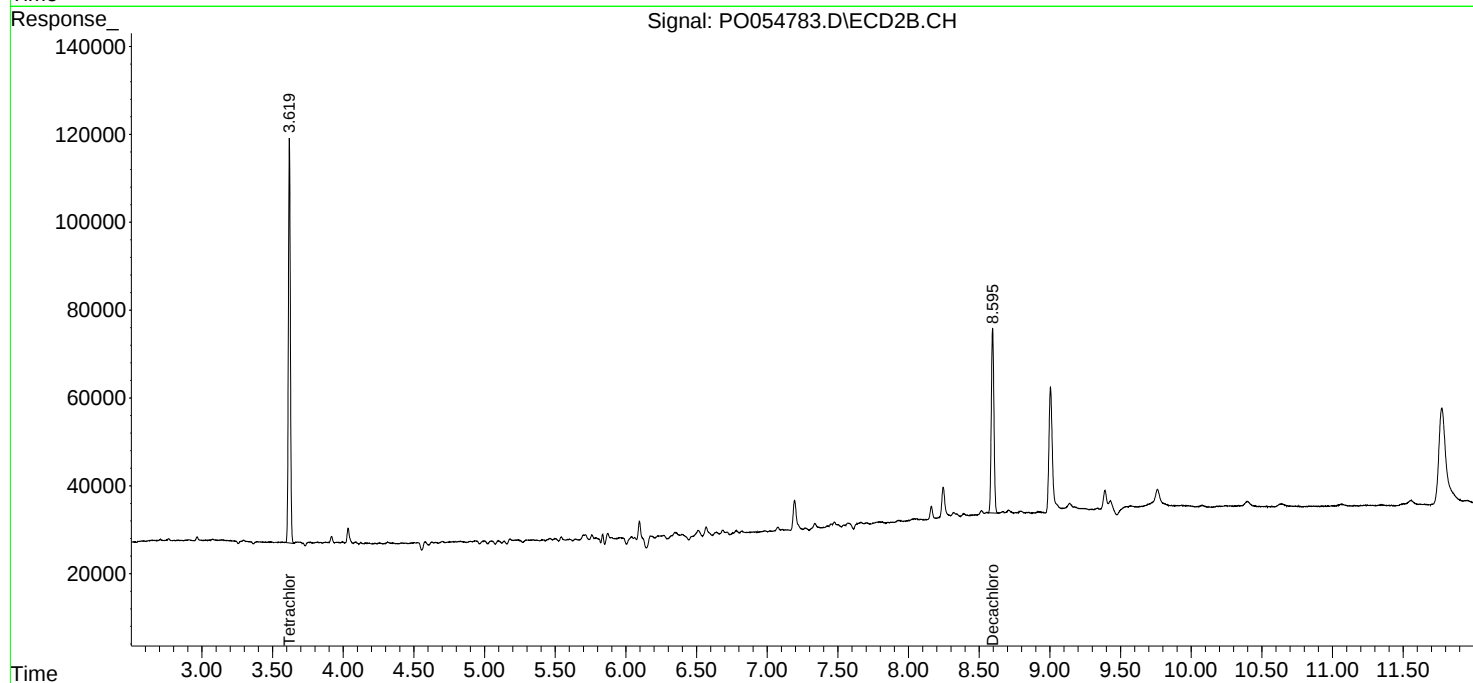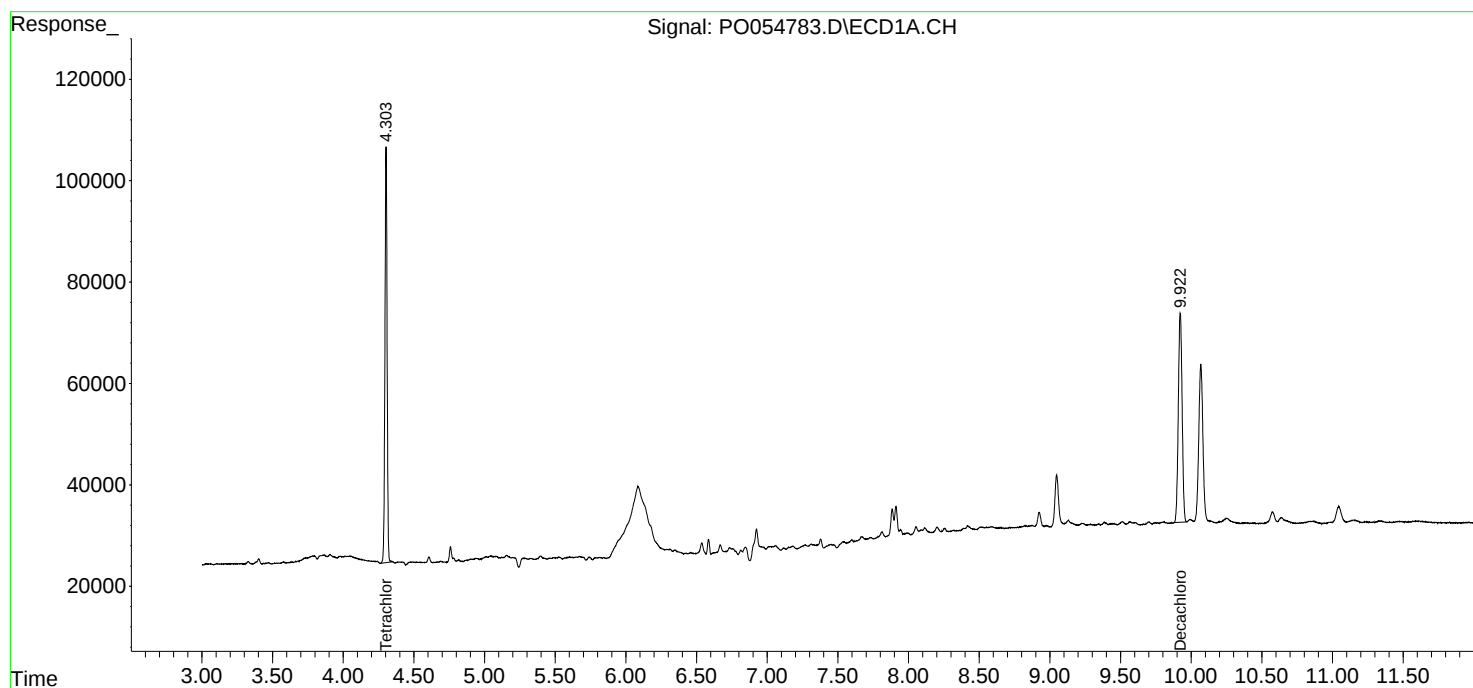


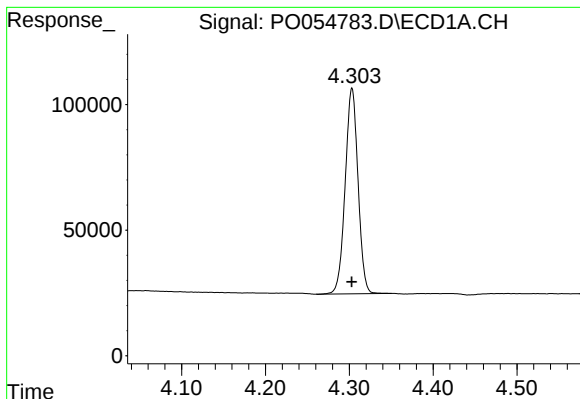

#1 Tetrachloro-m-xylene


R.T.: 4.303 min
Delta R.T.: 0.000 min
Response: 871620
Conc: 25.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-8

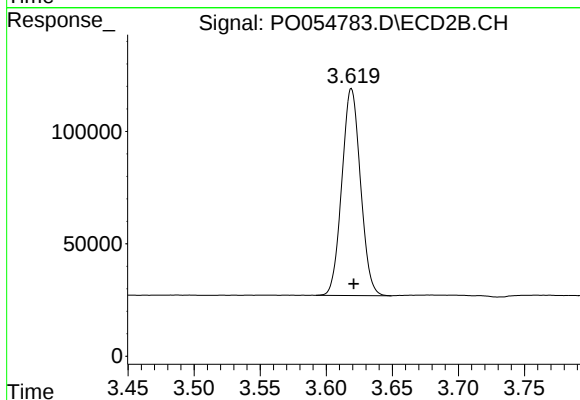


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 902496
Conc: 28.28 ng/ml

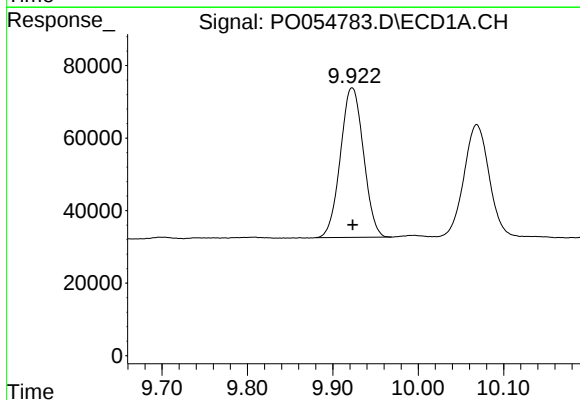

#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: 0.000 min
Response: 773045
Conc: 15.68 ng/ml

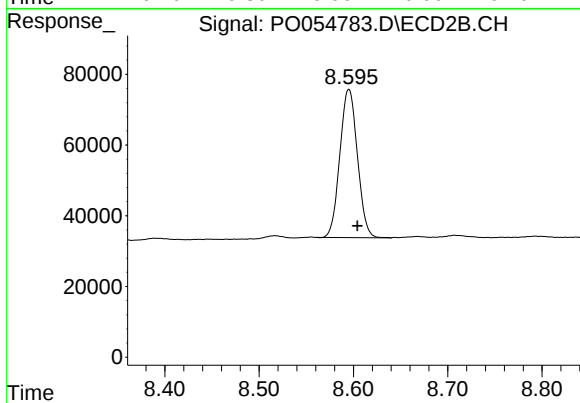

#2 Decachlorobiphenyl

R.T.: 8.595 min
Delta R.T.: -0.009 min
Response: 542298
Conc: 17.03 ng/ml