

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040121\
 Data File : P0076734.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 20:21
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:28:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 04:02:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 04:00:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.900	3.897	404454	217568	4.654	4.729
2) SA Decachlor...	10.874	9.144	439281	252026	4.980	5.509
Target Compounds						
26) L6 AR-1254-1	7.133	6.007	155367	143576	48.179	55.514m
27) L6 AR-1254-2	7.363	6.167	254345	123970	49.176	54.582
28) L6 AR-1254-3	7.744	6.584	258044	179881	45.965	50.527
29) L6 AR-1254-4	8.041	6.826	183530	111338	45.544	52.918
30) L6 AR-1254-5	8.467	7.248	218027	164229	49.211m	50.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040121\
Data File : P0076734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 20:21
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/2/2021 11:28:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 04:02:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 04:00:07 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

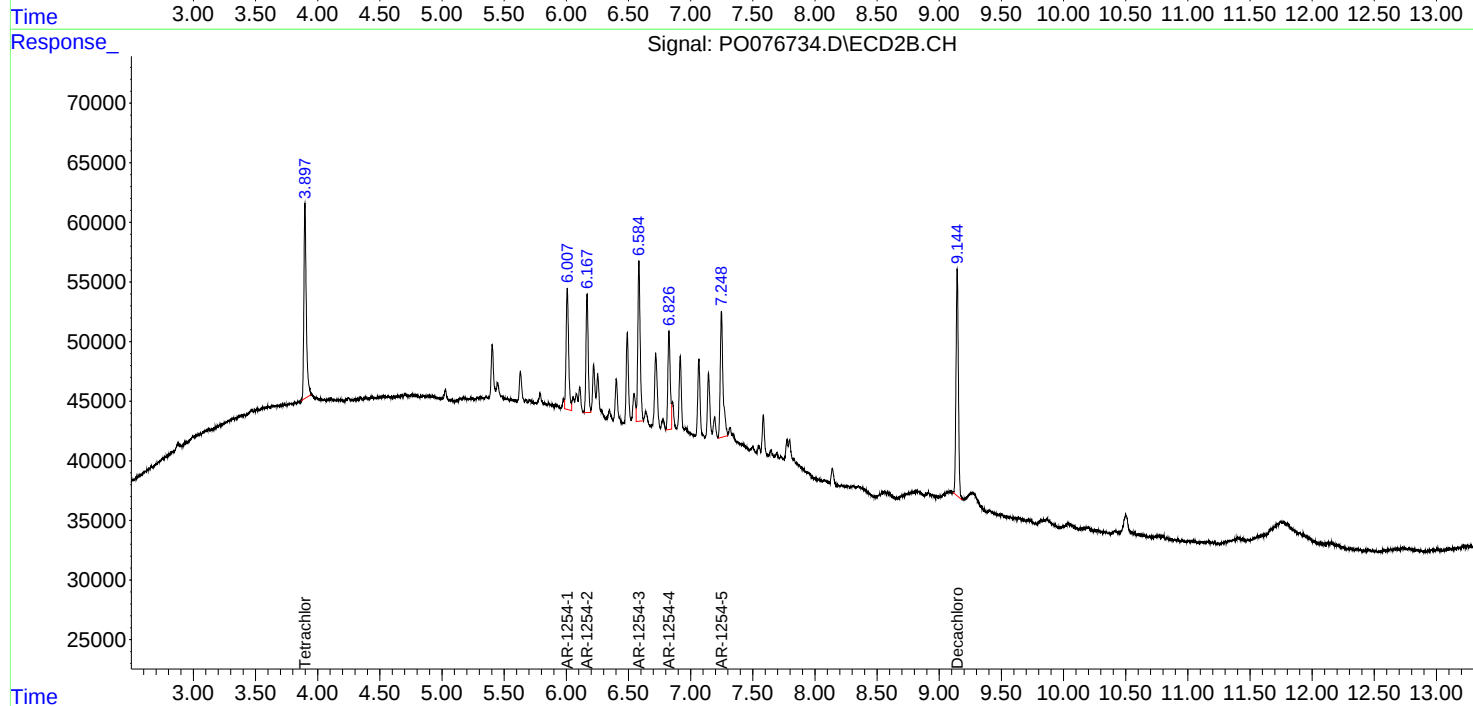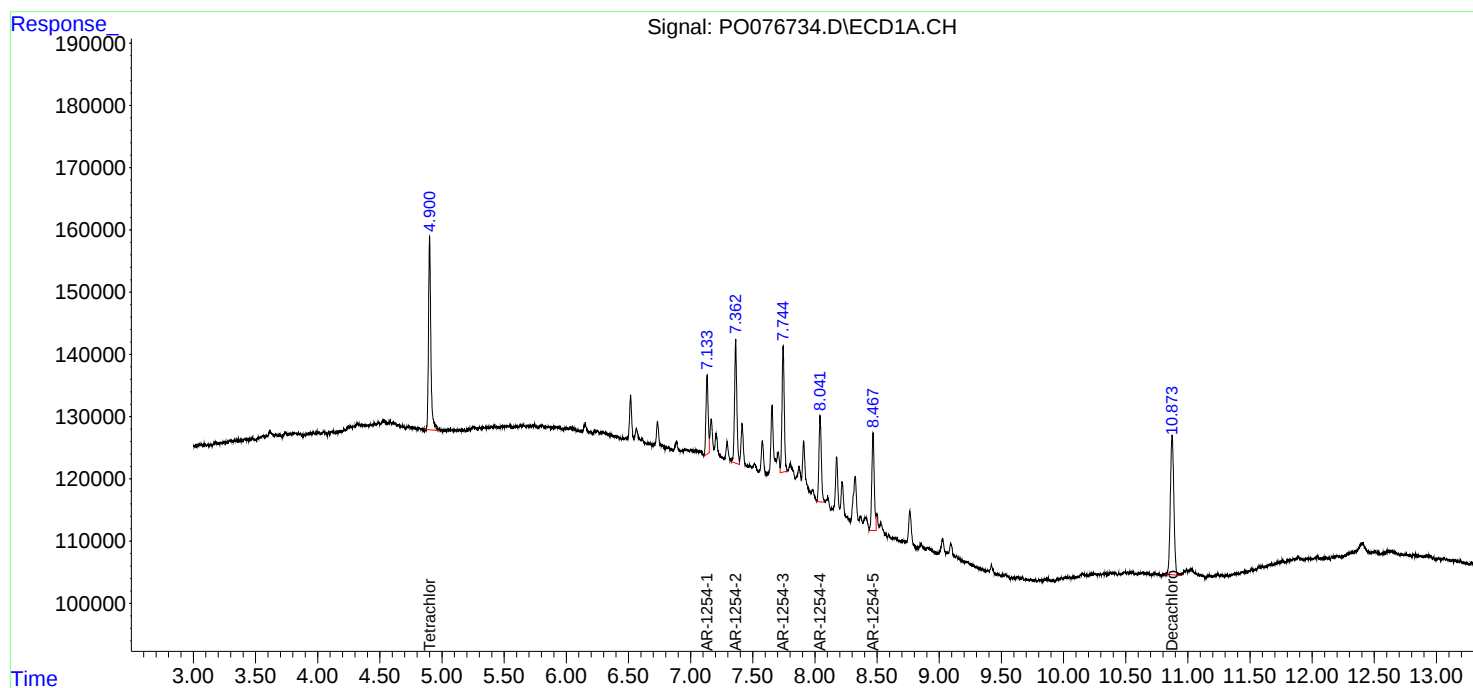

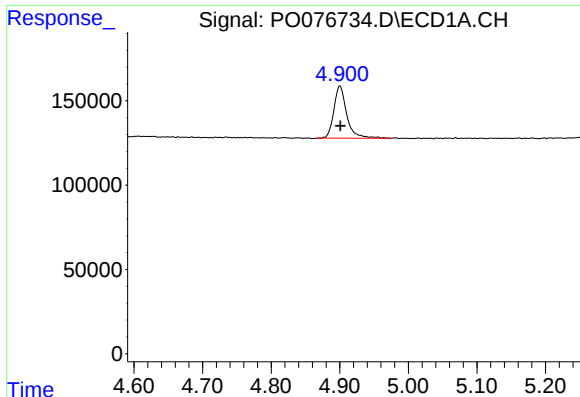


#1 Tetrachloro-m-xylene

R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 404454
Conc: 4.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/2/2021 11:28:16 AM

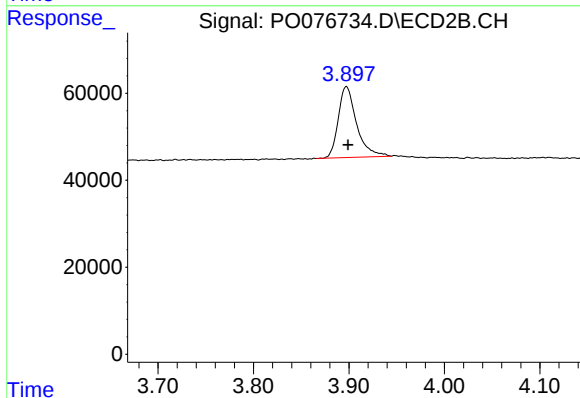


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: -0.001 min
Response: 217568
Conc: 4.73 ng/ml

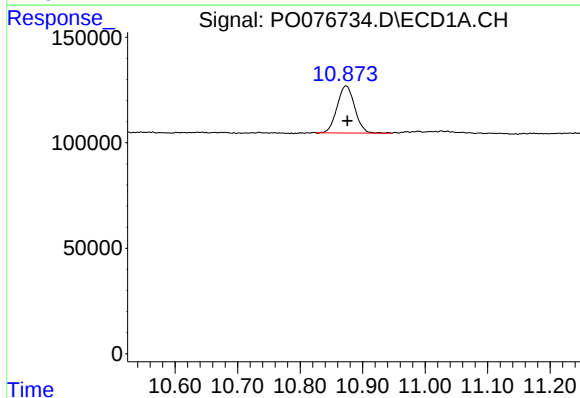


#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 439281
Conc: 4.98 ng/ml

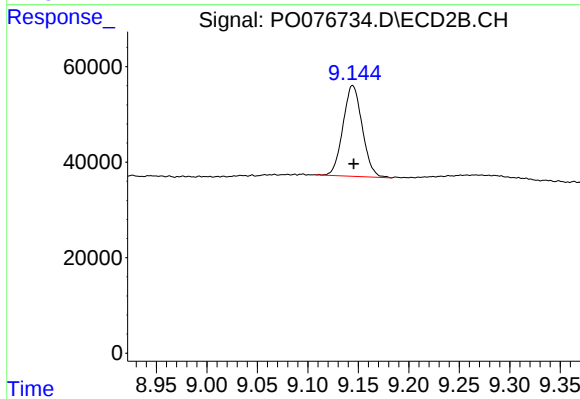

#2 Decachlorobiphenyl

R.T.: 9.144 min
Delta R.T.: -0.001 min
Response: 252026
Conc: 5.51 ng/ml

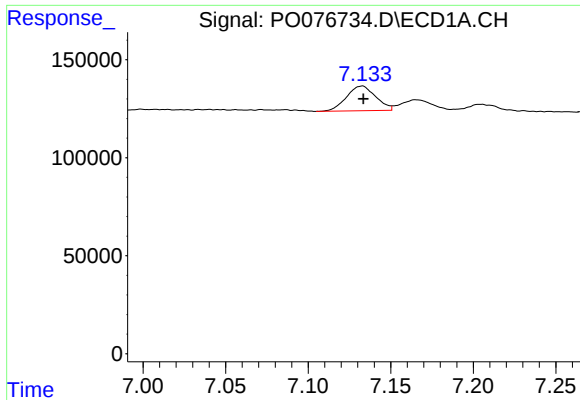


#26 AR-1254-1

R.T.: 7.133 min
Delta R.T.: 0.000 min
Response: 155367
Conc: 48.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/2/2021 11:28:16 AM

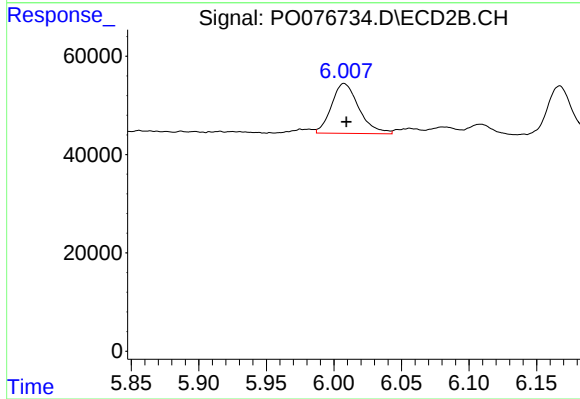


#26 AR-1254-1

R.T.: 6.007 min
Delta R.T.: -0.002 min
Response: 143576
Conc: 55.51 ng/ml m

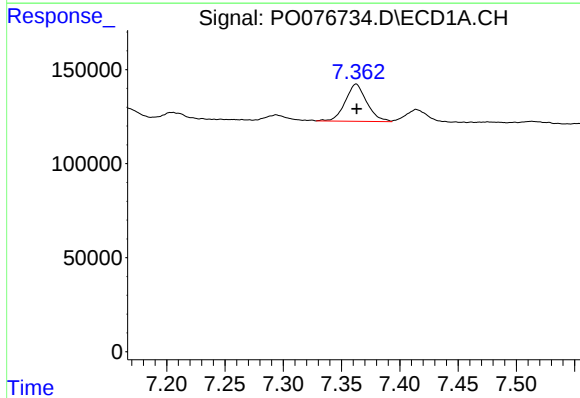


#27 AR-1254-2

R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 254345
Conc: 49.18 ng/ml

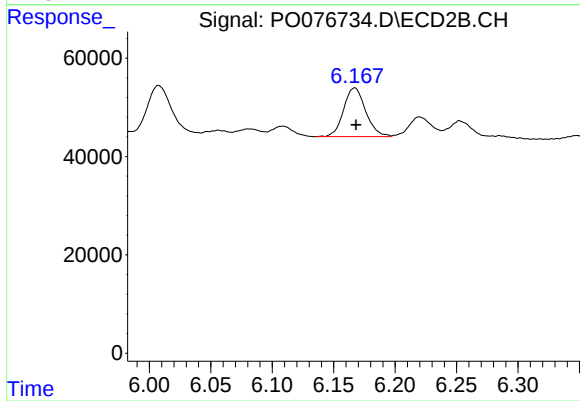

#27 AR-1254-2

R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 123970
Conc: 54.58 ng/ml

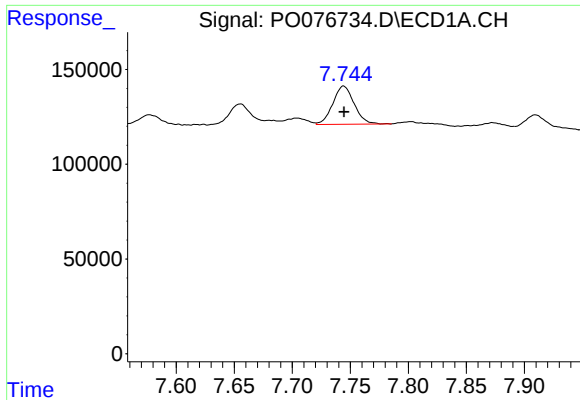


#28 AR-1254-3

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 258044
Conc: 45.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/2/2021 11:28:16 AM

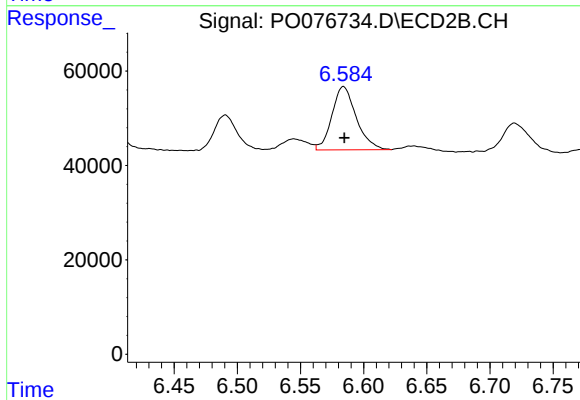


#28 AR-1254-3

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 179881
Conc: 50.53 ng/ml

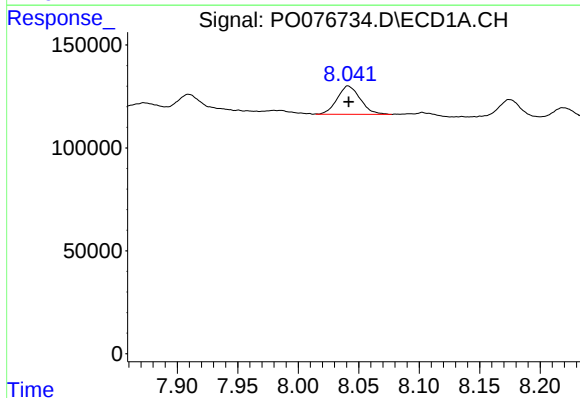


#29 AR-1254-4

R.T.: 8.041 min
Delta R.T.: 0.000 min
Response: 183530
Conc: 45.54 ng/ml

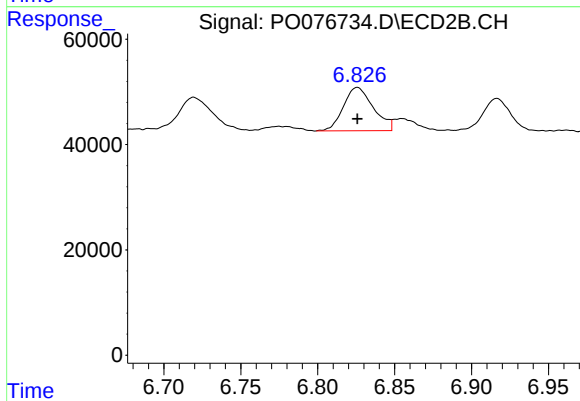

#29 AR-1254-4

R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 111338
Conc: 52.92 ng/ml

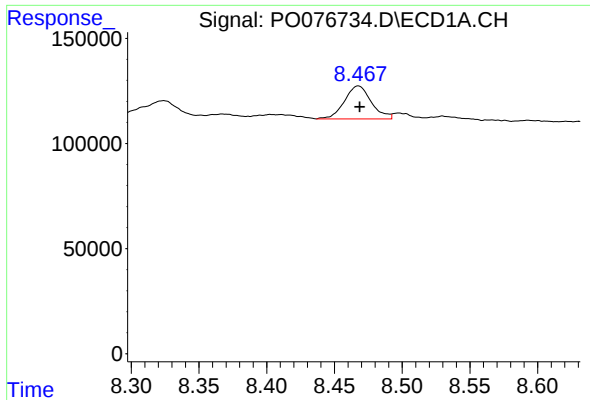


#30 AR-1254-5

R.T.: 8.467 min
Delta R.T.: -0.001 min
Response: 218027
Conc: 49.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
4/2/2021 11:28:16 AM

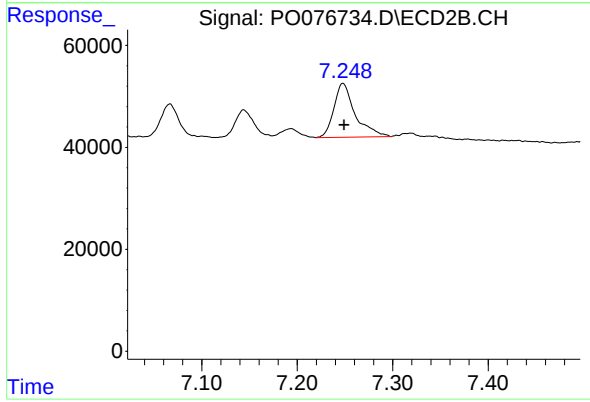

#30 AR-1254-5

R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 164229
Conc: 50.34 ng/ml