

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
 Data File : P0085813.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2022 14:48
 Operator : YP\AJ
 Sample : N2205-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-032322-SR-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 09:09:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.483	3.580	511424	117506	2.624	2.485
2) SA Decachlor...	10.391	8.602	344541	96292	2.685	2.743

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040122\
Data File : PO085813.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2022 14:48
Operator : YP\AJ
Sample : N2205-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 09:09:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

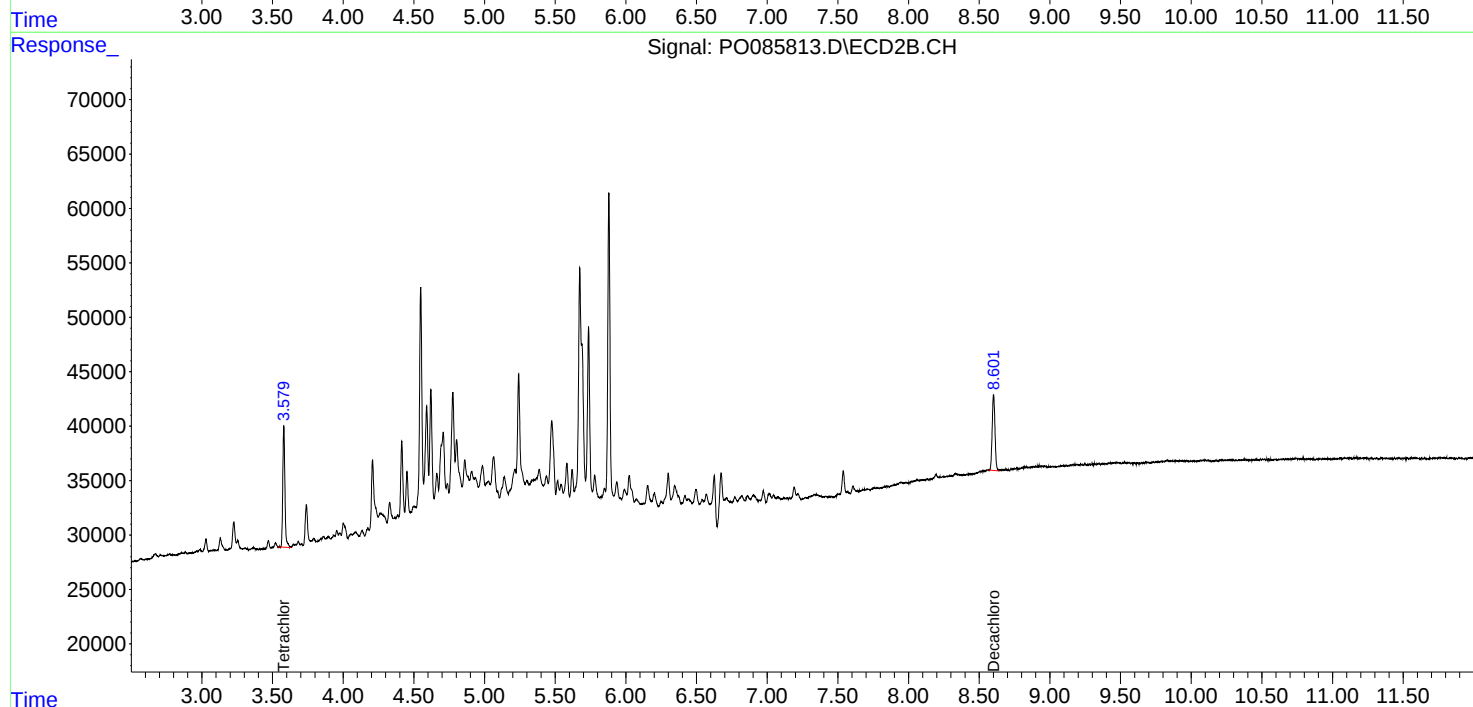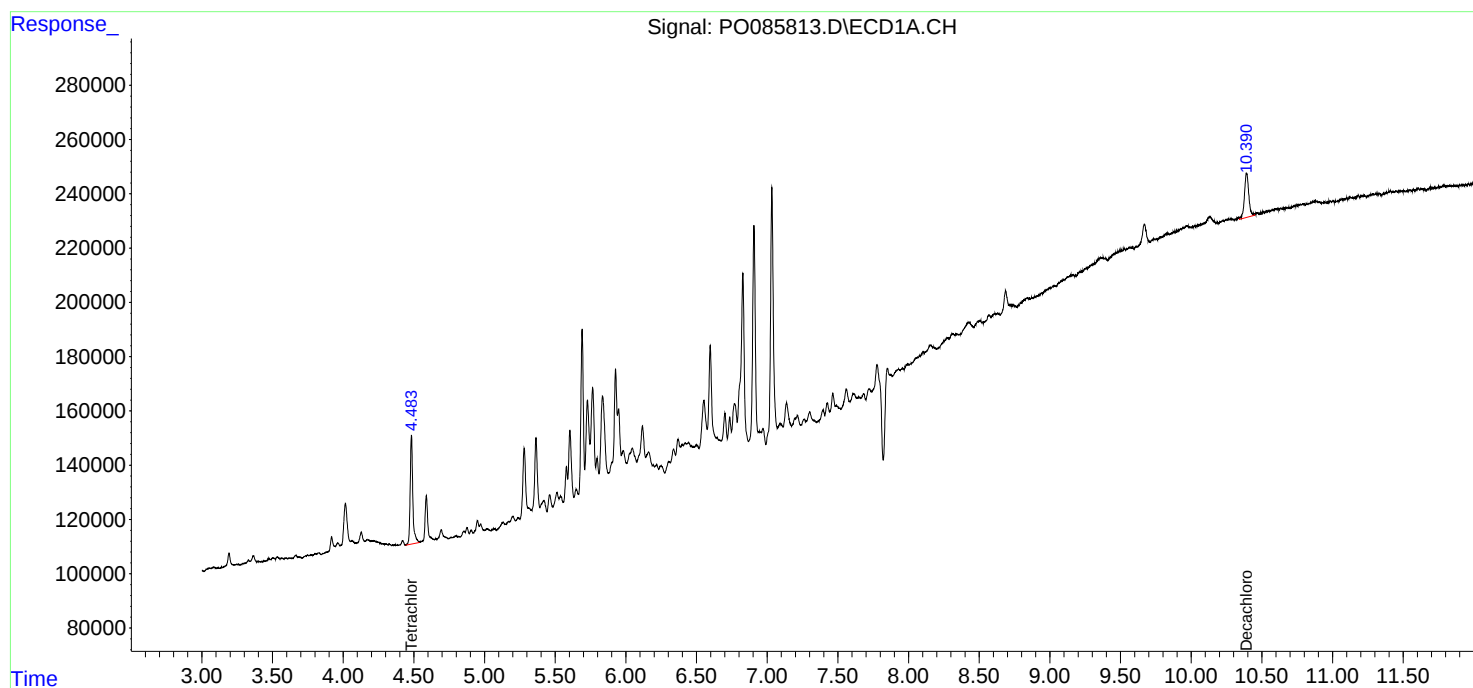


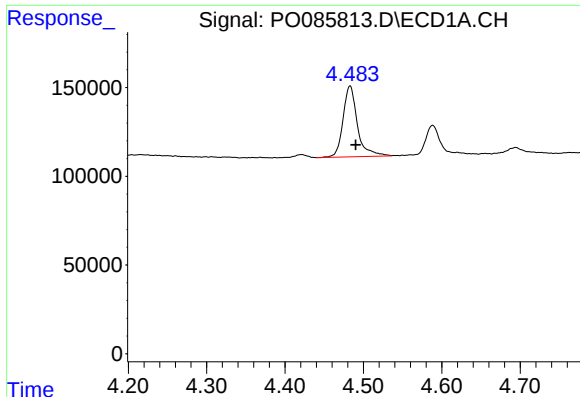

#1 Tetrachloro-m-xylene


R.T.: 4.483 min
Delta R.T.: -0.007 min
Response: 511424
Conc: 2.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-01

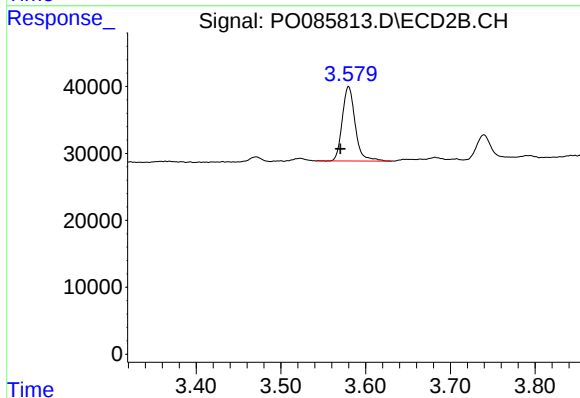


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.010 min
Response: 117506
Conc: 2.48 ng/ml

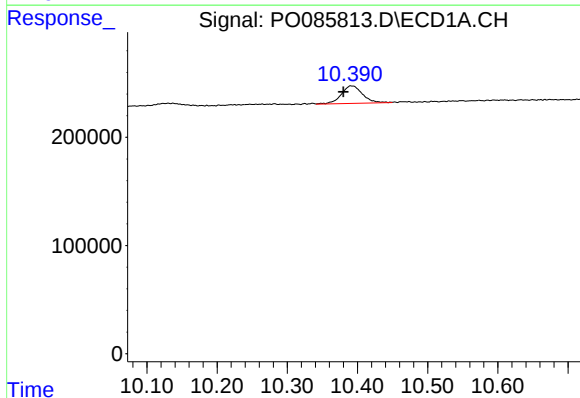

#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.011 min
Response: 344541
Conc: 2.69 ng/ml

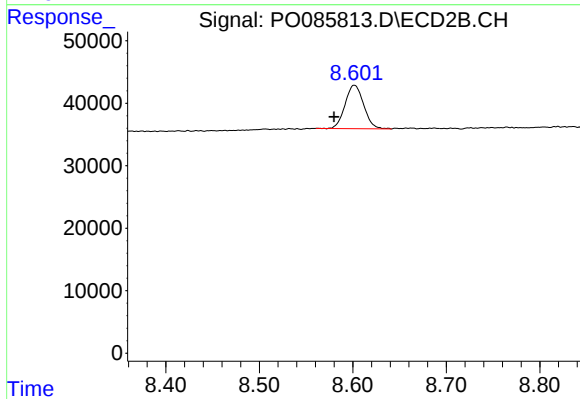

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: 0.022 min
Response: 96292
Conc: 2.74 ng/ml