

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
 Data File : P0085814.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2022 15:04
 Operator : YP\AJ
 Sample : N2205-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-032322-SR-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 09:12:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.472	3.570	540234	125120	2.772	2.646
2) SA Decachlor...	10.388	8.597	339253	94083	2.644	2.680

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040122\
Data File : PO085814.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2022 15:04
Operator : YP\AJ
Sample : N2205-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 09:12:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

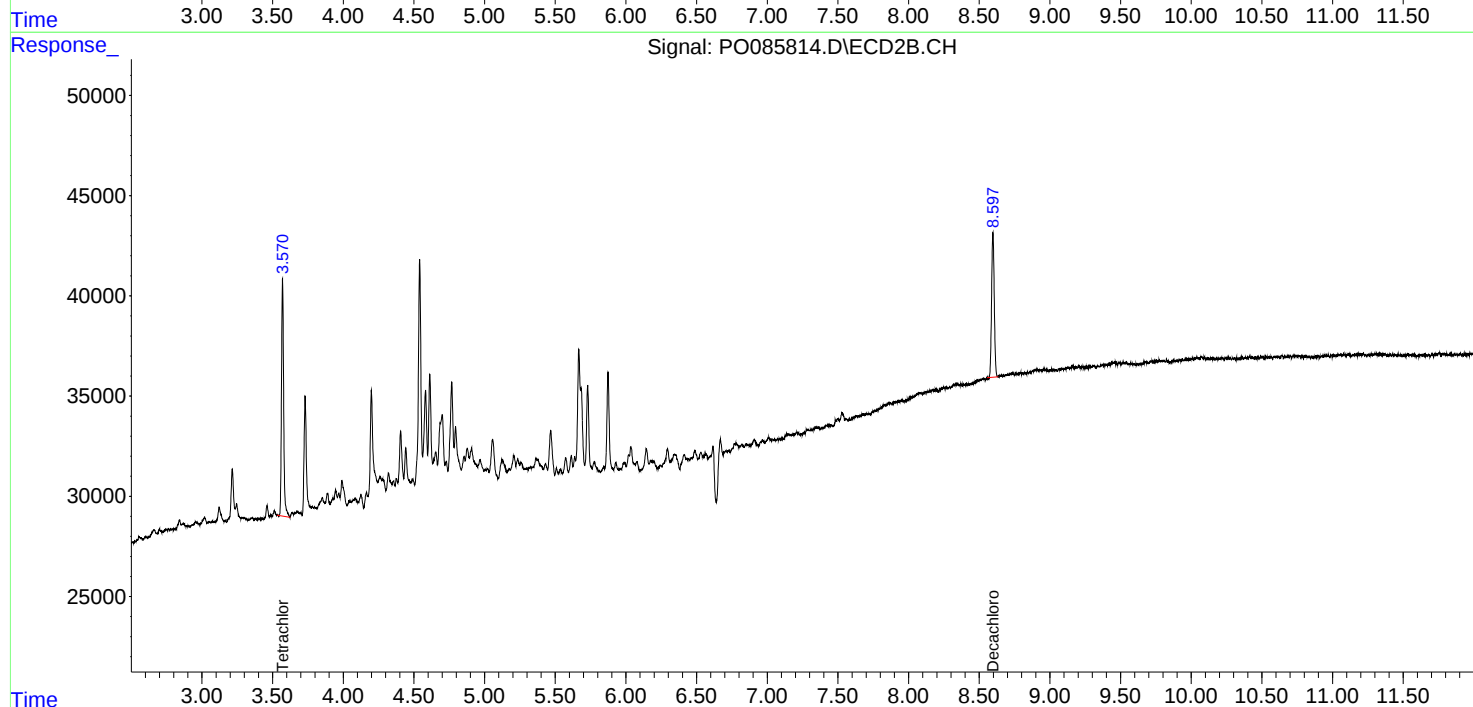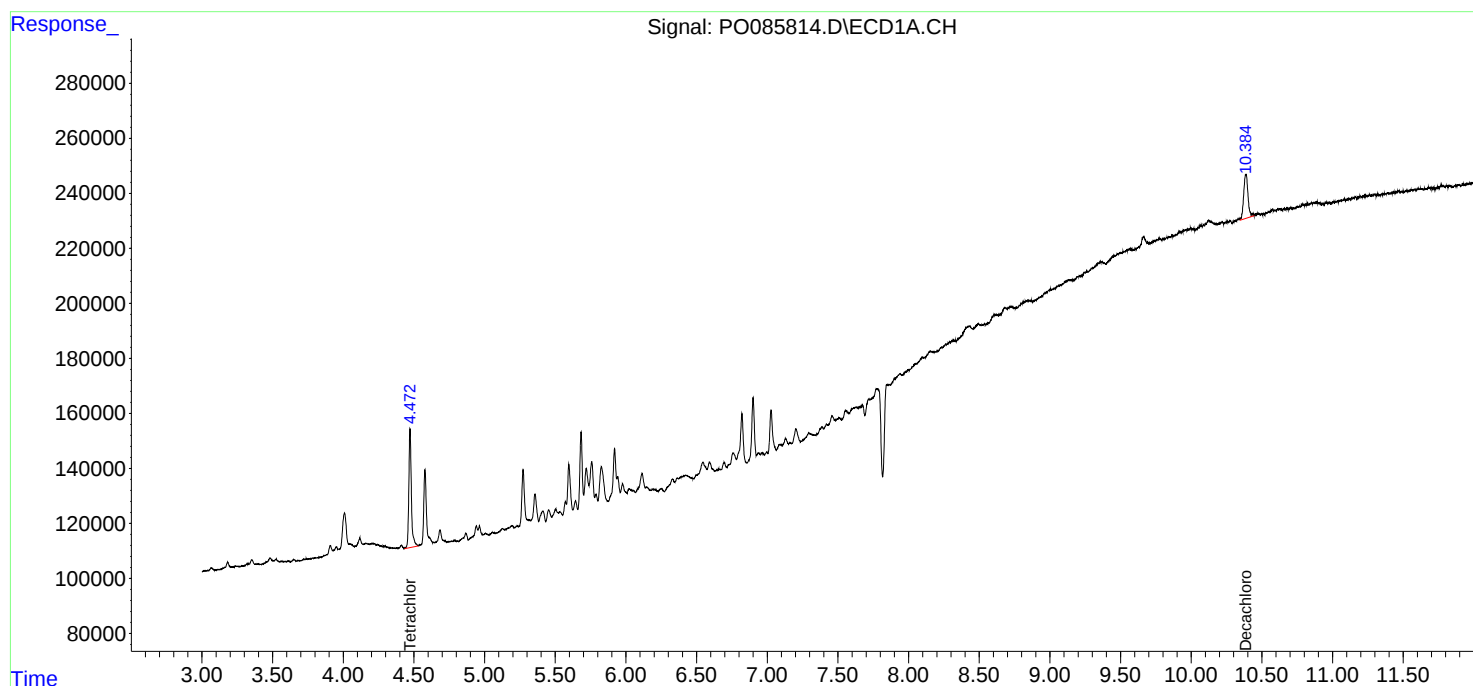


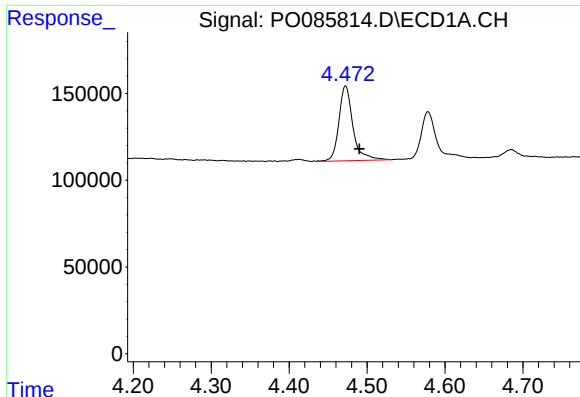

#1 Tetrachloro-m-xylene


R.T.: 4.472 min
Delta R.T.: -0.018 min
Response: 540234
Conc: 2.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-02

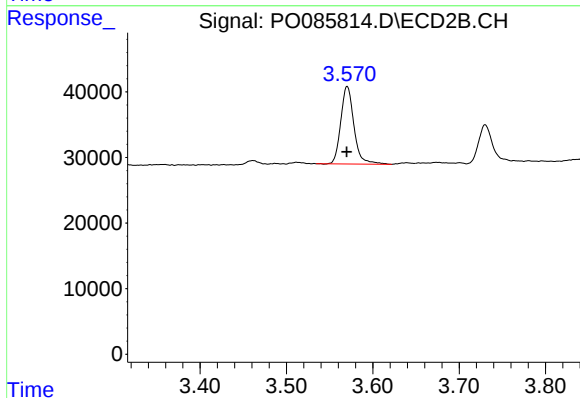


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 125120
Conc: 2.65 ng/ml

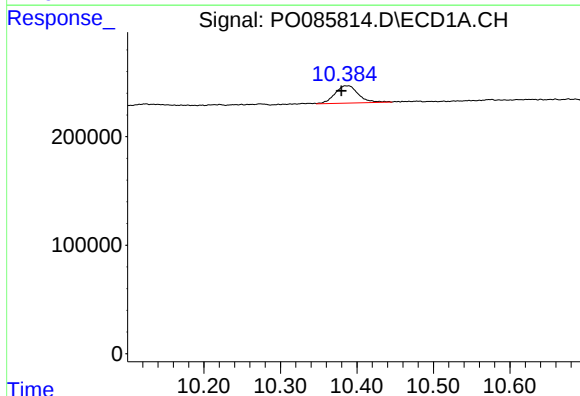

#2 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.008 min
Response: 339253
Conc: 2.64 ng/ml

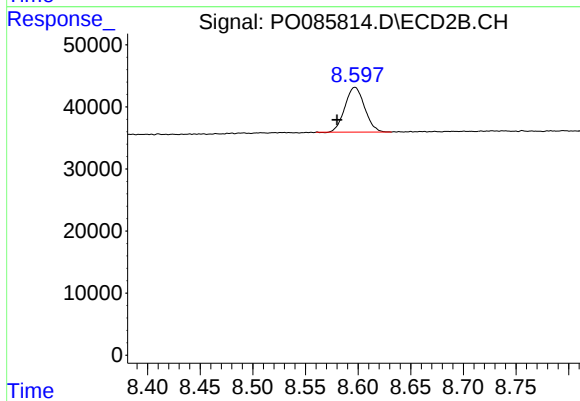

#2 Decachlorobiphenyl

R.T.: 8.597 min
Delta R.T.: 0.017 min
Response: 94083
Conc: 2.68 ng/ml