

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
 Data File : P0085818.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2022 16:08
 Operator : YP\AJ
 Sample : N2205-06 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-032322-SR-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 16:21:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.449	3.571	1553	124544	0.008	2.633 #
2)	SA Decachlor...	10.387	8.600	479203	98321	3.734	2.800 #
Target Compounds							
3)	L1 AR-1016-1	5.647	4.682	16727	858	2.505	0.479 #
4)	L1 AR-1016-2	5.686	4.682	35020	858	3.464	0.338 #
5)	L1 AR-1016-3	5.727	0.000	7499	0	1.237	N.D. #
6)	L1 AR-1016-4	5.833	0.000	2068	0	0.424	N.D. #
7)	L1 AR-1016-5	6.134	5.113	1298	389	0.286	0.287
8)	L2 AR-1221-1	4.684	0.000	41107	0	18.255	N.D. #
9)	L2 AR-1221-2	4.770	0.000	38398	0	20.733	N.D. #
10)	L2 AR-1221-3	4.875	3.961	172897	11888	31.835	8.384 #
11)	L3 AR-1232-1	4.875f	3.961	172897	11888	33.853	8.557 #
12)	L3 AR-1232-2	5.379	4.682	69935	858	26.698	0.661 #
13)	L3 AR-1232-3	5.686	0.000	35020	0	7.065	N.D. #
14)	L3 AR-1232-4	5.833	0.000	2068	0	0.842	N.D. #
15)	L3 AR-1232-5	5.928	5.113	3200	389	1.626	0.514 #
16)	L4 AR-1242-1	5.647	4.682	16727	858	3.107	0.608 #
17)	L4 AR-1242-2	5.686	4.682	35020	858	4.314	0.440 #
18)	L4 AR-1242-3	5.727	0.000	7499	0	1.495	N.D. #
19)	L4 AR-1242-4	5.833	0.000	2068	0	0.523	N.D. #
20)	L4 AR-1242-5	6.588	0.000	4918	0	1.103	N.D. #
21)	L5 AR-1248-1	5.658	4.682	21301	858	5.642	0.899 #
22)	L5 AR-1248-2	5.946	0.000	1973	0	0.371	N.D. #
23)	L5 AR-1248-3	6.148	0.000	3301	0	0.555	N.D. #
24)	L5 AR-1248-4	6.537	5.113	1615	389	0.319	0.229 #
25)	L5 AR-1248-5	6.597	0.000	4283	0	0.677	N.D. #
26)	L6 AR-1254-1	6.537	0.000	1615	0	0.232	N.D. #
27)	L6 AR-1254-2	6.769	0.000	41810	0	3.904	N.D. #
28)	L6 AR-1254-3	7.134	0.000	4008	0	0.358	N.D. #
29)	L6 AR-1254-4	7.420	0.000	23511	0	2.951	N.D. #
30)	L6 AR-1254-5	7.832	6.673	27097	3977	3.354	1.261 #
31)	L7 AR-1260-1	7.275	0.000	894	0	0.112	N.D. #
32)	L7 AR-1260-2	7.549	6.345	16351	4069	1.743	1.338
33)	L7 AR-1260-3	7.914	0.000	119860	0	16.988	N.D. #
34)	L7 AR-1260-4	8.125	7.004f	32678	8110	4.150	3.538
35)	L7 AR-1260-5	8.463	0.000	6335	0	0.412	N.D. #
36)	L8 AR-1262-1	7.914	6.755	119860	1579	10.983	1.070 #
37)	L8 AR-1262-2	8.463	7.004f	6335	8110	0.334	2.789 #
38)	L8 AR-1262-3	8.775	7.533f	3803	9436	0.335	1.840 #
39)	L8 AR-1262-4	8.886	7.533	17208	9436	3.156	1.864 #
40)	L8 AR-1262-5	9.562	0.000	5095	0	0.820	N.D. #
41)	L9 AR-1268-1	8.775	7.533f	3803	9436	0.185	0.948 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
Data File : P0085818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2022 16:08
Operator : YP\AJ
Sample : N2205-06 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 16:21:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.886	7.533	17208	9436	0.850	1.361 #
43)	L9 AR-1268-3	9.119	0.000	3089	0	0.188	N.D. #
44)	L9 AR-1268-4	9.562	0.000	5095	0	0.724	N.D. #
45)	L9 AR-1268-5	9.991	0.000	8449	0	0.150	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
Data File : P0085818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2022 16:08
Operator : YP\AJ
Sample : N2205-06 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 16:21:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

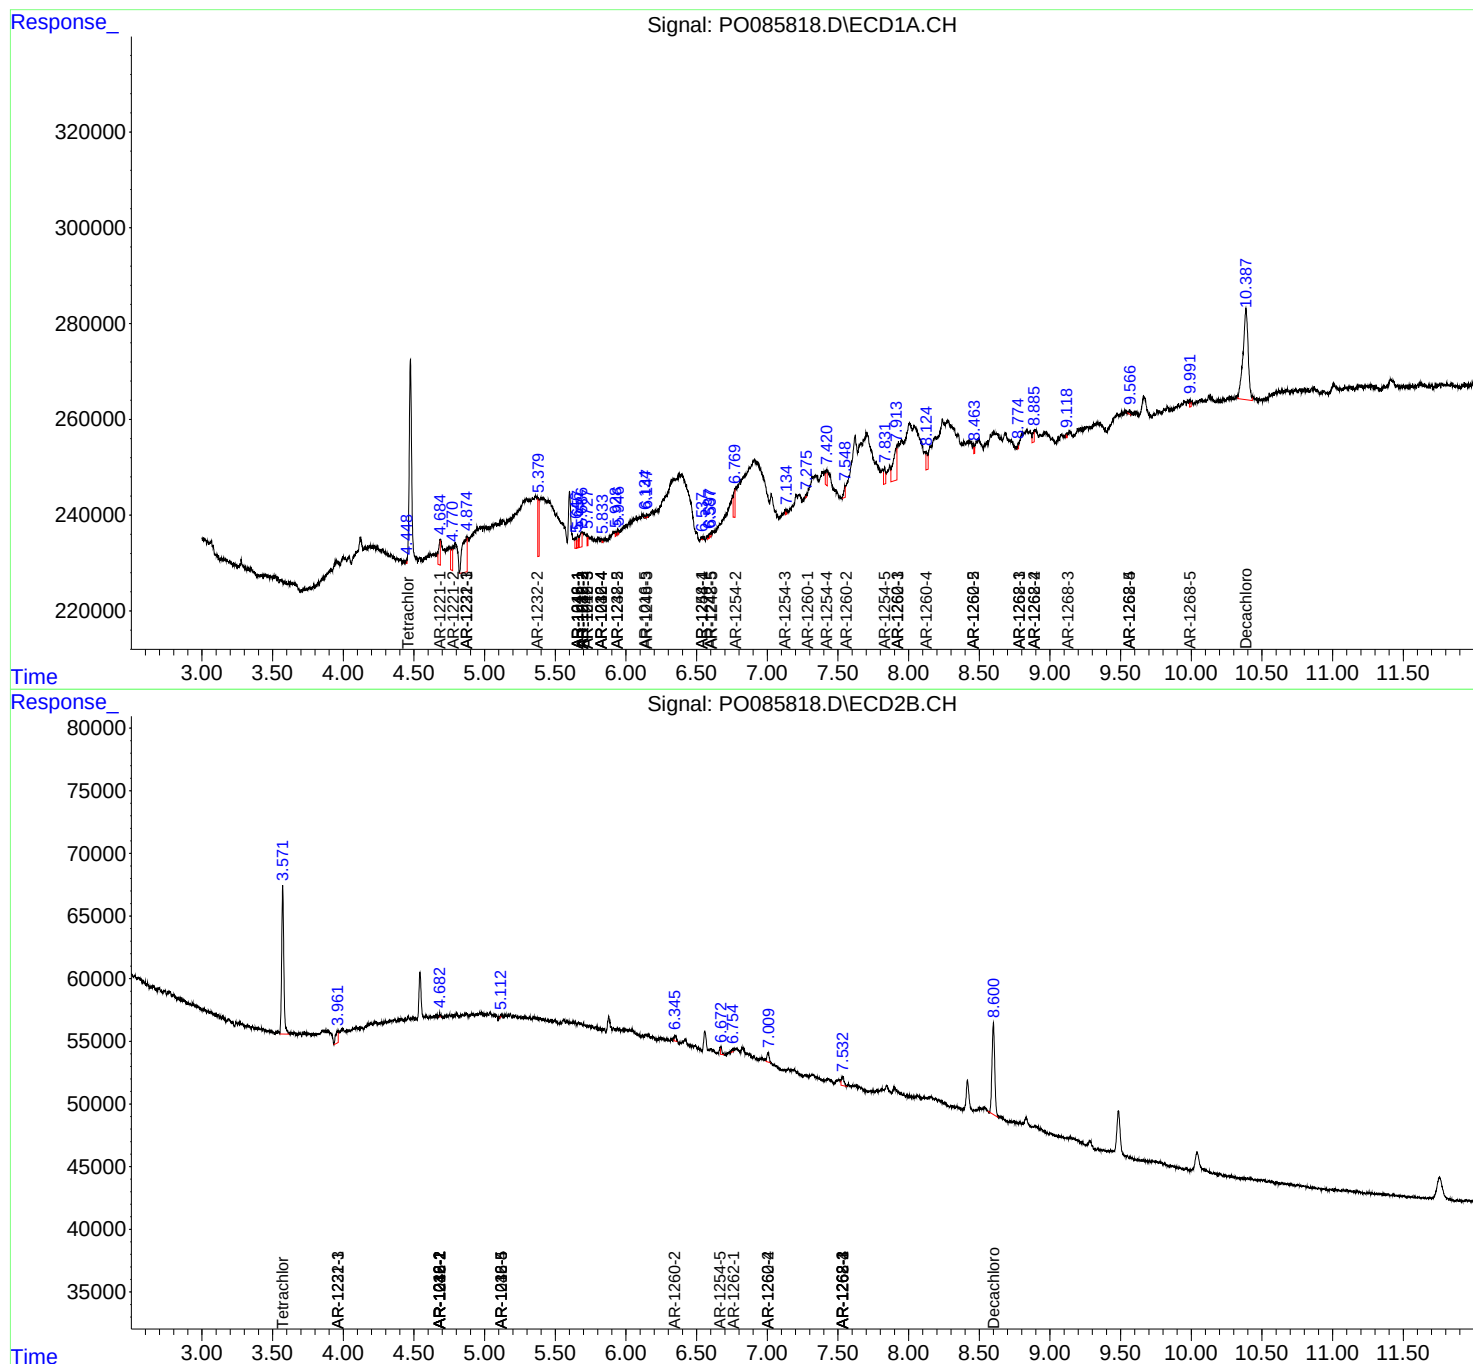


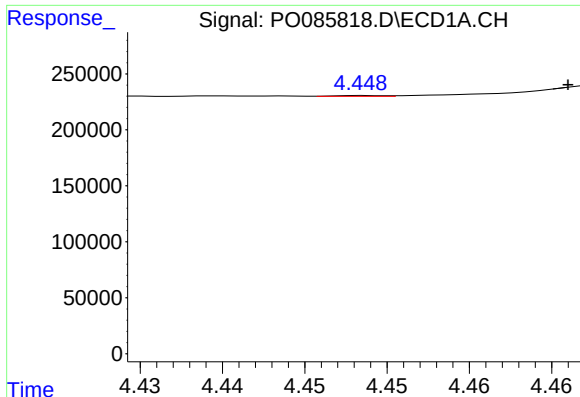

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.012 min
Response: 1553
Conc: 0.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

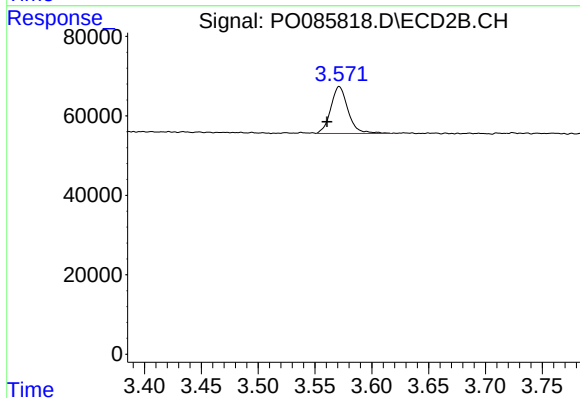


#1 Tetrachloro-m-xylene

R.T.: 3.571 min
Delta R.T.: 0.011 min
Response: 124544
Conc: 2.63 ng/ml

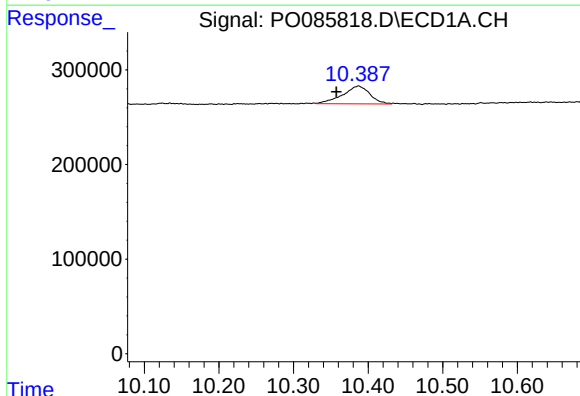


#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.030 min
Response: 479203
Conc: 3.73 ng/ml

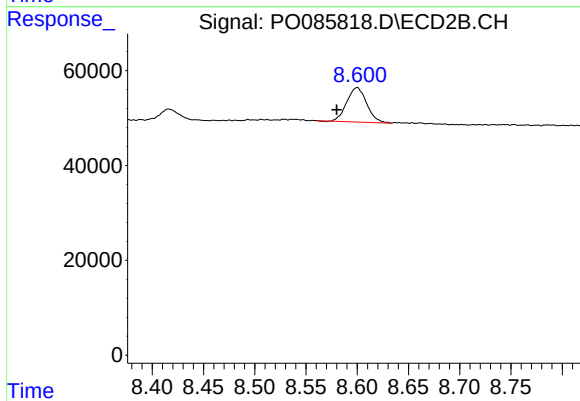

#2 Decachlorobiphenyl


R.T.: 8.600 min
Delta R.T.: 0.020 min
Response: 98321
Conc: 2.80 ng/ml

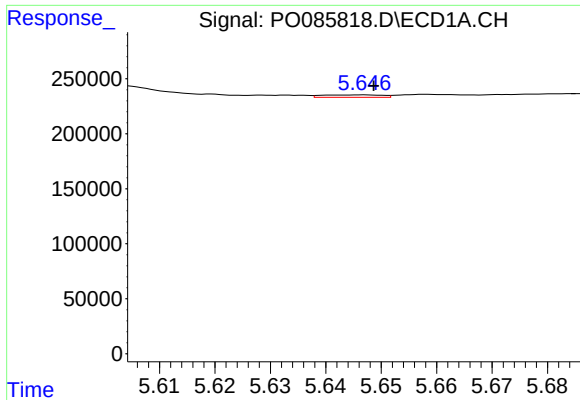

#3 AR-1016-1


R.T.: 5.647 min
Delta R.T.: -0.002 min
Response: 16727
Conc: 2.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

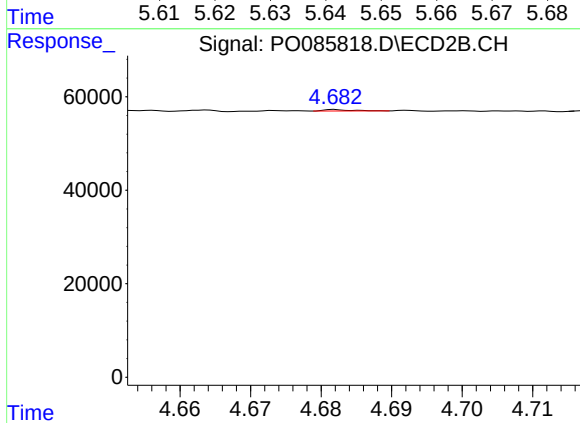


#3 AR-1016-1

R.T.: 4.682 min
Delta R.T.: 0.032 min
Response: 858
Conc: 0.48 ng/ml

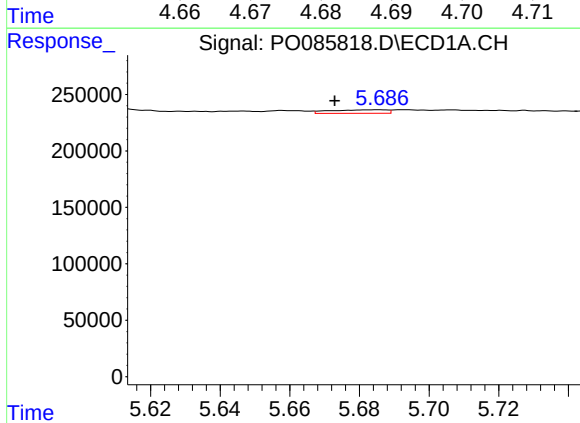


#4 AR-1016-2

R.T.: 5.686 min
Delta R.T.: 0.013 min
Response: 35020
Conc: 3.46 ng/ml

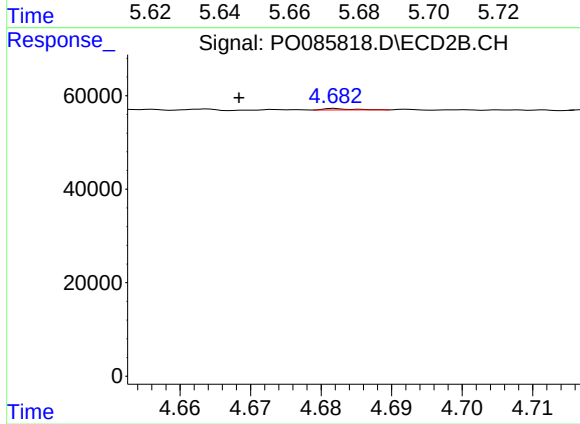

#4 AR-1016-2


R.T.: 4.682 min
Delta R.T.: 0.014 min
Response: 858
Conc: 0.34 ng/ml

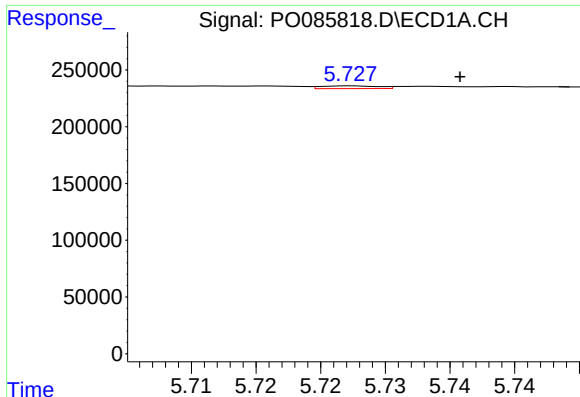

#5 AR-1016-3


R.T.: 5.727 min
Delta R.T.: -0.008 min
Response: 7499
Conc: 1.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

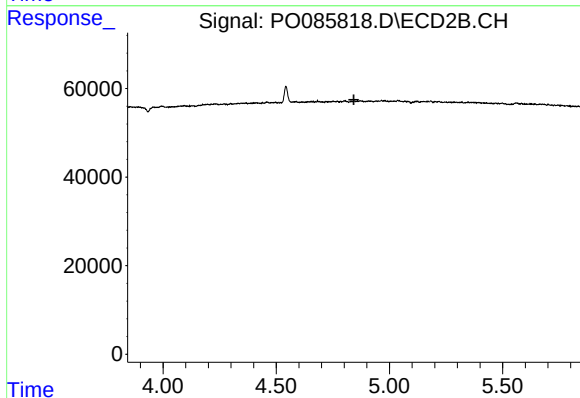


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.843 min
Response: 0
Conc: N.D.

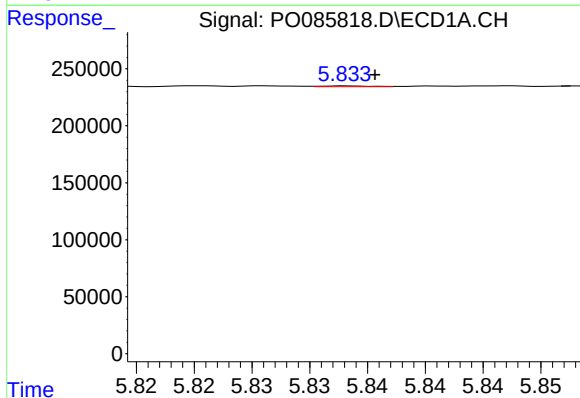


#6 AR-1016-4

R.T.: 5.833 min
Delta R.T.: -0.002 min
Response: 2068
Conc: 0.42 ng/ml

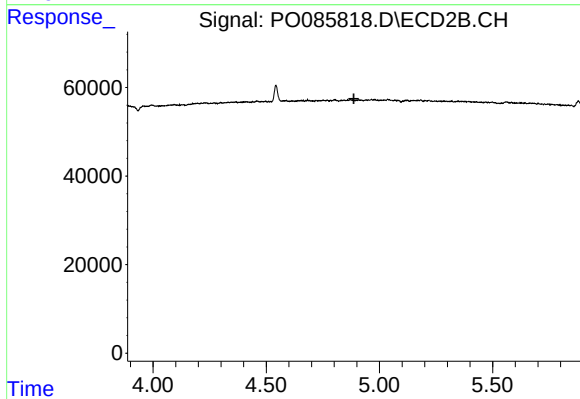

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 4.887 min
Response: 0
Conc: N.D.

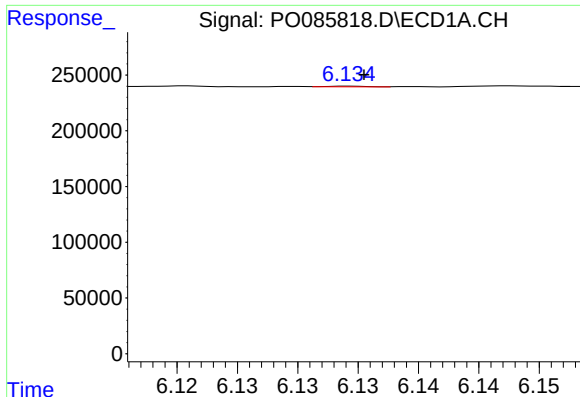

#7 AR-1016-5


R.T.: 6.134 min
Delta R.T.: -0.001 min
Response: 1298
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

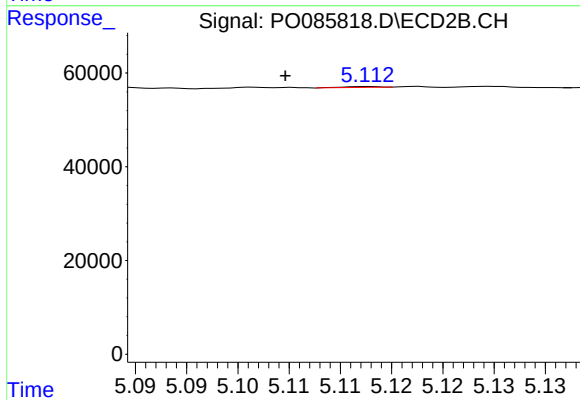


#7 AR-1016-5

R.T.: 5.113 min
Delta R.T.: 0.008 min
Response: 389
Conc: 0.29 ng/ml

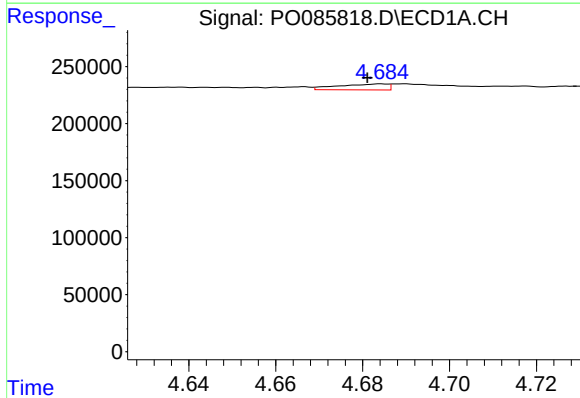


#8 AR-1221-1

R.T.: 4.684 min
Delta R.T.: 0.003 min
Response: 41107
Conc: 18.25 ng/ml

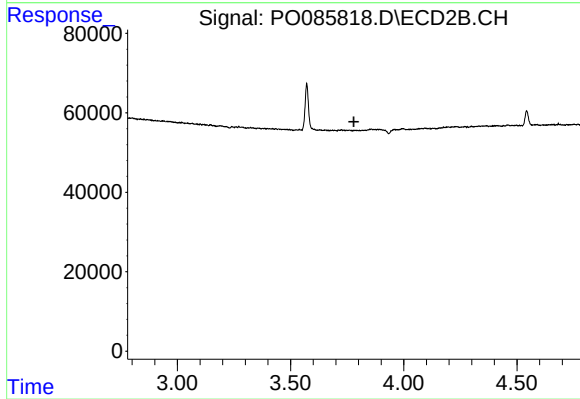

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.780 min
Response: 0
Conc: N.D.

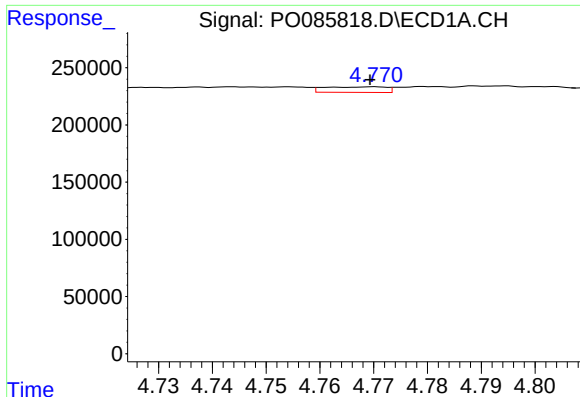

#9 AR-1221-2


R.T.: 4.770 min
Delta R.T.: 0.000 min
Response: 38398
Conc: 20.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

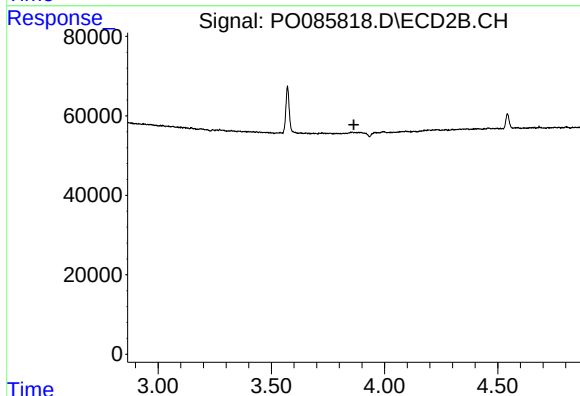


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.865 min
Response: 0
Conc: N.D.

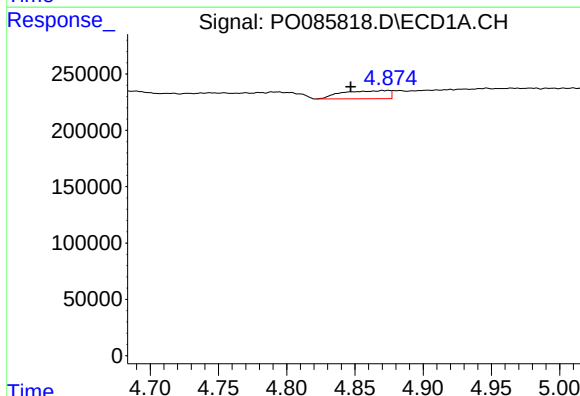


#10 AR-1221-3

R.T.: 4.875 min
Delta R.T.: 0.027 min
Response: 172897
Conc: 31.84 ng/ml

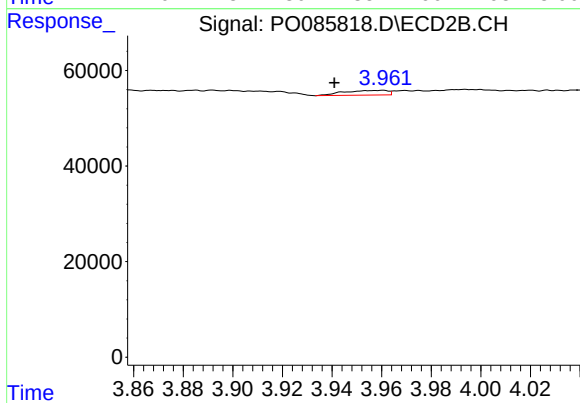

#10 AR-1221-3


R.T.: 3.961 min
Delta R.T.: 0.020 min
Response: 11888
Conc: 8.38 ng/ml

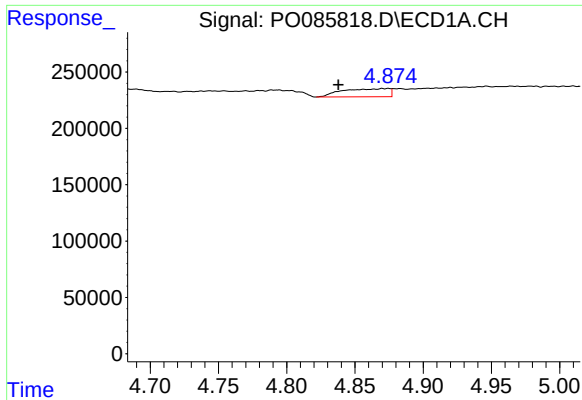

#11 AR-1232-1


R.T.: 4.875 min
Delta R.T.: 0.037 min
Response: 172897
Conc: 33.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

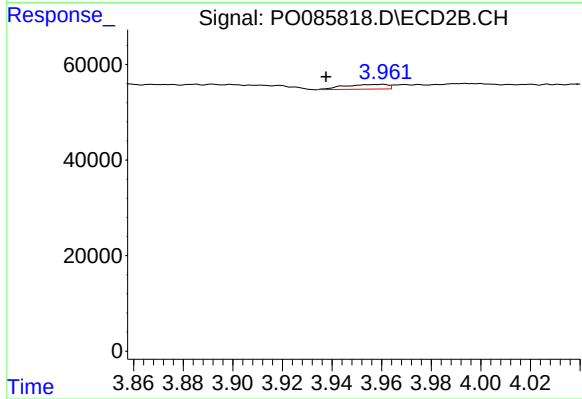


#11 AR-1232-1

R.T.: 3.961 min
Delta R.T.: 0.023 min
Response: 11888
Conc: 8.56 ng/ml

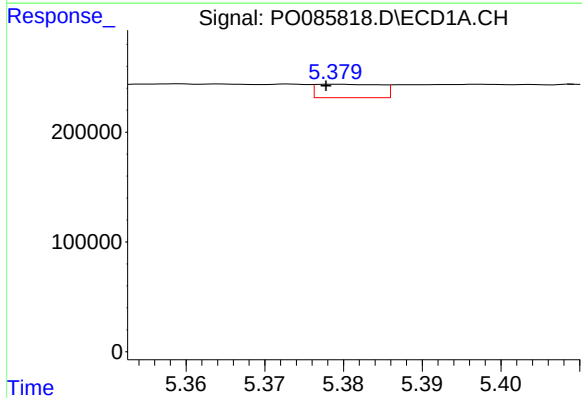


#12 AR-1232-2

R.T.: 5.379 min
Delta R.T.: 0.001 min
Response: 69935
Conc: 26.70 ng/ml

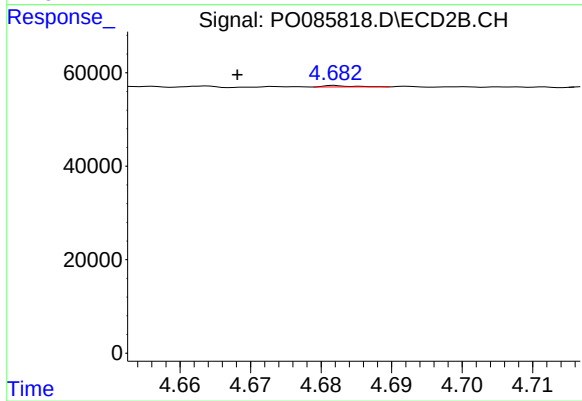

#12 AR-1232-2


R.T.: 4.682 min
Delta R.T.: 0.014 min
Response: 858
Conc: 0.66 ng/ml

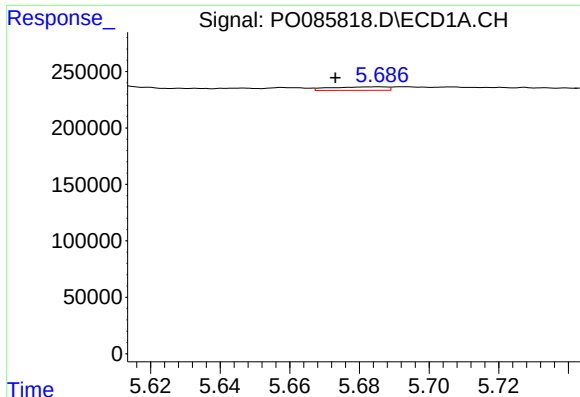

#13 AR-1232-3


R.T.: 5.686 min
Delta R.T.: 0.013 min
Response: 35020
Conc: 7.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

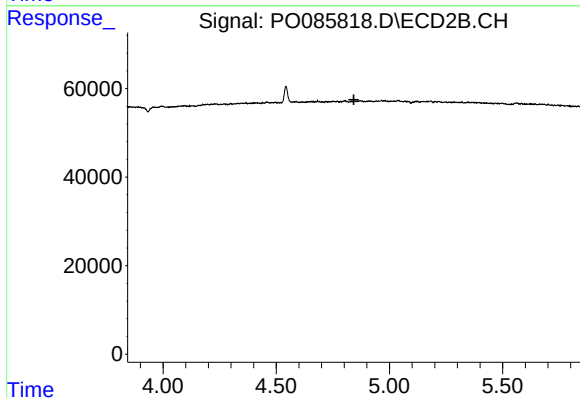


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.843 min
Response: 0
Conc: N.D.

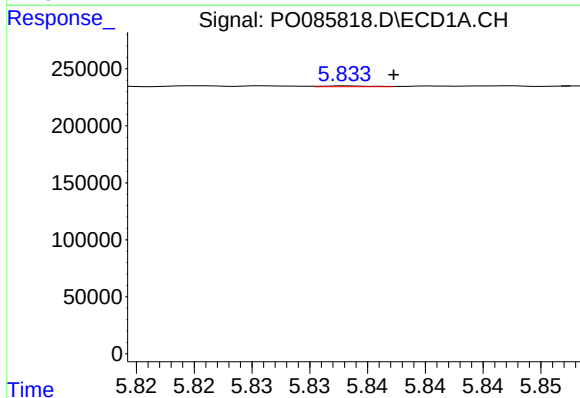


#14 AR-1232-4

R.T.: 5.833 min
Delta R.T.: -0.004 min
Response: 2068
Conc: 0.84 ng/ml

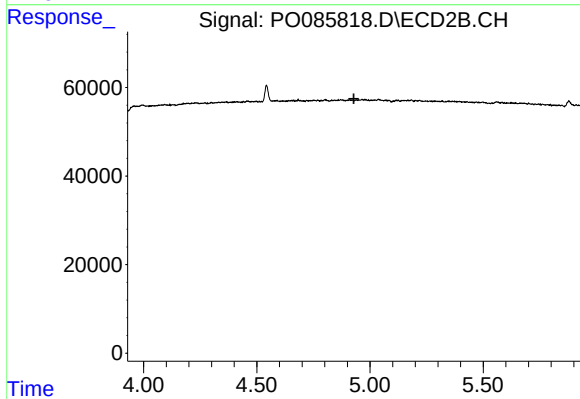

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

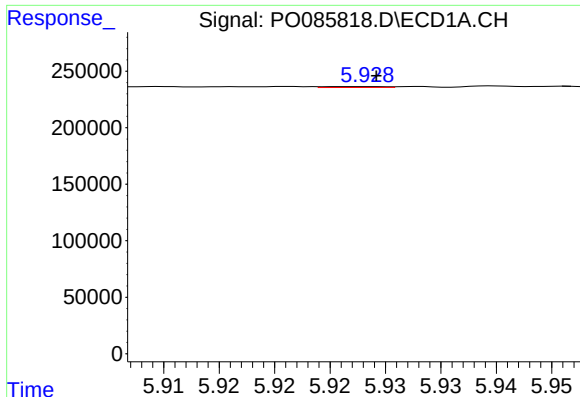

#15 AR-1232-5


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 3200
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

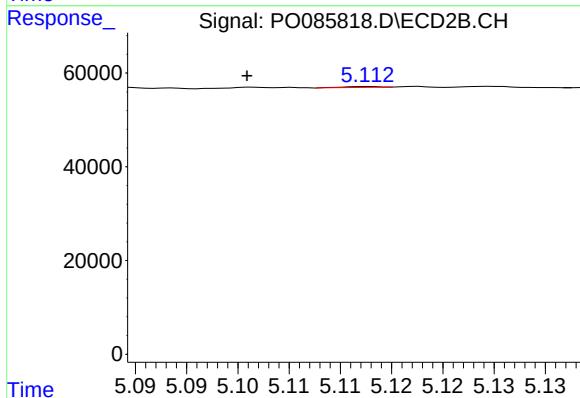


#15 AR-1232-5

R.T.: 5.113 min
Delta R.T.: 0.012 min
Response: 389
Conc: 0.51 ng/ml

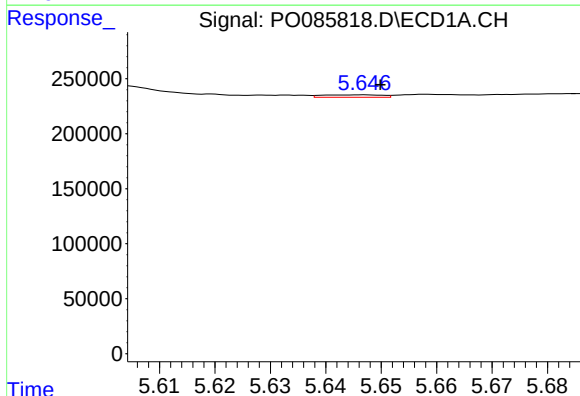


#16 AR-1242-1

R.T.: 5.647 min
Delta R.T.: -0.003 min
Response: 16727
Conc: 3.11 ng/ml

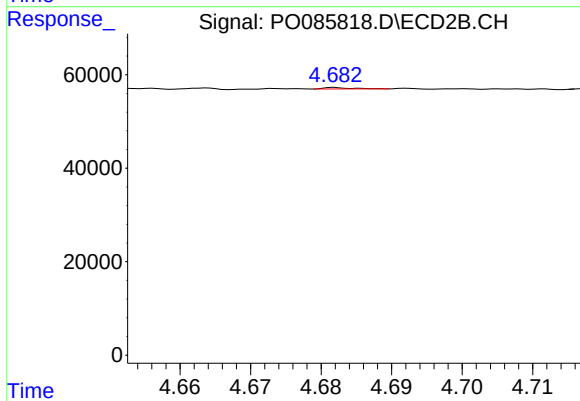

#16 AR-1242-1


R.T.: 4.682 min
Delta R.T.: 0.033 min
Response: 858
Conc: 0.61 ng/ml

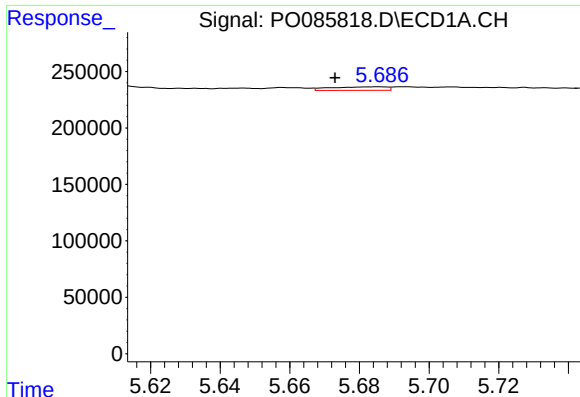

#17 AR-1242-2


R.T.: 5.686 min
Delta R.T.: 0.013 min
Response: 35020
Conc: 4.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

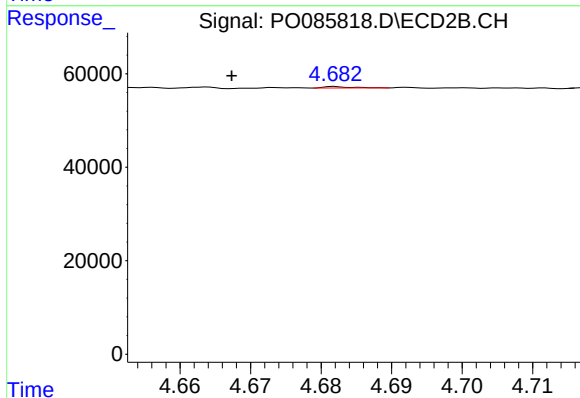


#17 AR-1242-2

R.T.: 4.682 min
Delta R.T.: 0.015 min
Response: 858
Conc: 0.44 ng/ml

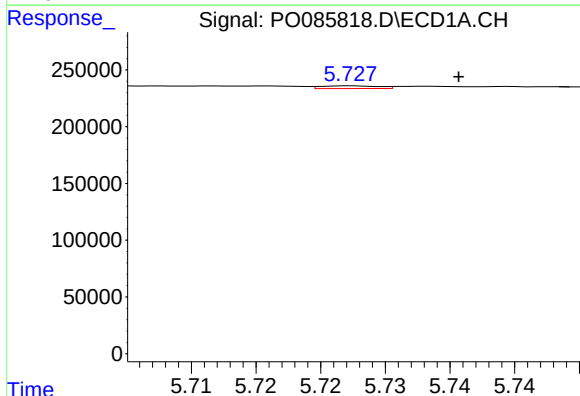


#18 AR-1242-3

R.T.: 5.727 min
Delta R.T.: -0.008 min
Response: 7499
Conc: 1.50 ng/ml

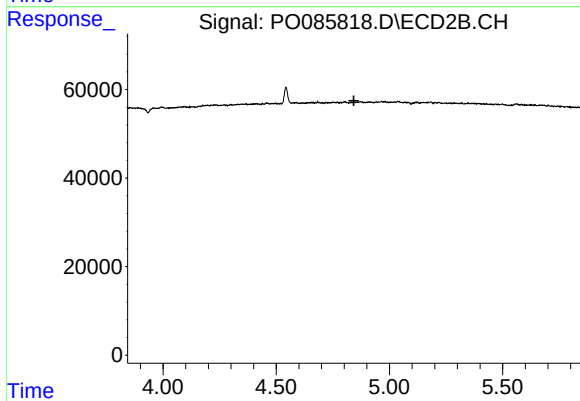

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 4.843 min
Response: 0
Conc: N.D.

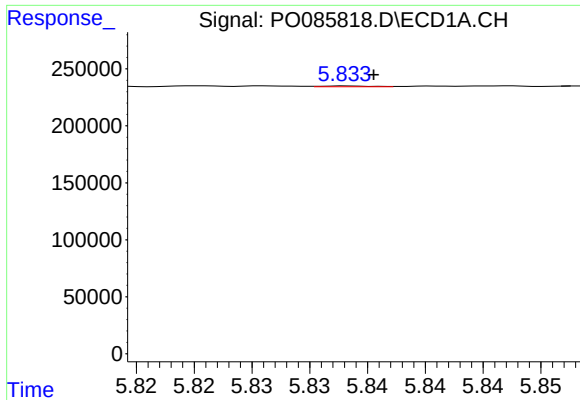

#19 AR-1242-4


R.T.: 5.833 min
Delta R.T.: -0.002 min
Response: 2068
Conc: 0.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

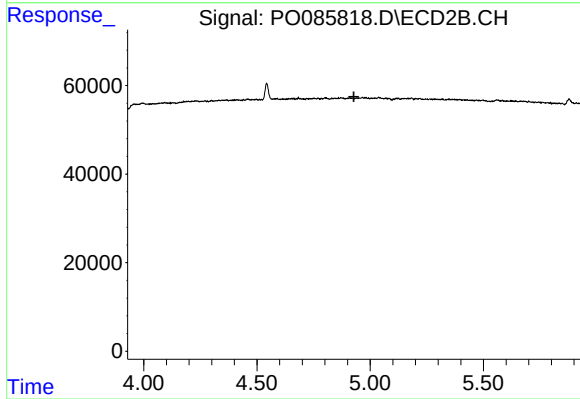


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 4.928 min
Response: 0
Conc: N.D.

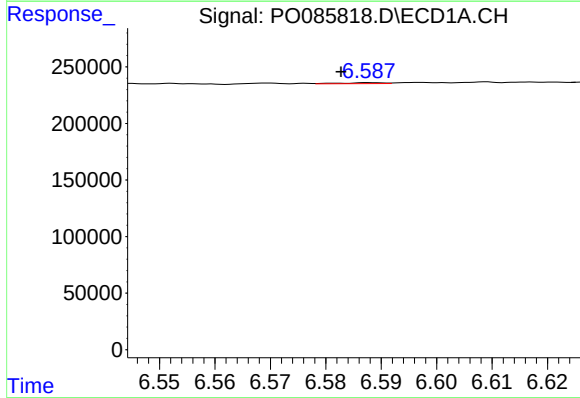


#20 AR-1242-5

R.T.: 6.588 min
Delta R.T.: 0.005 min
Response: 4918
Conc: 1.10 ng/ml

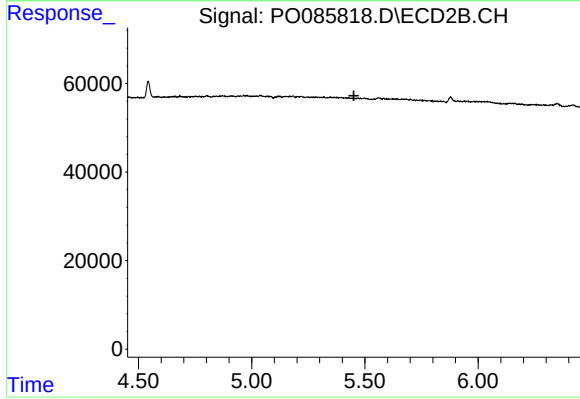

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.452 min
Response: 0
Conc: N.D.

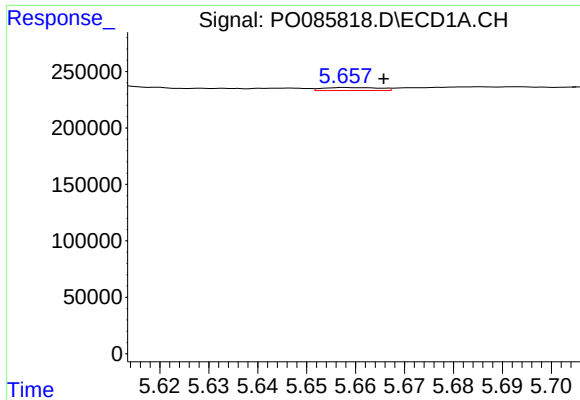

#21 AR-1248-1


R.T.: 5.658 min
Delta R.T.: -0.008 min
Response: 21301
Conc: 5.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

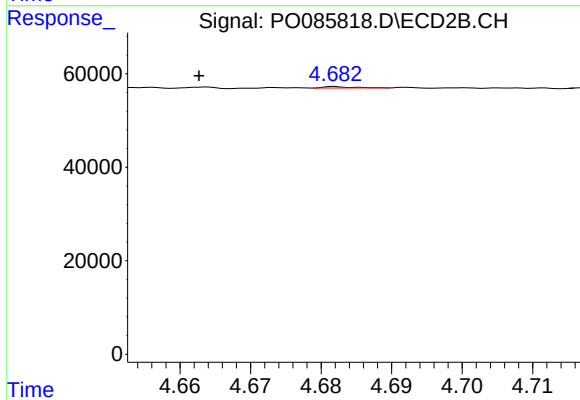


#21 AR-1248-1

R.T.: 4.682 min
Delta R.T.: 0.019 min
Response: 858
Conc: 0.90 ng/ml

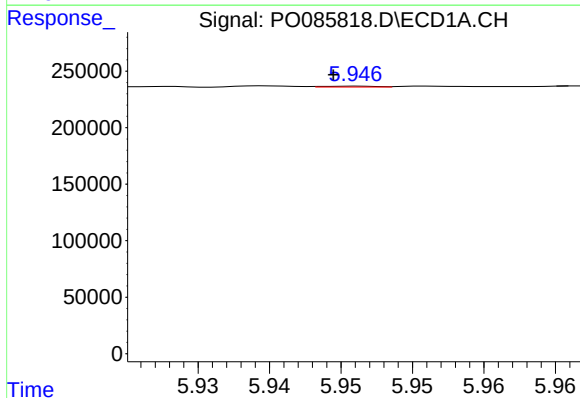


#22 AR-1248-2

R.T.: 5.946 min
Delta R.T.: 0.002 min
Response: 1973
Conc: 0.37 ng/ml

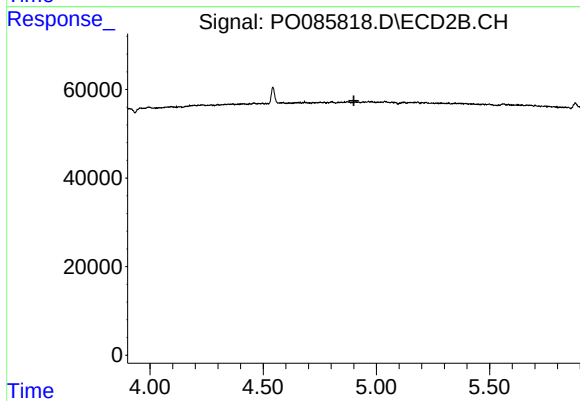

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 4.901 min
Response: 0
Conc: N.D.

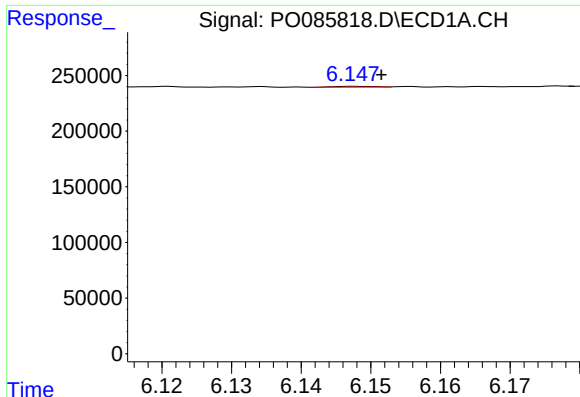

#23 AR-1248-3


R.T.: 6.148 min
Delta R.T.: -0.004 min
Response: 3301
Conc: 0.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

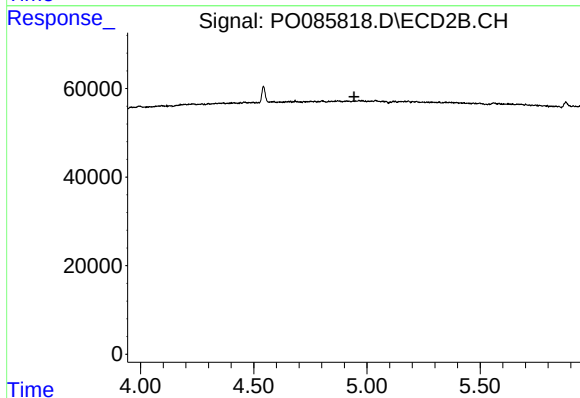


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

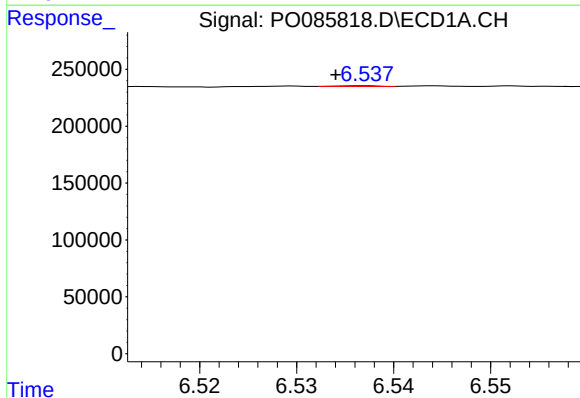


#24 AR-1248-4

R.T.: 6.537 min
Delta R.T.: 0.003 min
Response: 1615
Conc: 0.32 ng/ml

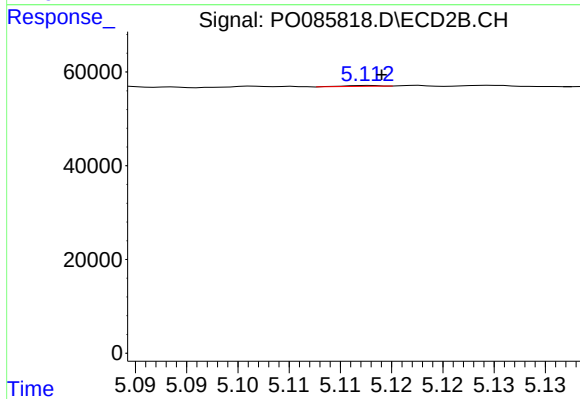

#24 AR-1248-4


R.T.: 5.113 min
Delta R.T.: -0.001 min
Response: 389
Conc: 0.23 ng/ml

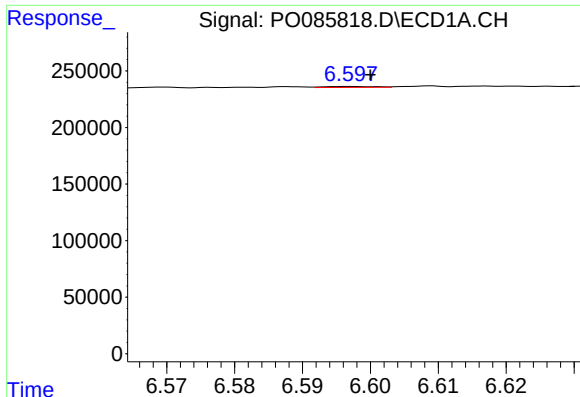

#25 AR-1248-5


R.T.: 6.597 min
Delta R.T.: -0.003 min
Response: 4283
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

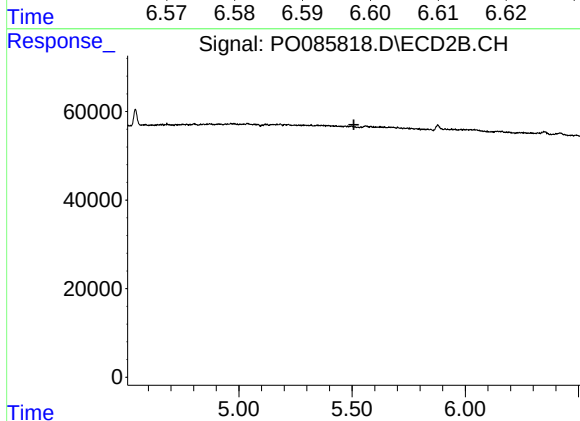


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

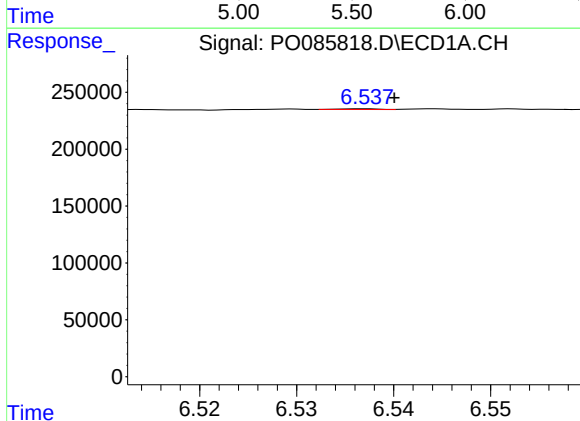


#26 AR-1254-1

R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 1615
Conc: 0.23 ng/ml

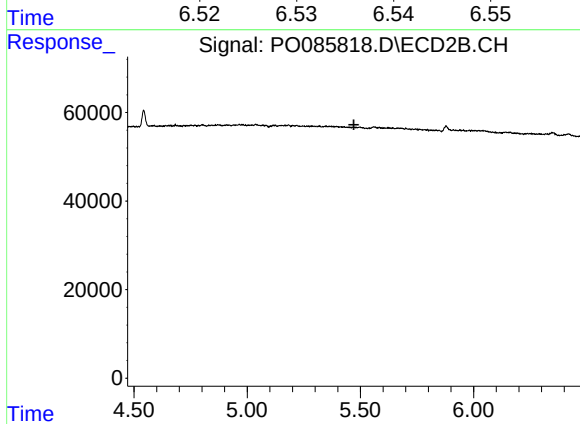

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.471 min
Response: 0
Conc: N.D.

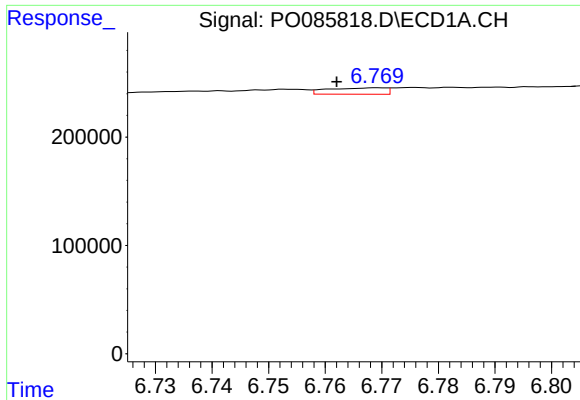

#27 AR-1254-2


R.T.: 6.769 min
Delta R.T.: 0.007 min
Response: 41810
Conc: 3.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

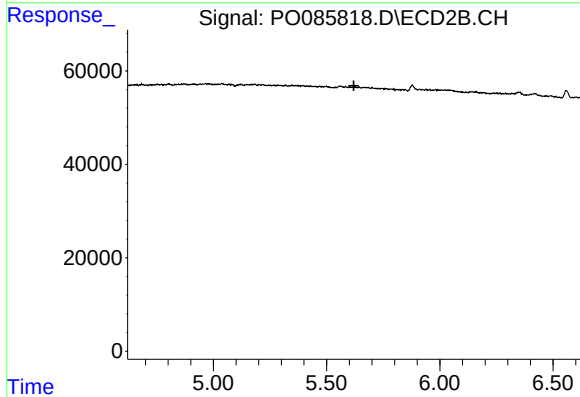


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.621 min
Response: 0
Conc: N.D.

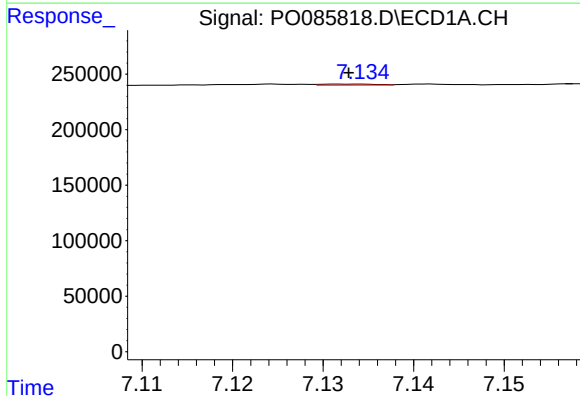


#28 AR-1254-3

R.T.: 7.134 min
Delta R.T.: 0.001 min
Response: 4008
Conc: 0.36 ng/ml

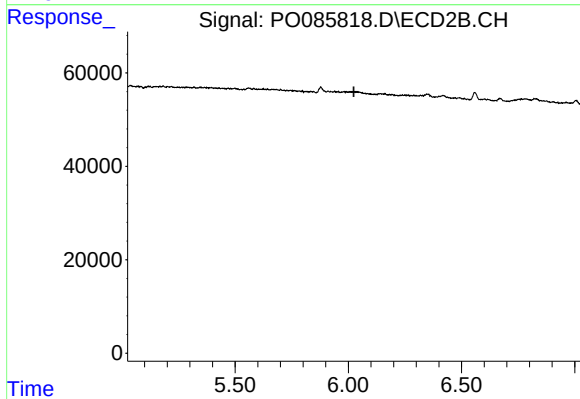

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

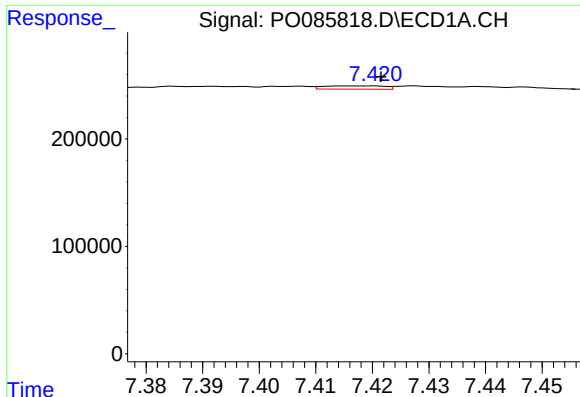

#29 AR-1254-4


R.T.: 7.420 min
Delta R.T.: -0.001 min
Response: 23511
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

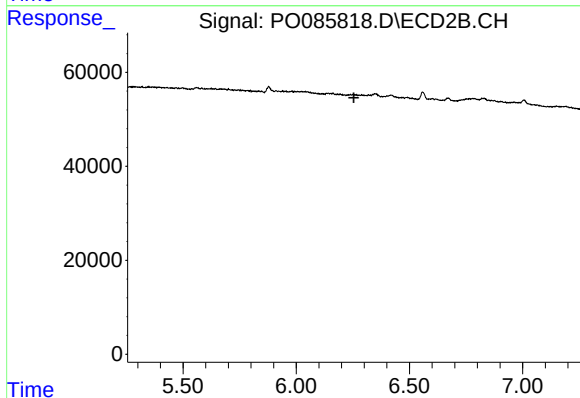


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.255 min
Response: 0
Conc: N.D.

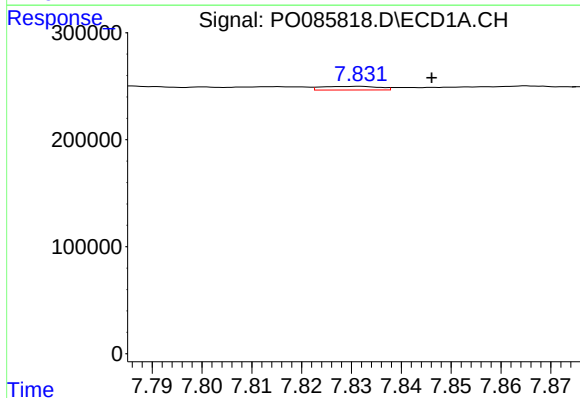


#30 AR-1254-5

R.T.: 7.832 min
Delta R.T.: -0.014 min
Response: 27097
Conc: 3.35 ng/ml

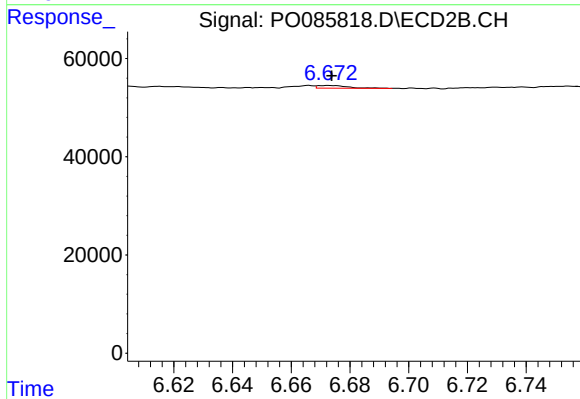

#30 AR-1254-5


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 3977
Conc: 1.26 ng/ml

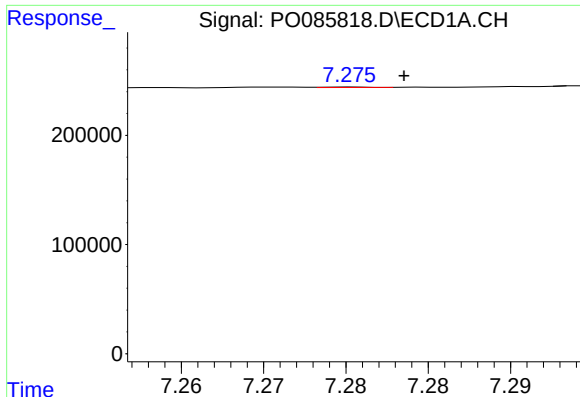

#31 AR-1260-1


R.T.: 7.275 min
Delta R.T.: -0.003 min
Response: 894
Conc: 0.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

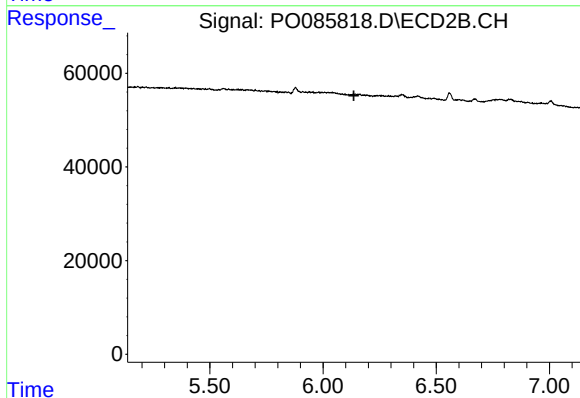


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

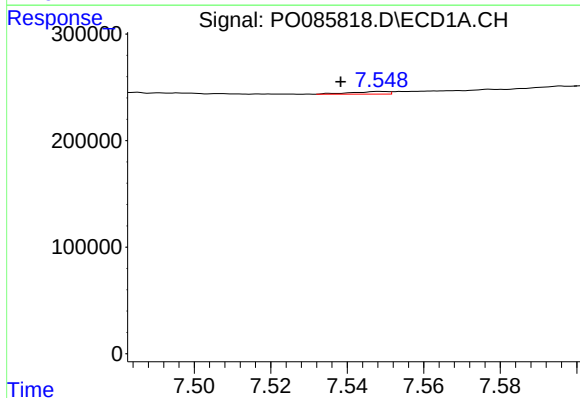


#32 AR-1260-2

R.T.: 7.549 min
Delta R.T.: 0.010 min
Response: 16351
Conc: 1.74 ng/ml

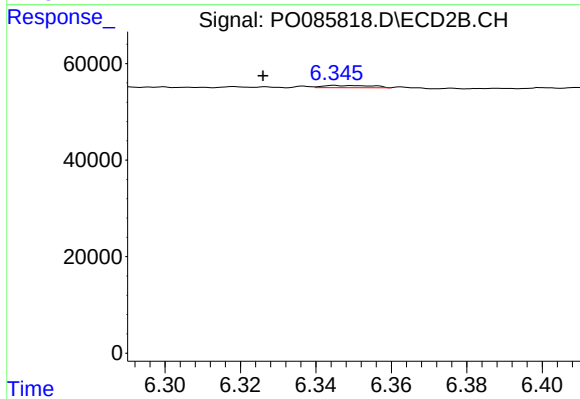

#32 AR-1260-2


R.T.: 6.345 min
Delta R.T.: 0.019 min
Response: 4069
Conc: 1.34 ng/ml

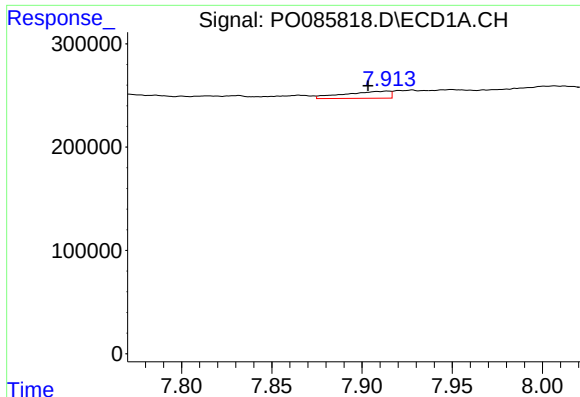

#33 AR-1260-3


R.T.: 7.914 min
Delta R.T.: 0.011 min
Response: 119860
Conc: 16.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

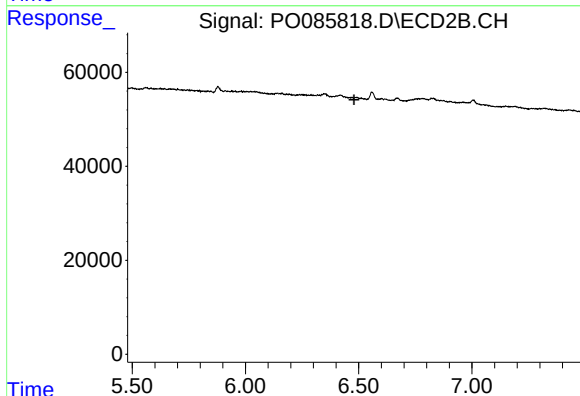


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.479 min
Response: 0
Conc: N.D.

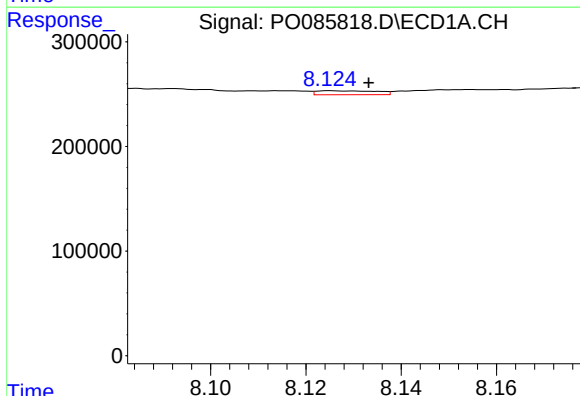


#34 AR-1260-4

R.T.: 8.125 min
Delta R.T.: -0.008 min
Response: 32678
Conc: 4.15 ng/ml

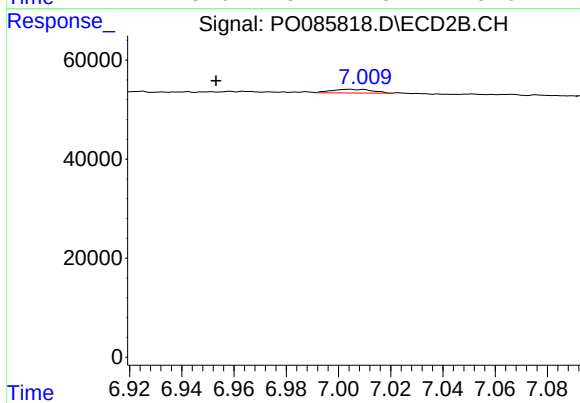

#34 AR-1260-4


R.T.: 7.004 min
Delta R.T.: 0.051 min
Response: 8110
Conc: 3.54 ng/ml

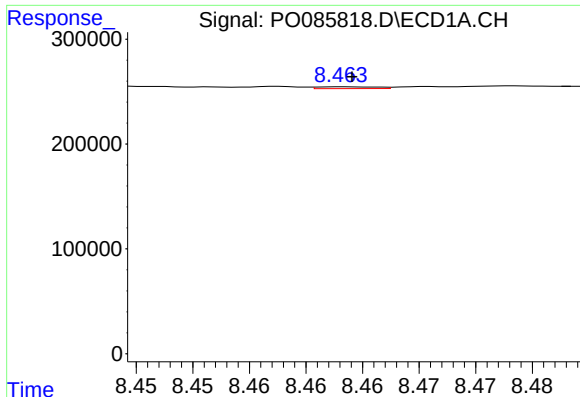

#35 AR-1260-5


R.T.: 8.463 min
Delta R.T.: 0.000 min
Response: 6335
Conc: 0.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

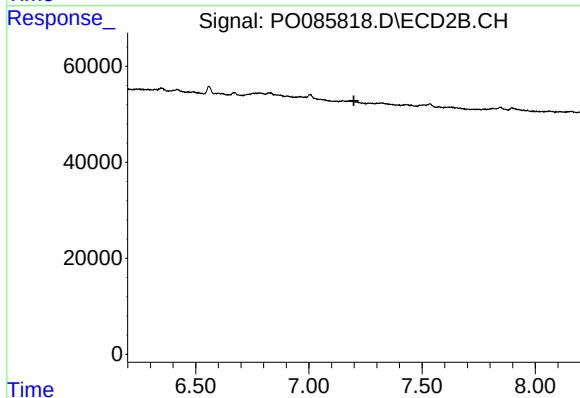


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

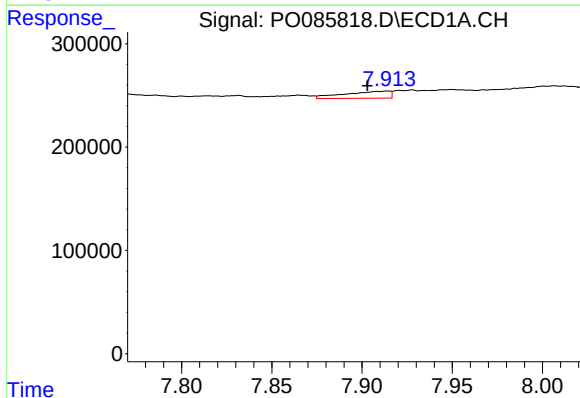


#36 AR-1262-1

R.T.: 7.914 min
Delta R.T.: 0.011 min
Response: 119860
Conc: 10.98 ng/ml

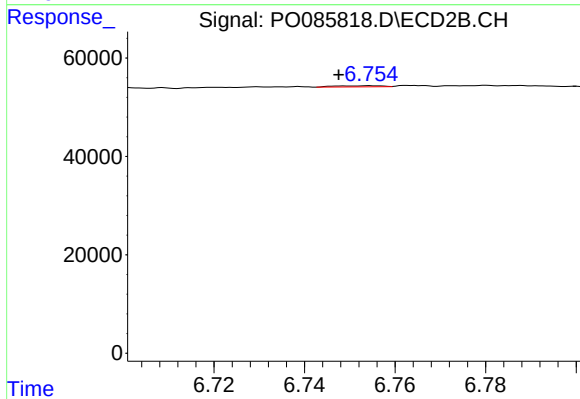

#36 AR-1262-1


R.T.: 6.755 min
Delta R.T.: 0.007 min
Response: 1579
Conc: 1.07 ng/ml

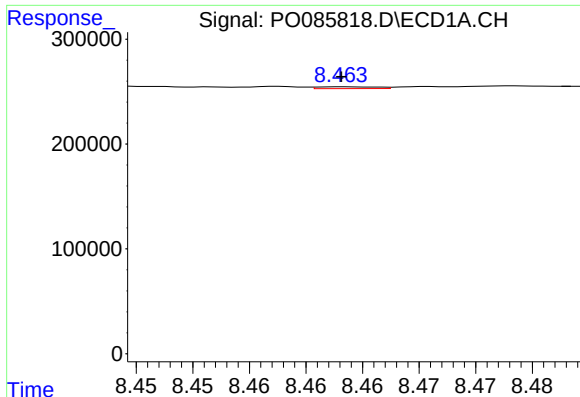

#37 AR-1262-2


R.T.: 8.463 min
Delta R.T.: 0.000 min
Response: 6335
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

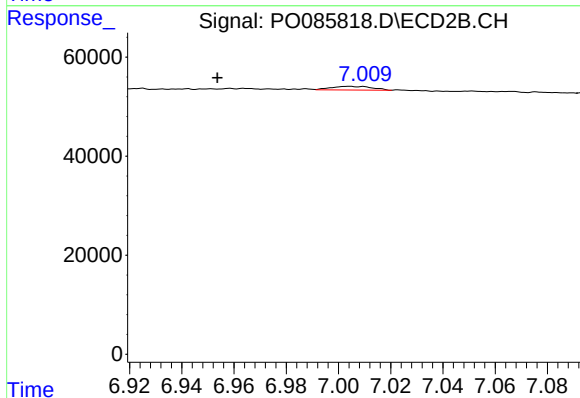


#37 AR-1262-2

R.T.: 7.004 min
Delta R.T.: 0.051 min
Response: 8110
Conc: 2.79 ng/ml

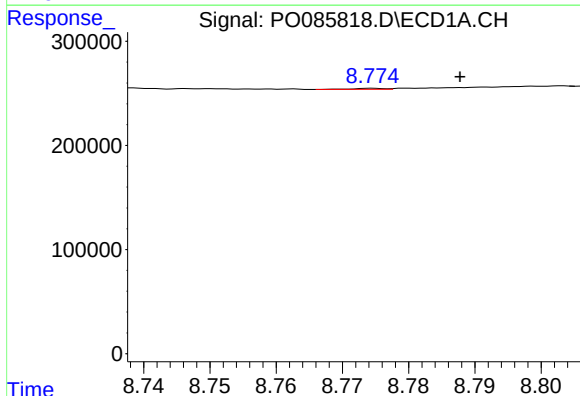


#38 AR-1262-3

R.T.: 8.775 min
Delta R.T.: -0.013 min
Response: 3803
Conc: 0.33 ng/ml

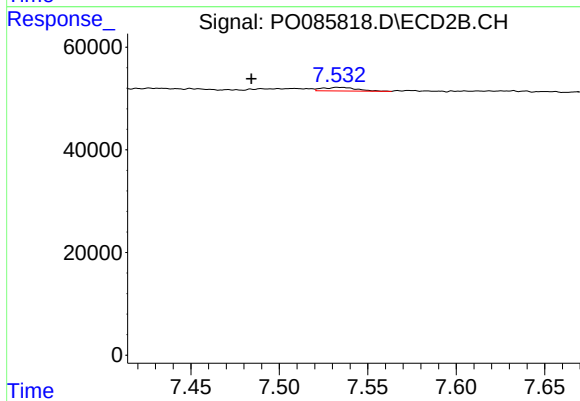

#38 AR-1262-3


R.T.: 7.533 min
Delta R.T.: 0.049 min
Response: 9436
Conc: 1.84 ng/ml

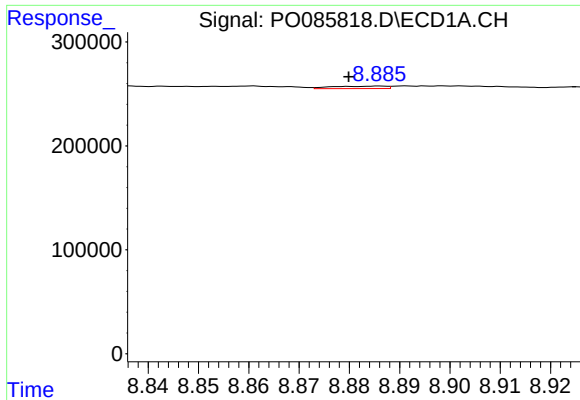

#39 AR-1262-4


R.T.: 8.886 min
Delta R.T.: 0.006 min
Response: 17208
Conc: 3.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

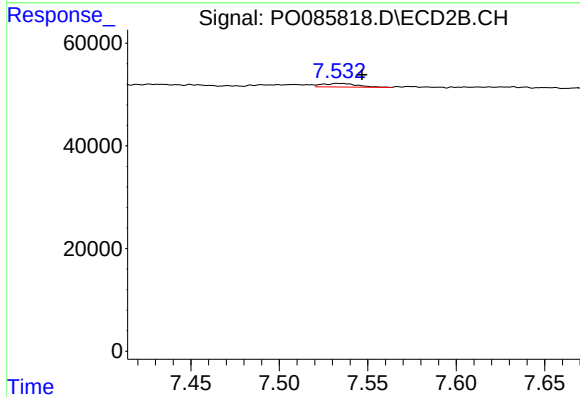


#39 AR-1262-4

R.T.: 7.533 min
Delta R.T.: -0.014 min
Response: 9436
Conc: 1.86 ng/ml

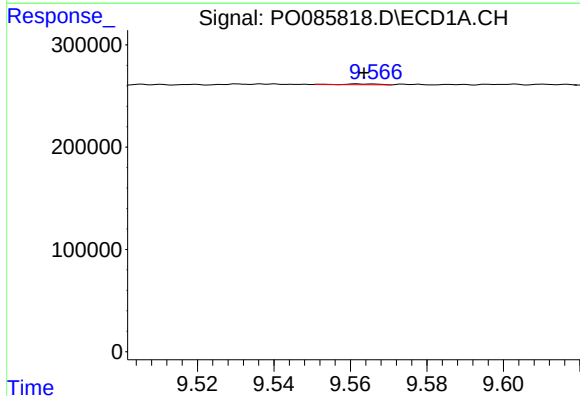


#40 AR-1262-5

R.T.: 9.562 min
Delta R.T.: -0.002 min
Response: 5095
Conc: 0.82 ng/ml

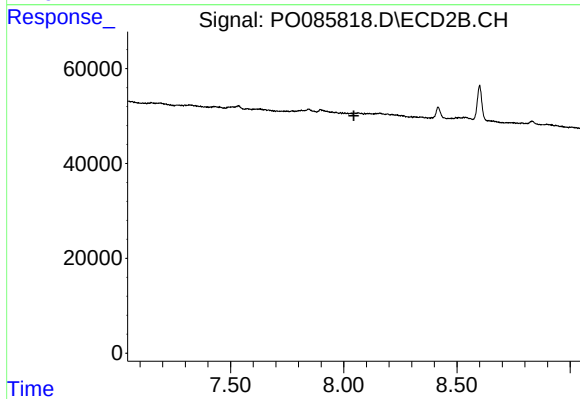

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.044 min
Response: 0
Conc: N.D.

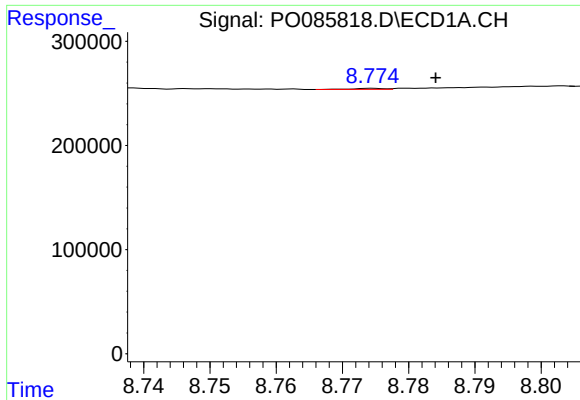

#41 AR-1268-1


R.T.: 8.775 min
Delta R.T.: -0.010 min
Response: 3803
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

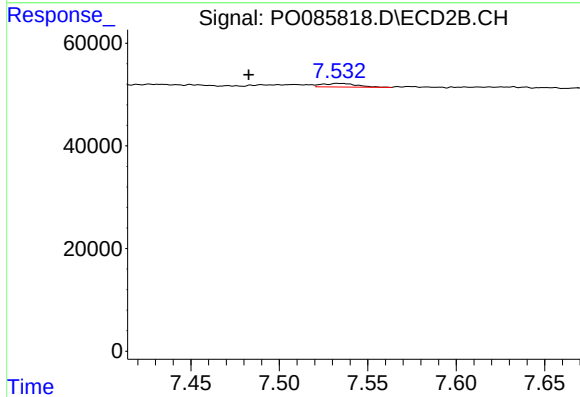


#41 AR-1268-1

R.T.: 7.533 min
Delta R.T.: 0.050 min
Response: 9436
Conc: 0.95 ng/ml

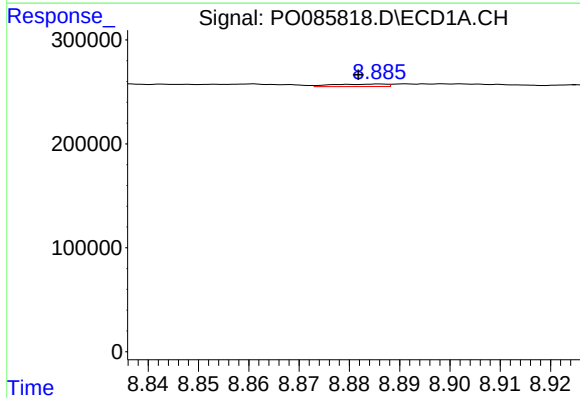


#42 AR-1268-2

R.T.: 8.886 min
Delta R.T.: 0.004 min
Response: 17208
Conc: 0.85 ng/ml

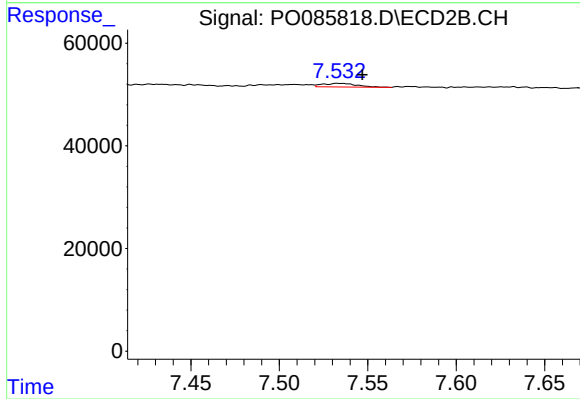

#42 AR-1268-2


R.T.: 7.533 min
Delta R.T.: -0.014 min
Response: 9436
Conc: 1.36 ng/ml

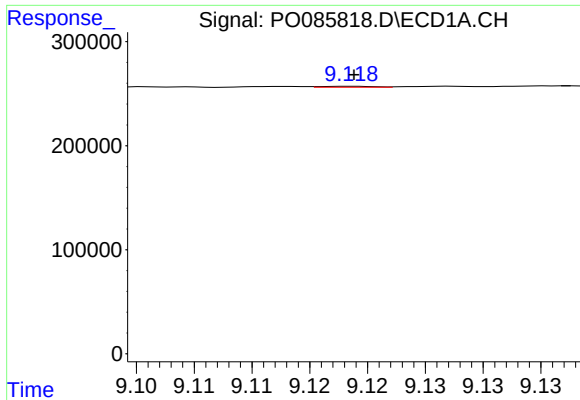

#43 AR-1268-3


R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 3089
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

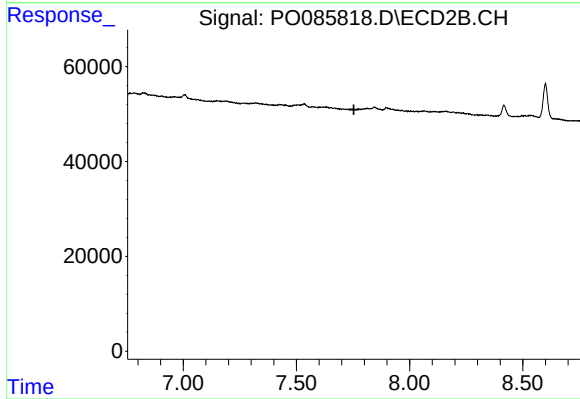


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.754 min
Response: 0
Conc: N.D.

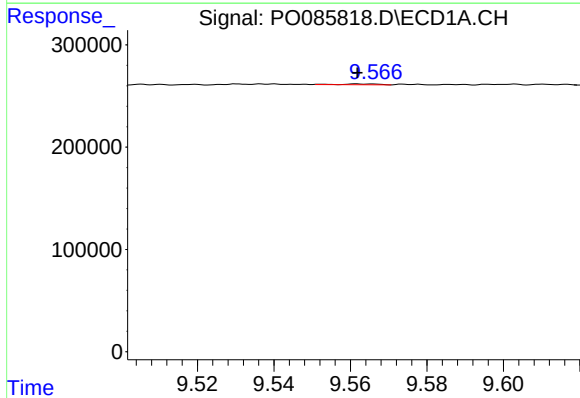


#44 AR-1268-4

R.T.: 9.562 min
Delta R.T.: 0.000 min
Response: 5095
Conc: 0.72 ng/ml

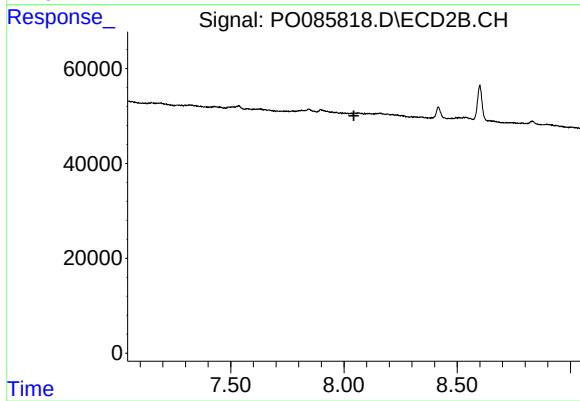

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.044 min
Response: 0
Conc: N.D.

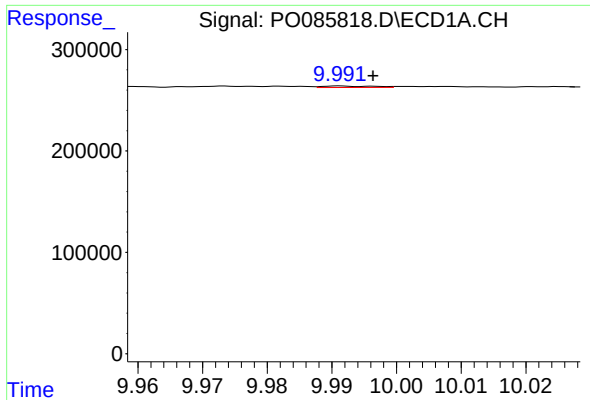

#45 AR-1268-5

R.T.: 9.991 min
Delta R.T.: -0.005 min
Response: 8449
Conc: 0.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-06

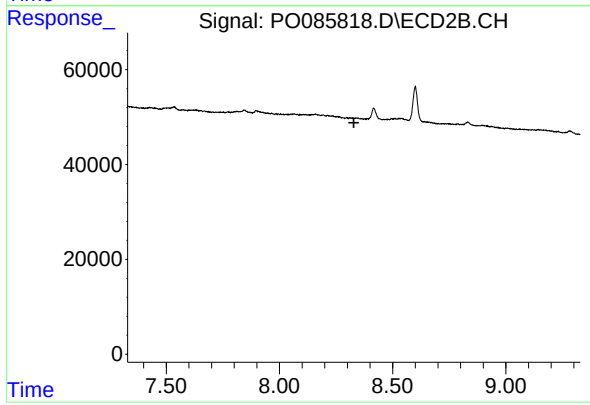

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.329 min
Response: 0
Conc: N.D.