

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
 Data File : P0085820.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2022 16:40
 Operator : YP\AJ
 Sample : N2205-08 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-032322-SR-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:42:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.504	3.566	3864	80380	0.020	1.700 #
2)	SA Decachlor...	10.379	8.586	919545	595256	7.166	16.954 #
Target Compounds							
3)	L1 AR-1016-1	5.637	4.652	18797	941	2.815	0.525 #
4)	L1 AR-1016-2	5.679	4.682	84314	4678	8.341	1.845 #
5)	L1 AR-1016-3	5.718	4.868	40649	15183	6.704	10.917 #
6)	L1 AR-1016-4	5.837	4.904	5529	27495	1.132	23.462 #
7)	L1 AR-1016-5	6.138	5.090	-3538	10752	N.D.	7.938 #
8)	L2 AR-1221-1	4.679	3.804	107818	6177	47.879	9.949 #
9)	L2 AR-1221-2	4.769	3.847	1155	14286	0.623	30.246 #
10)	L2 AR-1221-3	4.843	3.944	1779	4805	0.328	3.389 #
11)	L3 AR-1232-1	4.843	3.944	1779	4805	0.348	3.459 #
12)	L3 AR-1232-2	5.369	4.682	11764	4678	4.491	3.603
13)	L3 AR-1232-3	5.679	4.868	84314	15183	17.011	21.606 #
14)	L3 AR-1232-4	5.837	4.924	5529	24657	2.250	37.790 #
15)	L3 AR-1232-5	5.932	5.090	12381	10752	6.290	14.204 #
16)	L4 AR-1242-1	5.637	4.652	18797	941	3.491	0.666 #
17)	L4 AR-1242-2	5.718	4.682	40649	4678	5.007	2.400 #
18)	L4 AR-1242-3	5.755	4.868	54542	15183	10.876	14.182 #
19)	L4 AR-1242-4	5.837	4.924	5529	24657	1.398	22.728 #
20)	L4 AR-1242-5	6.591	5.461	98395	28385	22.069	21.216
21)	L5 AR-1248-1	5.679	4.652	84314	941	22.333	0.986 #
22)	L5 AR-1248-2	5.940	4.904	33560	27495	6.310	19.520 #
23)	L5 AR-1248-3	6.165	4.924	7579	24657	1.274	17.273 #
24)	L5 AR-1248-4	6.559	5.127	123195	8177	24.295	4.821 #
25)	L5 AR-1248-5	6.601	5.509	34449	10055	5.445	6.165
26)	L6 AR-1254-1	6.559	5.461	123195	28385	17.721	10.974 #
27)	L6 AR-1254-2	6.735	5.600	13848	9849	1.293	4.274 #
28)	L6 AR-1254-3	7.127	6.017	140084	174812	12.531	48.244 #
29)	L6 AR-1254-4	7.402	6.239	-26005	96073	N.D.	42.817 #
30)	L6 AR-1254-5	7.844	6.674	-2577	2197987	N.D.	696.820 #
31)	L7 AR-1260-1	7.286	6.141	357011	74837	44.572	29.971 #
32)	L7 AR-1260-2	7.521	6.311	100734	158403	10.736	52.062 #
33)	L7 AR-1260-3	7.886	6.483	25467	123621	3.610	45.041 #
34)	L7 AR-1260-4	8.141	6.967	10640300	2480093	1351.351	1081.961
35)	L7 AR-1260-5	8.461	7.228	859392	502428	55.941	99.378 #
36)	L8 AR-1262-1	7.886	6.733	25467	1936361	2.334	1311.814 #
37)	L8 AR-1262-2	8.461	6.967	859392	2480093	45.313	852.792 #
38)	L8 AR-1262-3	8.774	7.486	1623508	4970319	142.988	969.273 #
39)	L8 AR-1262-4	8.872	7.557	1062606	5044396	194.872	996.538 #
40)	L8 AR-1262-5	9.567	8.058	1243912	1701808	200.139	937.735 #
41)	L9 AR-1268-1	8.774	7.486	1623508	4970319	79.126	499.507 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
 Data File : P0085820.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2022 16:40
 Operator : YP\AJ
 Sample : N2205-08 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-032322-SR-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:42:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.872	7.557	1062606	5044396	52.503	727.619 #
43) L9	AR-1268-3	9.122	7.696f	1586198	359917	96.709	77.012
44) L9	AR-1268-4	9.567	8.058	1243912	1701808	176.878	812.929 #
45) L9	AR-1268-5	10.008	8.328	1374453	332750	24.361	24.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040122\
Data File : P0085820.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2022 16:40
Operator : YP\AJ
Sample : N2205-08 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 01:42:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

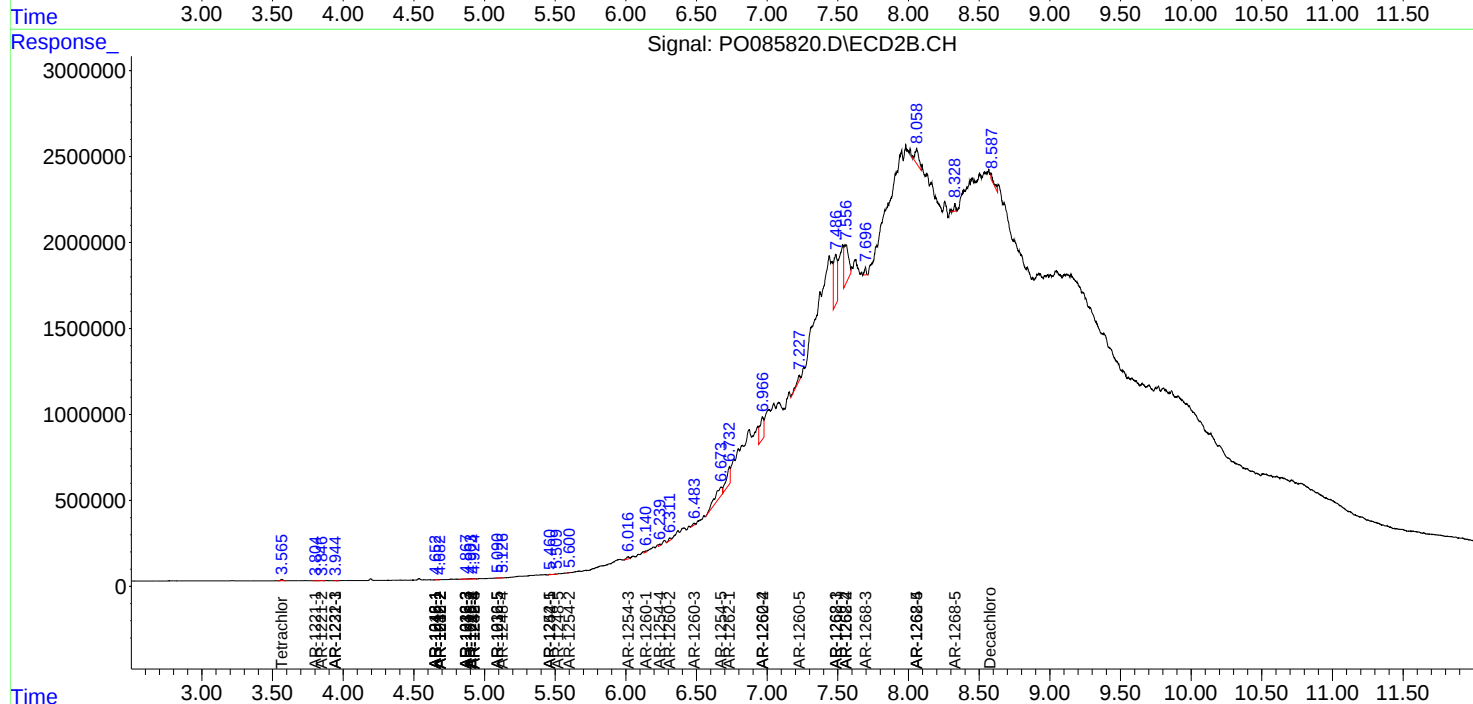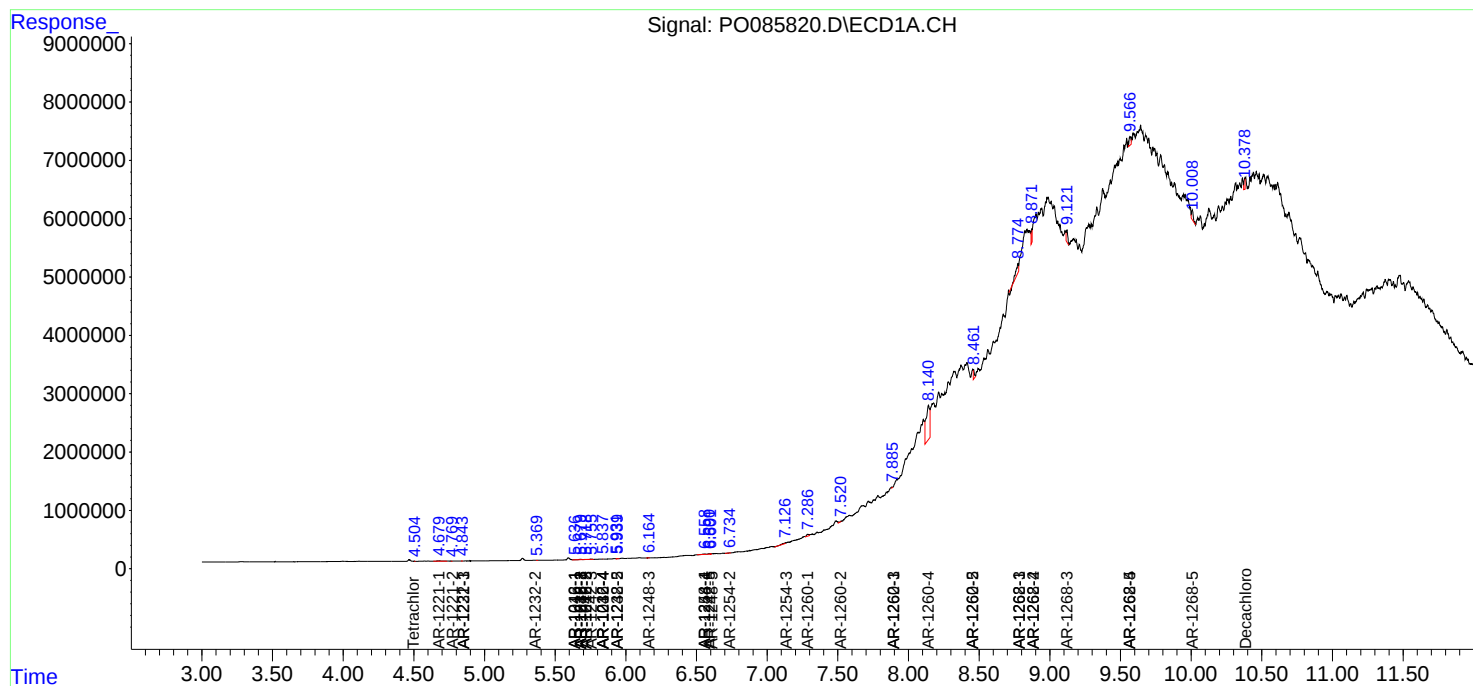


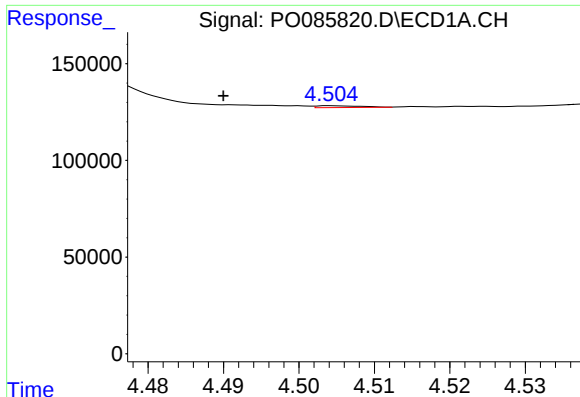

#1 Tetrachloro-m-xylene


R.T.: 4.504 min
Delta R.T.: 0.014 min
Response: 3864
Conc: 0.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

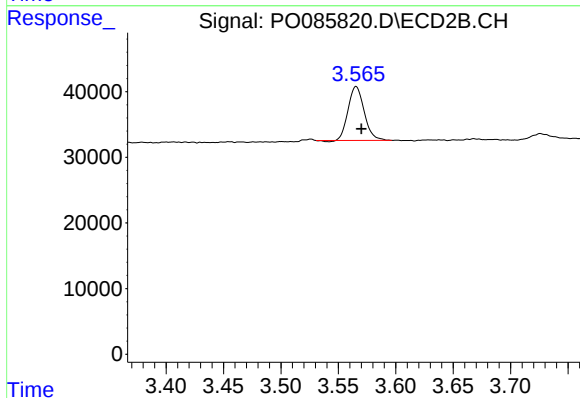


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.004 min
Response: 80380
Conc: 1.70 ng/ml

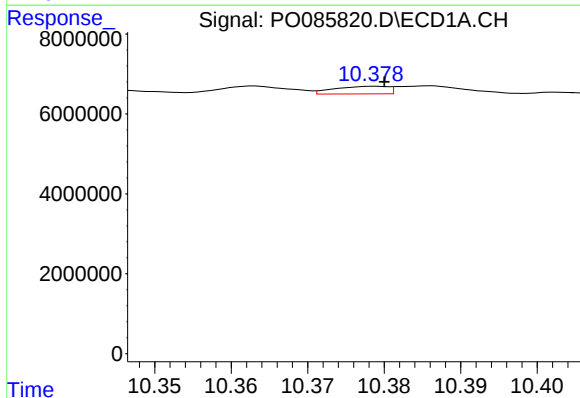


#2 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.001 min
Response: 919545
Conc: 7.17 ng/ml

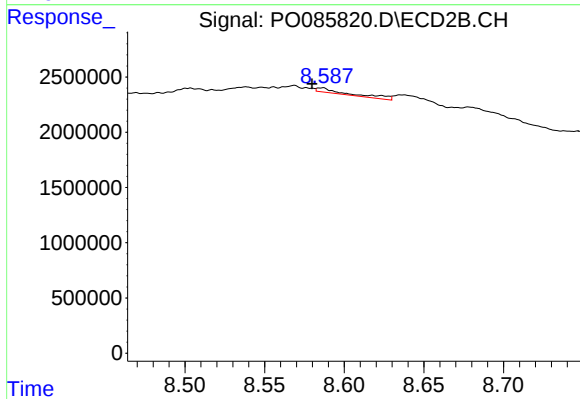

#2 Decachlorobiphenyl


R.T.: 8.586 min
Delta R.T.: 0.006 min
Response: 595256
Conc: 16.95 ng/ml

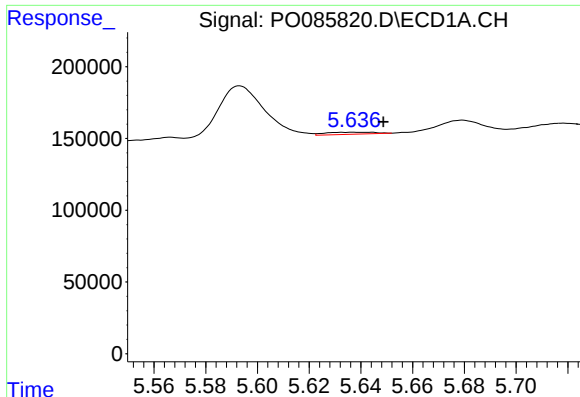

#3 AR-1016-1


R.T.: 5.637 min
Delta R.T.: -0.012 min
Response: 18797
Conc: 2.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

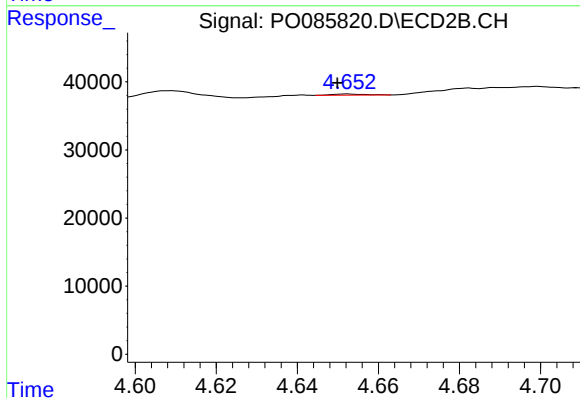


#3 AR-1016-1

R.T.: 4.652 min
Delta R.T.: 0.003 min
Response: 941
Conc: 0.53 ng/ml

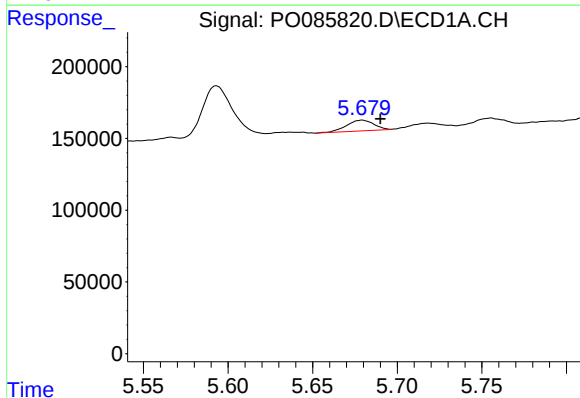


#4 AR-1016-2

R.T.: 5.679 min
Delta R.T.: -0.011 min
Response: 84314
Conc: 8.34 ng/ml

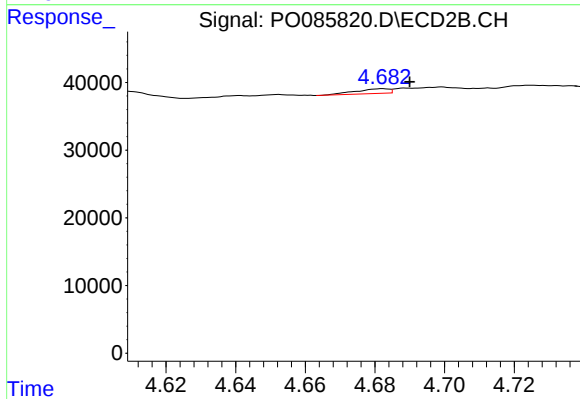

#4 AR-1016-2


R.T.: 4.682 min
Delta R.T.: -0.008 min
Response: 4678
Conc: 1.84 ng/ml

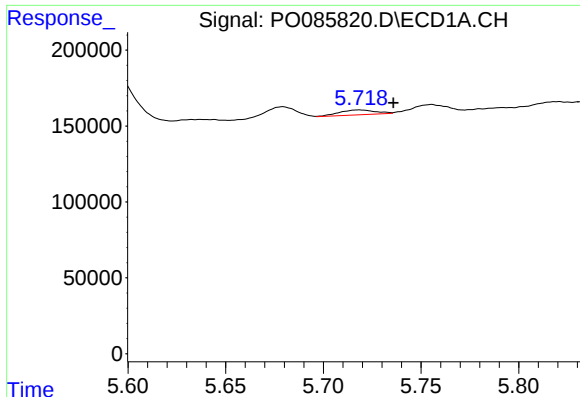

#5 AR-1016-3


R.T.: 5.718 min
Delta R.T.: -0.018 min
Response: 40649
Conc: 6.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

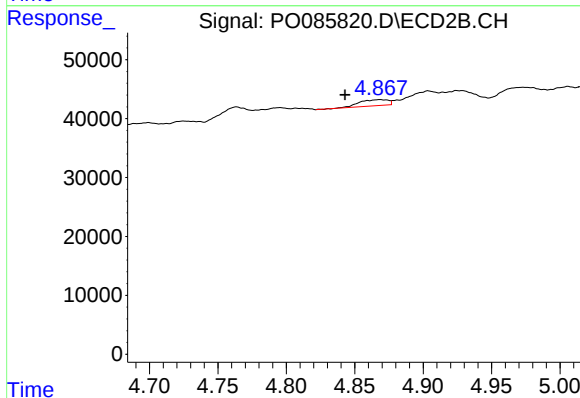


#5 AR-1016-3

R.T.: 4.868 min
Delta R.T.: 0.025 min
Response: 15183
Conc: 10.92 ng/ml

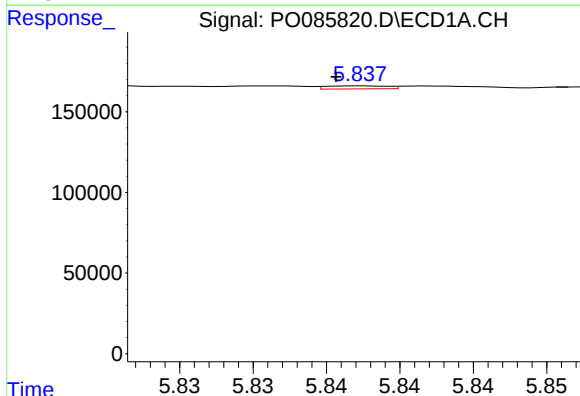


#6 AR-1016-4

R.T.: 5.837 min
Delta R.T.: 0.002 min
Response: 5529
Conc: 1.13 ng/ml

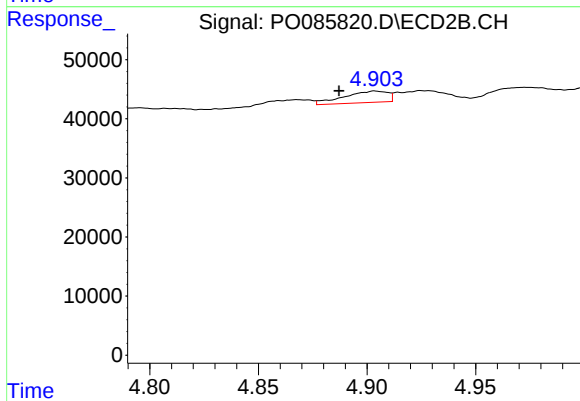

#6 AR-1016-4


R.T.: 4.904 min
Delta R.T.: 0.016 min
Response: 27495
Conc: 23.46 ng/ml

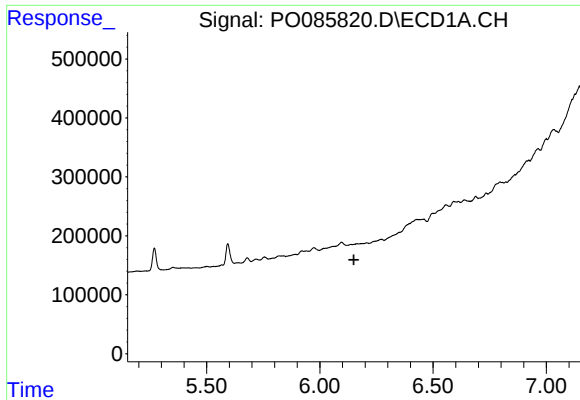

#7 AR-1016-5


R.T.: 6.138 min
Delta R.T.: -0.012 min
Response: -3538
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

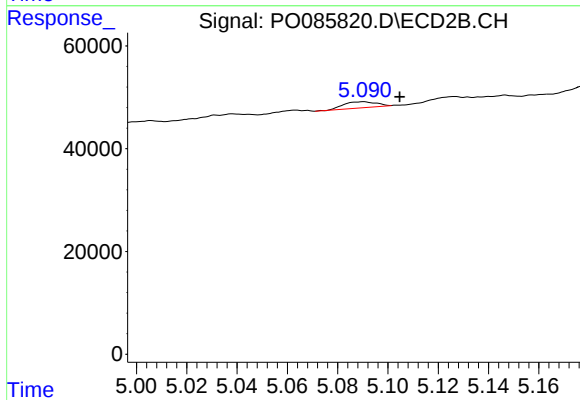


#7 AR-1016-5

R.T.: 5.090 min
Delta R.T.: -0.014 min
Response: 10752
Conc: 7.94 ng/ml

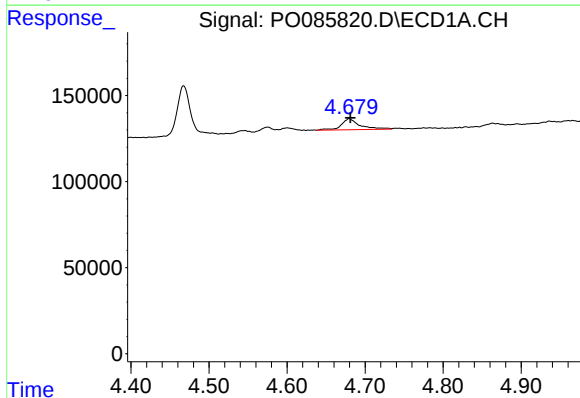


#8 AR-1221-1

R.T.: 4.679 min
Delta R.T.: -0.002 min
Response: 107818
Conc: 47.88 ng/ml

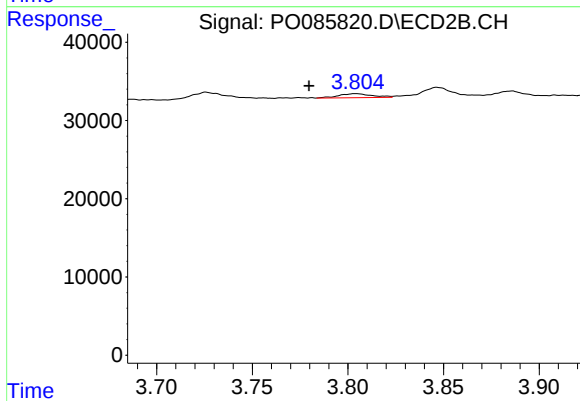

#8 AR-1221-1


R.T.: 3.804 min
Delta R.T.: 0.024 min
Response: 6177
Conc: 9.95 ng/ml

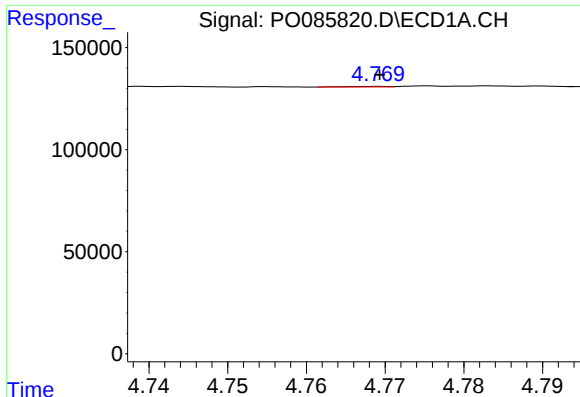

#9 AR-1221-2


R.T.: 4.769 min
Delta R.T.: 0.000 min
Response: 1155
Conc: 0.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

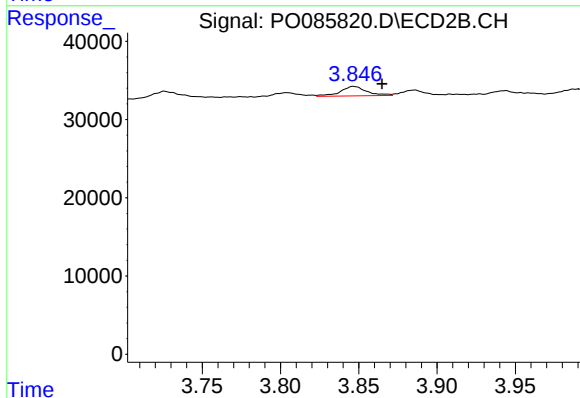


#9 AR-1221-2

R.T.: 3.847 min
Delta R.T.: -0.018 min
Response: 14286
Conc: 30.25 ng/ml

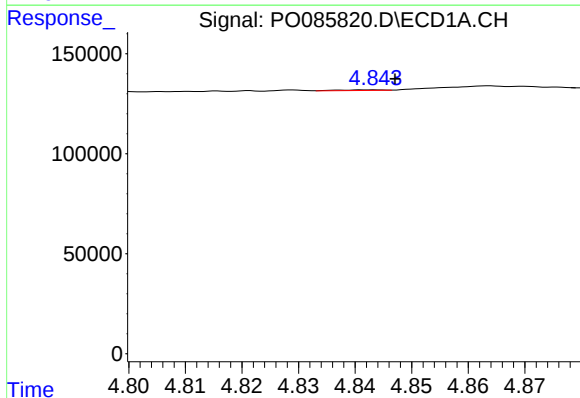


#10 AR-1221-3

R.T.: 4.843 min
Delta R.T.: -0.004 min
Response: 1779
Conc: 0.33 ng/ml

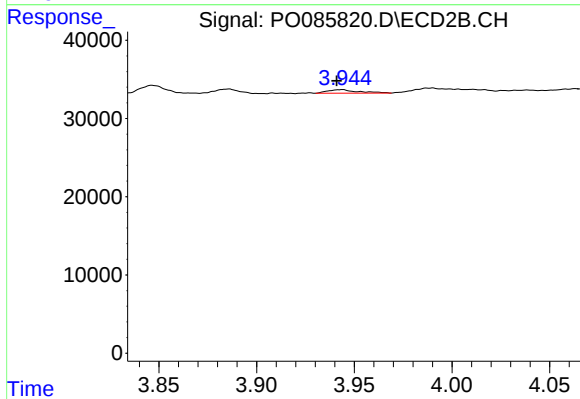

#10 AR-1221-3


R.T.: 3.944 min
Delta R.T.: 0.003 min
Response: 4805
Conc: 3.39 ng/ml

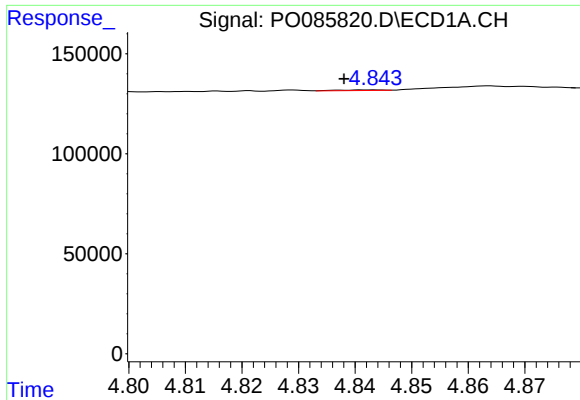

#11 AR-1232-1


R.T.: 4.843 min
Delta R.T.: 0.005 min
Response: 1779
Conc: 0.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

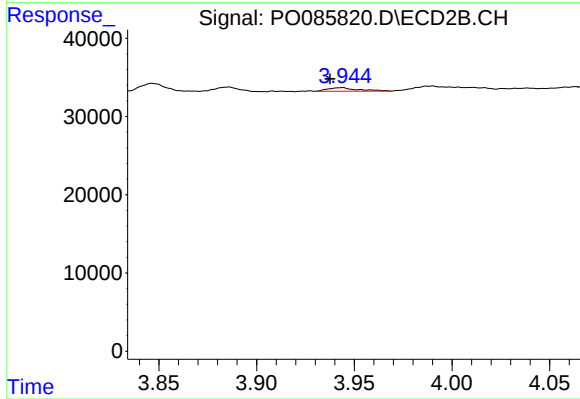


#11 AR-1232-1

R.T.: 3.944 min
Delta R.T.: 0.006 min
Response: 4805
Conc: 3.46 ng/ml

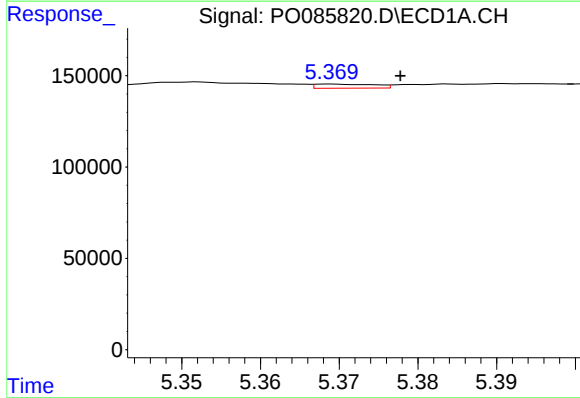


#12 AR-1232-2

R.T.: 5.369 min
Delta R.T.: -0.009 min
Response: 11764
Conc: 4.49 ng/ml

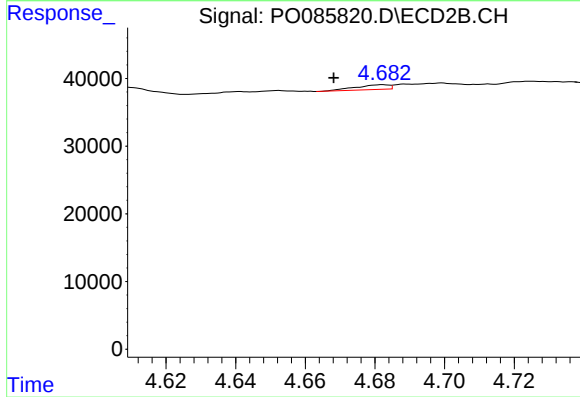

#12 AR-1232-2


R.T.: 4.682 min
Delta R.T.: 0.014 min
Response: 4678
Conc: 3.60 ng/ml

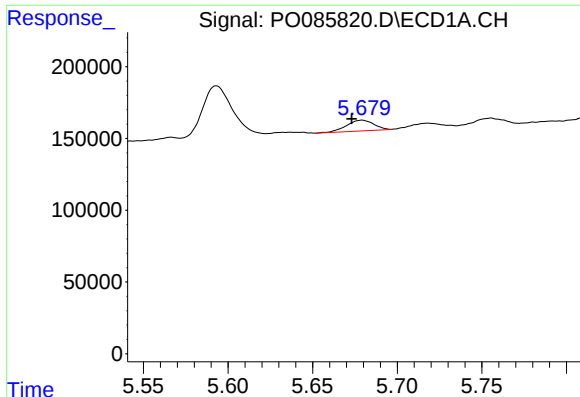

#13 AR-1232-3


R.T.: 5.679 min
Delta R.T.: 0.006 min
Response: 84314
Conc: 17.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

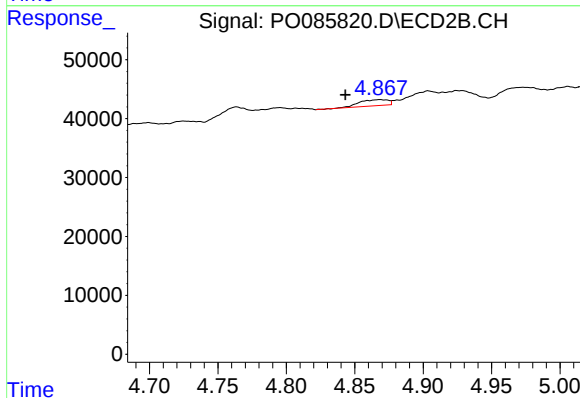


#13 AR-1232-3

R.T.: 4.868 min
Delta R.T.: 0.025 min
Response: 15183
Conc: 21.61 ng/ml

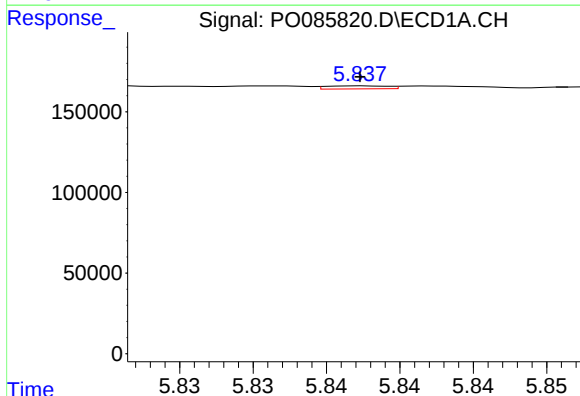


#14 AR-1232-4

R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 5529
Conc: 2.25 ng/ml

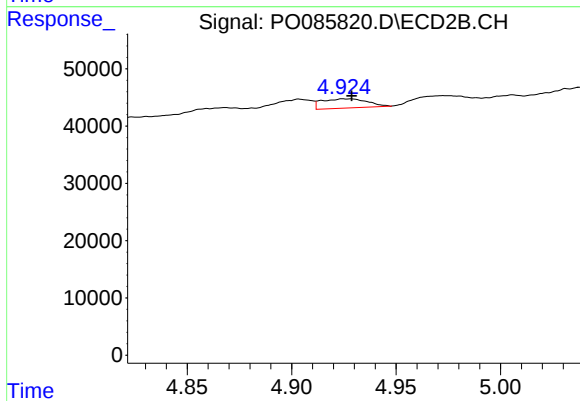

#14 AR-1232-4


R.T.: 4.924 min
Delta R.T.: -0.004 min
Response: 24657
Conc: 37.79 ng/ml

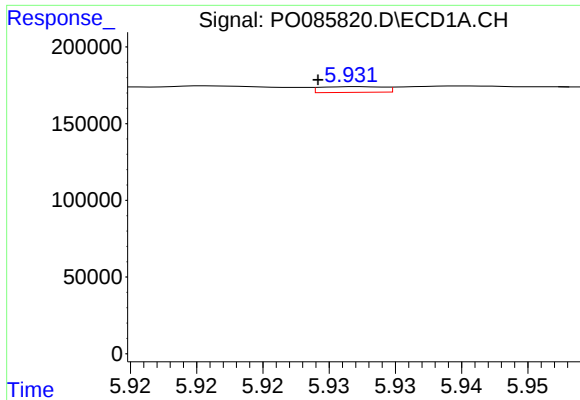

#15 AR-1232-5


R.T.: 5.932 min
Delta R.T.: 0.003 min
Response: 12381
Conc: 6.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

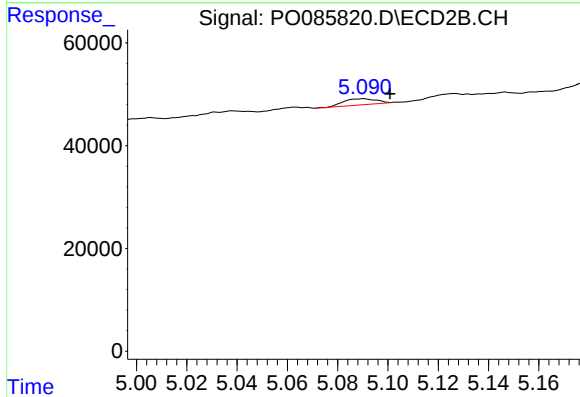


#15 AR-1232-5

R.T.: 5.090 min
Delta R.T.: -0.010 min
Response: 10752
Conc: 14.20 ng/ml

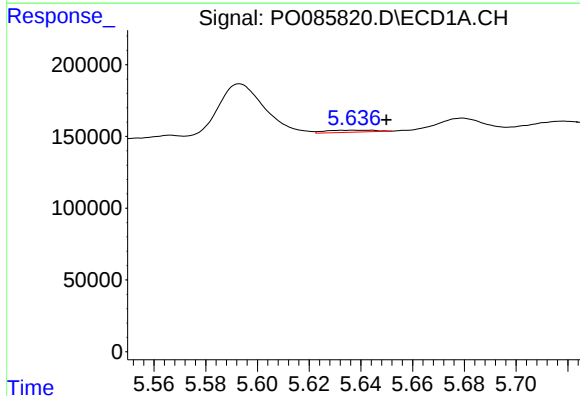


#16 AR-1242-1

R.T.: 5.637 min
Delta R.T.: -0.013 min
Response: 18797
Conc: 3.49 ng/ml

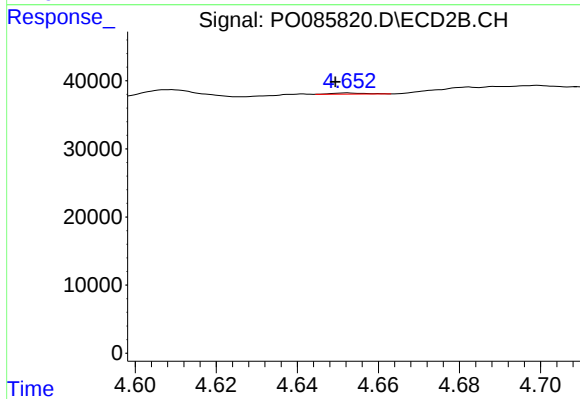

#16 AR-1242-1


R.T.: 4.652 min
Delta R.T.: 0.003 min
Response: 941
Conc: 0.67 ng/ml

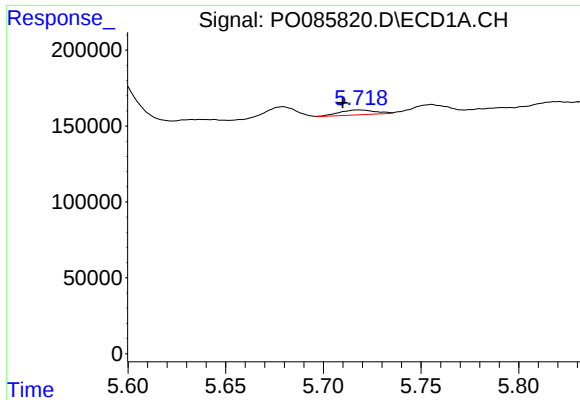

#17 AR-1242-2


R.T.: 5.718 min
Delta R.T.: 0.008 min
Response: 40649
Conc: 5.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

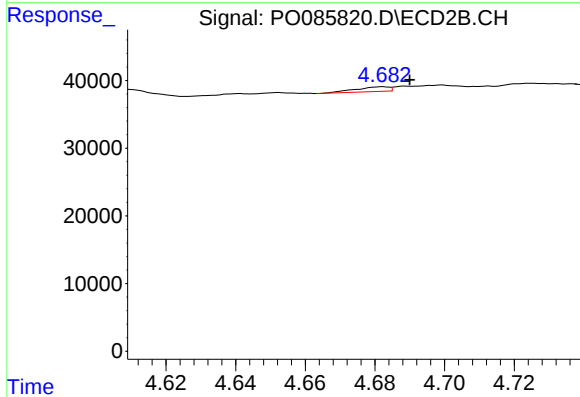


#17 AR-1242-2

R.T.: 4.682 min
Delta R.T.: -0.008 min
Response: 4678
Conc: 2.40 ng/ml

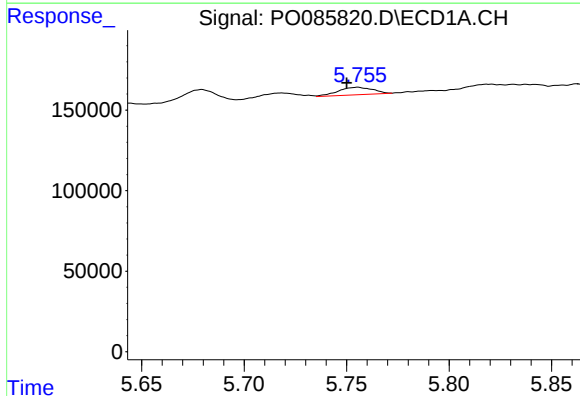


#18 AR-1242-3

R.T.: 5.755 min
Delta R.T.: 0.005 min
Response: 54542
Conc: 10.88 ng/ml

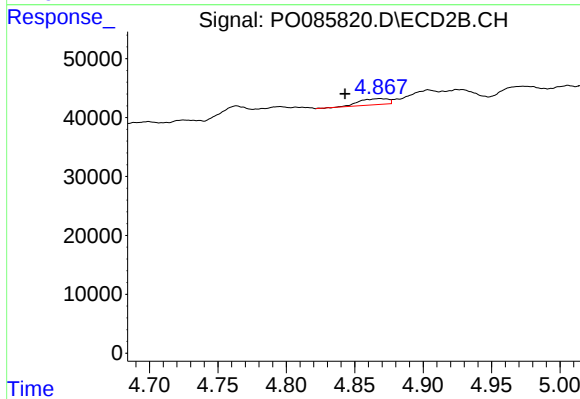

#18 AR-1242-3


R.T.: 4.868 min
Delta R.T.: 0.025 min
Response: 15183
Conc: 14.18 ng/ml

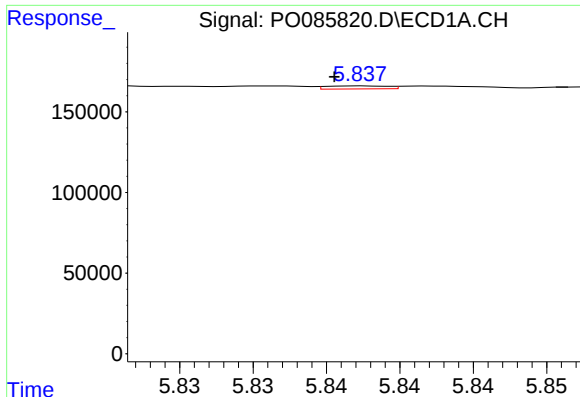

#19 AR-1242-4


R.T.: 5.837 min
Delta R.T.: 0.002 min
Response: 5529
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

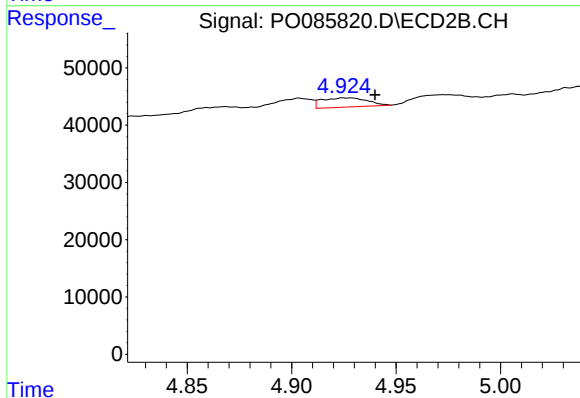


#19 AR-1242-4

R.T.: 4.924 min
Delta R.T.: -0.016 min
Response: 24657
Conc: 22.73 ng/ml

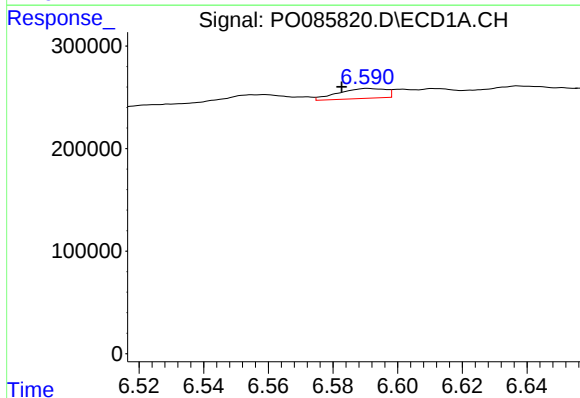


#20 AR-1242-5

R.T.: 6.591 min
Delta R.T.: 0.008 min
Response: 98395
Conc: 22.07 ng/ml

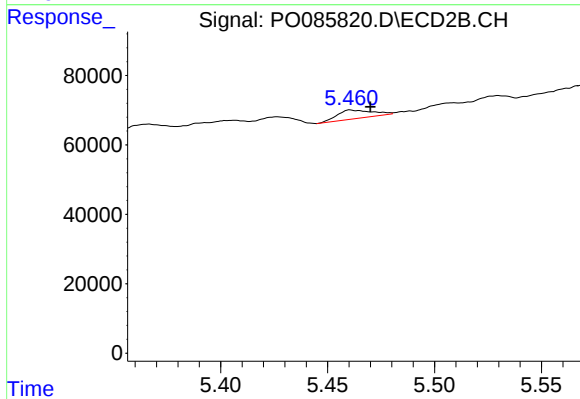

#20 AR-1242-5


R.T.: 5.461 min
Delta R.T.: -0.009 min
Response: 28385
Conc: 21.22 ng/ml

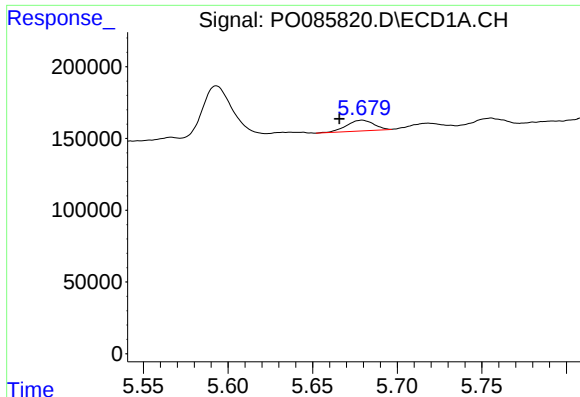

#21 AR-1248-1


R.T.: 5.679 min
Delta R.T.: 0.014 min
Response: 84314
Conc: 22.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

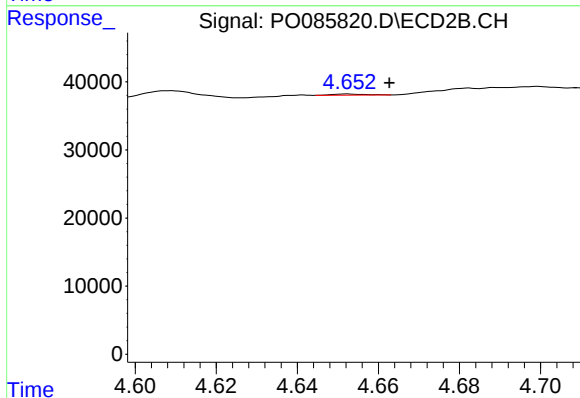


#21 AR-1248-1

R.T.: 4.652 min
Delta R.T.: -0.010 min
Response: 941
Conc: 0.99 ng/ml

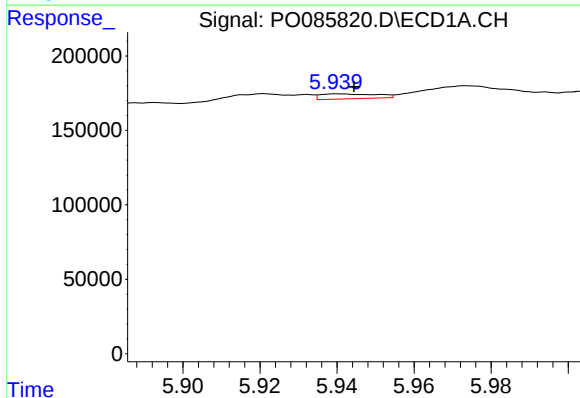


#22 AR-1248-2

R.T.: 5.940 min
Delta R.T.: -0.004 min
Response: 33560
Conc: 6.31 ng/ml

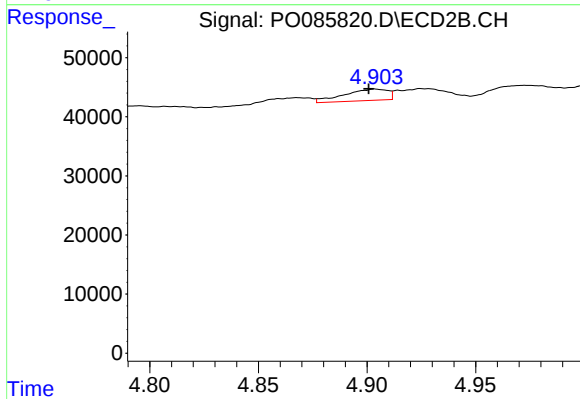

#22 AR-1248-2


R.T.: 4.904 min
Delta R.T.: 0.003 min
Response: 27495
Conc: 19.52 ng/ml

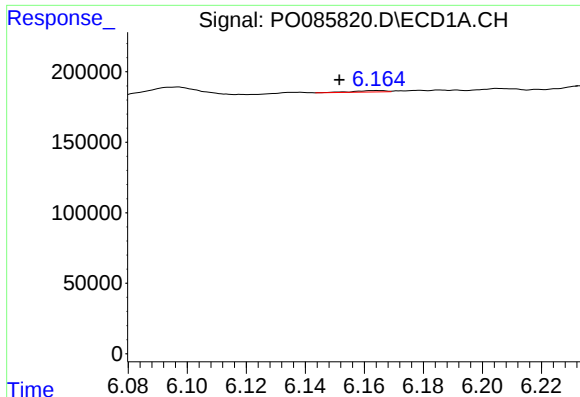

#23 AR-1248-3


R.T.: 6.165 min
Delta R.T.: 0.013 min
Response: 7579
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

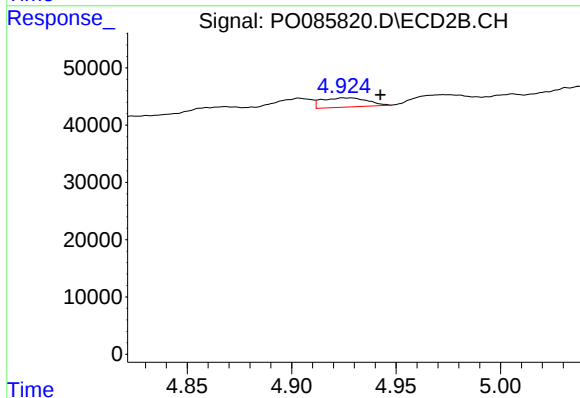


#23 AR-1248-3

R.T.: 4.924 min
Delta R.T.: -0.018 min
Response: 24657
Conc: 17.27 ng/ml

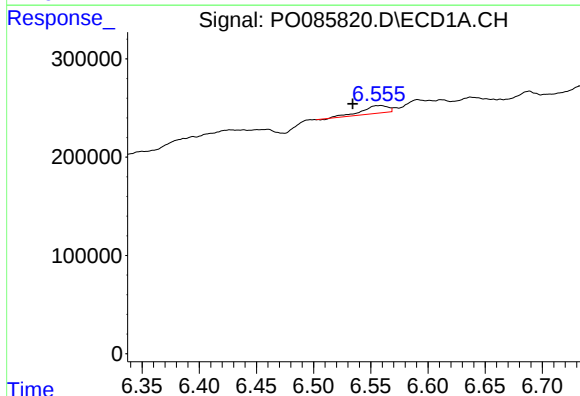


#24 AR-1248-4

R.T.: 6.559 min
Delta R.T.: 0.025 min
Response: 123195
Conc: 24.29 ng/ml

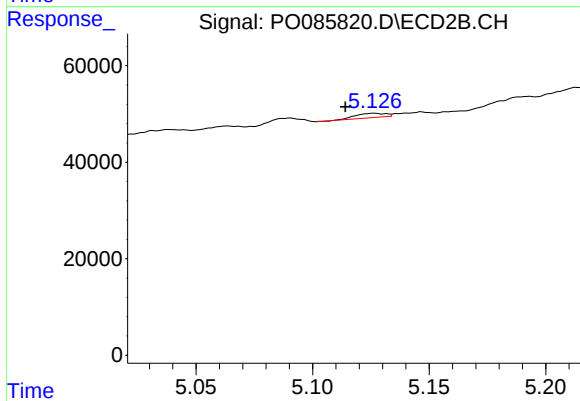

#24 AR-1248-4


R.T.: 5.127 min
Delta R.T.: 0.012 min
Response: 8177
Conc: 4.82 ng/ml

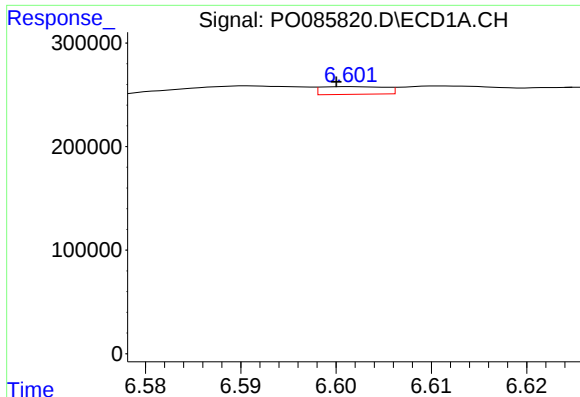

#25 AR-1248-5


R.T.: 6.601 min
Delta R.T.: 0.001 min
Response: 34449
Conc: 5.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

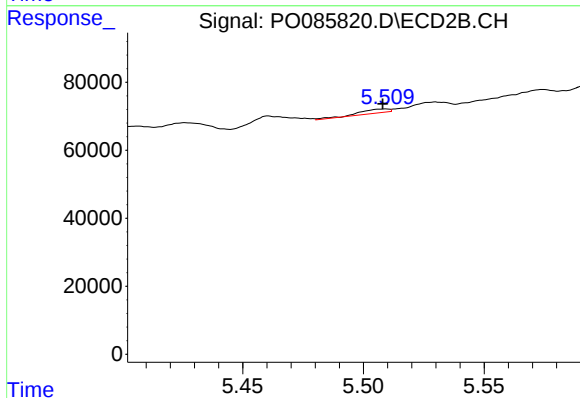


#25 AR-1248-5

R.T.: 5.509 min
Delta R.T.: 0.001 min
Response: 10055
Conc: 6.16 ng/ml

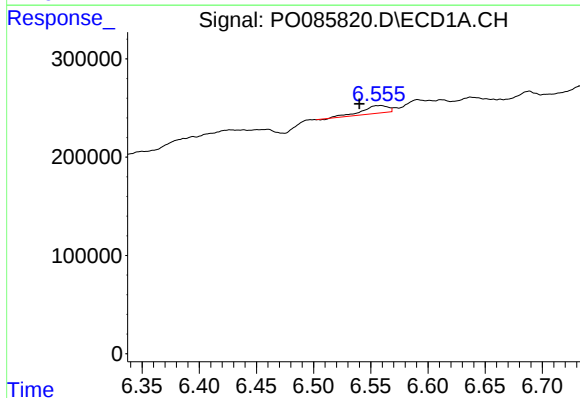


#26 AR-1254-1

R.T.: 6.559 min
Delta R.T.: 0.019 min
Response: 123195
Conc: 17.72 ng/ml

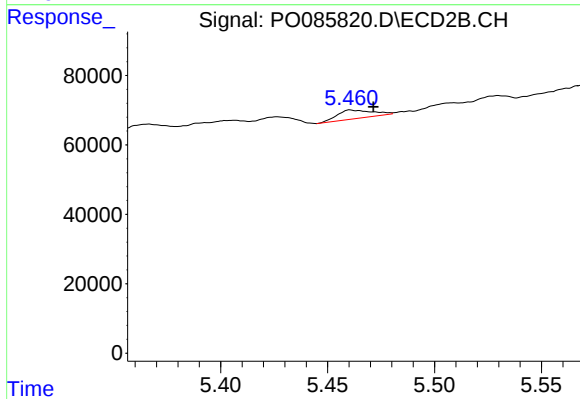

#26 AR-1254-1


R.T.: 5.461 min
Delta R.T.: -0.011 min
Response: 28385
Conc: 10.97 ng/ml

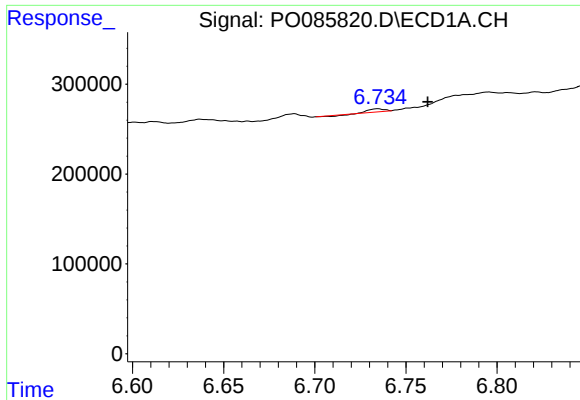

#27 AR-1254-2


R.T.: 6.735 min
Delta R.T.: -0.027 min
Response: 13848
Conc: 1.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

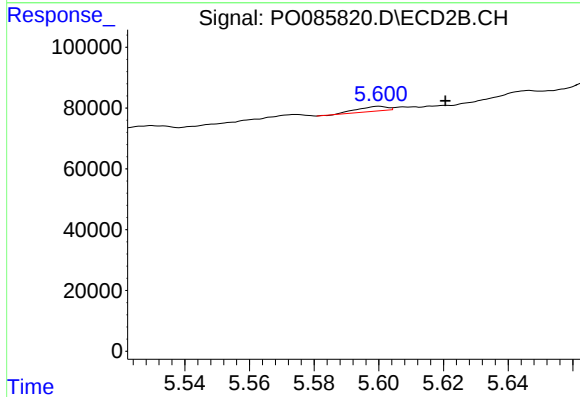


#27 AR-1254-2

R.T.: 5.600 min
Delta R.T.: -0.020 min
Response: 9849
Conc: 4.27 ng/ml

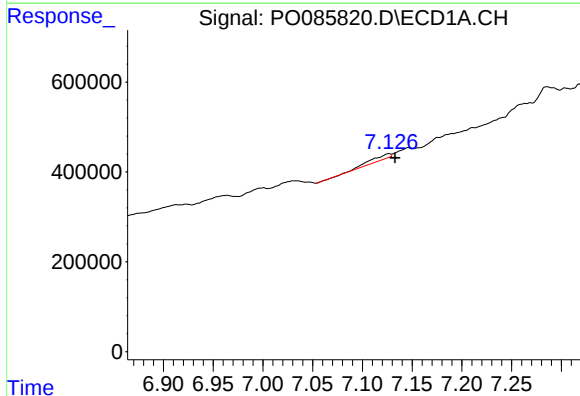


#28 AR-1254-3

R.T.: 7.127 min
Delta R.T.: -0.006 min
Response: 140084
Conc: 12.53 ng/ml

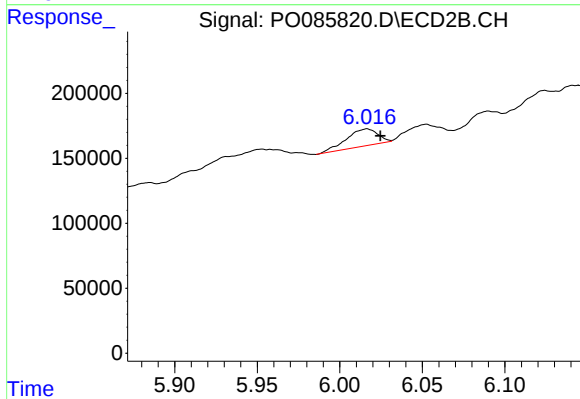

#28 AR-1254-3


R.T.: 6.017 min
Delta R.T.: -0.008 min
Response: 174812
Conc: 48.24 ng/ml

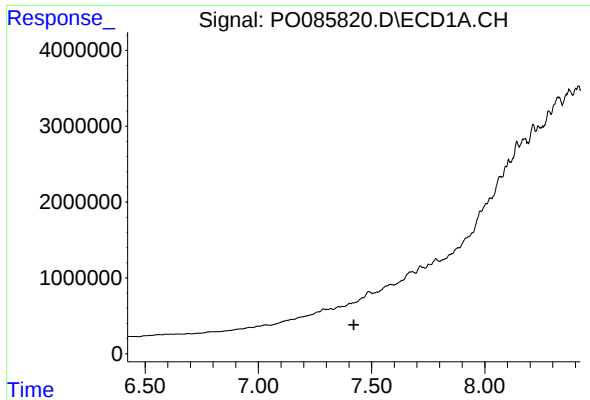

#29 AR-1254-4


R.T.: 7.402 min
Delta R.T.: -0.019 min
Response: -26005
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

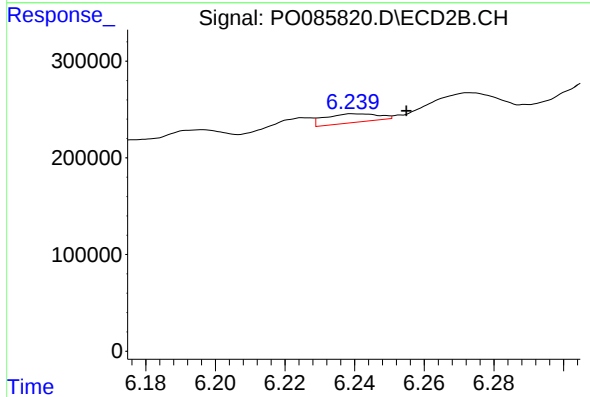


#29 AR-1254-4

R.T.: 6.239 min
Delta R.T.: -0.016 min
Response: 96073
Conc: 42.82 ng/ml

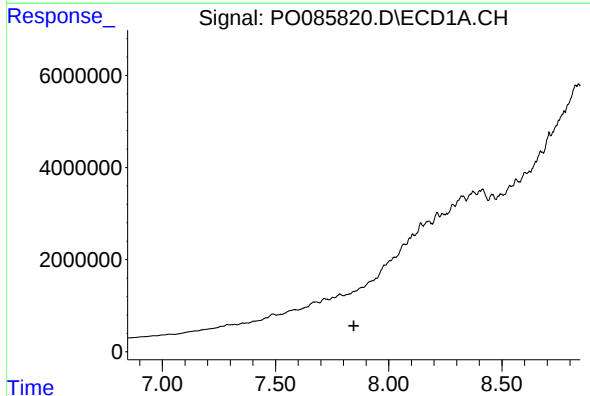


#30 AR-1254-5

R.T.: 7.844 min
Delta R.T.: -0.002 min
Response: -2577
Conc: N.D.

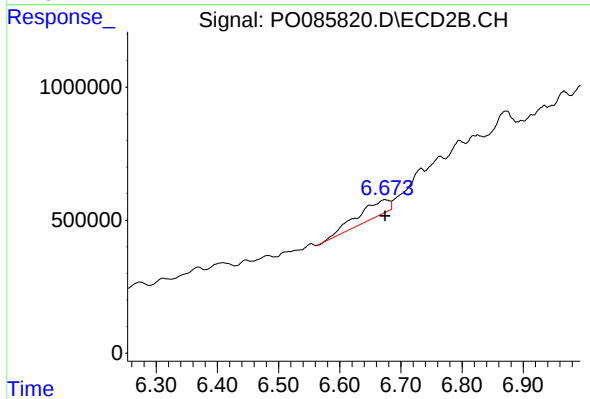

#30 AR-1254-5


R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 2197987
Conc: 696.82 ng/ml

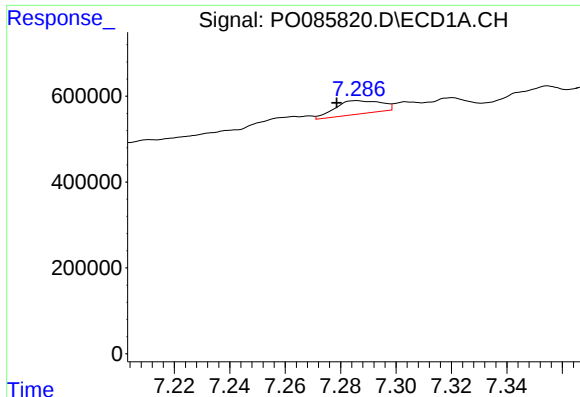

#31 AR-1260-1


R.T.: 7.286 min
Delta R.T.: 0.007 min
Response: 357011
Conc: 44.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

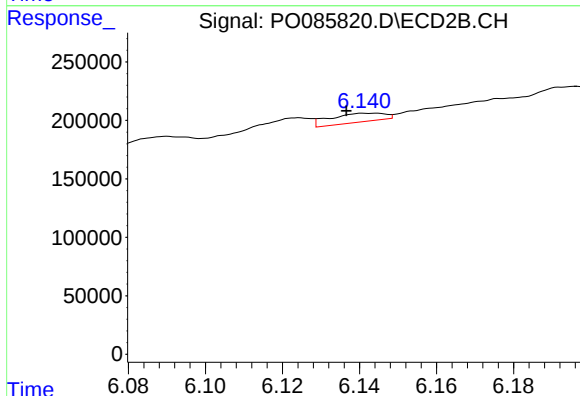


#31 AR-1260-1

R.T.: 6.141 min
Delta R.T.: 0.004 min
Response: 74837
Conc: 29.97 ng/ml

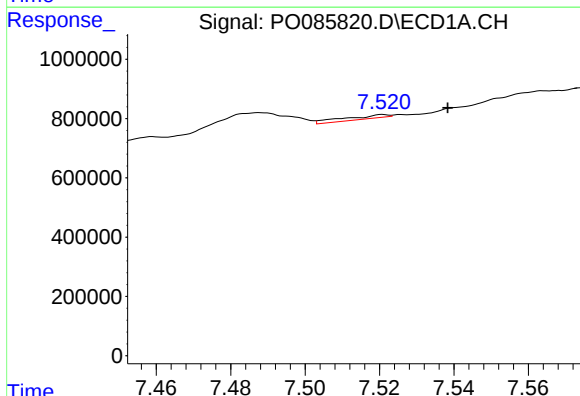


#32 AR-1260-2

R.T.: 7.521 min
Delta R.T.: -0.017 min
Response: 100734
Conc: 10.74 ng/ml

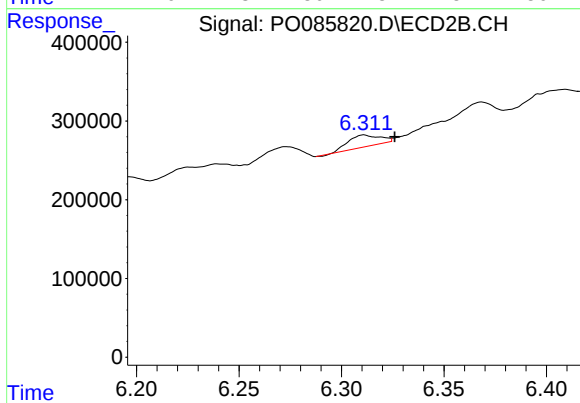

#32 AR-1260-2


R.T.: 6.311 min
Delta R.T.: -0.015 min
Response: 158403
Conc: 52.06 ng/ml

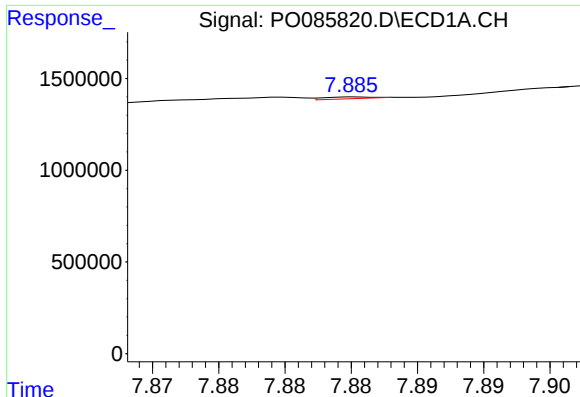

#33 AR-1260-3


R.T.: 7.886 min
Delta R.T.: -0.024 min
Response: 25467
Conc: 3.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

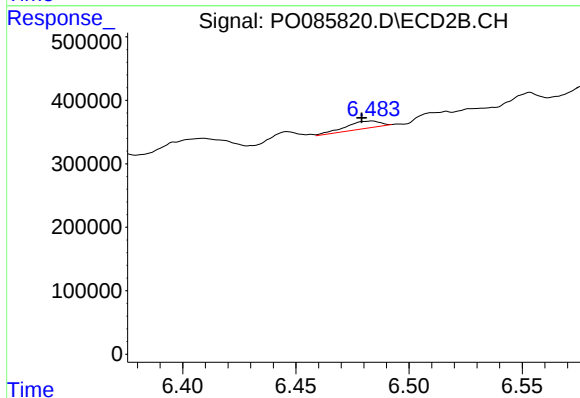


#33 AR-1260-3

R.T.: 6.483 min
Delta R.T.: 0.004 min
Response: 123621
Conc: 45.04 ng/ml

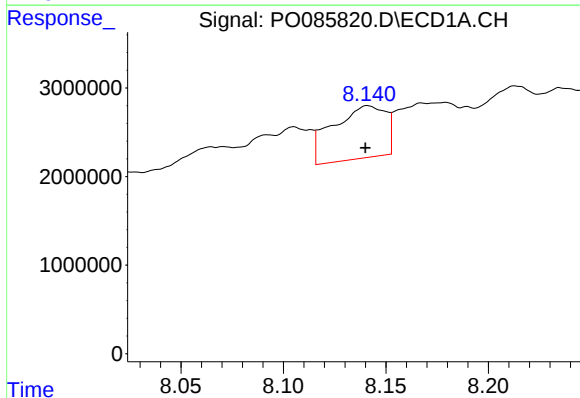


#34 AR-1260-4

R.T.: 8.141 min
Delta R.T.: 0.000 min
Response: 10640300
Conc: 1351.35 ng/ml

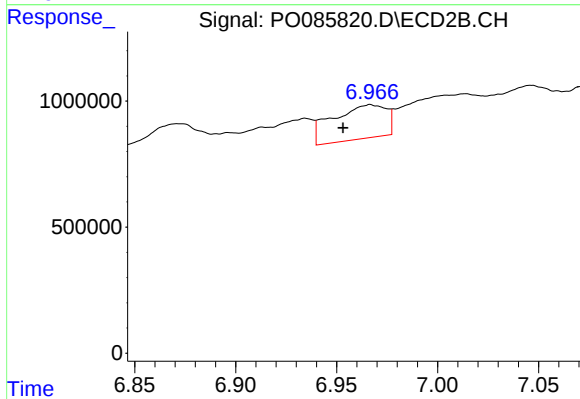

#34 AR-1260-4


R.T.: 6.967 min
Delta R.T.: 0.014 min
Response: 2480093
Conc: 1081.96 ng/ml

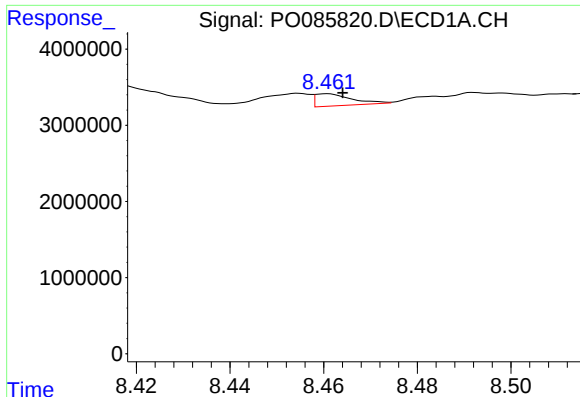

#35 AR-1260-5


R.T.: 8.461 min
Delta R.T.: -0.003 min
Response: 859392
Conc: 55.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

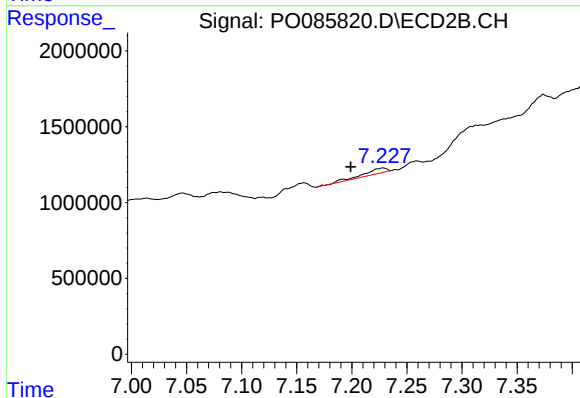


#35 AR-1260-5

R.T.: 7.228 min
Delta R.T.: 0.029 min
Response: 502428
Conc: 99.38 ng/ml

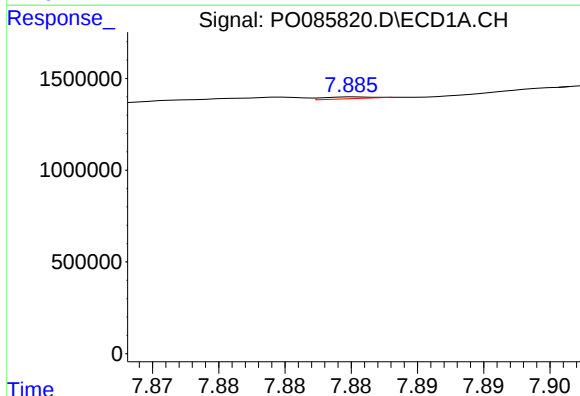


#36 AR-1262-1

R.T.: 7.886 min
Delta R.T.: -0.017 min
Response: 25467
Conc: 2.33 ng/ml

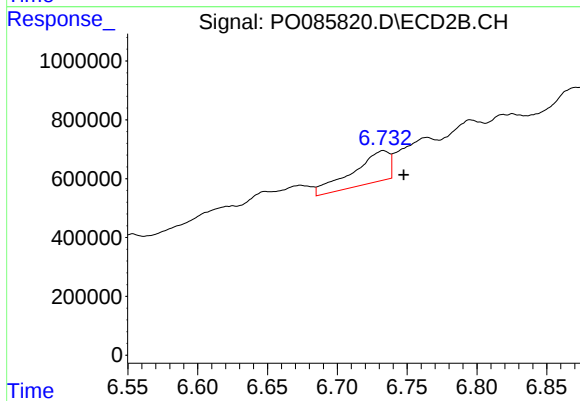

#36 AR-1262-1


R.T.: 6.733 min
Delta R.T.: -0.015 min
Response: 1936361
Conc: 1311.81 ng/ml

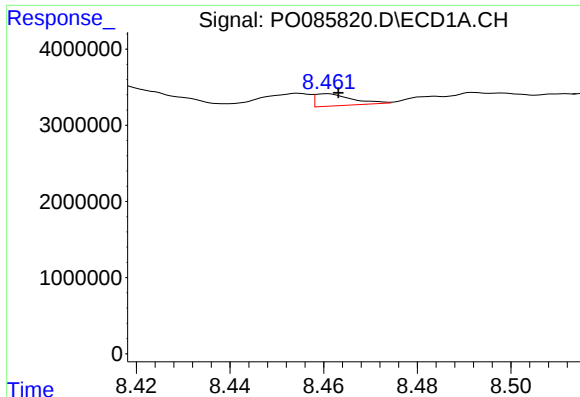

#37 AR-1262-2


R.T.: 8.461 min
Delta R.T.: -0.002 min
Response: 859392
Conc: 45.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

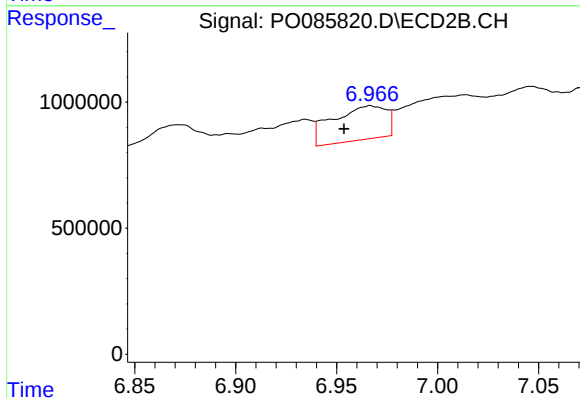


#37 AR-1262-2

R.T.: 6.967 min
Delta R.T.: 0.013 min
Response: 2480093
Conc: 852.79 ng/ml

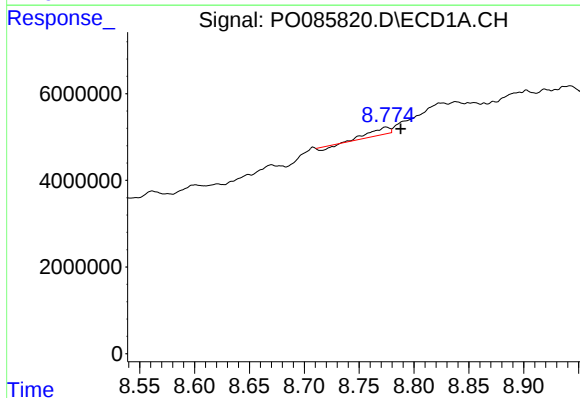


#38 AR-1262-3

R.T.: 8.774 min
Delta R.T.: -0.013 min
Response: 1623508
Conc: 142.99 ng/ml

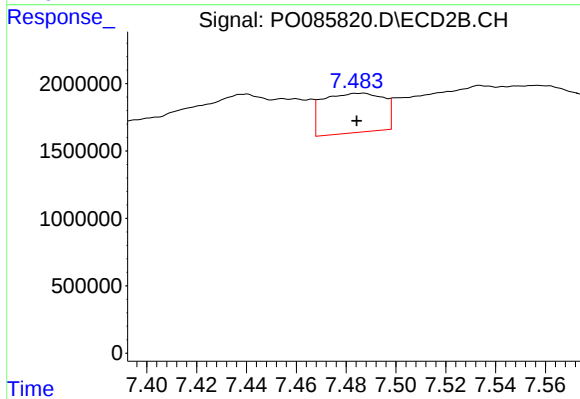

#38 AR-1262-3


R.T.: 7.486 min
Delta R.T.: 0.002 min
Response: 4970319
Conc: 969.27 ng/ml

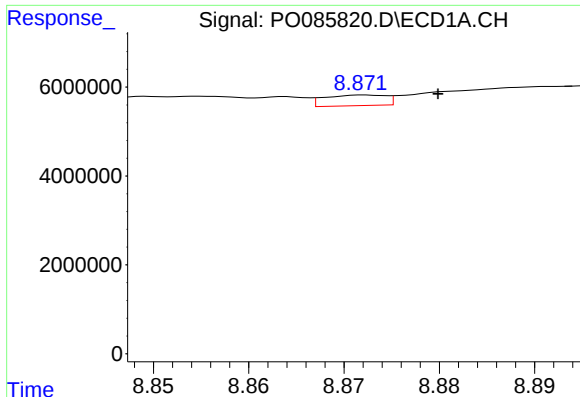

#39 AR-1262-4


R.T.: 8.872 min
Delta R.T.: -0.008 min
Response: 1062606
Conc: 194.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

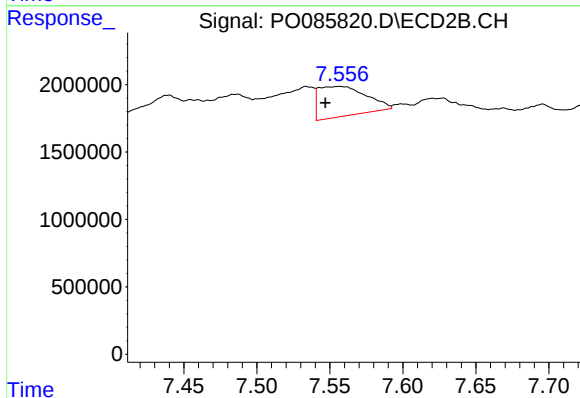


#39 AR-1262-4

R.T.: 7.557 min
Delta R.T.: 0.010 min
Response: 5044396
Conc: 996.54 ng/ml

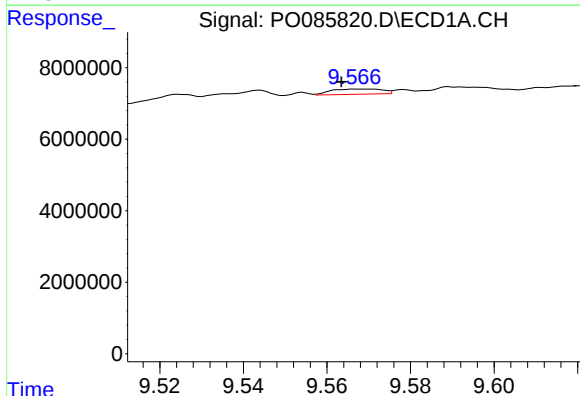


#40 AR-1262-5

R.T.: 9.567 min
Delta R.T.: 0.004 min
Response: 1243912
Conc: 200.14 ng/ml

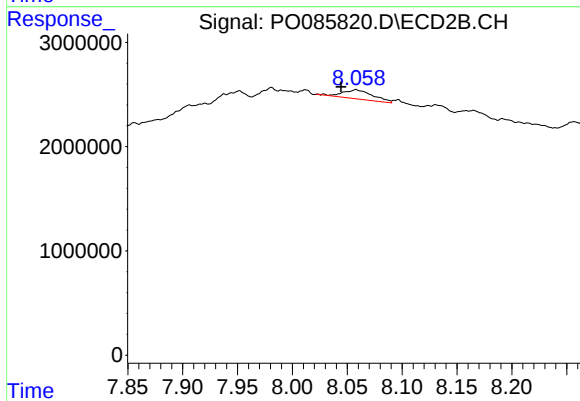

#40 AR-1262-5


R.T.: 8.058 min
Delta R.T.: 0.013 min
Response: 1701808
Conc: 937.73 ng/ml

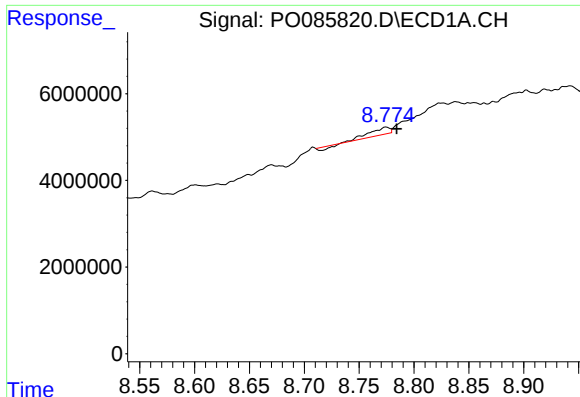

#41 AR-1268-1


R.T.: 8.774 min
Delta R.T.: -0.010 min
Response: 1623508
Conc: 79.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

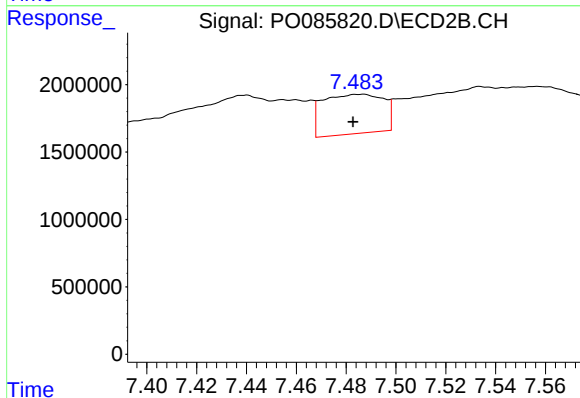


#41 AR-1268-1

R.T.: 7.486 min
Delta R.T.: 0.003 min
Response: 4970319
Conc: 499.51 ng/ml

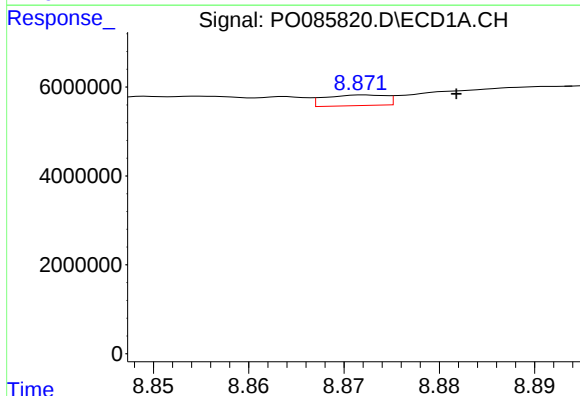


#42 AR-1268-2

R.T.: 8.872 min
Delta R.T.: -0.010 min
Response: 1062606
Conc: 52.50 ng/ml

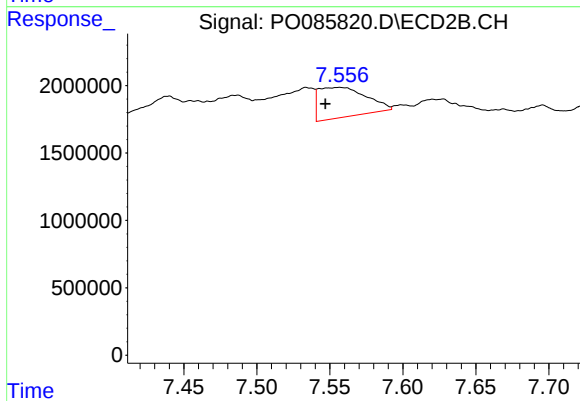

#42 AR-1268-2


R.T.: 7.557 min
Delta R.T.: 0.010 min
Response: 5044396
Conc: 727.62 ng/ml

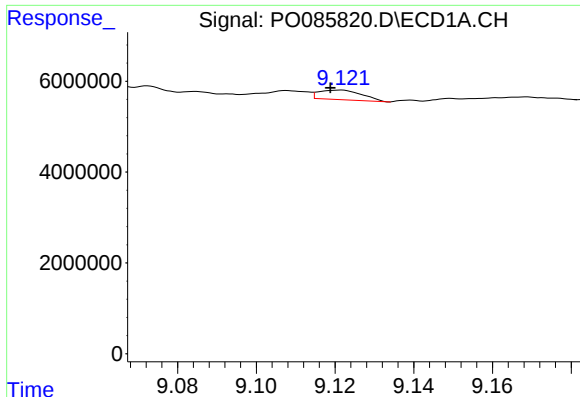

#43 AR-1268-3


R.T.: 9.122 min
Delta R.T.: 0.003 min
Response: 1586198
Conc: 96.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

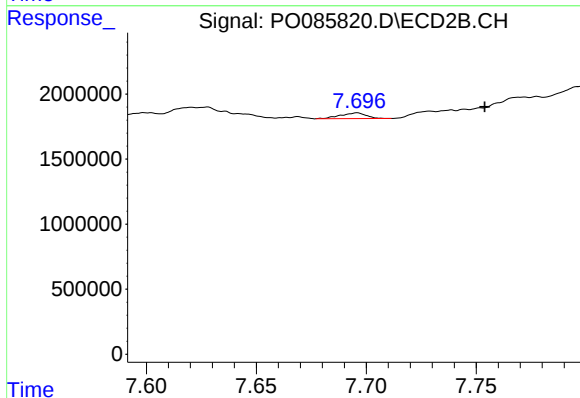


#43 AR-1268-3

R.T.: 7.696 min
Delta R.T.: -0.058 min
Response: 359917
Conc: 77.01 ng/ml

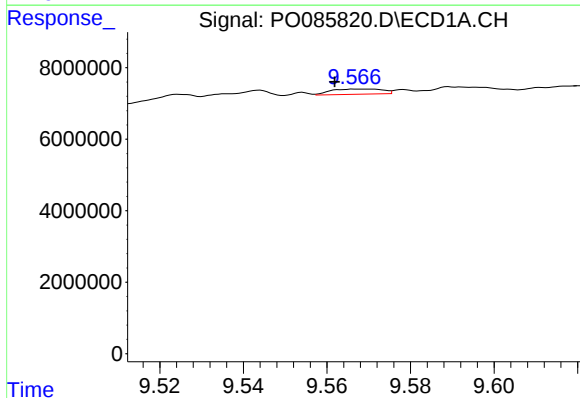


#44 AR-1268-4

R.T.: 9.567 min
Delta R.T.: 0.005 min
Response: 1243912
Conc: 176.88 ng/ml

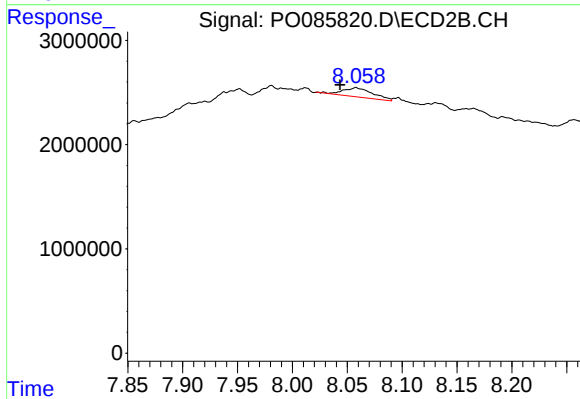

#44 AR-1268-4


R.T.: 8.058 min
Delta R.T.: 0.014 min
Response: 1701808
Conc: 812.93 ng/ml

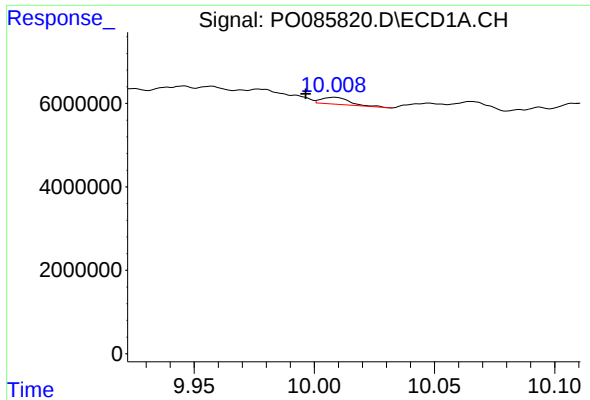

#45 AR-1268-5

R.T.: 10.008 min
Delta R.T.: 0.012 min
Response: 1374453
Conc: 24.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-032322-SR-08

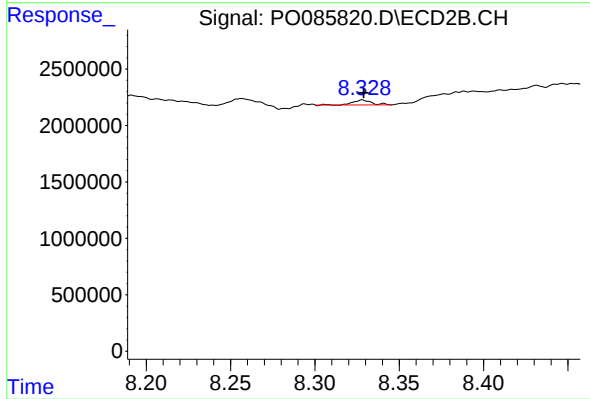

#45 AR-1268-5

R.T.: 8.328 min
Delta R.T.: 0.000 min
Response: 332750
Conc: 24.67 ng/ml