

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040221\
 Data File : P0076768.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 14:46
 Operator : DD\AJ
 Sample : M1898-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 32998

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:32:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 08:50:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.897	94873	33613	1.020	0.670m#
2)	SA Decachlor...	10.871	9.142	78704	34924	0.850m	0.720
Target Compounds							
16)	L4 AR-1242-1	6.222	5.142	470843	290818	223.062	293.769 #
17)	L4 AR-1242-2	6.246	5.162	766923	432852	217.719	203.315
18)	L4 AR-1242-3	6.311	5.351	376873	175929	169.705	188.787
19)	L4 AR-1242-4	6.434	5.447	2546298	145978	1530.789	150.932 #
20)	L4 AR-1242-5	7.202	6.008	145753	100563	74.458	83.379

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040221\
Data File : PO076768.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 14:46
Operator : DD\AJ
Sample : M1898-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
32998


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 08:50:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

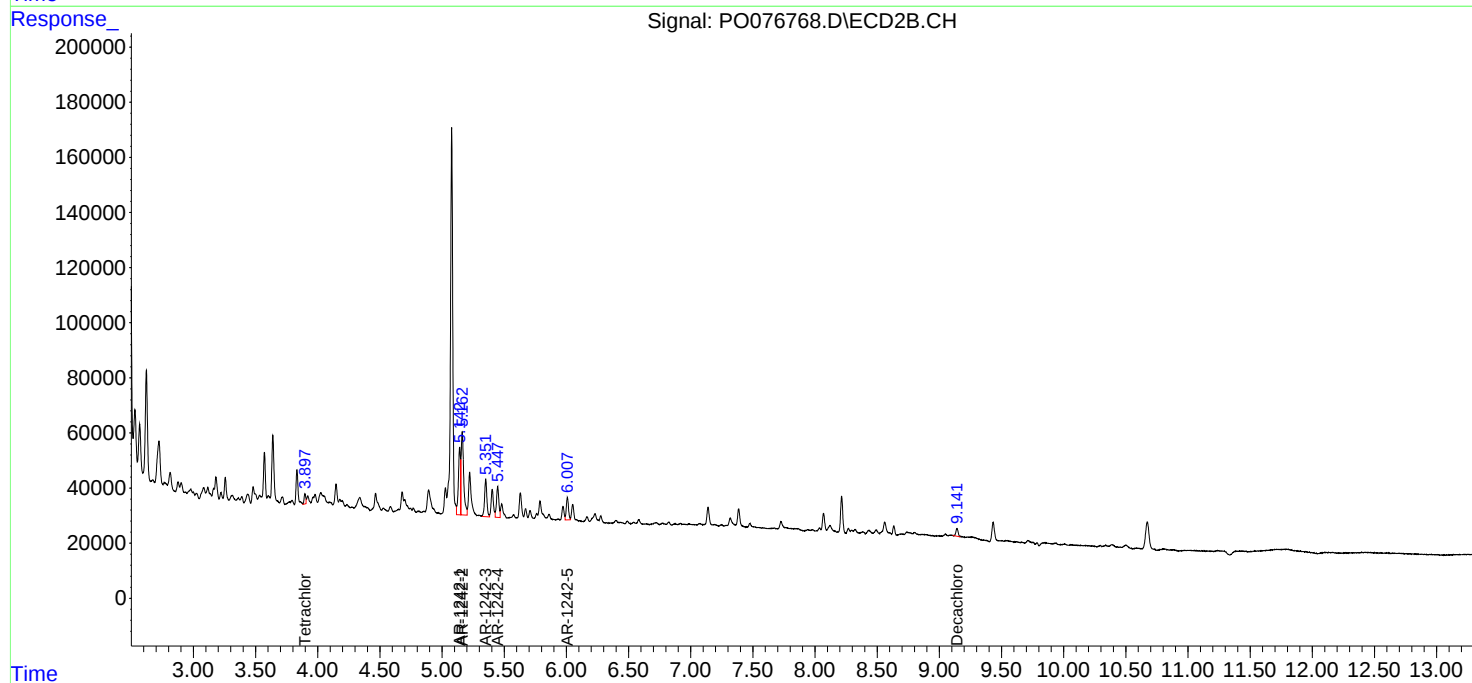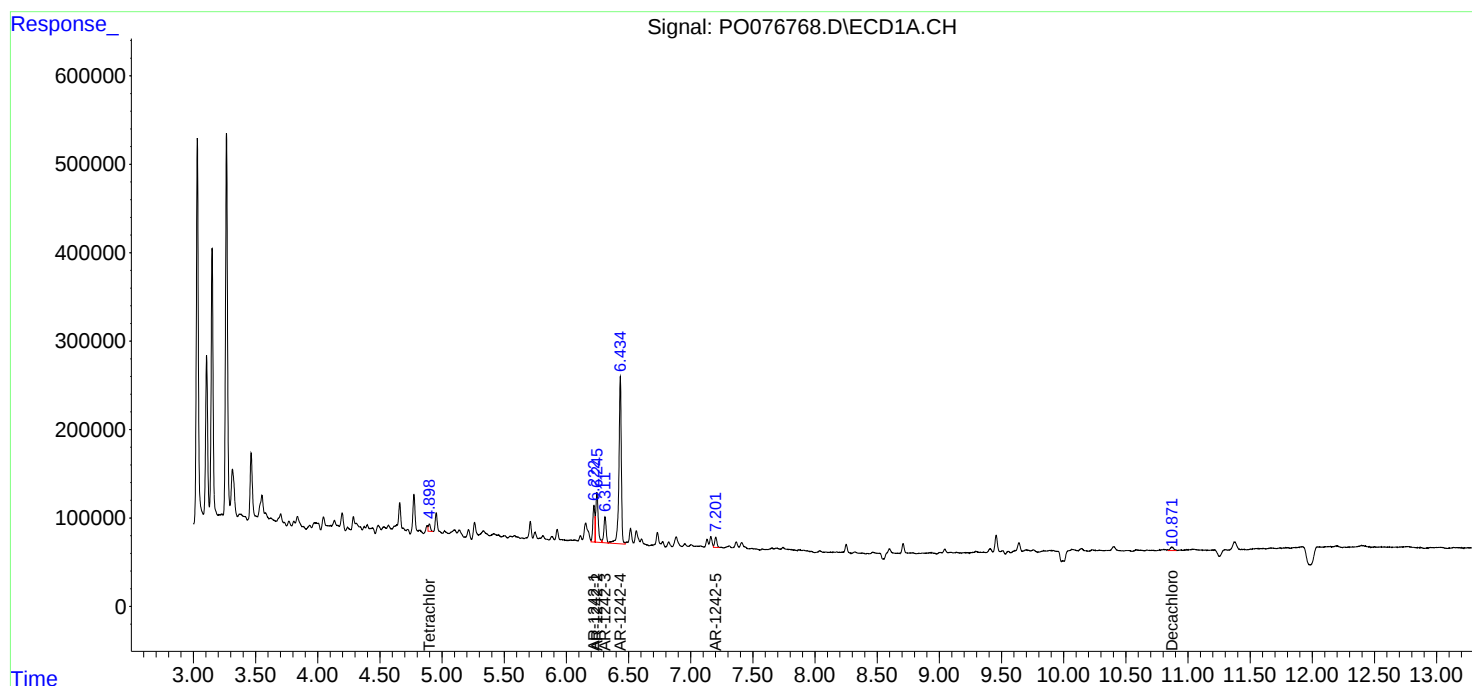

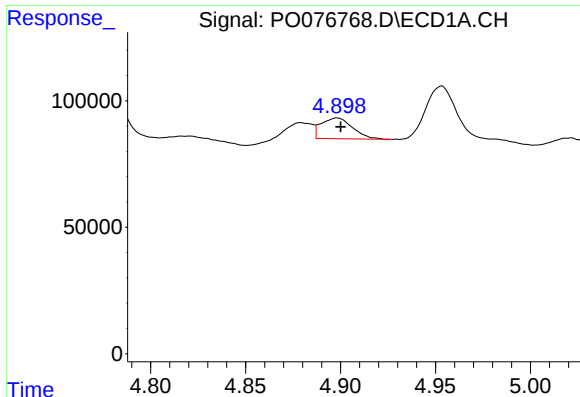


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 94873
Conc: 1.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
32998


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:49 PM

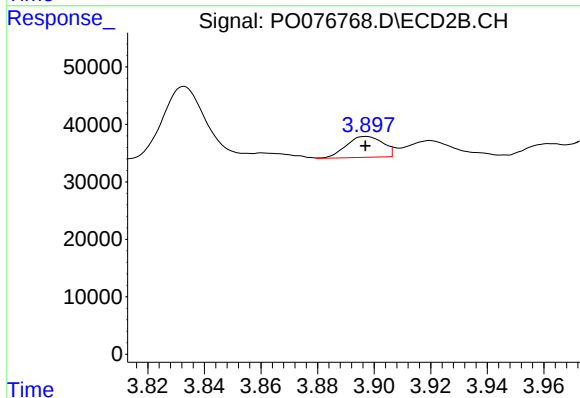


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 33613
Conc: 0.67 ng/ml m

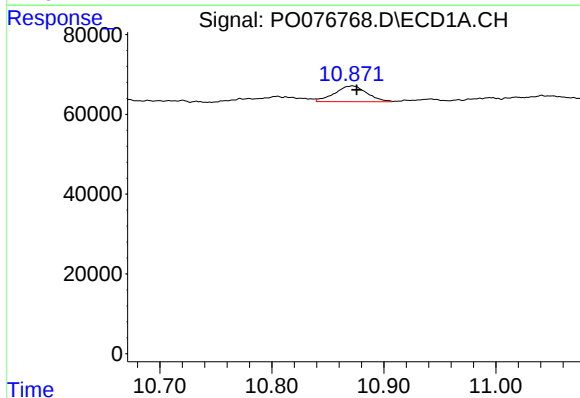


#2 Decachlorobiphenyl

R.T.: 10.871 min
Delta R.T.: -0.004 min
Response: 78704
Conc: 0.85 ng/ml m

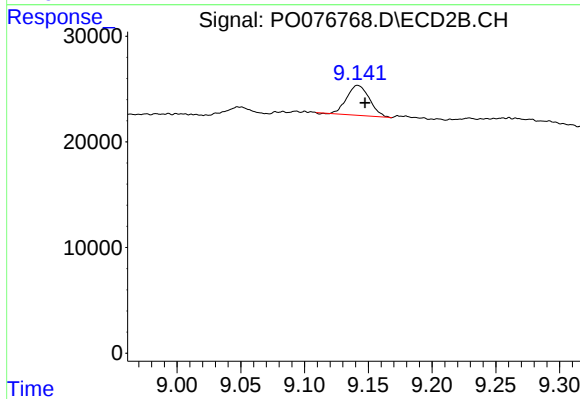

#2 Decachlorobiphenyl

R.T.: 9.142 min
Delta R.T.: -0.005 min
Response: 34924
Conc: 0.72 ng/ml

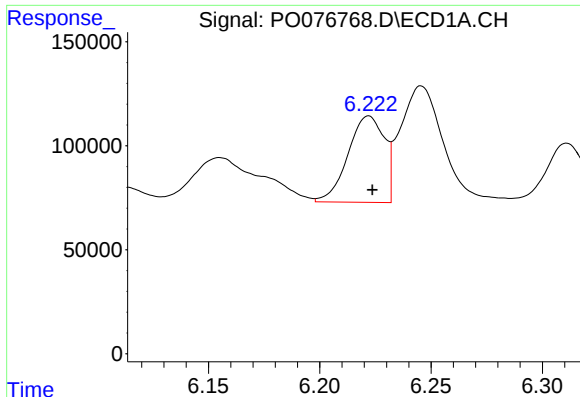


#16 AR-1242-1

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 470843
Conc: 223.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
32998


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:49 PM

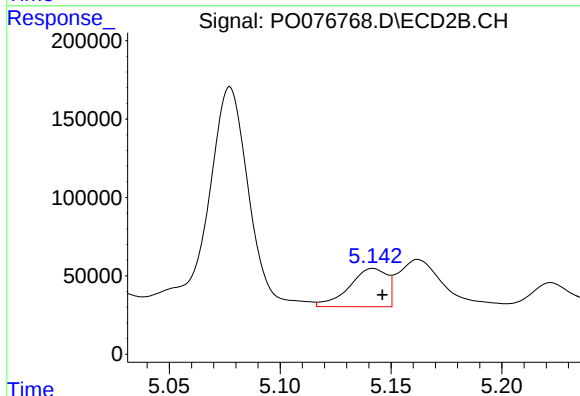


#16 AR-1242-1

R.T.: 5.142 min
Delta R.T.: -0.004 min
Response: 290818
Conc: 293.77 ng/ml

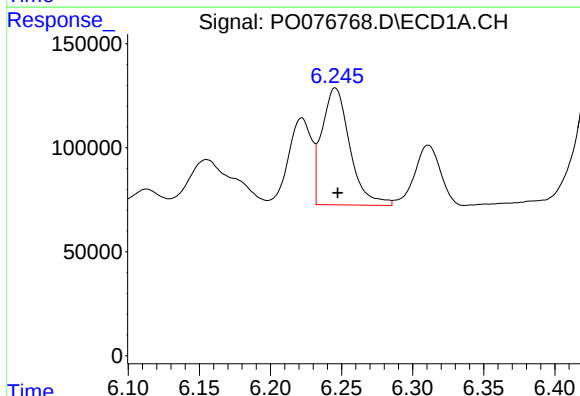


#17 AR-1242-2

R.T.: 6.246 min
Delta R.T.: -0.002 min
Response: 766923
Conc: 217.72 ng/ml

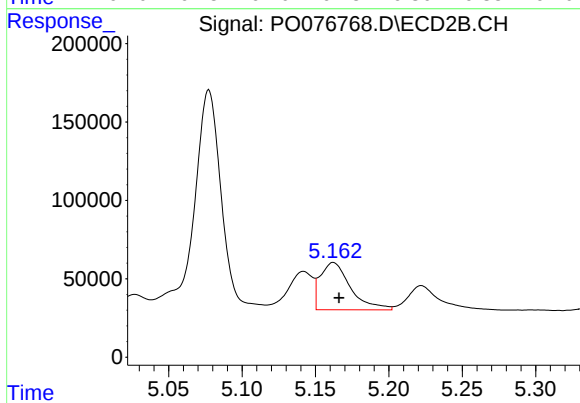

#17 AR-1242-2

R.T.: 5.162 min
Delta R.T.: -0.004 min
Response: 432852
Conc: 203.32 ng/ml

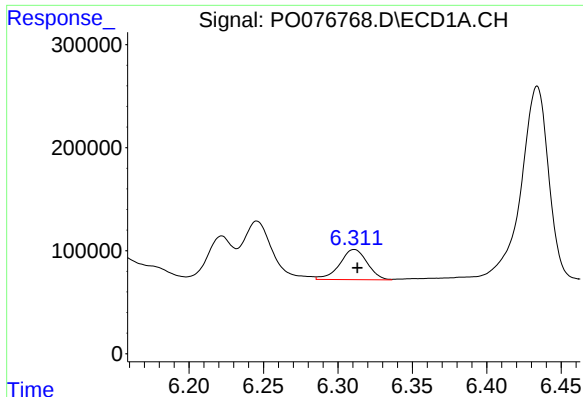


#18 AR-1242-3

R.T.: 6.311 min
Delta R.T.: -0.002 min
Response: 376873
Conc: 169.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
32998


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:49 PM

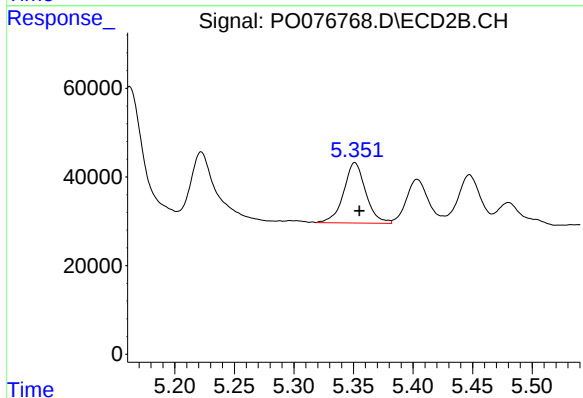


#18 AR-1242-3

R.T.: 5.351 min
Delta R.T.: -0.004 min
Response: 175929
Conc: 188.79 ng/ml

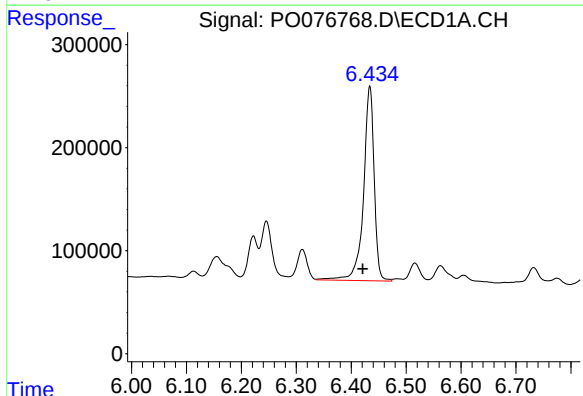


#19 AR-1242-4

R.T.: 6.434 min
Delta R.T.: 0.013 min
Response: 2546298
Conc: 1530.79 ng/ml

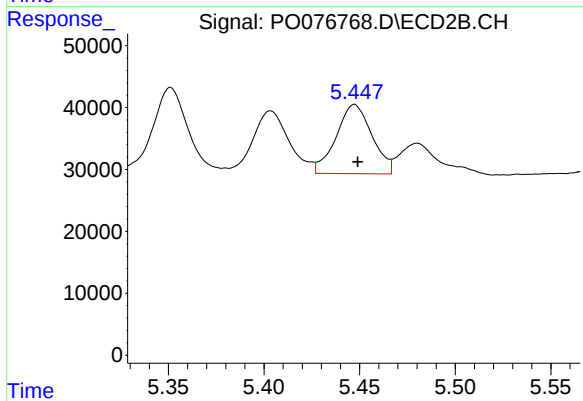

#19 AR-1242-4

R.T.: 5.447 min
Delta R.T.: -0.002 min
Response: 145978
Conc: 150.93 ng/ml

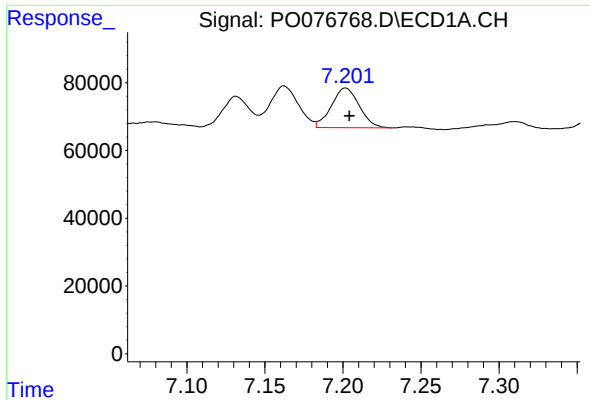


#20 AR-1242-5

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 145753
Conc: 74.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
32998

Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:49 PM

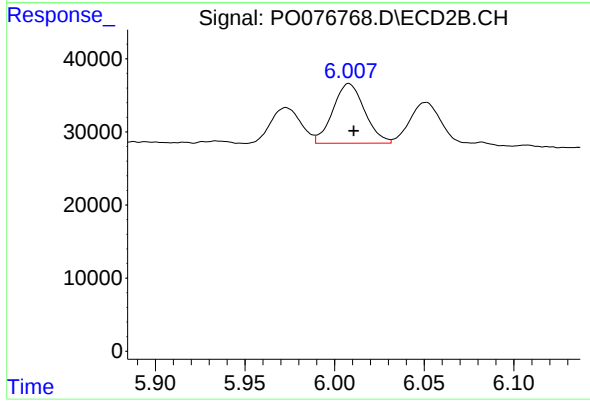

#20 AR-1242-5

R.T.: 6.008 min
Delta R.T.: -0.003 min
Response: 100563
Conc: 83.38 ng/ml