

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040221\
 Data File : P0076781.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 18:46
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:32:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:07:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.899	3.897	4885473	2554171	52.524	50.898
2) SA Decachlor...	10.870	9.141	4654388	2148814	50.252	44.282
Target Compounds						
26) L6 AR-1254-1	7.130	6.005	1708306	1465751	537.451m	559.206m
27) L6 AR-1254-2	7.360	6.164	2898397	1270316	565.687	554.720m
28) L6 AR-1254-3	7.741	6.581	3225412	1921858	585.315	543.776m
29) L6 AR-1254-4	8.038	6.821	2278057	1164540	578.588m	554.890m
30) L6 AR-1254-5	8.466	7.245	2453574	1797886	557.868	551.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040221\
Data File : P0076781.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 18:46
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:07:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

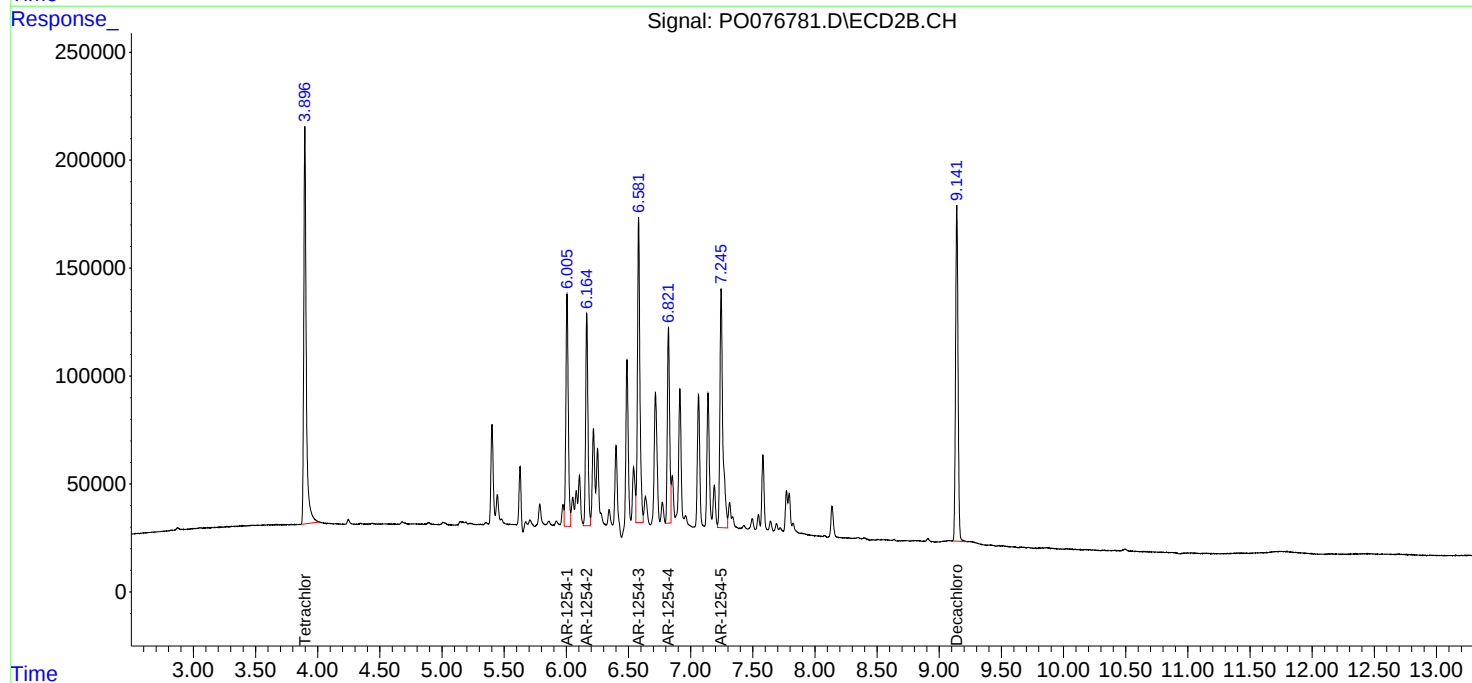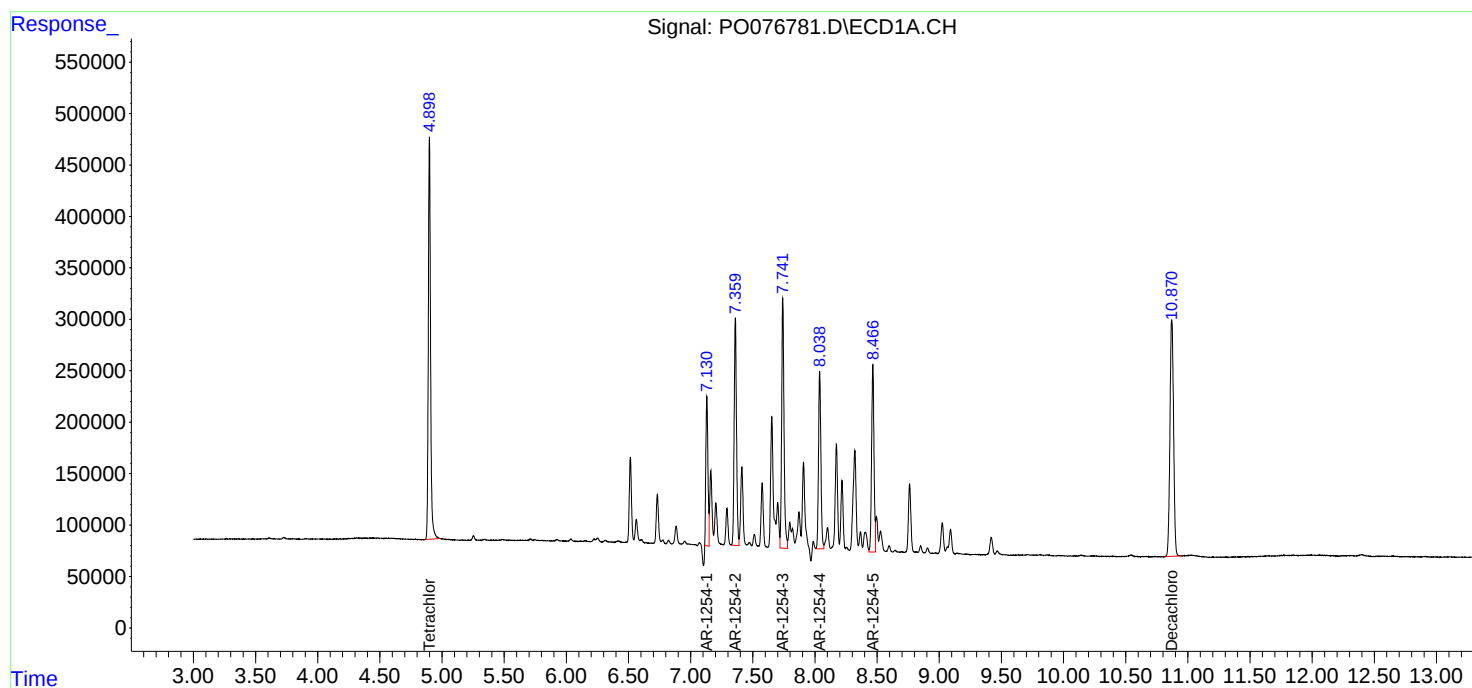

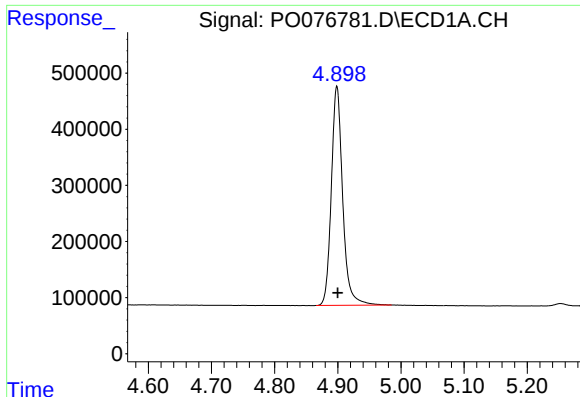


#1 Tetrachloro-m-xylene

R.T.: 4.899 min
Delta R.T.: -0.001 min
Response: 4885473
Conc: 52.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:58 PM

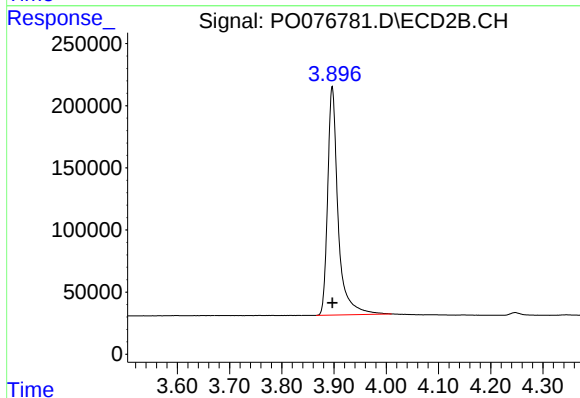


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 2554171
Conc: 50.90 ng/ml

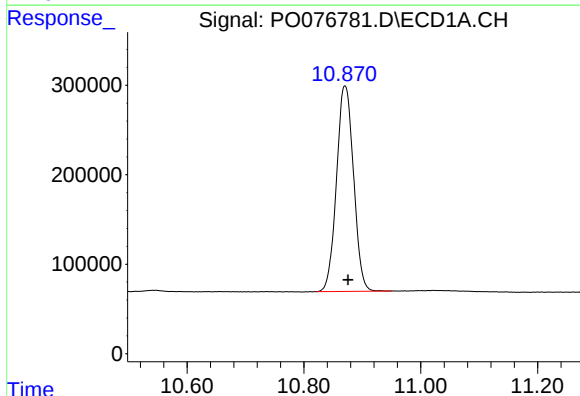


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.006 min
Response: 4654388
Conc: 50.25 ng/ml

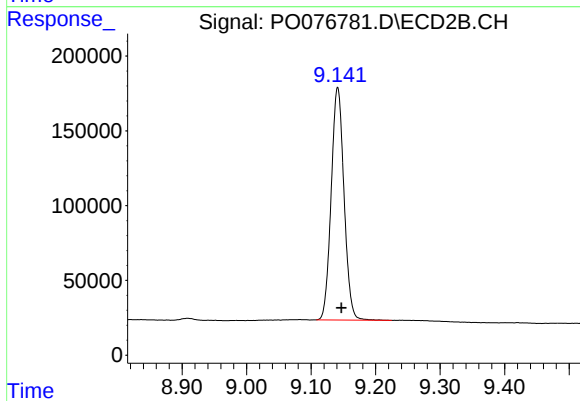

#2 Decachlorobiphenyl

R.T.: 9.141 min
Delta R.T.: -0.006 min
Response: 2148814
Conc: 44.28 ng/ml

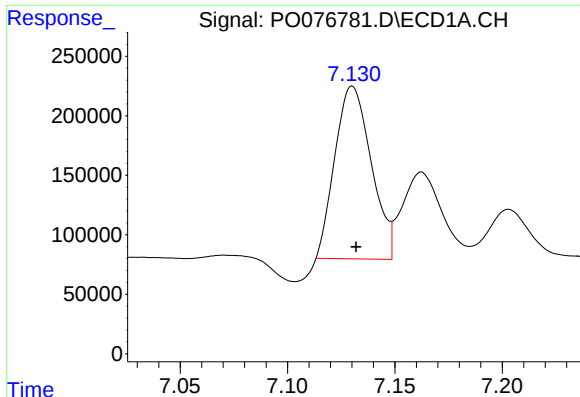


#26 AR-1254-1

R.T.: 7.130 min
Delta R.T.: -0.002 min
Response: 1708306
Conc: 537.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:58 PM

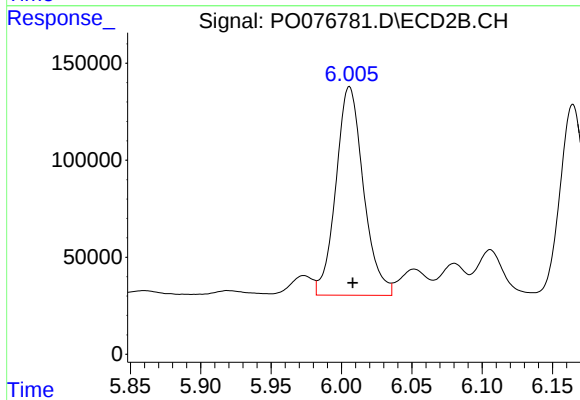


#26 AR-1254-1

R.T.: 6.005 min
Delta R.T.: -0.003 min
Response: 1465751
Conc: 559.21 ng/ml m

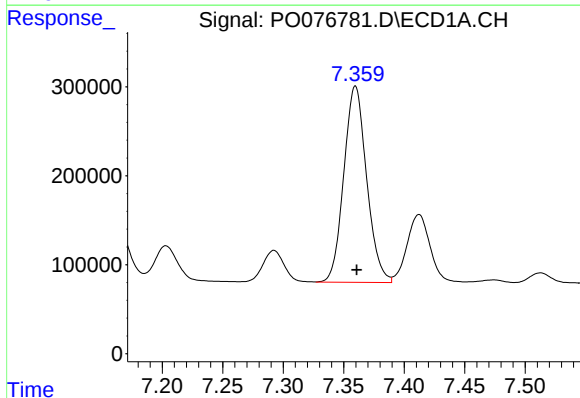


#27 AR-1254-2

R.T.: 7.360 min
Delta R.T.: -0.001 min
Response: 2898397
Conc: 565.69 ng/ml

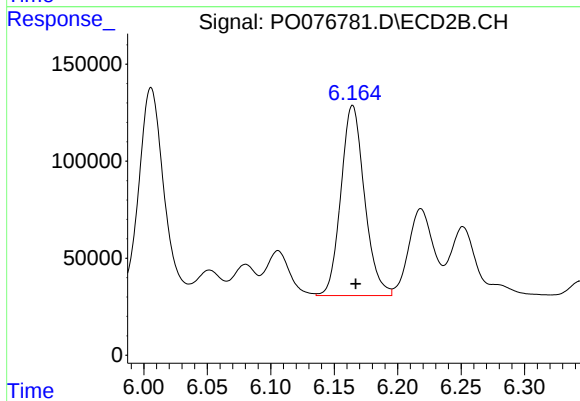

#27 AR-1254-2

R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 1270316
Conc: 554.72 ng/ml m

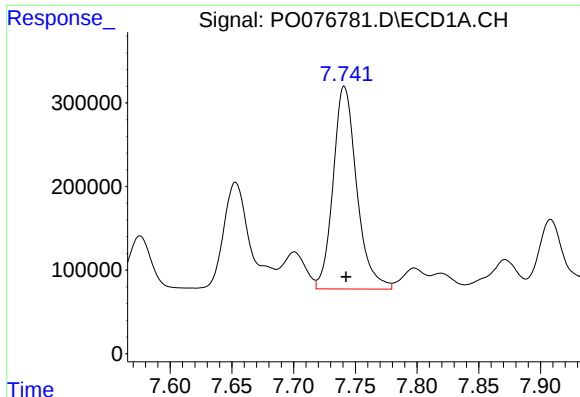


#28 AR-1254-3

R.T.: 7.741 min
Delta R.T.: -0.001 min
Response: 3225412
Conc: 585.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:58 PM

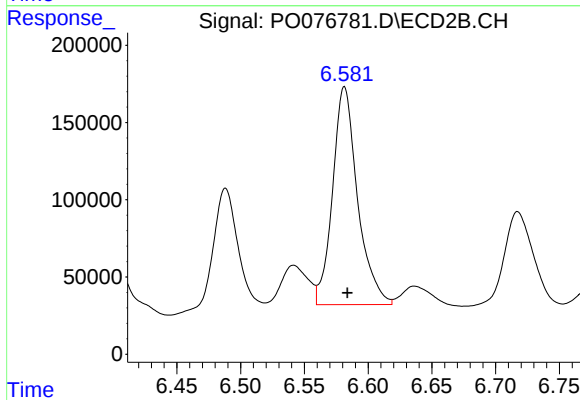


#28 AR-1254-3

R.T.: 6.581 min
Delta R.T.: -0.003 min
Response: 1921858
Conc: 543.78 ng/ml m

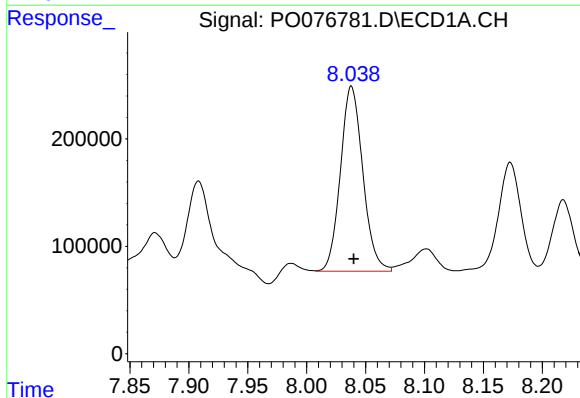


#29 AR-1254-4

R.T.: 8.038 min
Delta R.T.: -0.003 min
Response: 2278057
Conc: 578.59 ng/ml m

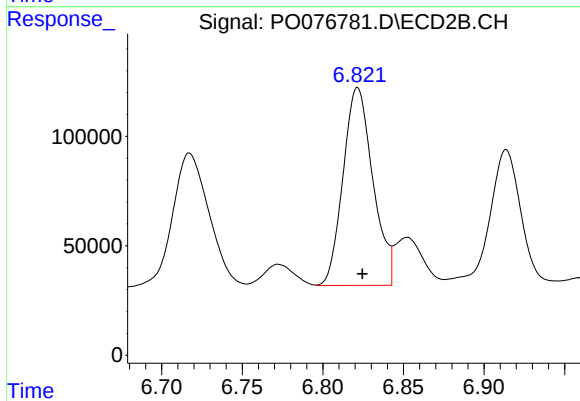

#29 AR-1254-4

R.T.: 6.821 min
Delta R.T.: -0.003 min
Response: 1164540
Conc: 554.89 ng/ml m

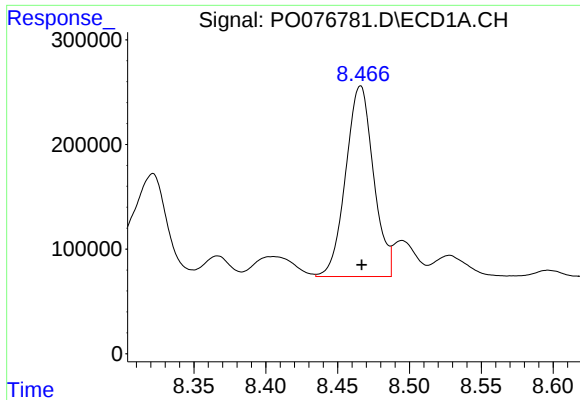


#30 AR-1254-5

R.T.: 8.466 min
Delta R.T.: 0.000 min
Response: 2453574
Conc: 557.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
4/5/2021 3:32:58 PM

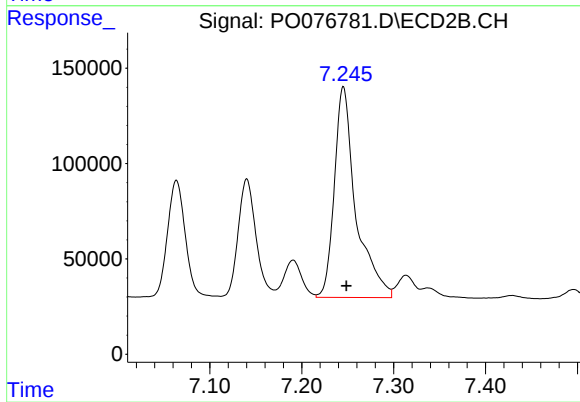

#30 AR-1254-5

R.T.: 7.245 min
Delta R.T.: -0.003 min
Response: 1797886
Conc: 551.50 ng/ml