

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040221\
 Data File : P0076785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 19:55
 Operator : DD\AJ
 Sample : M1903-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41749

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:33:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:10:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.896	1437086	797457	15.450	15.891
2) SA Decachlor...	10.870	9.141	608059	297558	6.565m	6.132m
Target Compounds						
16) L4 AR-1242-1	6.219	5.141	401984	134486	190.440	135.851 #
17) L4 AR-1242-2	6.245	5.161	306050	237662	86.883	111.632 #
18) L4 AR-1242-3	6.310	5.350	198805	117253	89.522	125.822 #
19) L4 AR-1242-4	6.417	5.446	144509	154505	86.876	159.750 #
20) L4 AR-1242-5	7.201	6.006	290519	245811	148.412	203.807 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040221\
Data File : PO076785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 19:55
Operator : DD\AJ
Sample : M1903-06
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41749


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:10:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

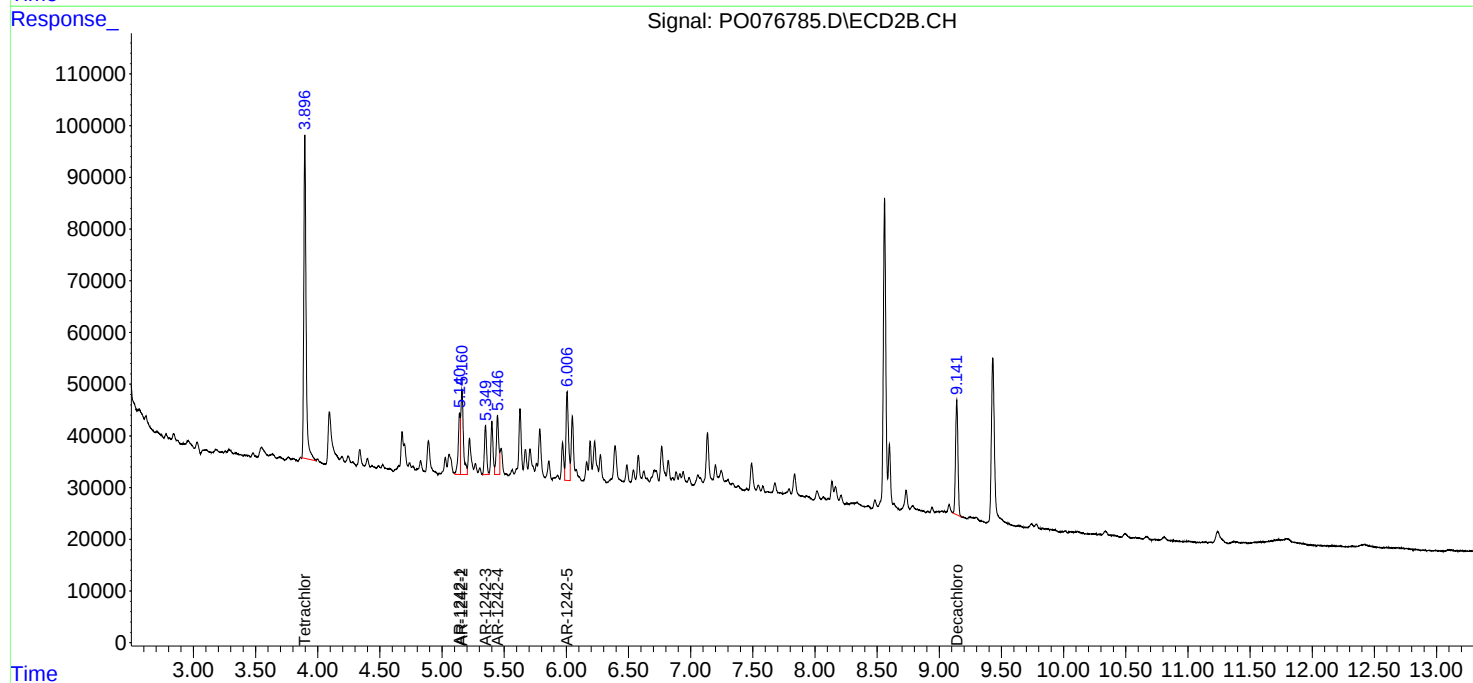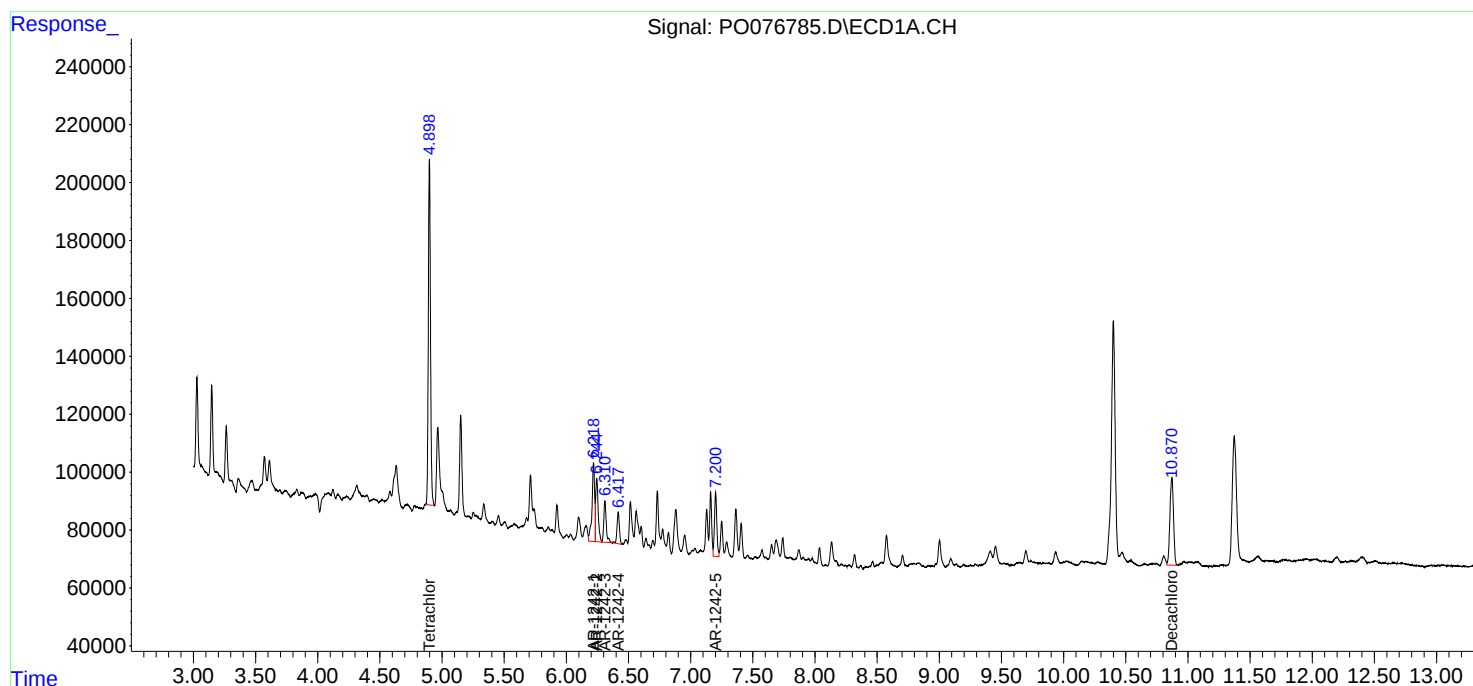

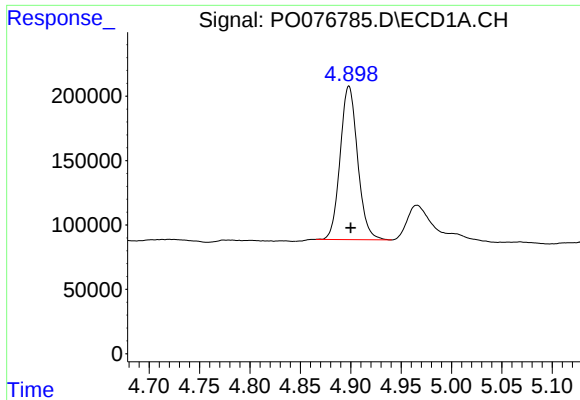


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 1437086
Conc: 15.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
41749


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:03 PM

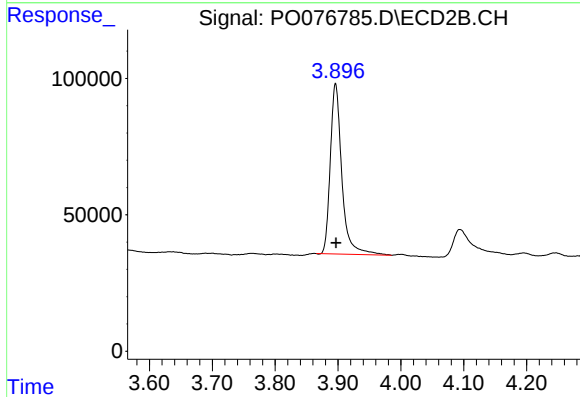


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 797457
Conc: 15.89 ng/ml

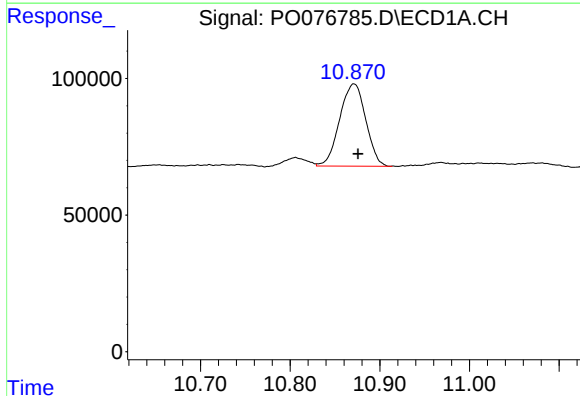


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.005 min
Response: 608059
Conc: 6.57 ng/ml m

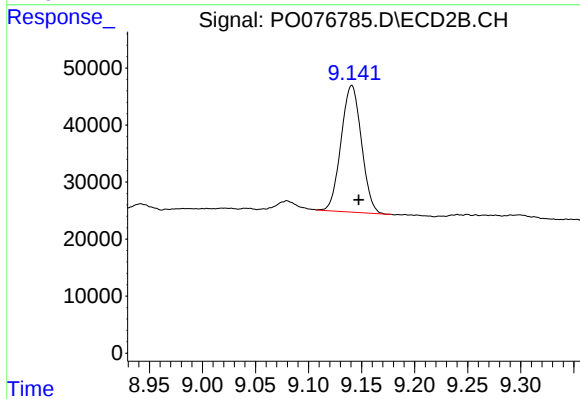

#2 Decachlorobiphenyl

R.T.: 9.141 min
Delta R.T.: -0.007 min
Response: 297558
Conc: 6.13 ng/ml m

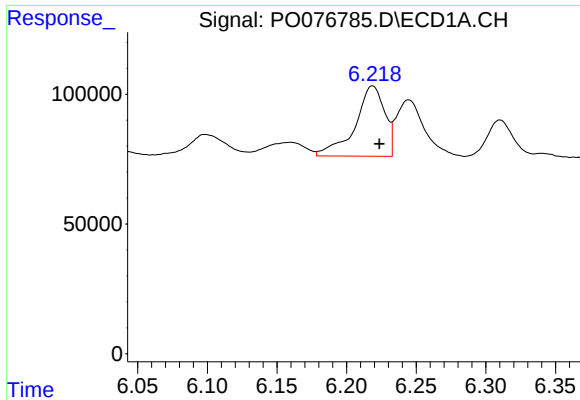


#16 AR-1242-1

R.T.: 6.219 min
Delta R.T.: -0.005 min
Response: 401984
Conc: 190.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
41749


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:03 PM

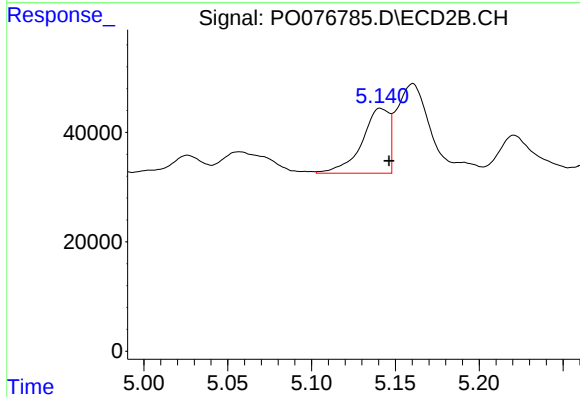


#16 AR-1242-1

R.T.: 5.141 min
Delta R.T.: -0.005 min
Response: 134486
Conc: 135.85 ng/ml

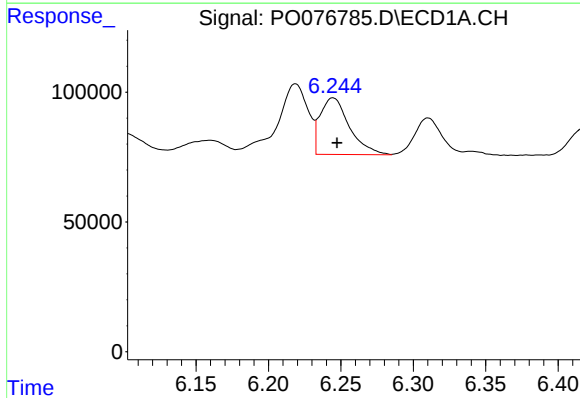


#17 AR-1242-2

R.T.: 6.245 min
Delta R.T.: -0.003 min
Response: 306050
Conc: 86.88 ng/ml

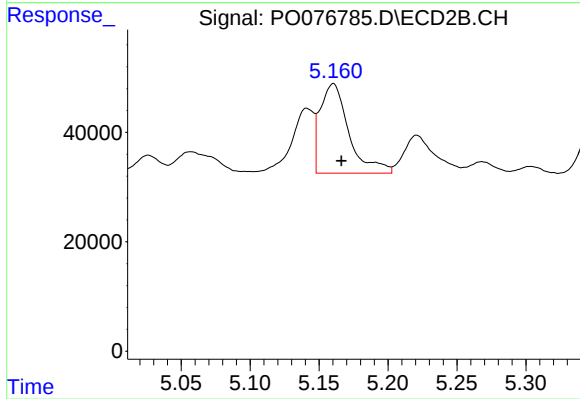

#17 AR-1242-2

R.T.: 5.161 min
Delta R.T.: -0.005 min
Response: 237662
Conc: 111.63 ng/ml

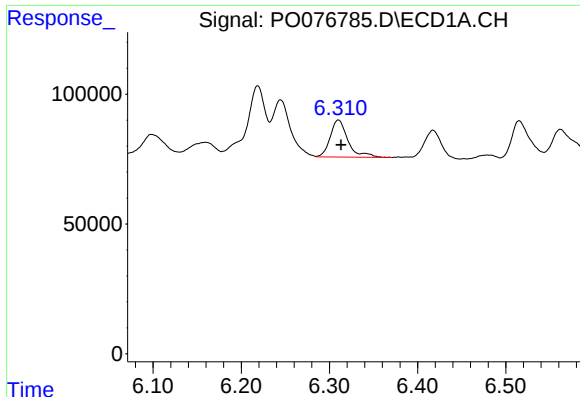


#18 AR-1242-3

R.T.: 6.310 min
Delta R.T.: -0.003 min
Response: 198805
Conc: 89.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
41749


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:03 PM

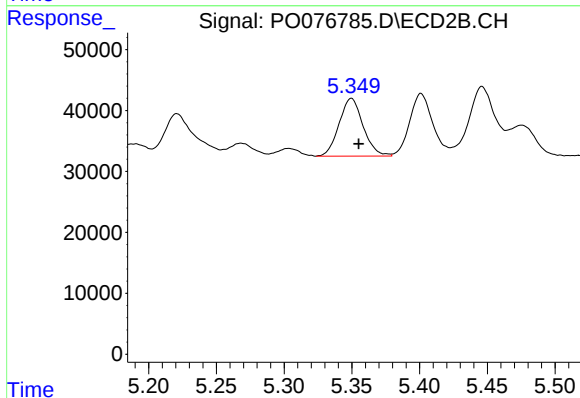


#18 AR-1242-3

R.T.: 5.350 min
Delta R.T.: -0.005 min
Response: 117253
Conc: 125.82 ng/ml

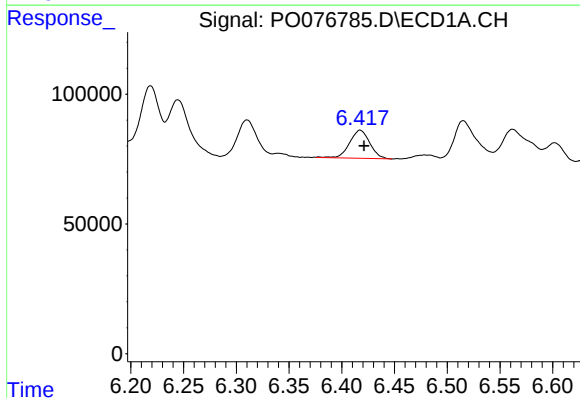


#19 AR-1242-4

R.T.: 6.417 min
Delta R.T.: -0.003 min
Response: 144509
Conc: 86.88 ng/ml

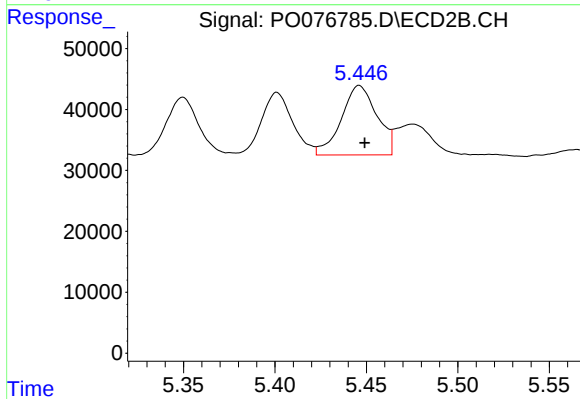

#19 AR-1242-4

R.T.: 5.446 min
Delta R.T.: -0.003 min
Response: 154505
Conc: 159.75 ng/ml

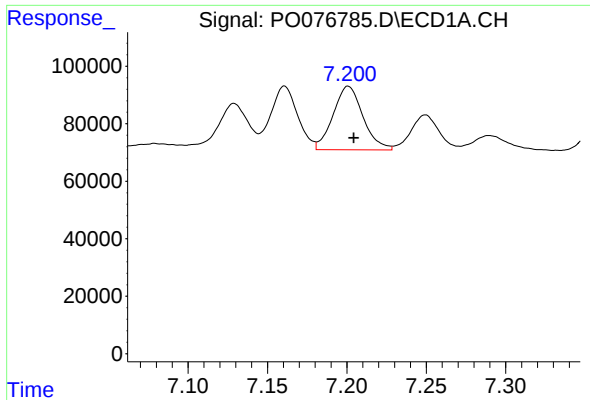


#20 AR-1242-5

R.T.: 7.201 min
Delta R.T.: -0.003 min
Response: 290519
Conc: 148.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
41749

Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:03 PM

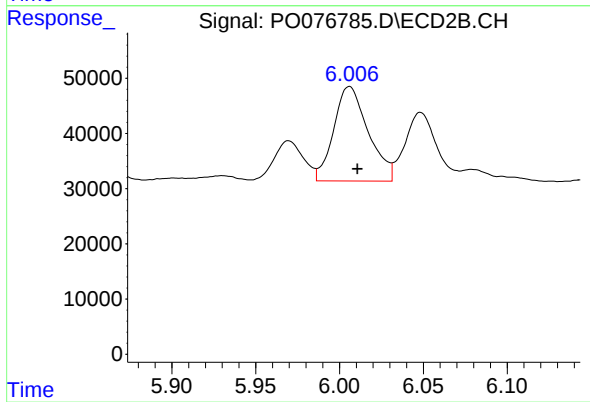

#20 AR-1242-5

R.T.: 6.006 min
Delta R.T.: -0.005 min
Response: 245811
Conc: 203.81 ng/ml