

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040221\
 Data File : P0076787.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 20:29
 Operator : DD\AJ
 Sample : M1903-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31030

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:33:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 01:11:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.899	3.896	1519970	838195	16.341	16.703
2) SA Decachlor...	10.871	9.141	777361	381532	8.393	7.862
Target Compounds						
16) L4 AR-1242-1	6.218	5.142	322001	90611	152.548	91.530 #
17) L4 AR-1242-2	6.245	5.161	205503	164947	58.339	77.477 #
18) L4 AR-1242-3	6.310	5.350	133225	76813	59.991m	82.427 #
19) L4 AR-1242-4	6.418	5.446	98502	101809	59.218	105.265 #
20) L4 AR-1242-5	7.200	6.006	204476	146428	104.457	121.407

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040221\
Data File : PO076787.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 20:29
Operator : DD\AJ
Sample : M1903-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31030


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 01:11:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

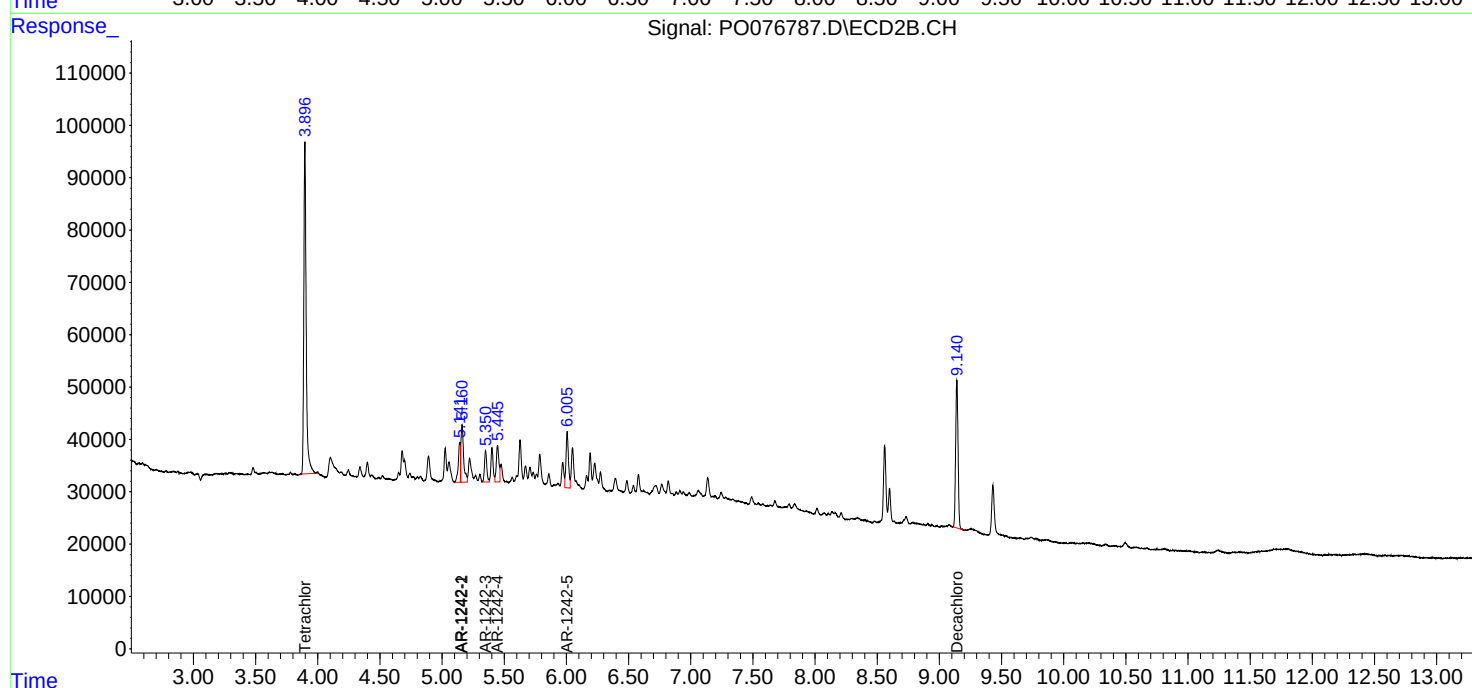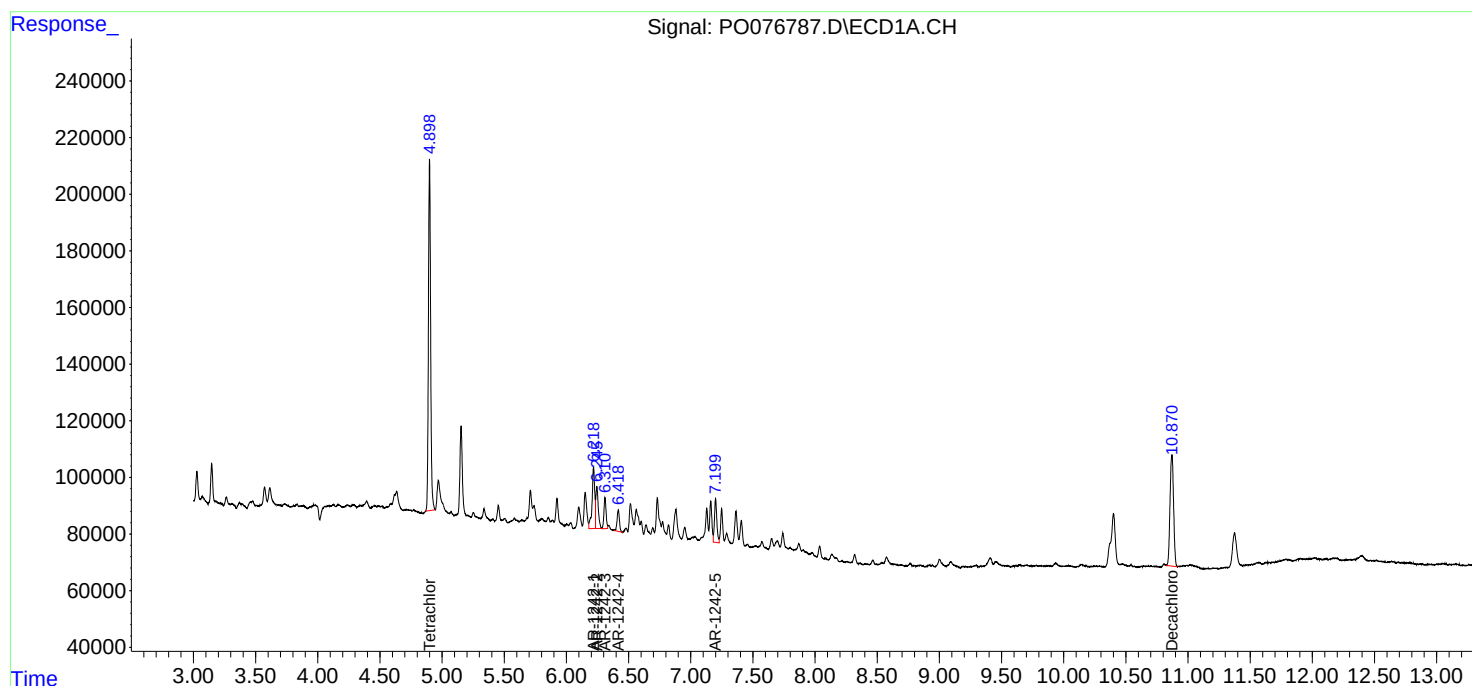

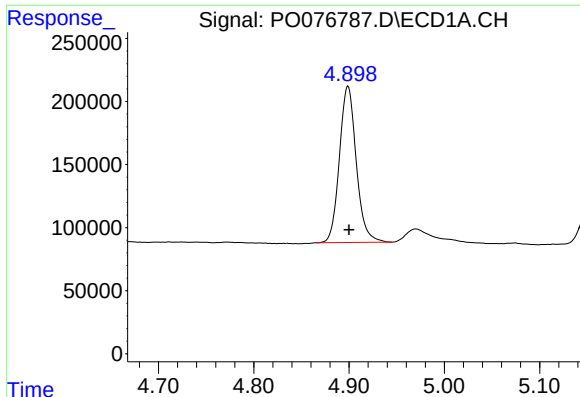


#1 Tetrachloro-m-xylene

R.T.: 4.899 min
Delta R.T.: -0.001 min
Response: 1519970
Conc: 16.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
31030


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:05 PM

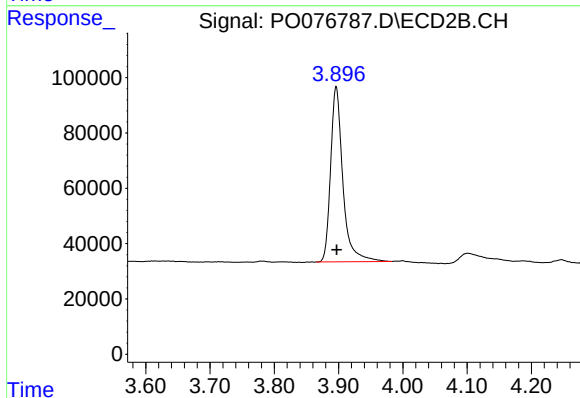


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 838195
Conc: 16.70 ng/ml

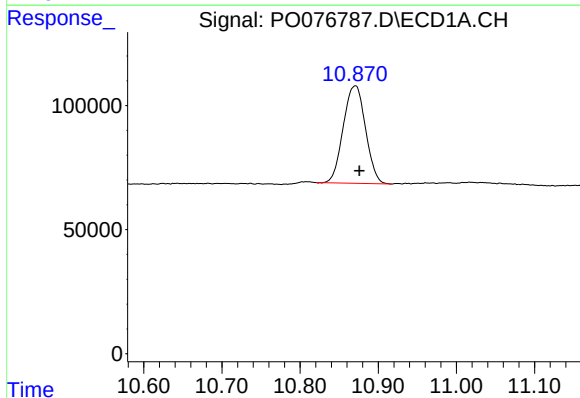


#2 Decachlorobiphenyl

R.T.: 10.871 min
Delta R.T.: -0.005 min
Response: 777361
Conc: 8.39 ng/ml

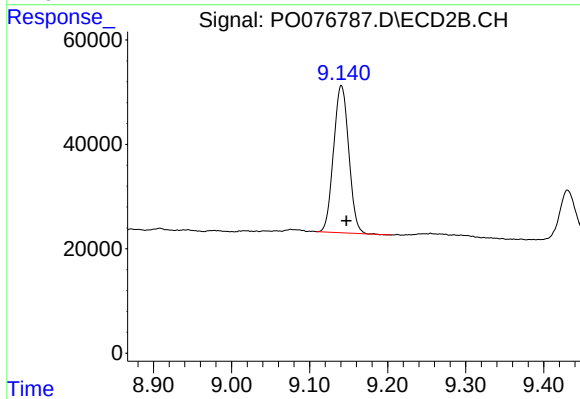

#2 Decachlorobiphenyl

R.T.: 9.141 min
Delta R.T.: -0.007 min
Response: 381532
Conc: 7.86 ng/ml

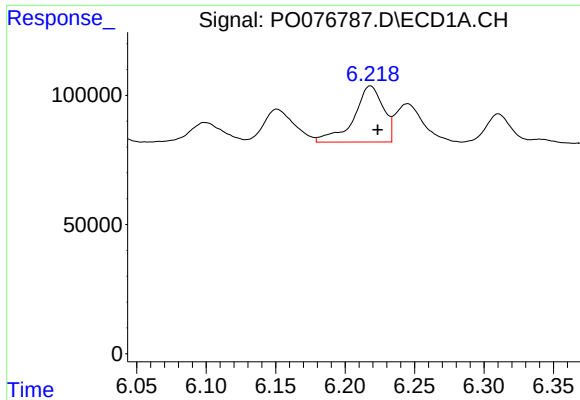


#16 AR-1242-1

R.T.: 6.218 min
Delta R.T.: -0.005 min
Response: 322001
Conc: 152.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
31030


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:05 PM

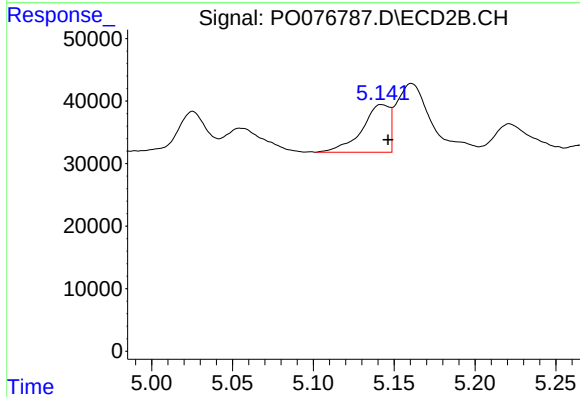


#16 AR-1242-1

R.T.: 5.142 min
Delta R.T.: -0.004 min
Response: 90611
Conc: 91.53 ng/ml

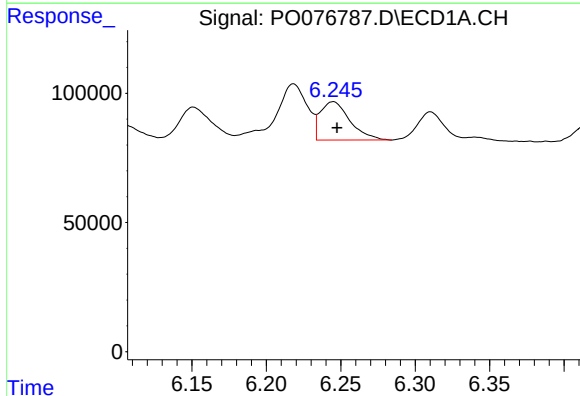


#17 AR-1242-2

R.T.: 6.245 min
Delta R.T.: -0.002 min
Response: 205503
Conc: 58.34 ng/ml

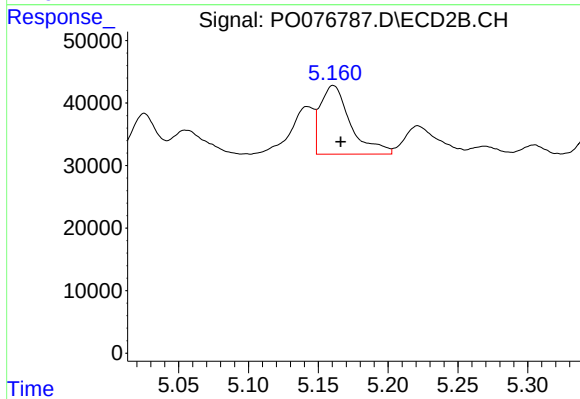

#17 AR-1242-2

R.T.: 5.161 min
Delta R.T.: -0.005 min
Response: 164947
Conc: 77.48 ng/ml

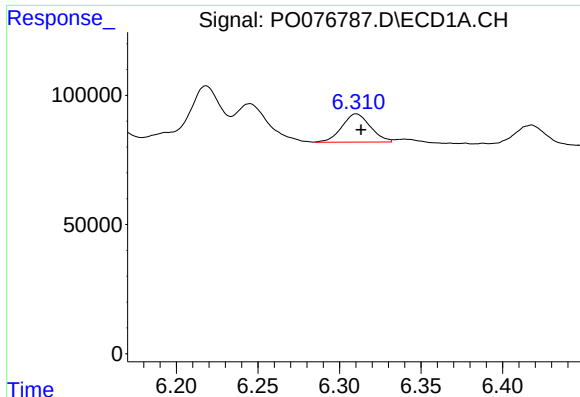


#18 AR-1242-3

R.T.: 6.310 min
Delta R.T.: -0.003 min
Response: 133225
Conc: 59.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31030


Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:05 PM

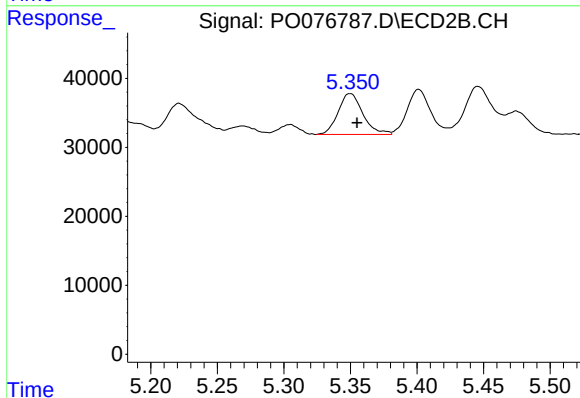


#18 AR-1242-3

R.T.: 5.350 min
Delta R.T.: -0.005 min
Response: 76813
Conc: 82.43 ng/ml

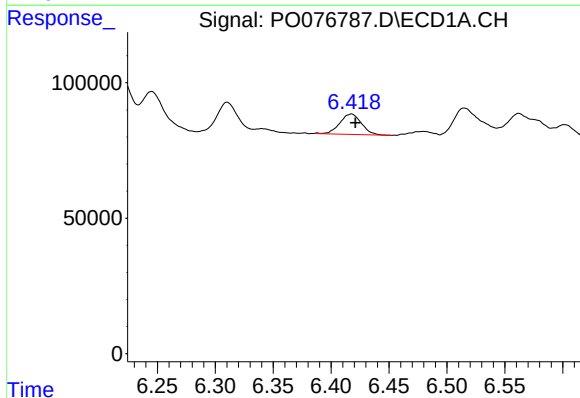


#19 AR-1242-4

R.T.: 6.418 min
Delta R.T.: -0.003 min
Response: 98502
Conc: 59.22 ng/ml

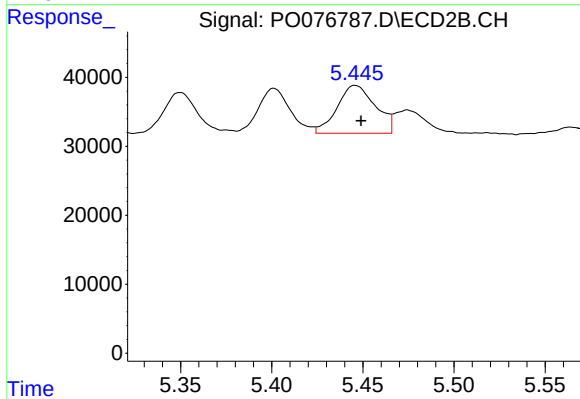

#19 AR-1242-4

R.T.: 5.446 min
Delta R.T.: -0.003 min
Response: 101809
Conc: 105.26 ng/ml

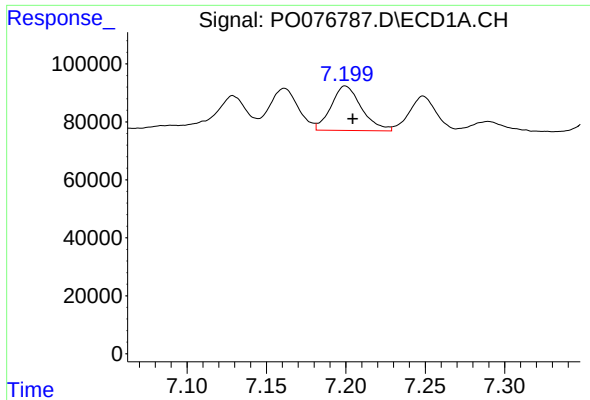


#20 AR-1242-5

R.T.: 7.200 min
Delta R.T.: -0.005 min
Response: 204476
Conc: 104.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
31030

Manual Integrations
APPROVED

Ankita
4/5/2021 3:33:05 PM

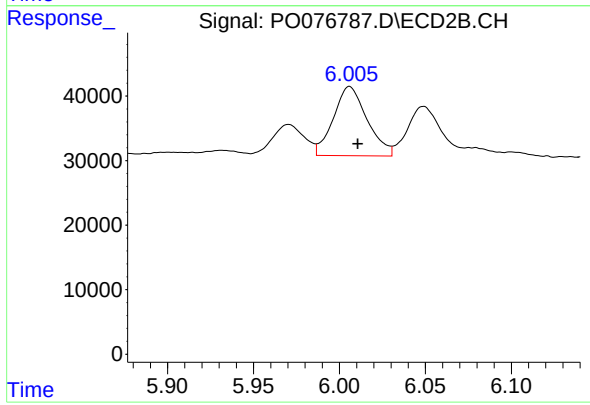

#20 AR-1242-5

R.T.: 6.006 min
Delta R.T.: -0.005 min
Response: 146428
Conc: 121.41 ng/ml