

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040225\
 Data File : P0110190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2025 14:05
 Operator : YP/AJ
 Sample : Q1693-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WCS-TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 14:19:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.689	3.687	179.6E6	101.5E6	19.730	19.364
2) SA Decachlor...	8.737	8.687	131.6E6	37386798	17.113	15.410

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040225\
Data File : PO110190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2025 14:05
Operator : YP/AJ
Sample : Q1693-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WCS-TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 14:19:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

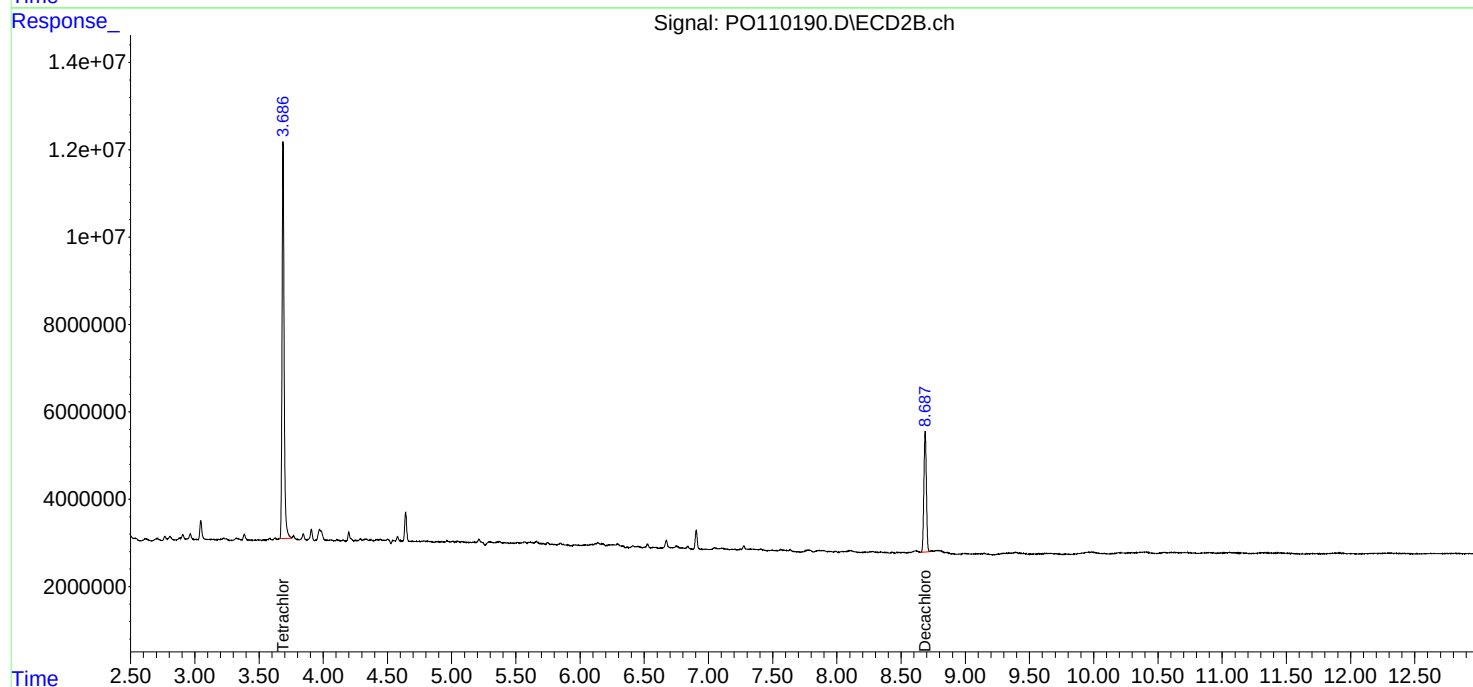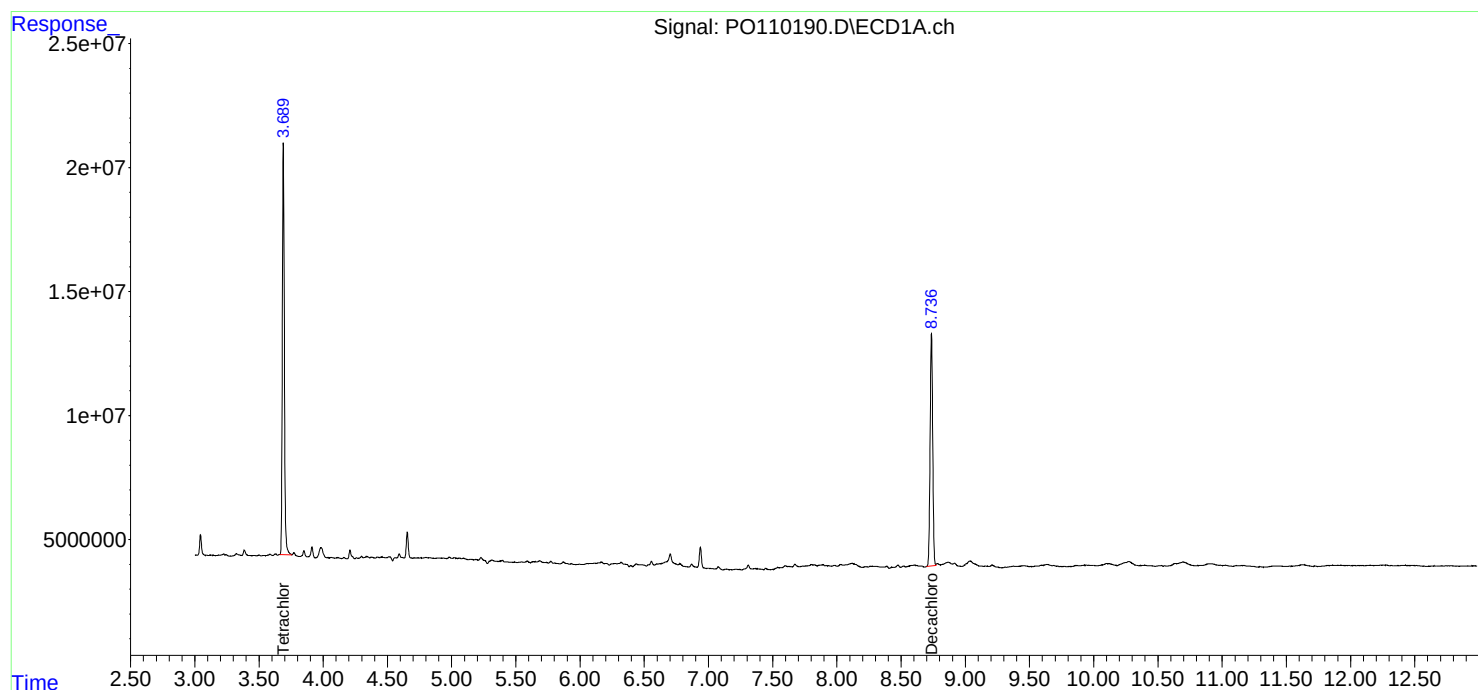


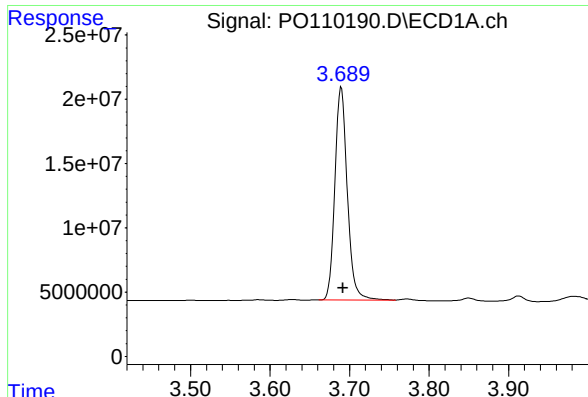

#1 Tetrachloro-m-xylene


R.T.: 3.689 min
Delta R.T.: -0.003 min
Response: 179571076
Conc: 19.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
WCS-TP-3

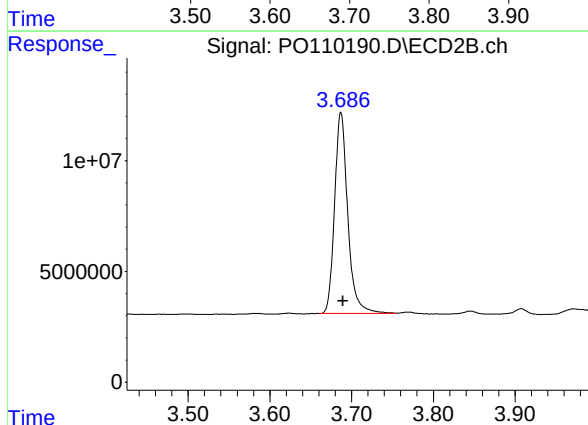


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: -0.003 min
Response: 101549309
Conc: 19.36 ng/ml

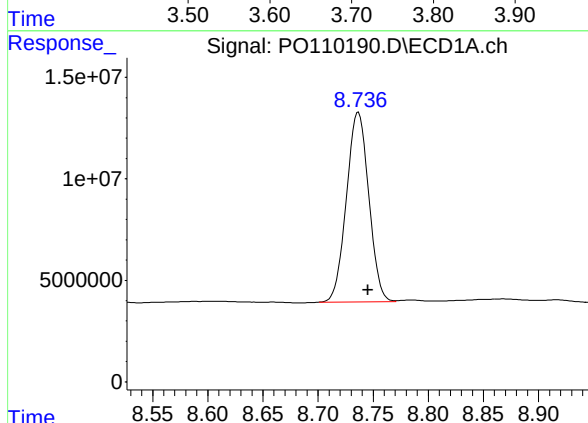

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.009 min
Response: 131574809
Conc: 17.11 ng/ml

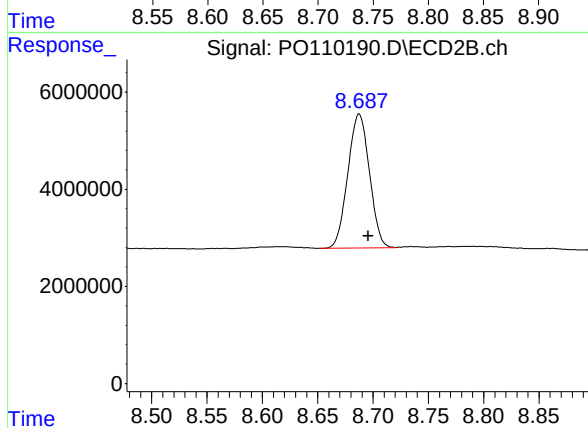

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: -0.008 min
Response: 37386798
Conc: 15.41 ng/ml