

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040321\
 Data File : P0076798.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2021 2:36
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 4/6/2021 2:58:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 15:56:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.899	3.897	4851254	2507273	52.156	49.963
2) SA Decachlor...	10.870	9.141	4654476	2140296	50.253	44.106
Target Compounds						
26) L6 AR-1254-1	7.131	6.005	1801090	1418101	566.642m	541.027m
27) L6 AR-1254-2	7.361	6.164	2971938	1284290	580.041	560.823m
28) L6 AR-1254-3	7.743	6.581	3354709	2032764	608.778	575.156m
29) L6 AR-1254-4	8.039	6.821	2402592	1200400	610.217	571.977m
30) L6 AR-1254-5	8.466	7.245	2455419	1798843	558.288	551.790

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040321\
Data File : P0076798.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2021 2:36
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/6/2021 2:58:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 15:56:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

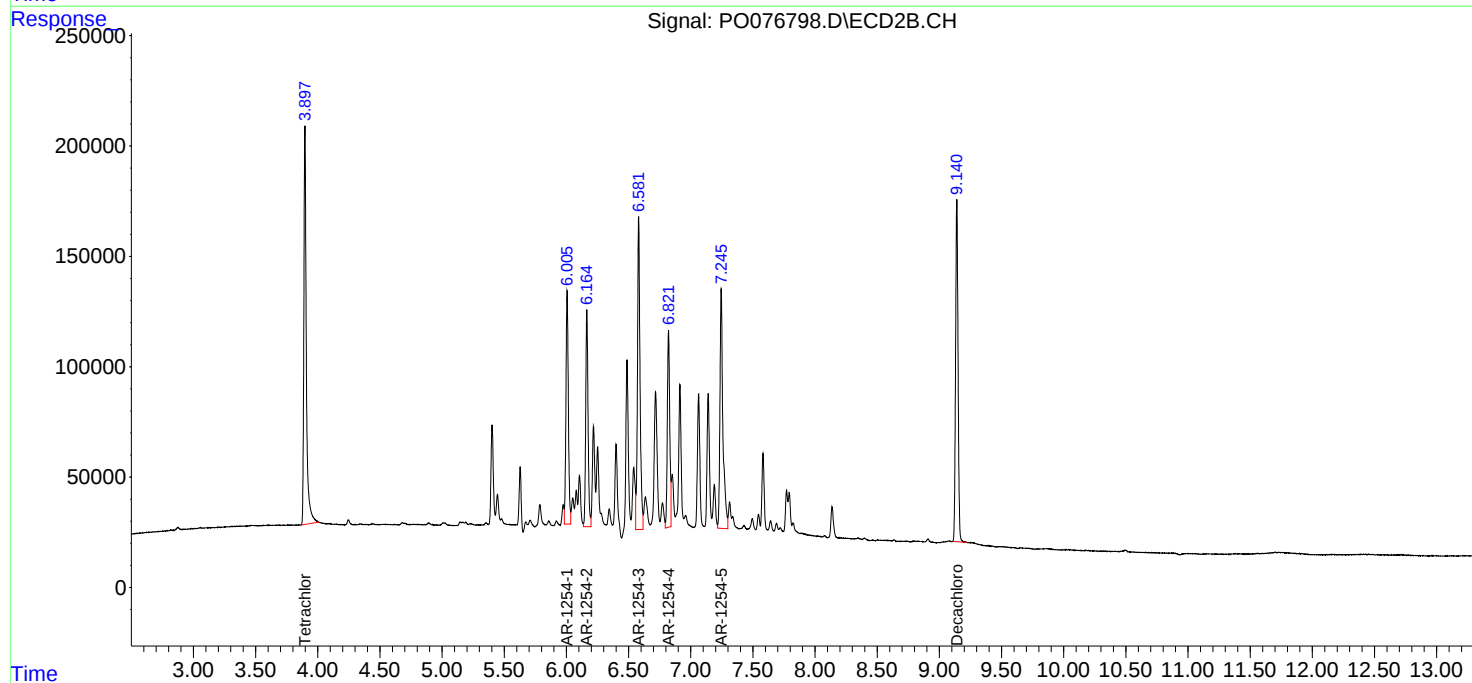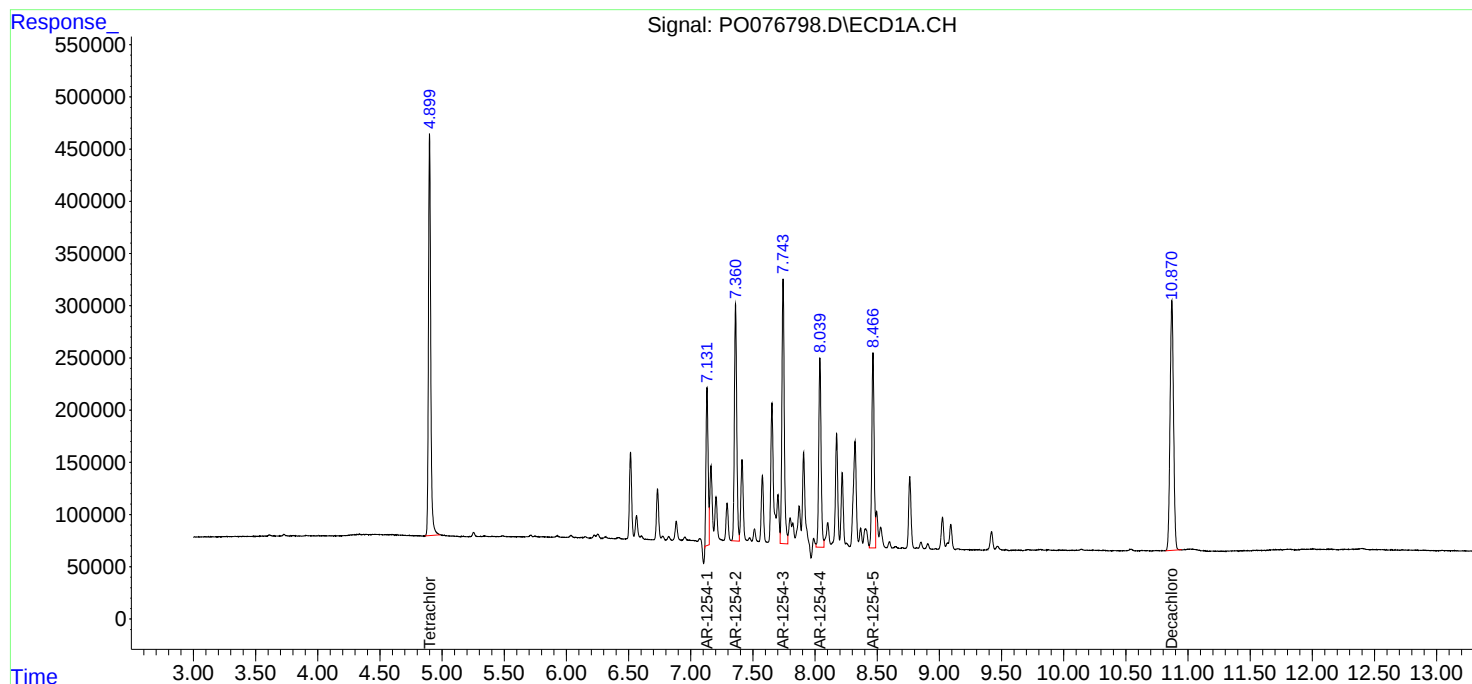

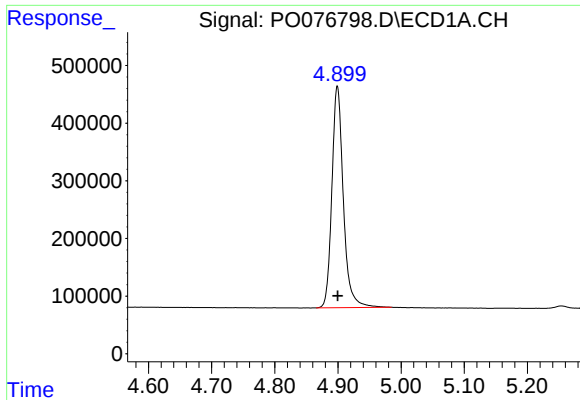


#1 Tetrachloro-m-xylene

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 4851254
Conc: 52.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/6/2021 2:58:16 PM

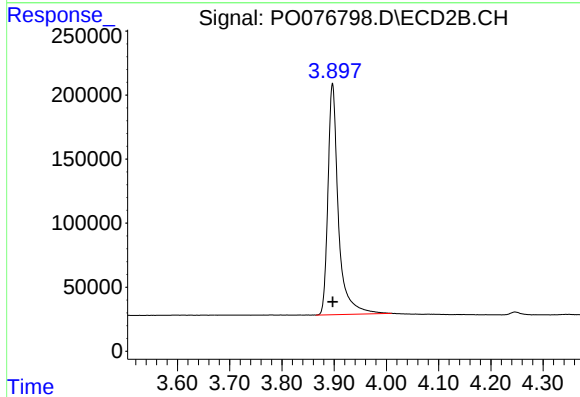


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 2507273
Conc: 49.96 ng/ml

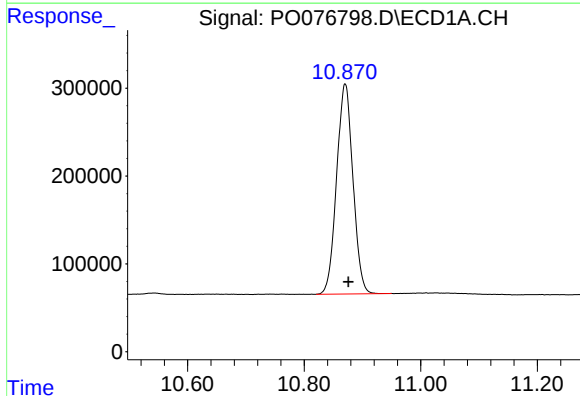


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.005 min
Response: 4654476
Conc: 50.25 ng/ml

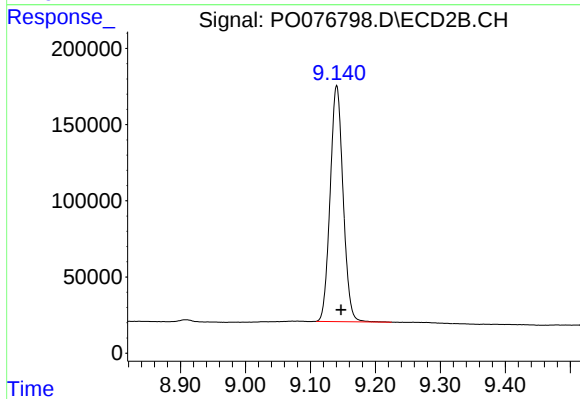

#2 Decachlorobiphenyl

R.T.: 9.141 min
Delta R.T.: -0.007 min
Response: 2140296
Conc: 44.11 ng/ml

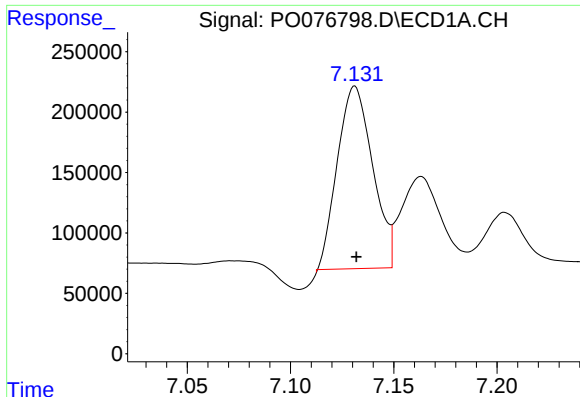


#26 AR-1254-1

R.T.: 7.131 min
Delta R.T.: -0.001 min
Response: 1801090
Conc: 566.64 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/6/2021 2:58:16 PM

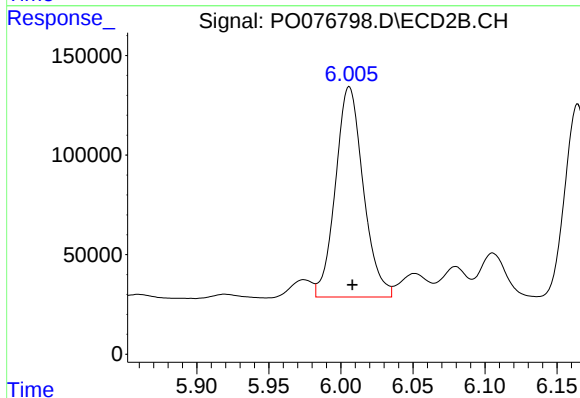


#26 AR-1254-1

R.T.: 6.005 min
Delta R.T.: -0.002 min
Response: 1418101
Conc: 541.03 ng/ml m

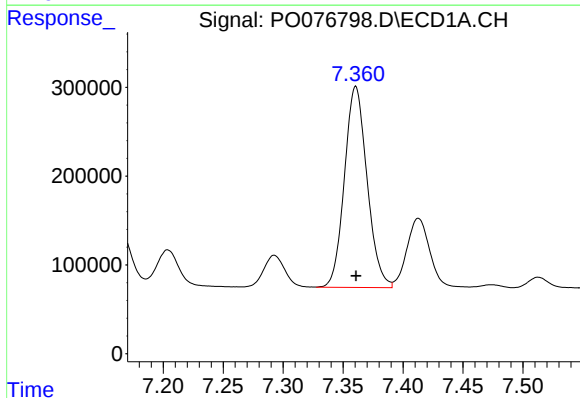


#27 AR-1254-2

R.T.: 7.361 min
Delta R.T.: 0.000 min
Response: 2971938
Conc: 580.04 ng/ml

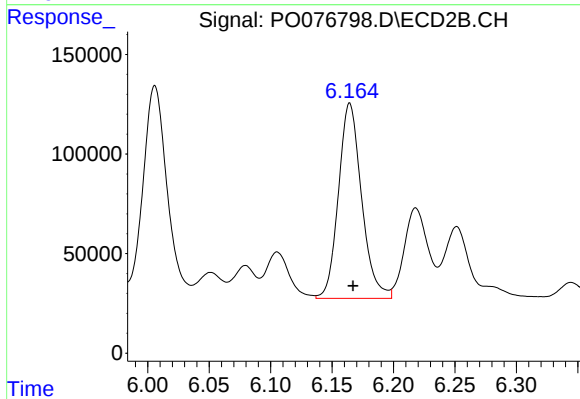

#27 AR-1254-2

R.T.: 6.164 min
Delta R.T.: -0.003 min
Response: 1284290
Conc: 560.82 ng/ml m

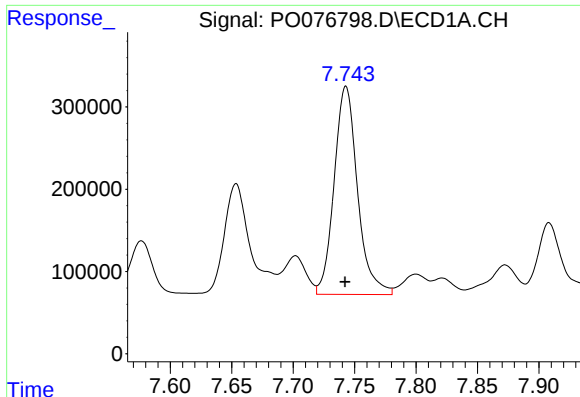


#28 AR-1254-3

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 3354709
Conc: 608.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/6/2021 2:58:16 PM

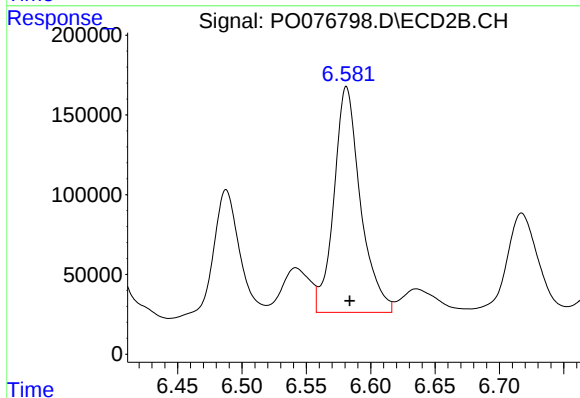


#28 AR-1254-3

R.T.: 6.581 min
Delta R.T.: -0.003 min
Response: 2032764
Conc: 575.16 ng/ml m

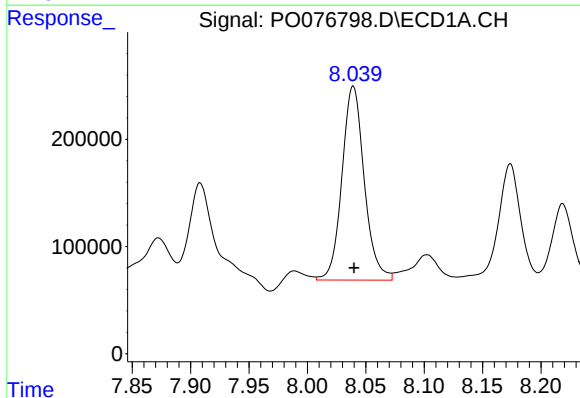


#29 AR-1254-4

R.T.: 8.039 min
Delta R.T.: 0.000 min
Response: 2402592
Conc: 610.22 ng/ml

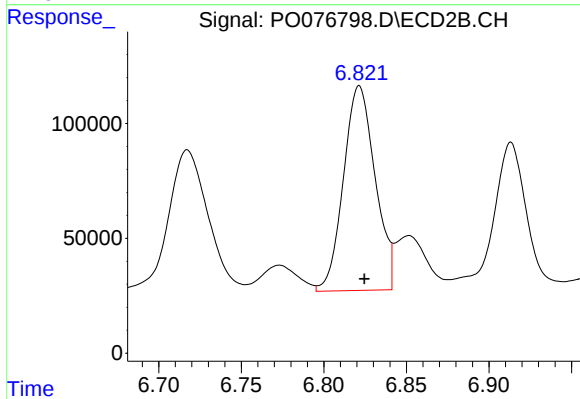

#29 AR-1254-4

R.T.: 6.821 min
Delta R.T.: -0.003 min
Response: 1200400
Conc: 571.98 ng/ml m

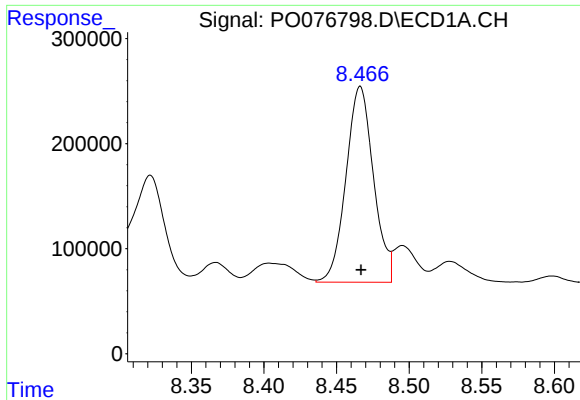


#30 AR-1254-5

R.T.: 8.466 min
Delta R.T.: 0.000 min
Response: 2455419
Conc: 558.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
4/6/2021 2:58:16 PM

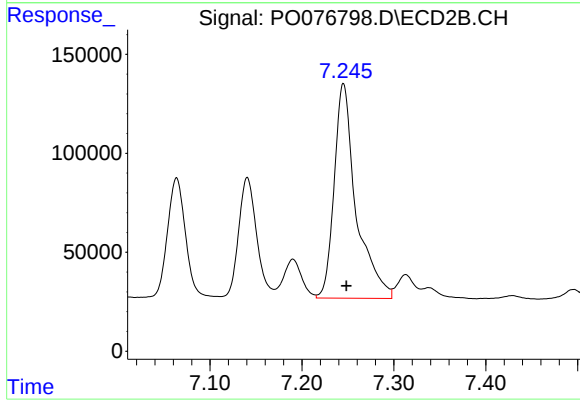

#30 AR-1254-5

R.T.: 7.245 min
Delta R.T.: -0.003 min
Response: 1798843
Conc: 551.79 ng/ml