

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040324\
 Data File : P0102696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 13:35
 Operator : YP/AJ
 Sample : P1962-03 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2308-003-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2024
 Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 16:52:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.379	6197978	3898350	1.406	1.355m
2) SA Decachlor...	9.799	8.242	3245584	2320220	1.169m	1.279

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040324\
Data File : PO102696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 13:35
Operator : YP/AJ
Sample : P1962-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2308-003-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 16:52:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

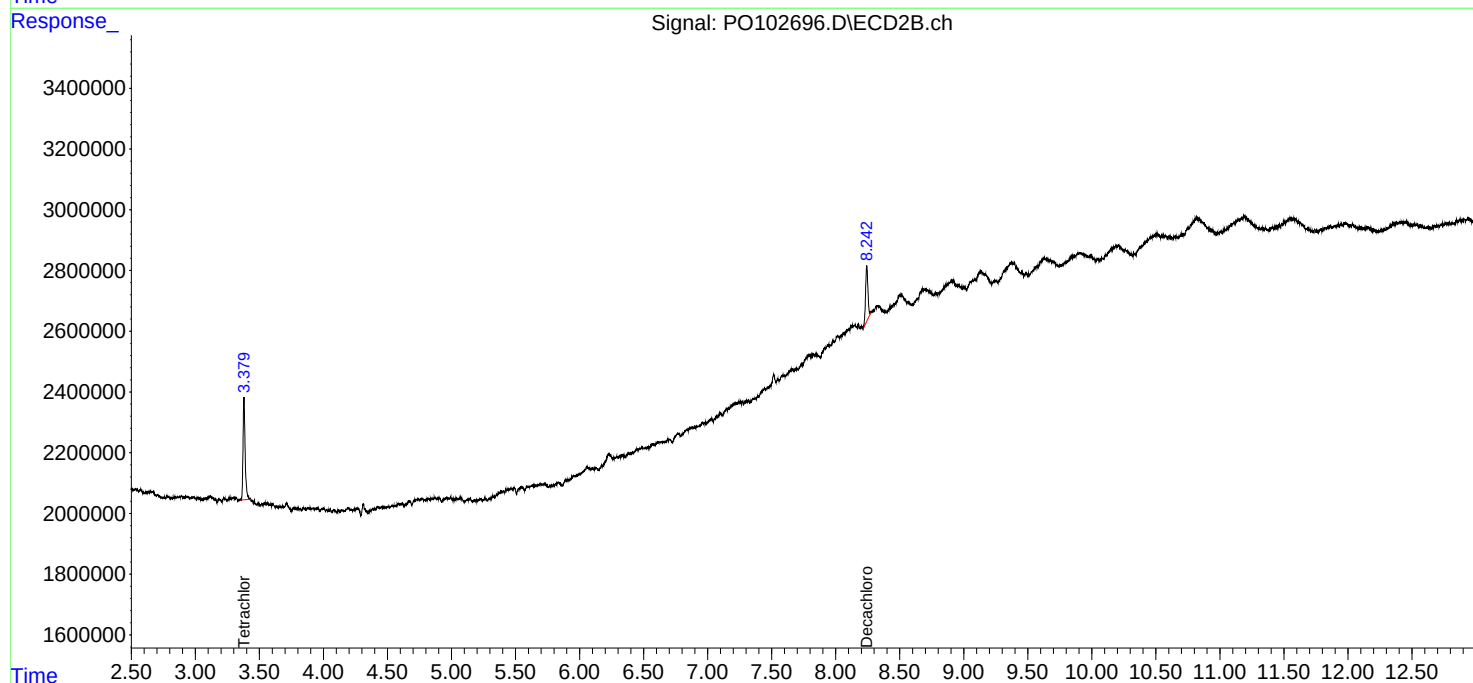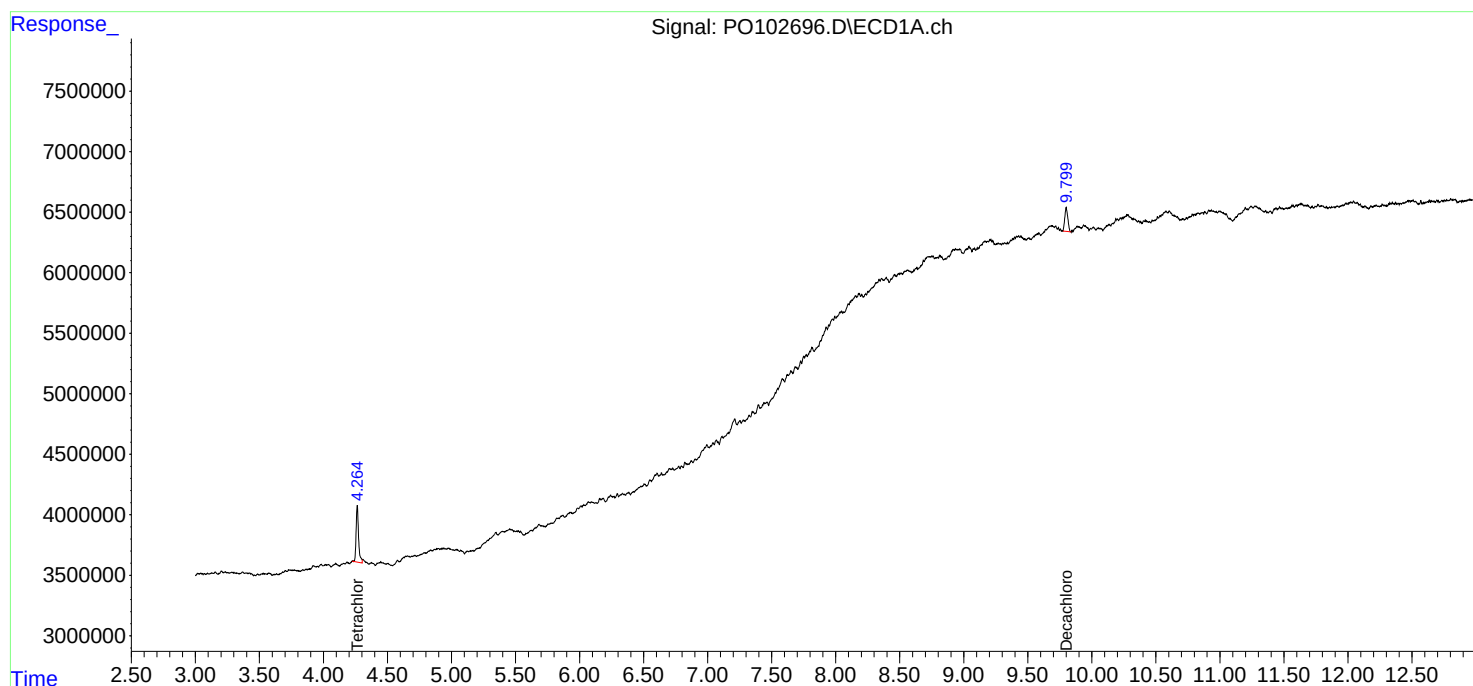

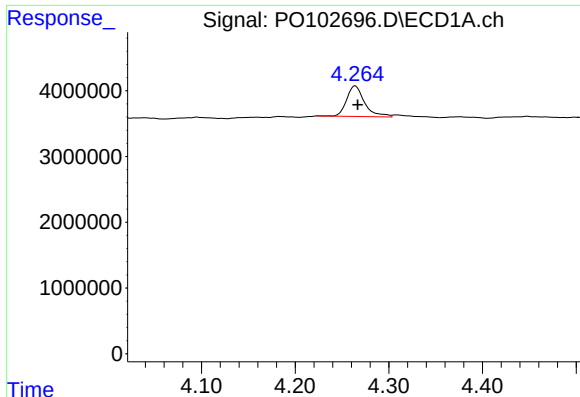


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.003 min
Response: 6197978
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2308-003-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

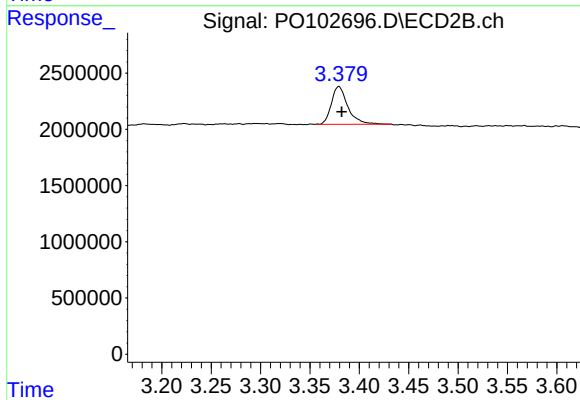


#1 Tetrachloro-m-xylene

R.T.: 3.379 min
Delta R.T.: -0.003 min
Response: 3898350
Conc: 1.35 ng/ml m

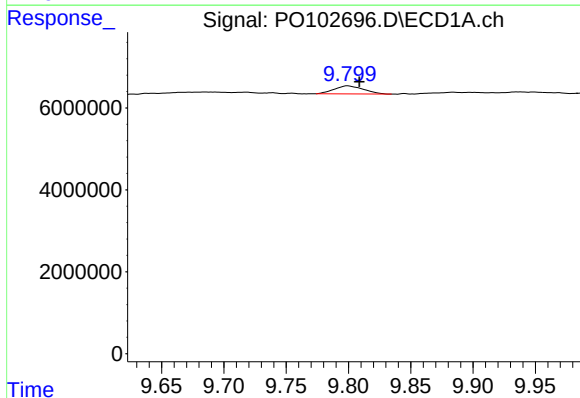

#2 Decachlorobiphenyl

R.T.: 9.799 min
Delta R.T.: -0.010 min
Response: 3245584
Conc: 1.17 ng/ml m

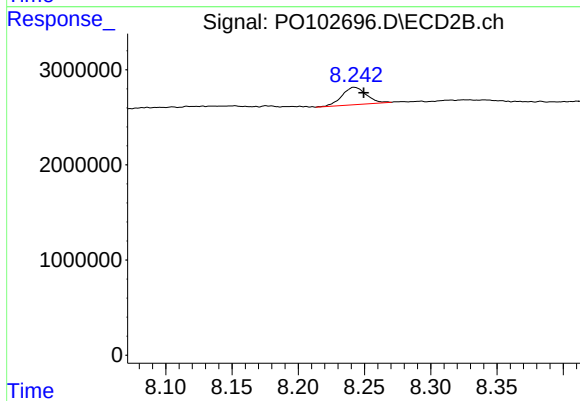

#2 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: -0.007 min
Response: 2320220
Conc: 1.28 ng/ml