

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040324\
 Data File : P0102697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 13:52
 Operator : YP/AJ
 Sample : P1962-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2308-003-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2024
 Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 16:52:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.378	7418142	4310966	1.683	1.498m
2) SA Decachlor...	9.800	8.243	4301655	3602841	1.549	1.986 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040324\
Data File : PO102697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 13:52
Operator : YP/AJ
Sample : P1962-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
Y2308-003-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 16:52:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

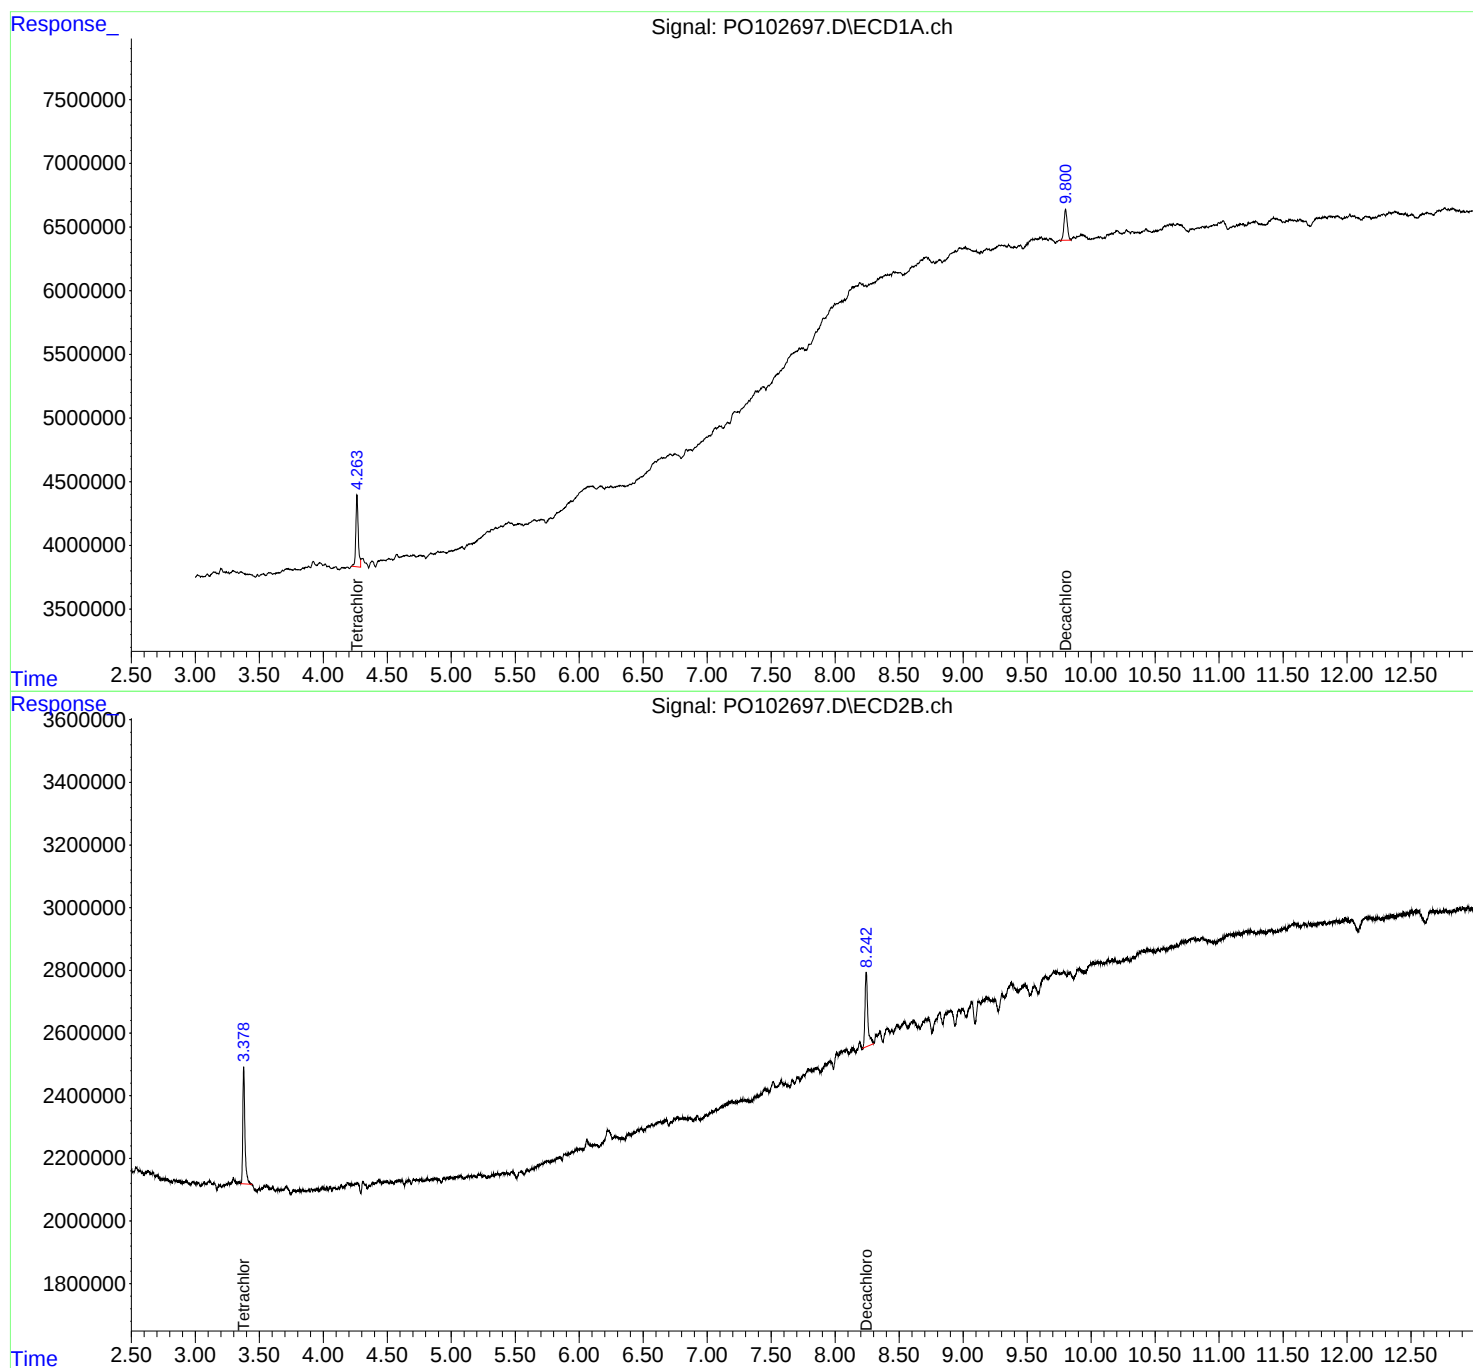

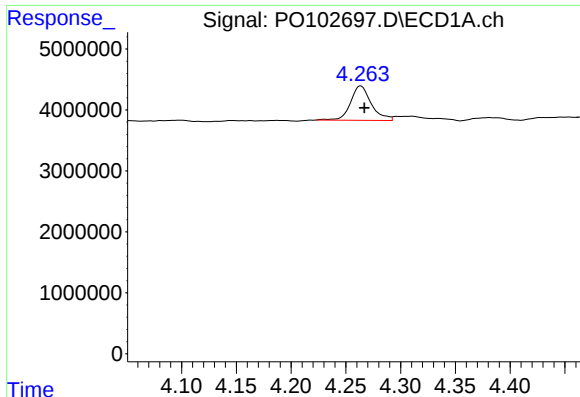


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.003 min
Response: 7418142
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2308-003-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

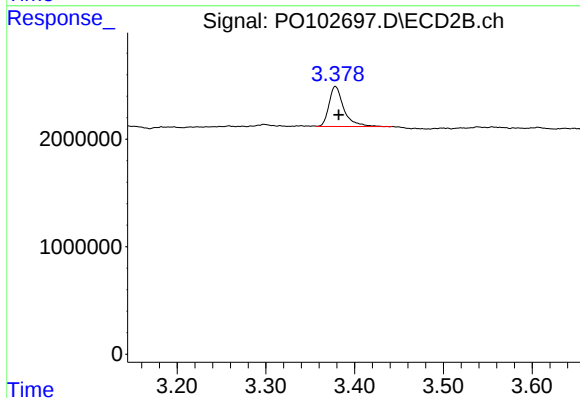


#1 Tetrachloro-m-xylene

R.T.: 3.378 min
Delta R.T.: -0.004 min
Response: 4310966
Conc: 1.50 ng/ml m

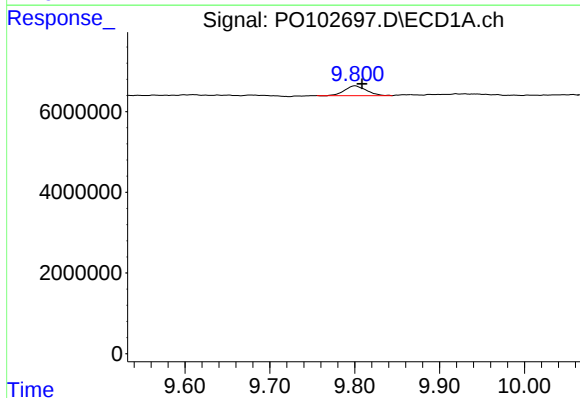

#2 Decachlorobiphenyl

R.T.: 9.800 min
Delta R.T.: -0.008 min
Response: 4301655
Conc: 1.55 ng/ml

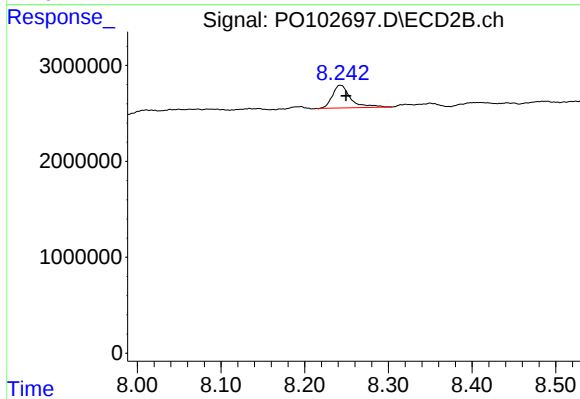

#2 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: -0.007 min
Response: 3602841
Conc: 1.99 ng/ml