

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040324\
 Data File : P0102703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 15:36
 Operator : YP/AJ
 Sample : P1962-05 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2310-0287-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2024
 Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 17:16:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.378	7912543	5477000	1.795	1.904m
2) SA Decachlor...	9.803	8.243	5071028	3085253	1.826	1.701

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040324\
Data File : PO102703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 15:36
Operator : YP/AJ
Sample : P1962-05 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2310-0287-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 17:16:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

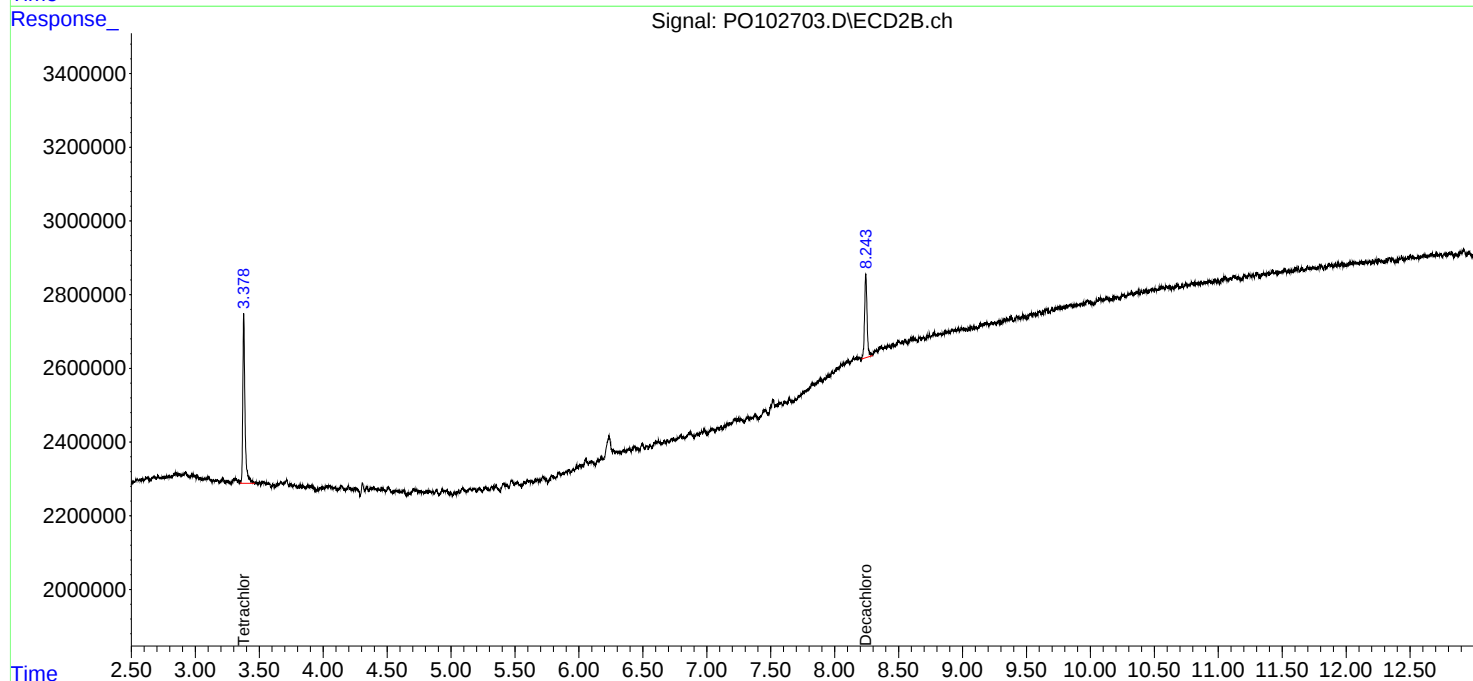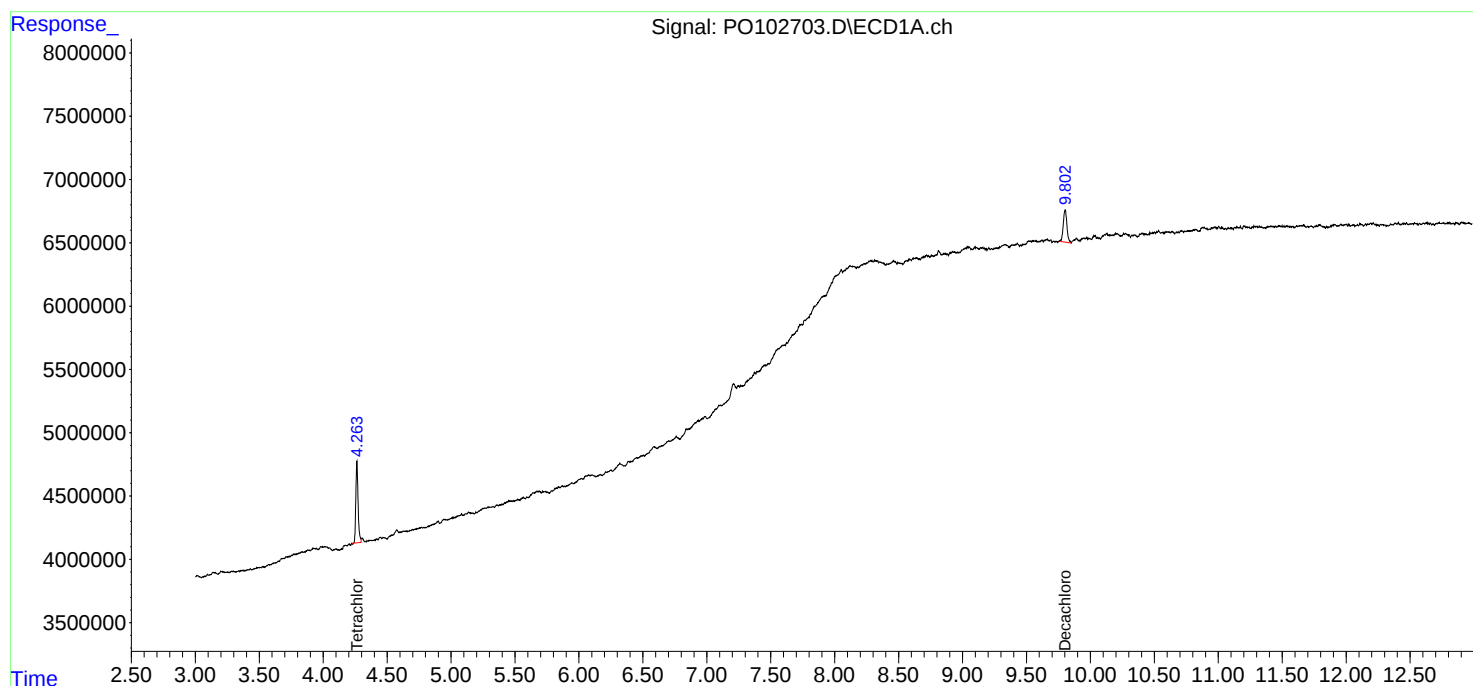

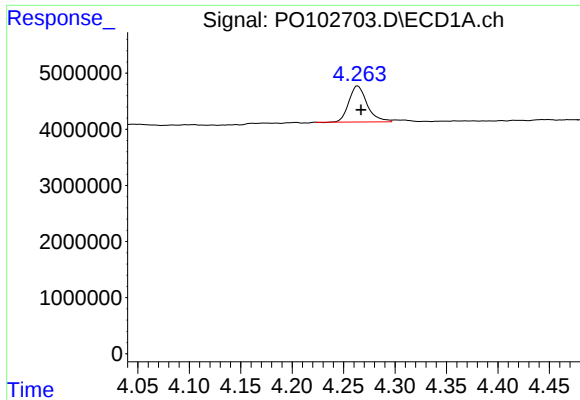


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.003 min
Response: 7912543
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2310-0287-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

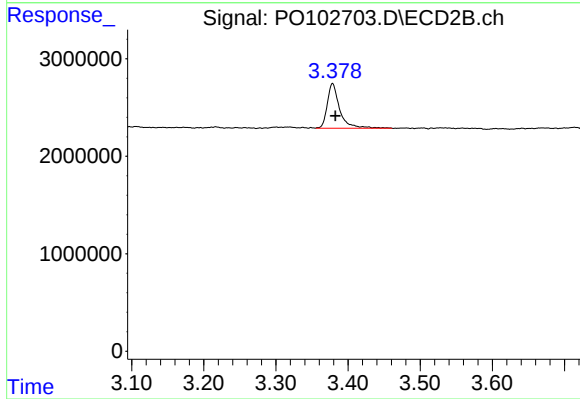


#1 Tetrachloro-m-xylene

R.T.: 3.378 min
Delta R.T.: -0.004 min
Response: 5477000
Conc: 1.90 ng/ml m

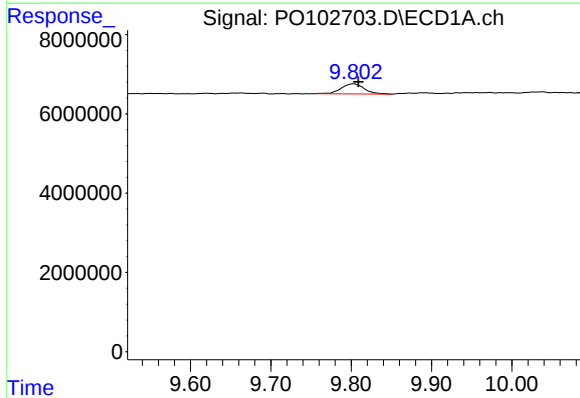

#2 Decachlorobiphenyl

R.T.: 9.803 min
Delta R.T.: -0.006 min
Response: 5071028
Conc: 1.83 ng/ml

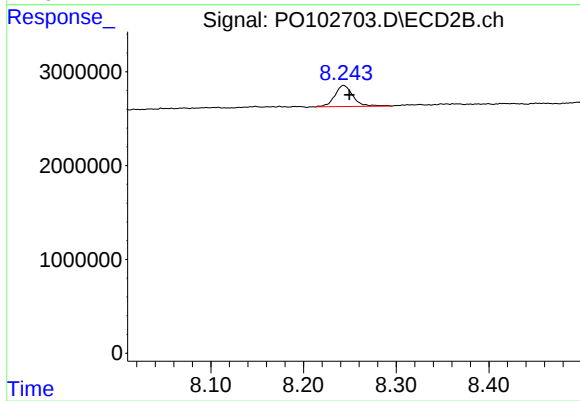

#2 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: -0.006 min
Response: 3085253
Conc: 1.70 ng/ml