

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040324\
 Data File : P0102705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2024 16:10
 Operator : YP/AJ
 Sample : P1962-07 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2308-0013-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2024
 Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 17:17:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.378	7829804	4751261	1.776	1.651m
2) SA Decachlor...	9.802	8.245	4200735	2962564	1.513	1.633

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040324\
Data File : PO102705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2024 16:10
Operator : YP/AJ
Sample : P1962-07 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2308-0013-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 17:17:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

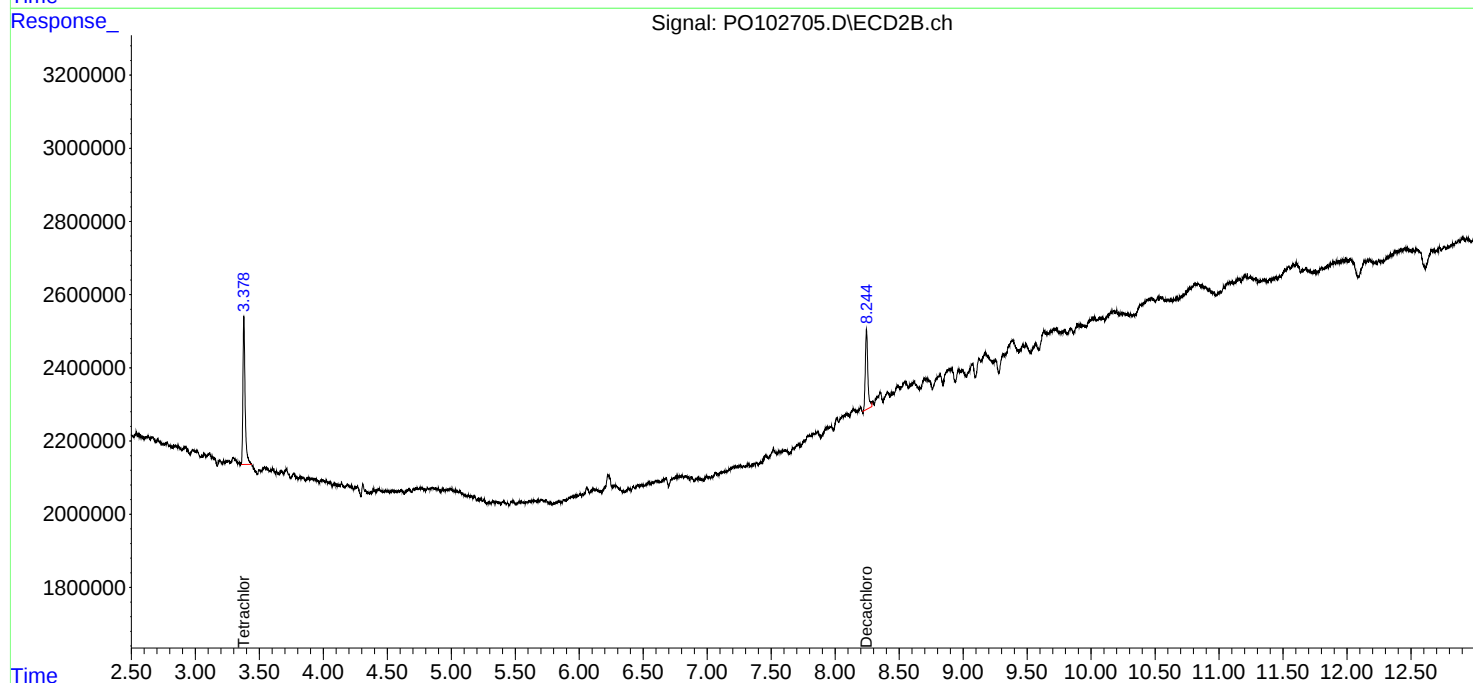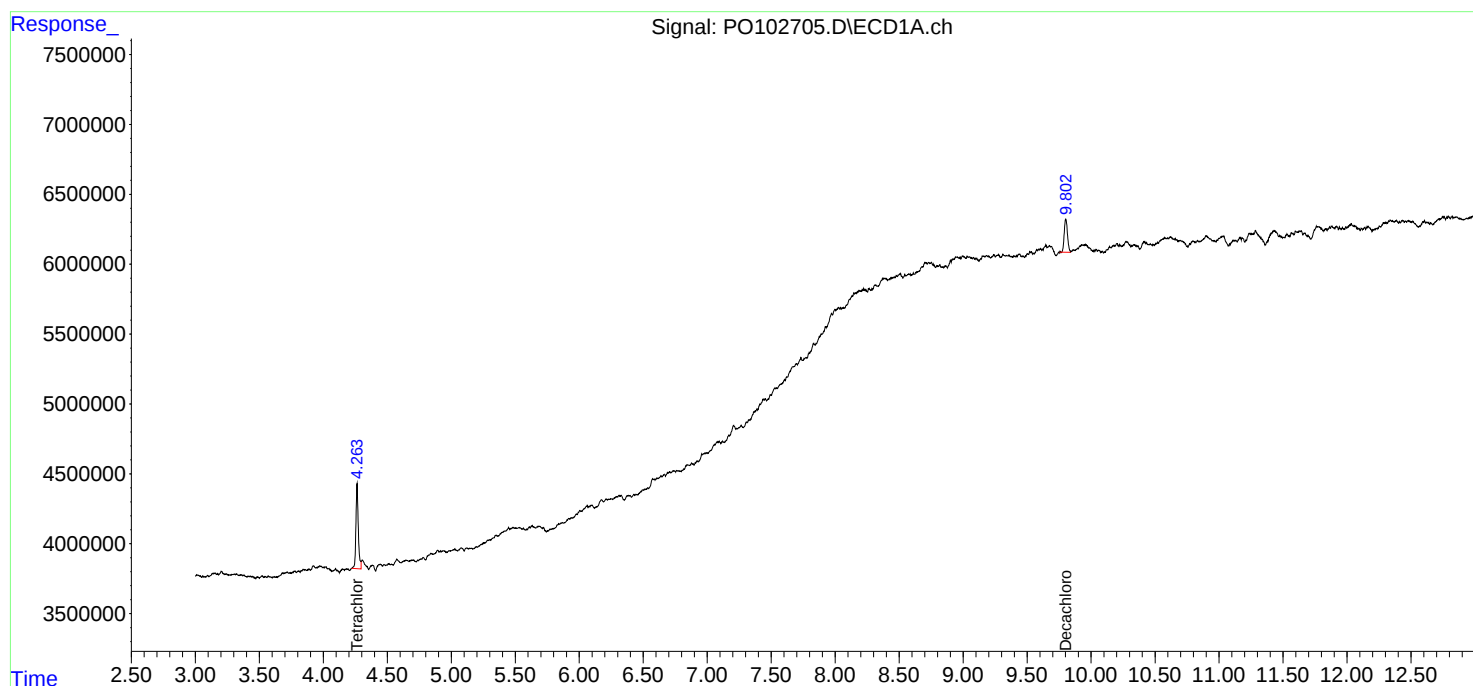

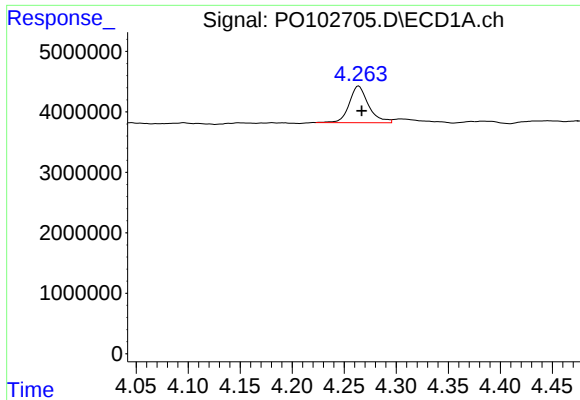


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.003 min
Response: 7829804
Conc: 1.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2308-0013-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2024
Supervised By :Ankita Jodhani 04/04/2024

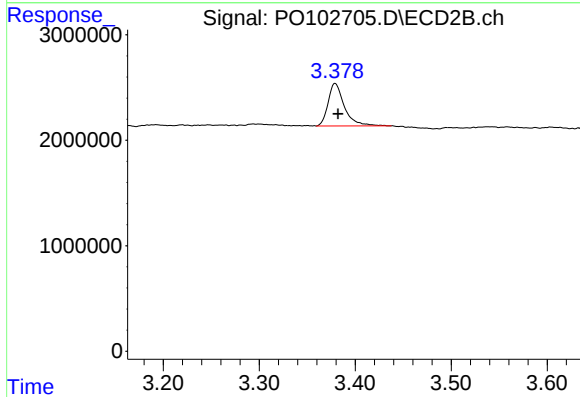


#1 Tetrachloro-m-xylene

R.T.: 3.378 min
Delta R.T.: -0.004 min
Response: 4751261
Conc: 1.65 ng/ml m

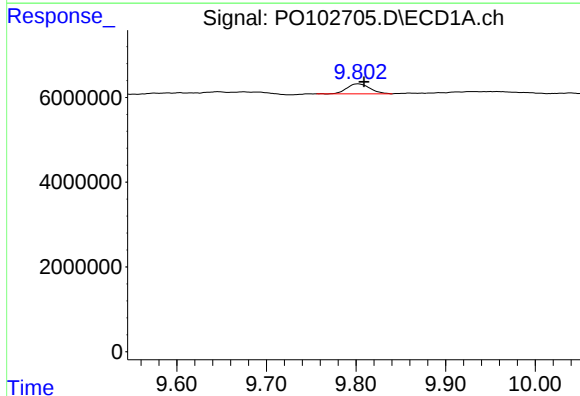

#2 Decachlorobiphenyl

R.T.: 9.802 min
Delta R.T.: -0.006 min
Response: 4200735
Conc: 1.51 ng/ml

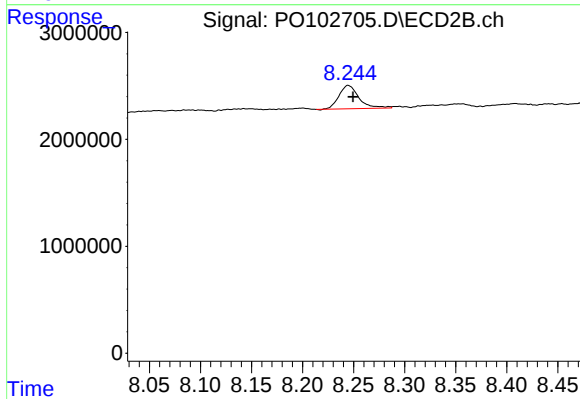

#2 Decachlorobiphenyl

R.T.: 8.245 min
Delta R.T.: -0.005 min
Response: 2962564
Conc: 1.63 ng/ml