

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040422\
 Data File : P0085858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2022 14:38
 Operator : YP\AJ
 Sample : N2207-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220349-AMENDED-096-21-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:22:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.583	4503467	1061443	23.110	22.443
2) SA Decachlor...	10.390	8.601	2494258	640086	19.438	18.231

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040422\
Data File : P0085858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2022 14:38
Operator : YP\AJ
Sample : N2207-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220349-AMENDED-096-21-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:22:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

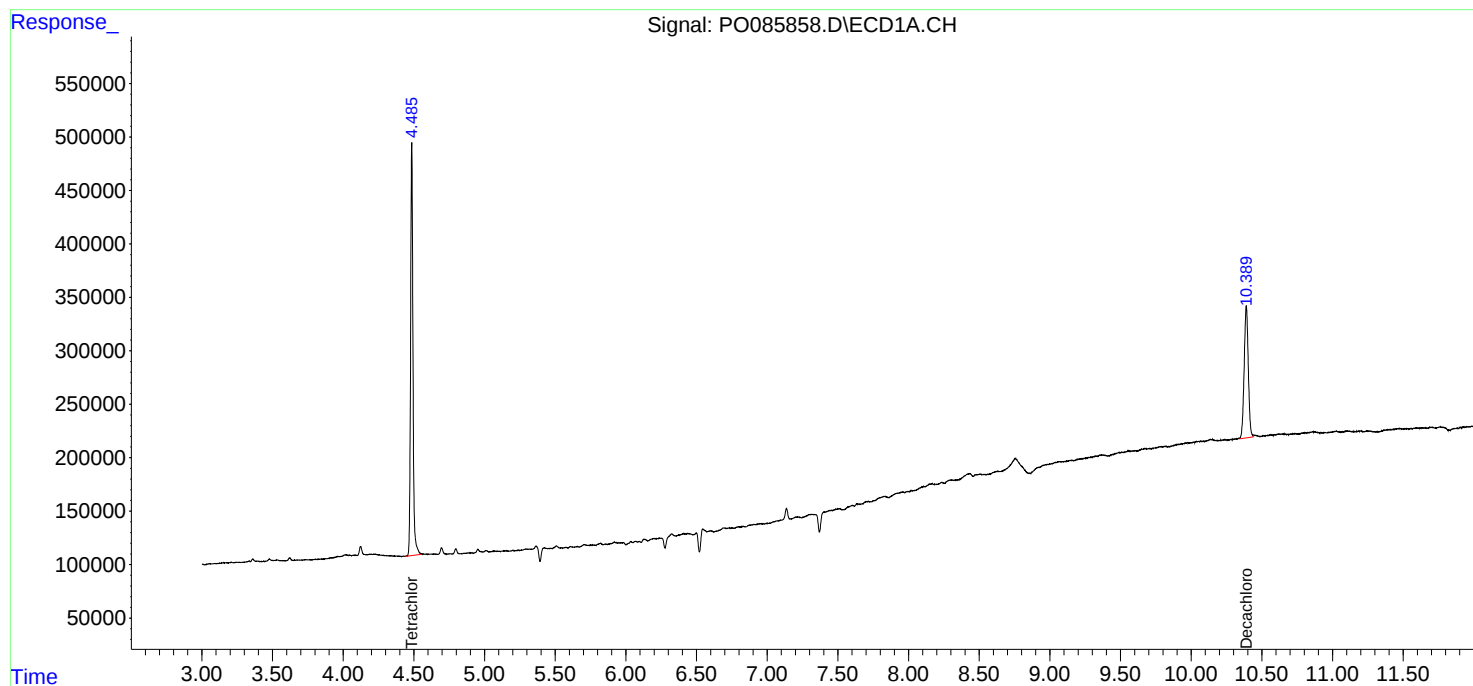


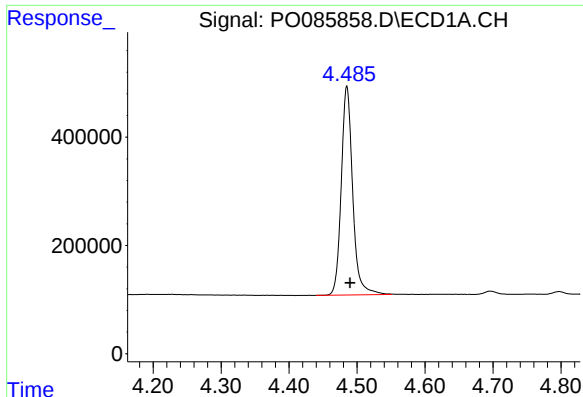

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.005 min
Response: 4503467
Conc: 23.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220349-AMENDED-096-21-01

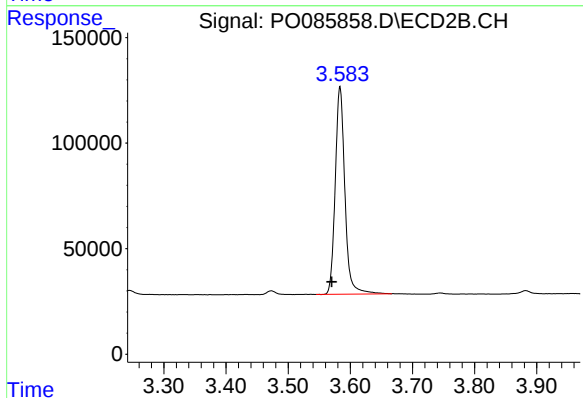


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: 0.013 min
Response: 1061443
Conc: 22.44 ng/ml

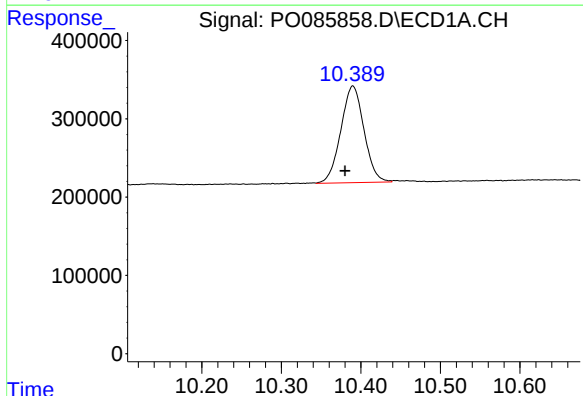

#2 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: 0.010 min
Response: 2494258
Conc: 19.44 ng/ml

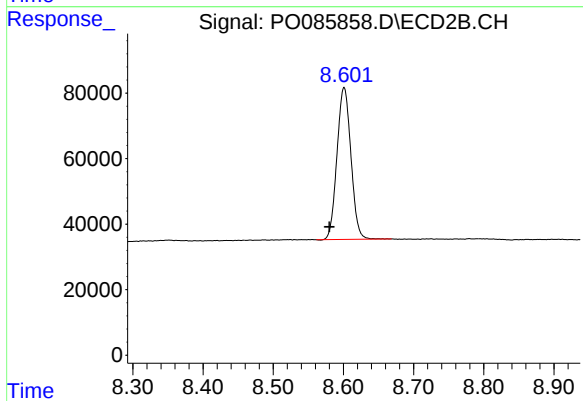

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: 0.021 min
Response: 640086
Conc: 18.23 ng/ml