

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040422\
 Data File : P0085877.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Apr 2022 21:52
 Operator : YP\AJ
 Sample : N2241-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-040122

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:48:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.482	3.581	3776133	924489	19.378	19.547
2)	SA Decachlor...	10.385	8.599	2827058	638040	22.032	18.172

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040422\
Data File : P0085877.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Apr 2022 21:52
Operator : YP\AJ
Sample : N2241-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-040122

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:48:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

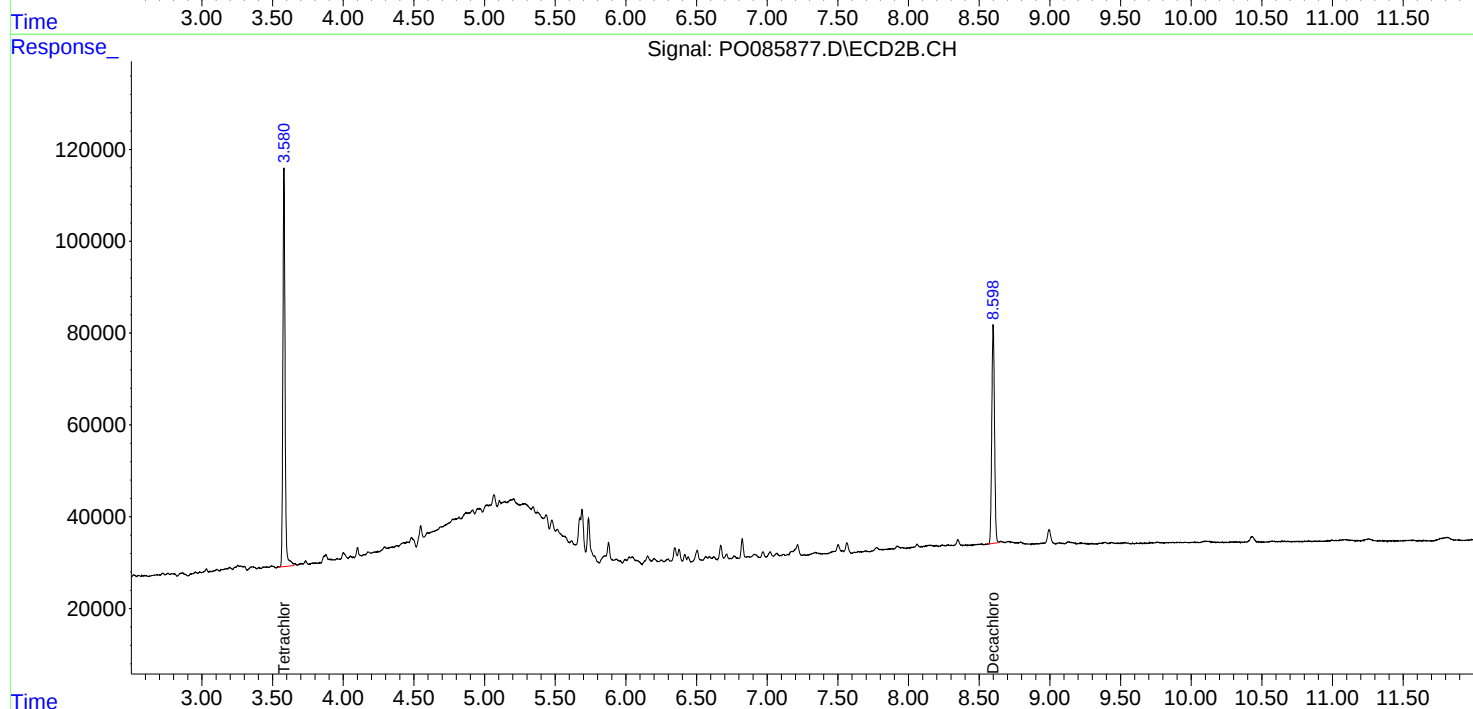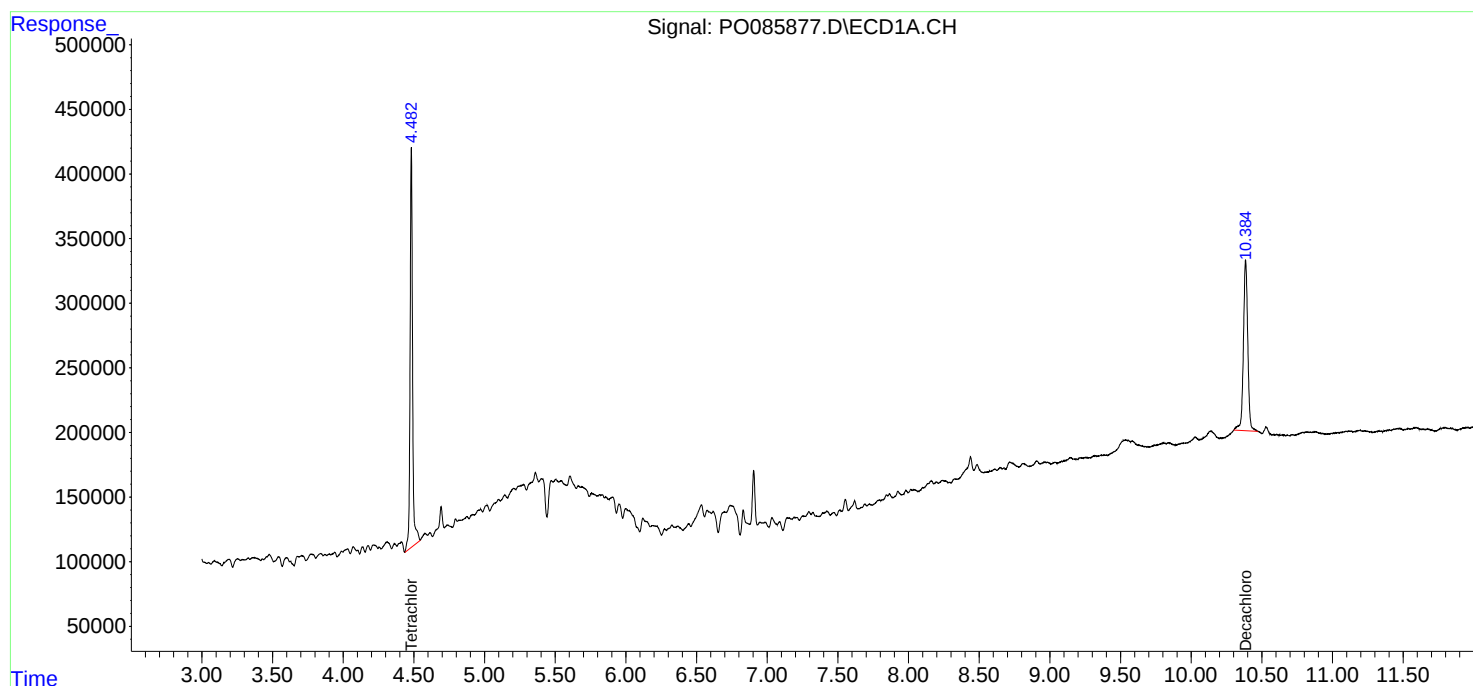


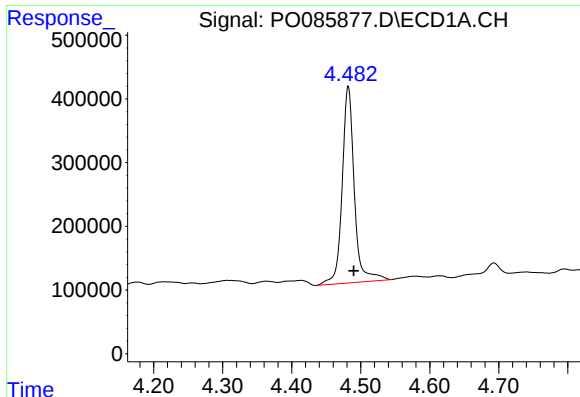

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: -0.008 min
Response: 3776133
Conc: 19.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-040122

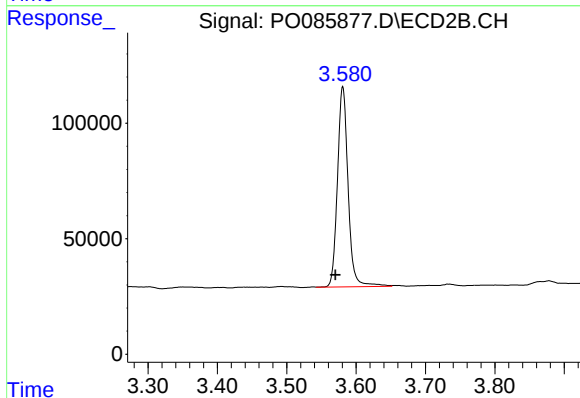


#1 Tetrachloro-m-xylene

R.T.: 3.581 min
Delta R.T.: 0.011 min
Response: 924489
Conc: 19.55 ng/ml

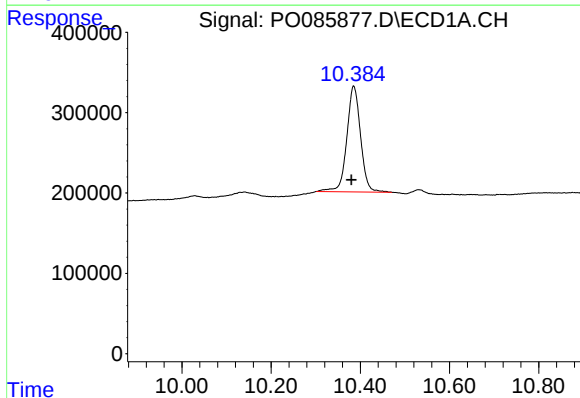

#2 Decachlorobiphenyl

R.T.: 10.385 min
Delta R.T.: 0.005 min
Response: 2827058
Conc: 22.03 ng/ml

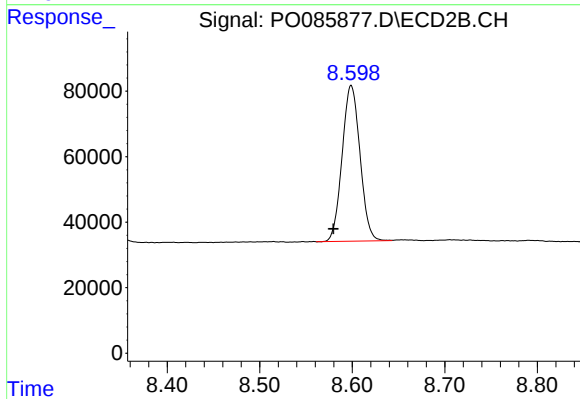

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: 0.019 min
Response: 638040
Conc: 18.17 ng/ml