

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040422\
 Data File : P0085887.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2022 8:36
 Operator : YP\AJ
 Sample : N2234-12 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOM-2022-16B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 12:23:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.588	326759	83810	1.677	1.772
2) SA Decachlor...	10.399	8.605	354955	70436	2.766	2.006 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040422\
Data File : PO085887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2022 8:36
Operator : YP\AJ
Sample : N2234-12 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOM-2022-16B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 12:23:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

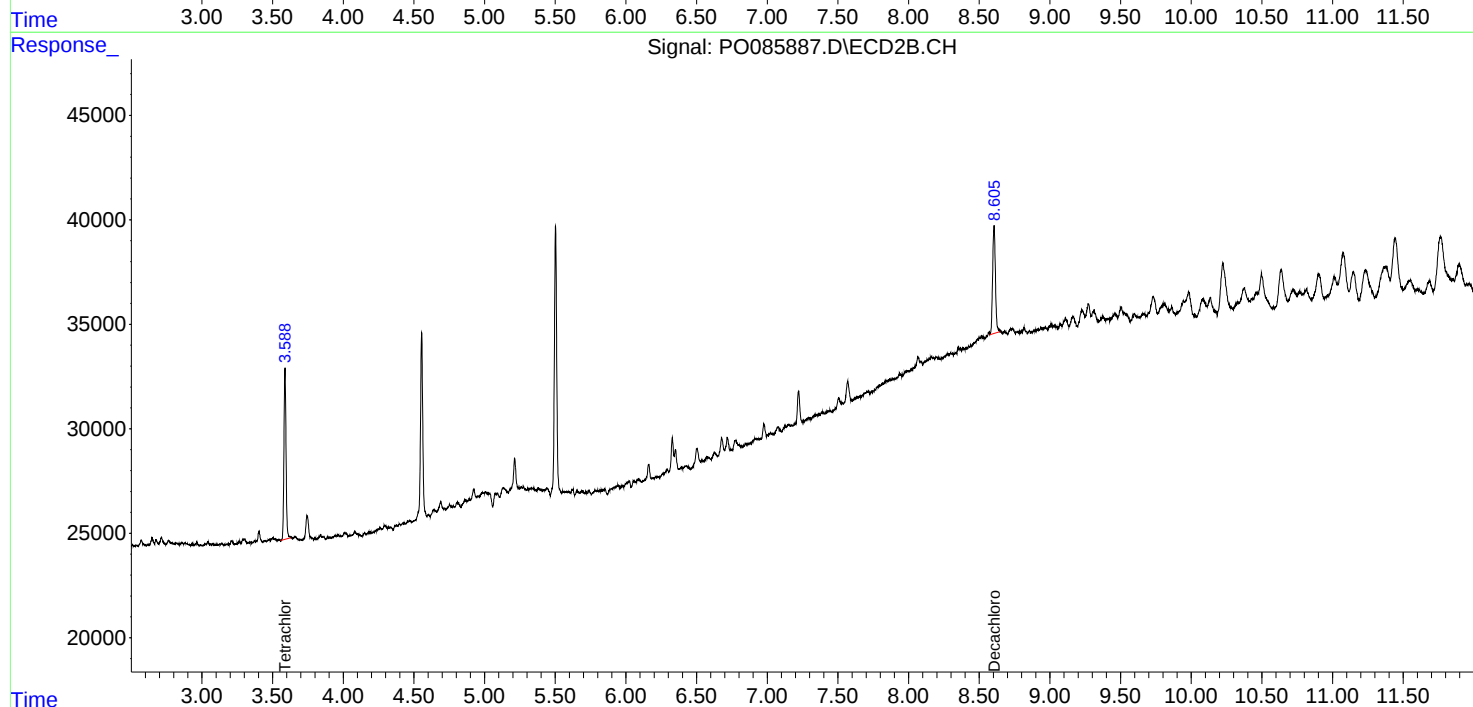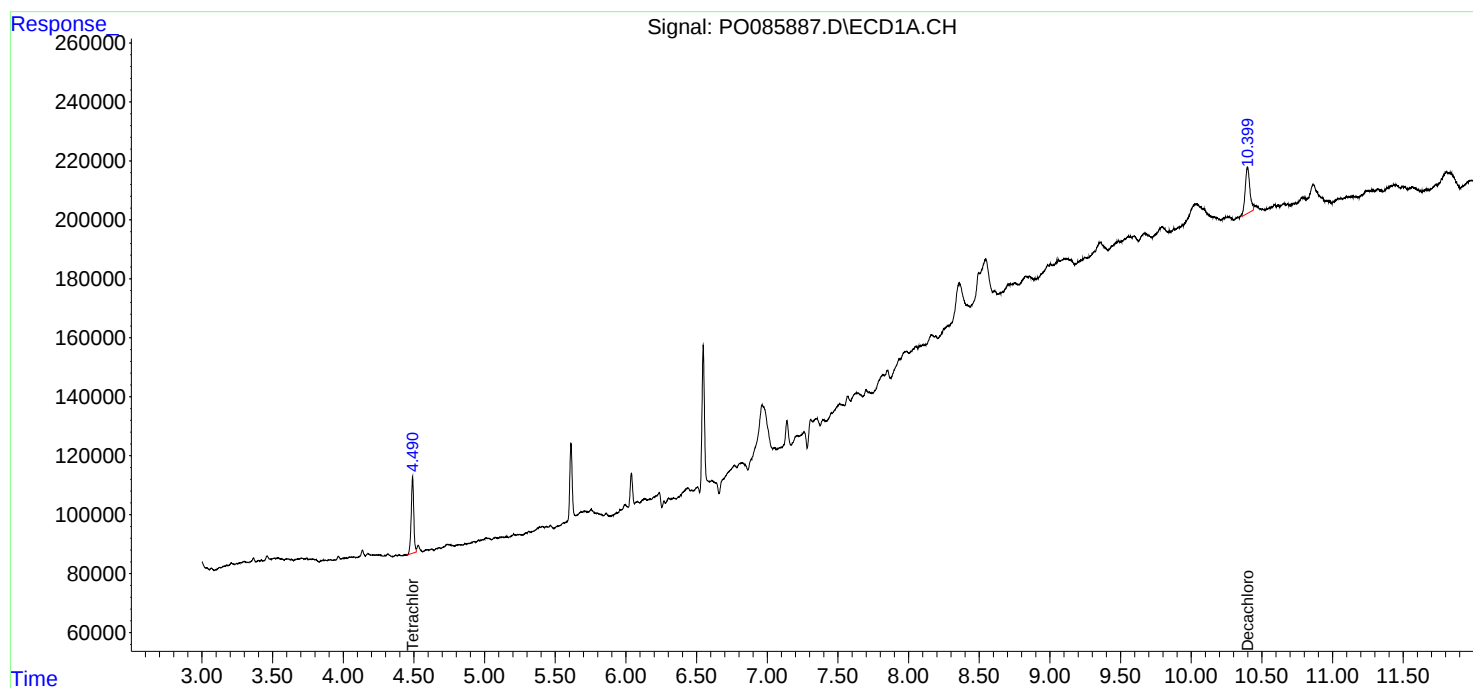


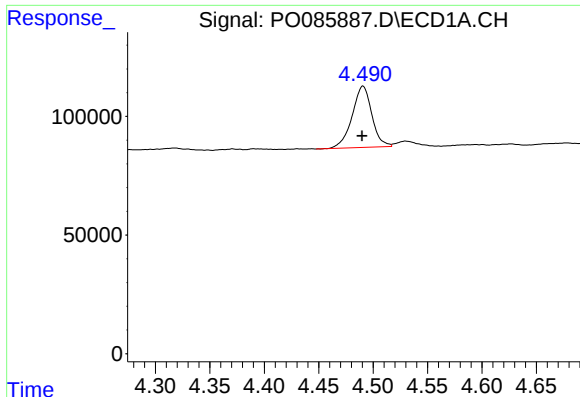

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 326759
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOM-2022-16B

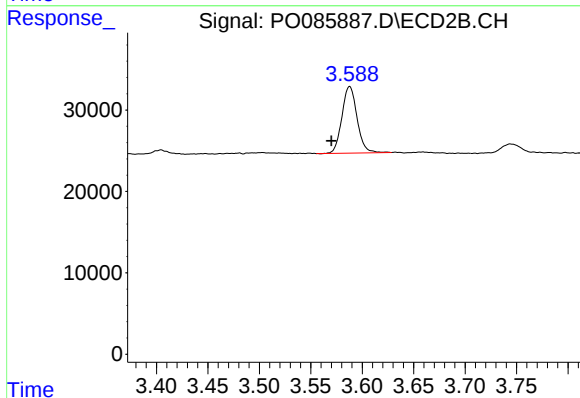


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: 0.018 min
Response: 83810
Conc: 1.77 ng/ml

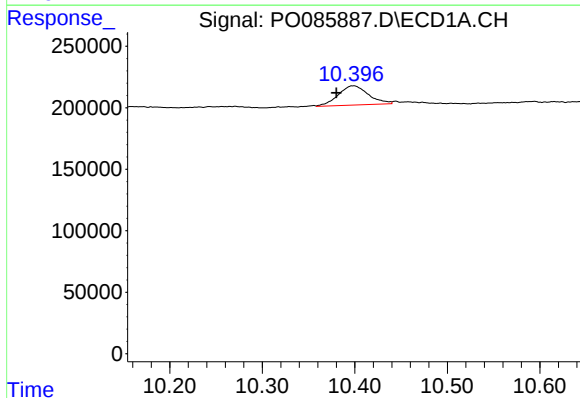

#2 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: 0.019 min
Response: 354955
Conc: 2.77 ng/ml

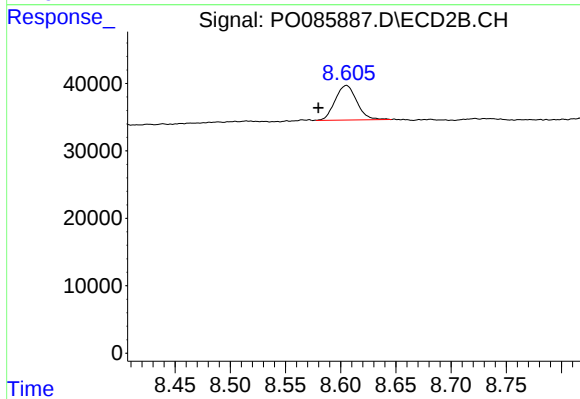

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: 0.025 min
Response: 70436
Conc: 2.01 ng/ml