

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040423\
 Data File : P0093788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2023 15:18
 Operator : YP/AJ
 Sample : 02173-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33972

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/05/2023
 Supervised By :Ankita Jodhani 04/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 21:59:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.629	75240381	27845620	20.127	21.867m
2) SA Decachlor...	10.254	8.653	53676686	22852000	23.996	22.857

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040423\
Data File : P0093788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2023 15:18
Operator : YP/AJ
Sample : 02173-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33972


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2023
Supervised By :Ankita Jodhani 04/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 21:59:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

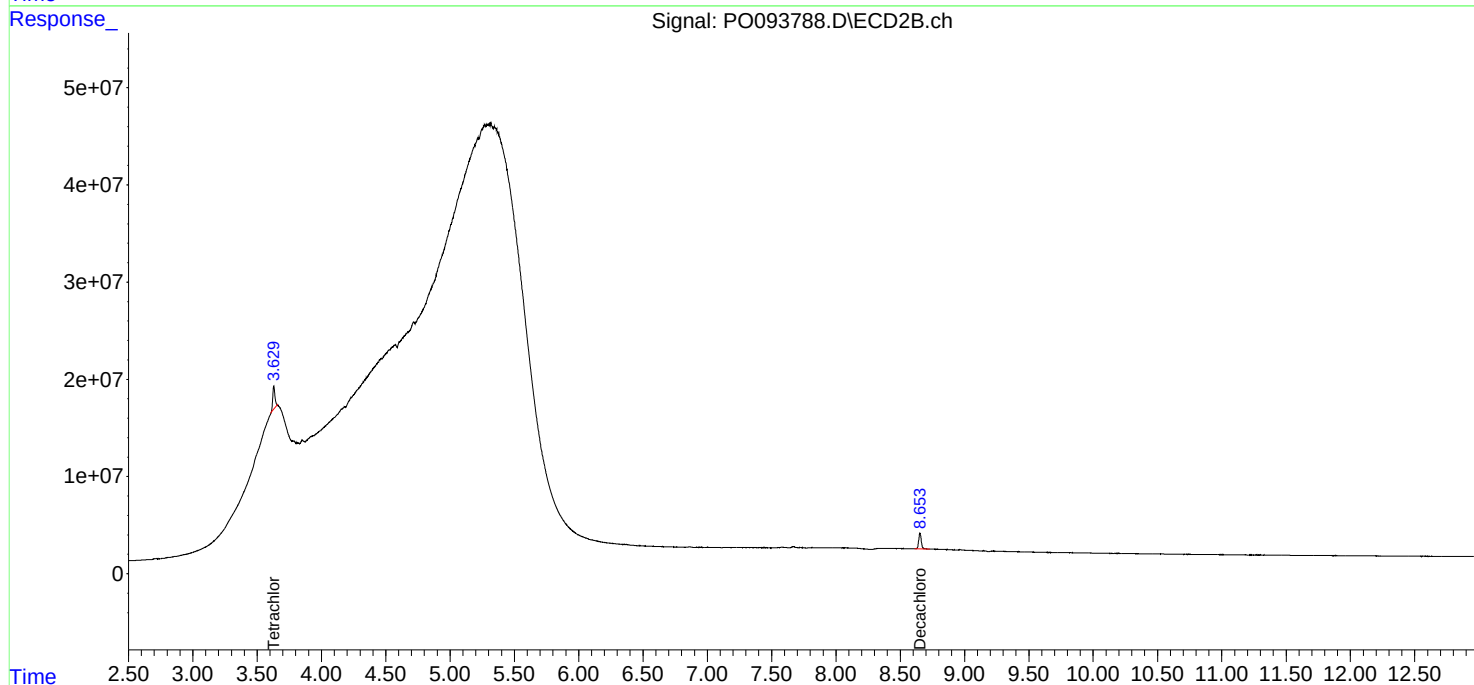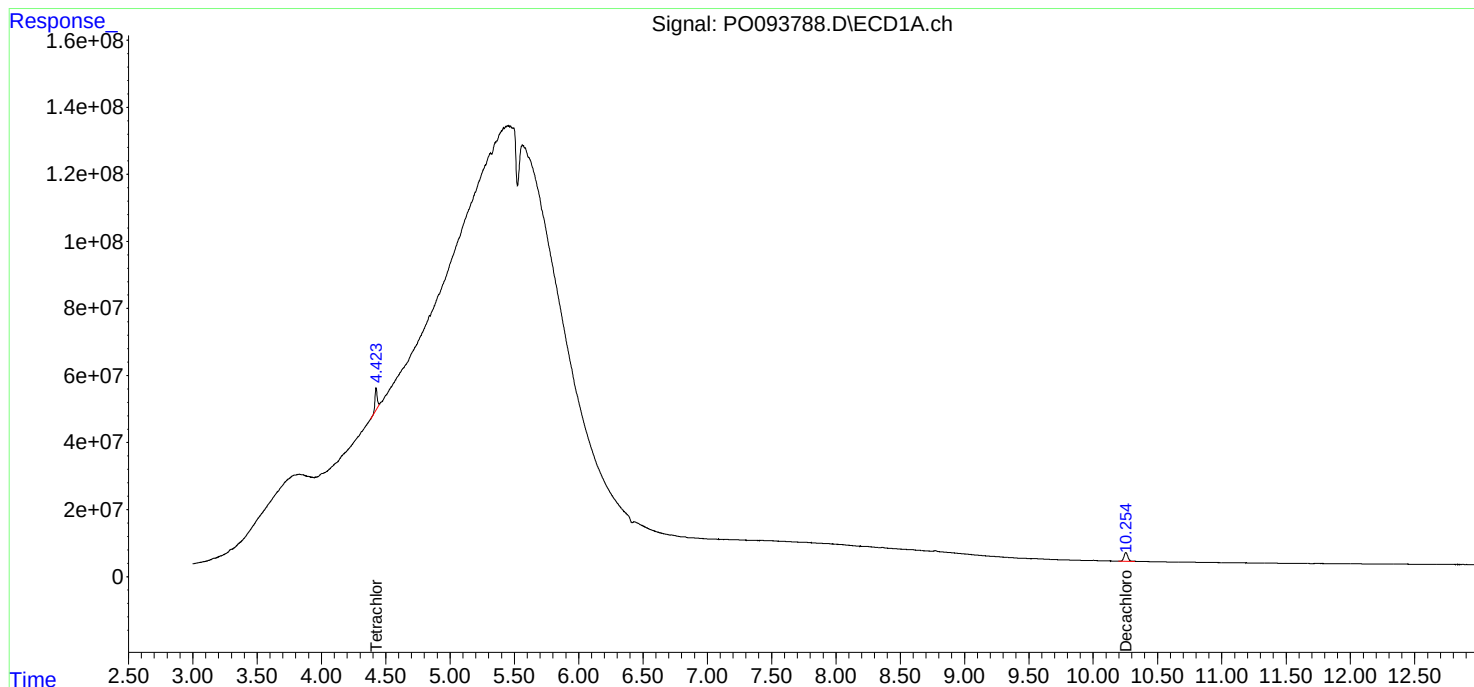

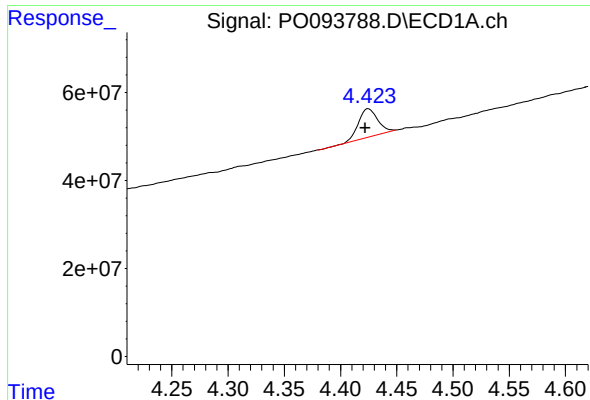

#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.003 min
Response: 75240381
Conc: 20.13 ng/ml


Instrument :

ECD_O

ClientSampleId :
33972


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2023
Supervised By :Ankita Jodhani 04/05/2023

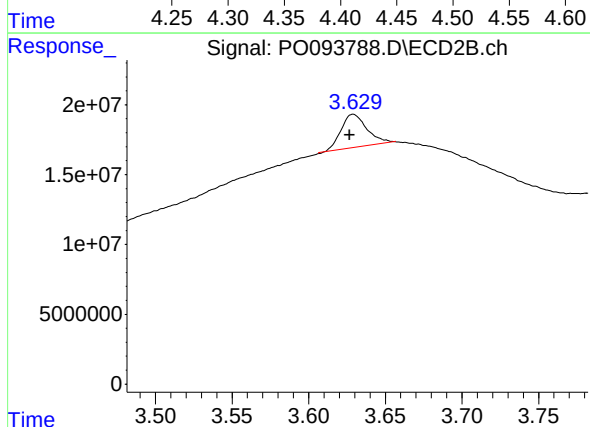


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: 0.002 min
Response: 27845620
Conc: 21.87 ng/ml

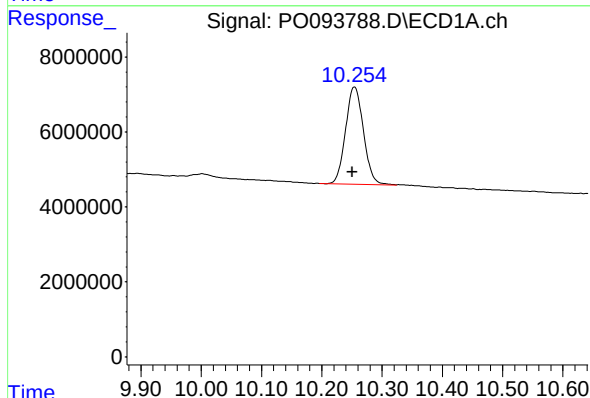

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: 0.004 min
Response: 53676686
Conc: 24.00 ng/ml

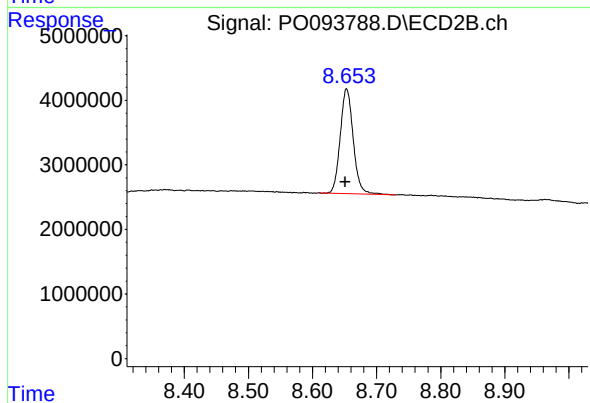

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: 0.002 min
Response: 22852000
Conc: 22.86 ng/ml